


tR = [1,6167 min]
Intensity [%]
100
80
60
40
20
0
200
210
220
230
240
250
260
270
280
290
300
Wavelength [nm]

Chromatogram

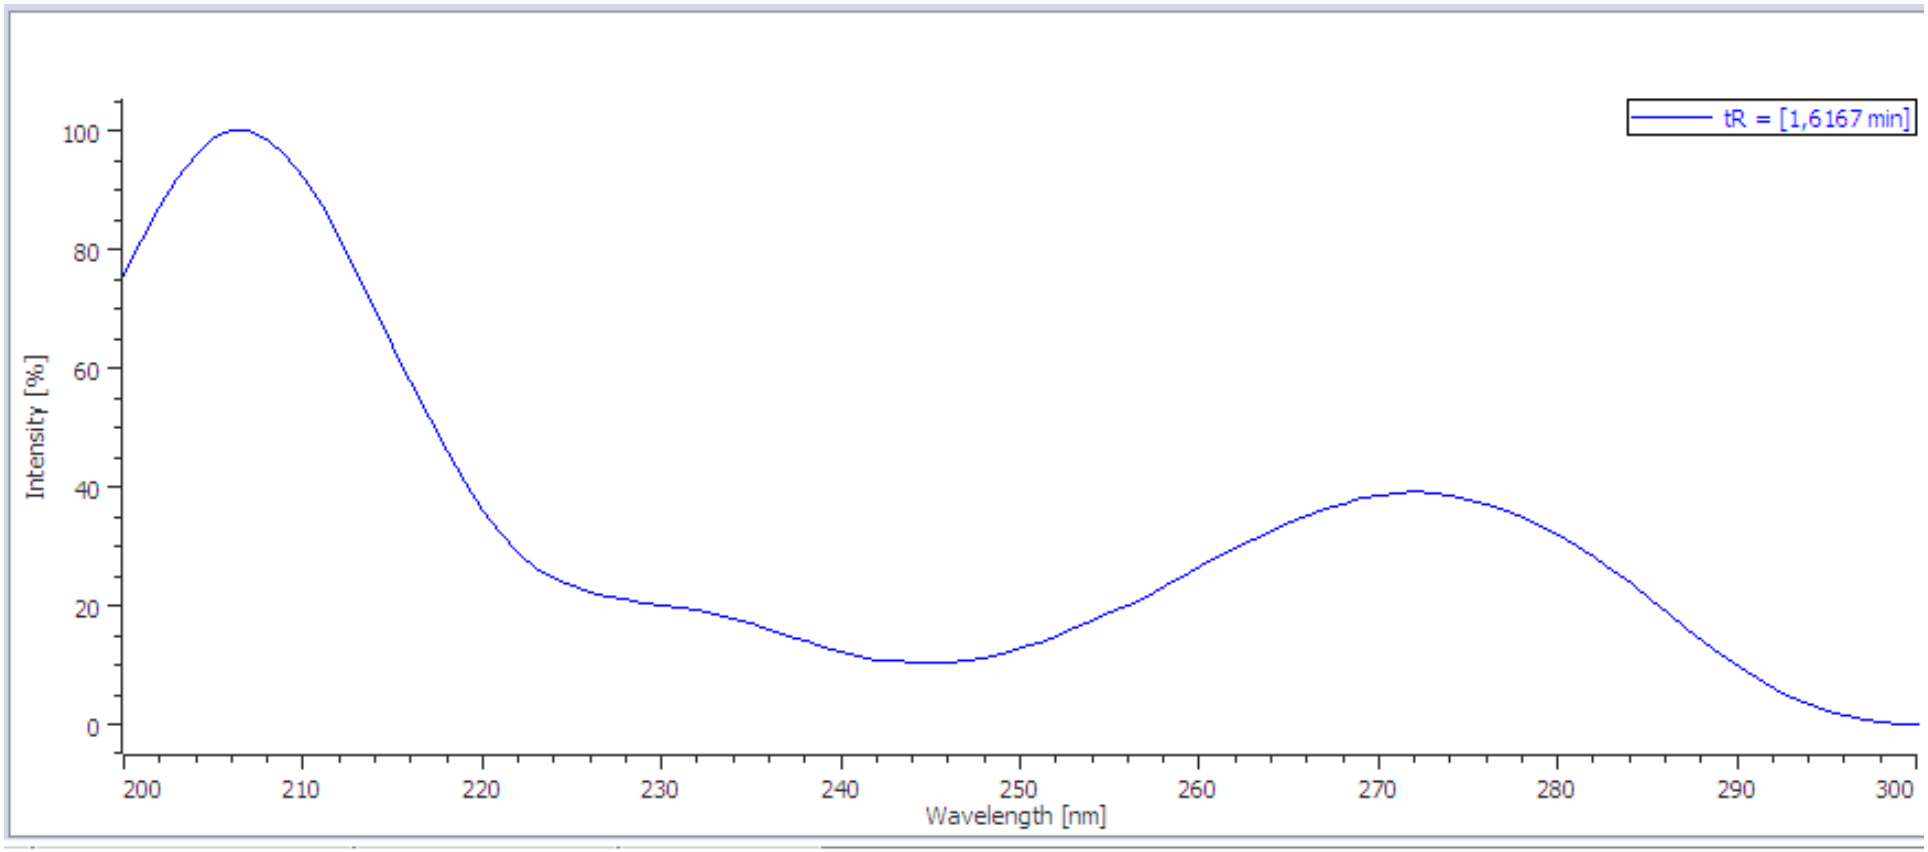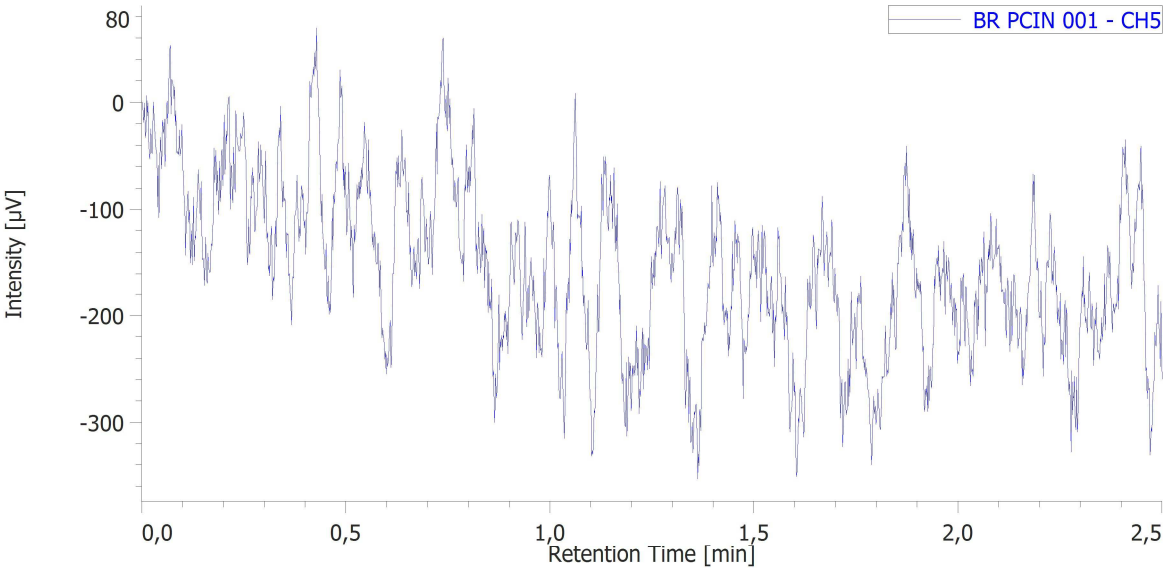


Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 13:41:01
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:38:29
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

Creator
Reviewer
Approver

Chromatogram

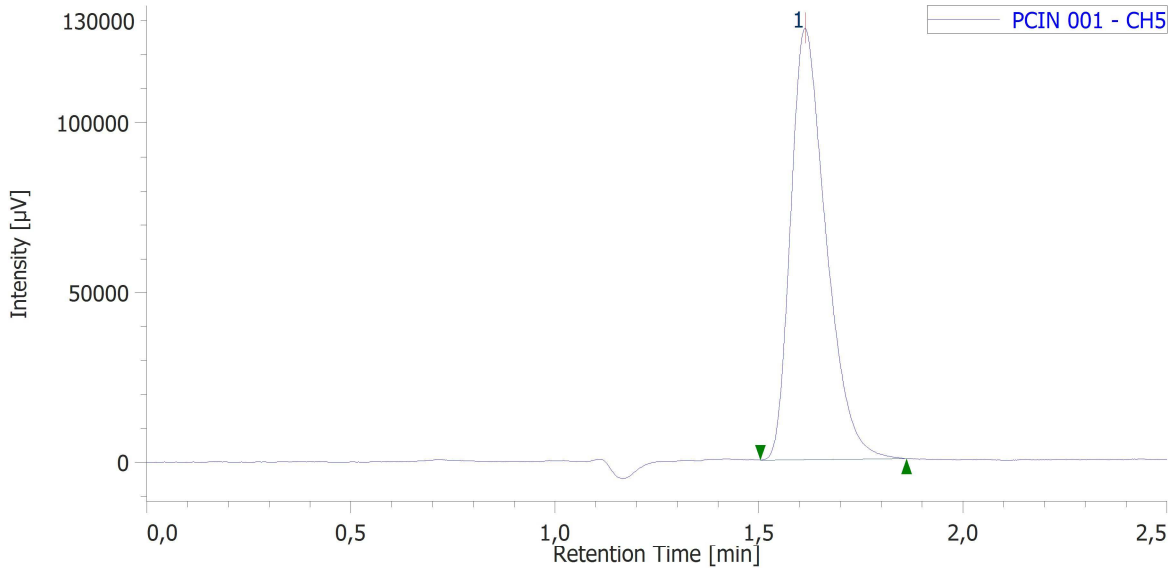

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 13:43:43
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:41:12
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	765952	126969	100,000	100,000	N/A	1703	N/A	1,393	

Creator
Reviewer
Approver

Chromatogram

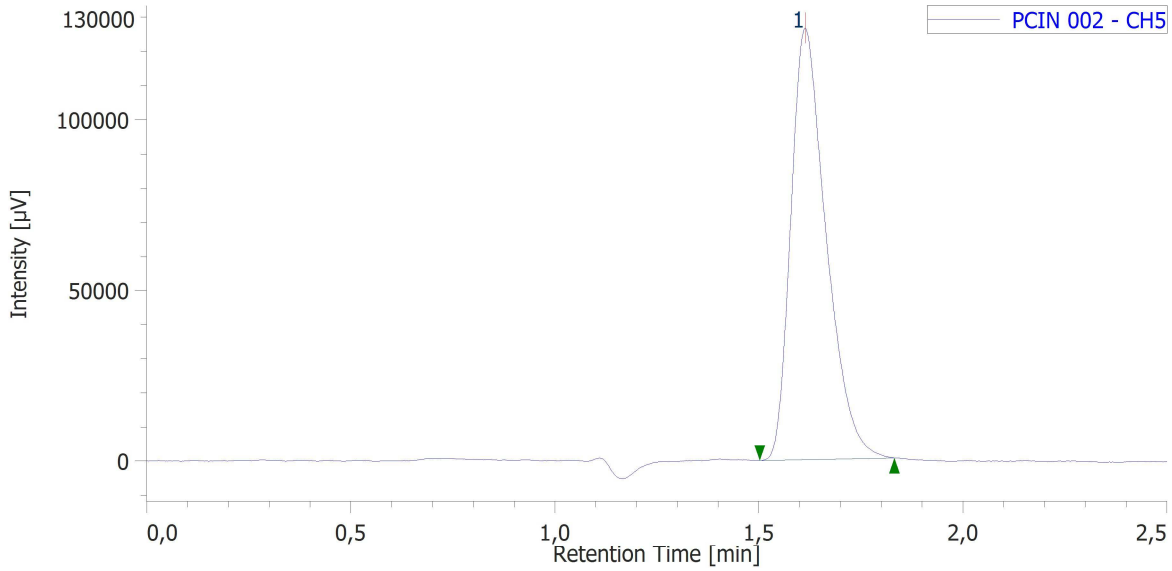

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 13:46:27
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:43:55
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	761235	126278	100,000	100,000	N/A	1708	N/A	1,408	

Creator
Reviewer
Approver

Chromatogram

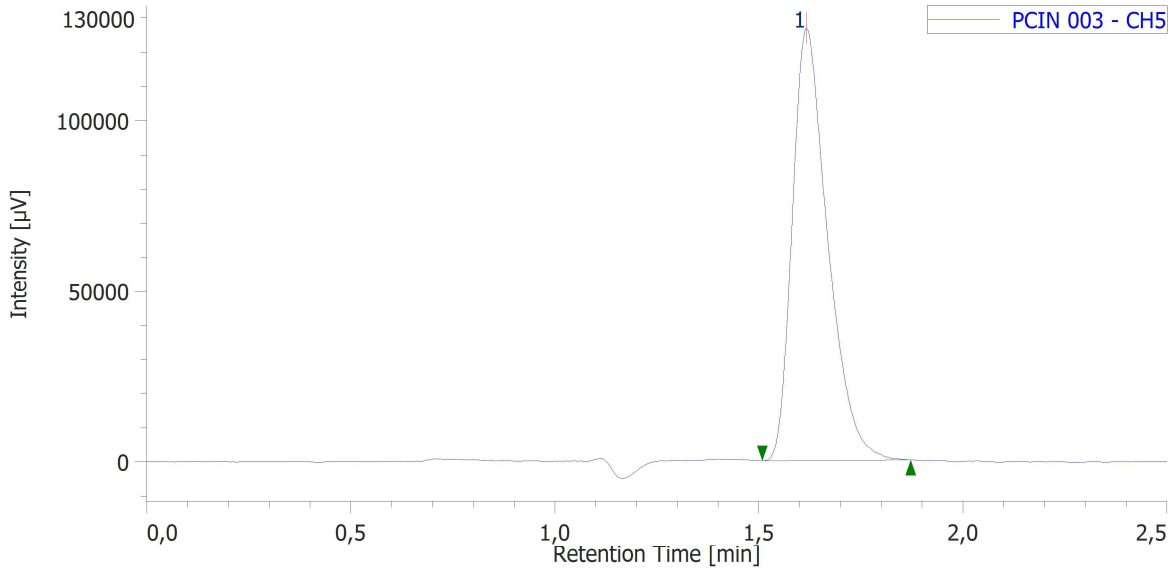

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 13:49:09
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:46:37
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,617	764473	126561	100,000	100,000	N/A	1728	N/A	1,425	

Creator
Reviewer
Approver

Chromatogram

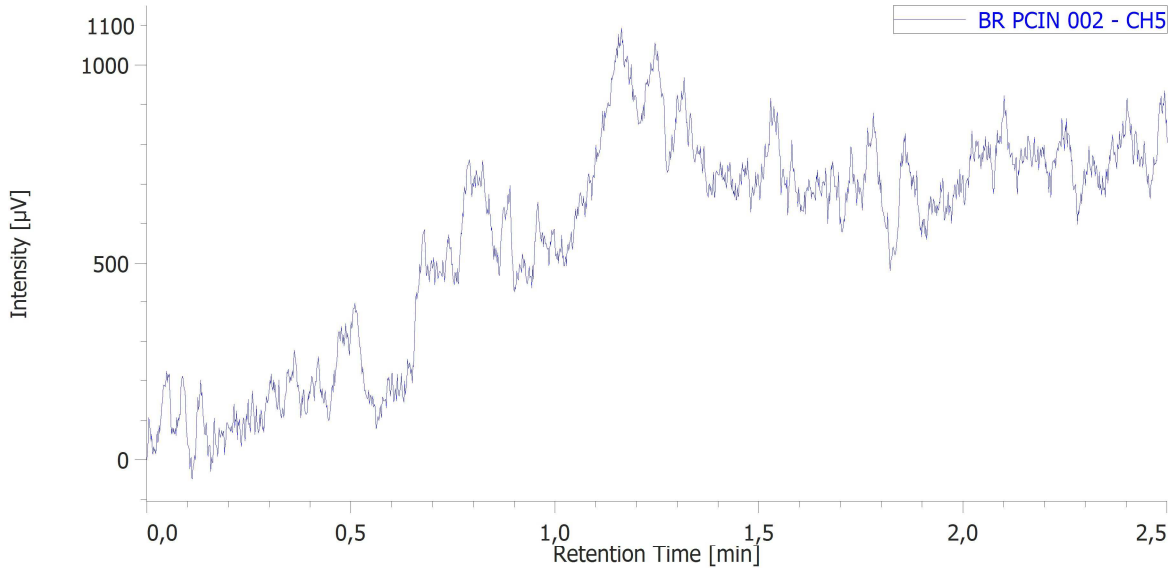


Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 13:51:53
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:49:20
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	

Creator Jasco
Reviewer
Approver

Chromatogram

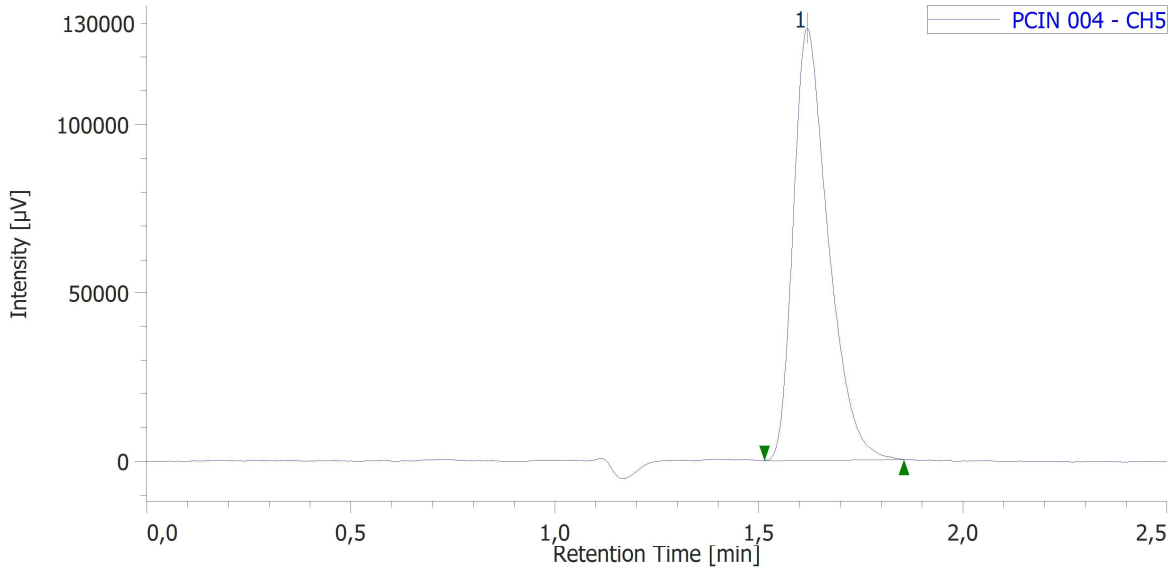

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 13:54:35
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:52:03
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,618	765462	128190	100,000	100,000	N/A	1773	N/A	1,434	

Creator
Reviewer
Approver

Chromatogram

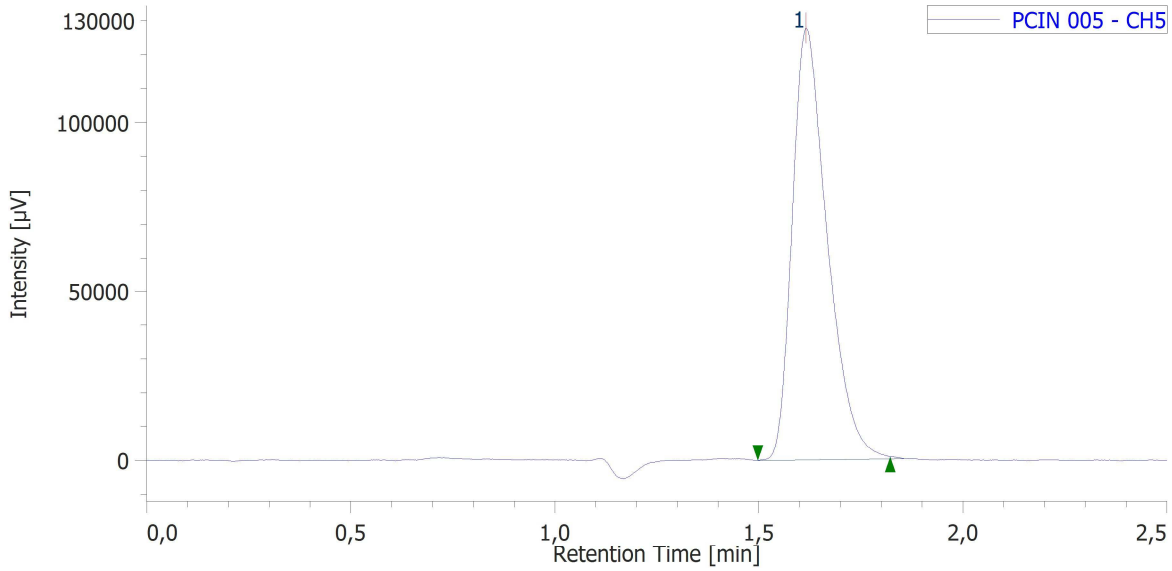

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 13:57:17
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:54:45
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,615	762625	127600	100,000	100,000	N/A	1760	N/A	1,449	

Creator
Reviewer
Approver

Chromatogram

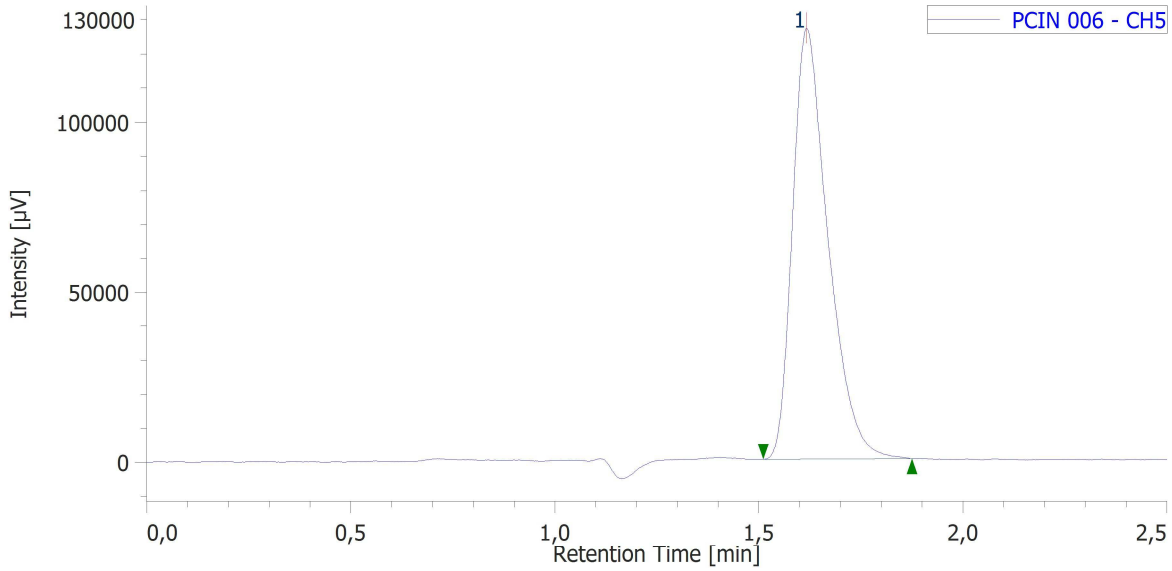

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 14:00:01
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 13:57:28
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 006-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,617	767370	126598	100,000	100,000	N/A	1726	N/A	1,444	

Creator
Reviewer
Approver

Chromatogram

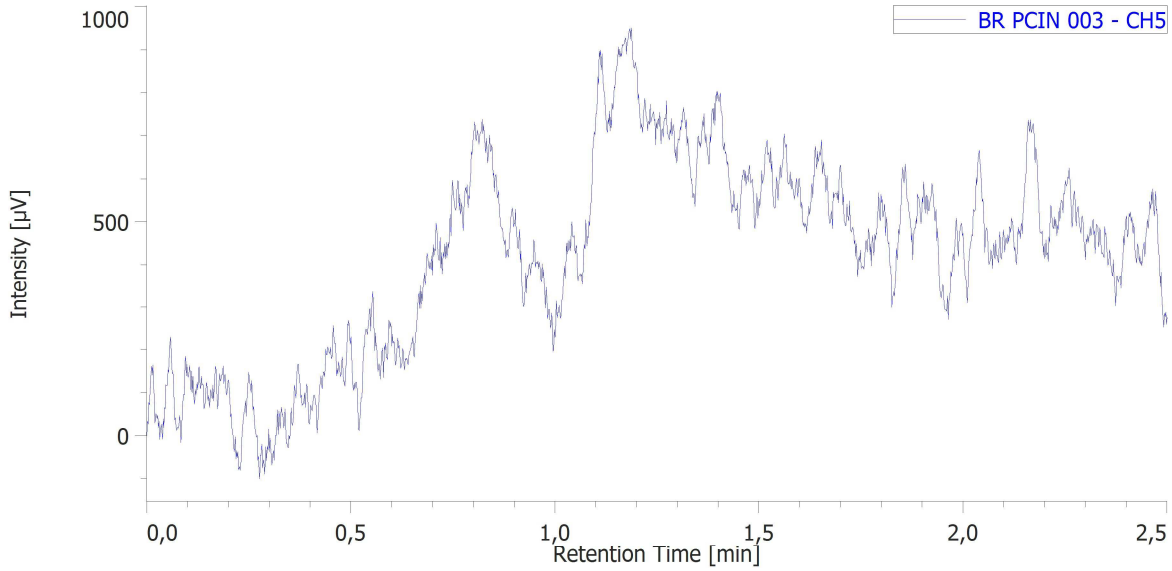


Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 14:02:43
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 14:00:11
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	

Creator Jasco
Reviewer
Approver

Chromatogram

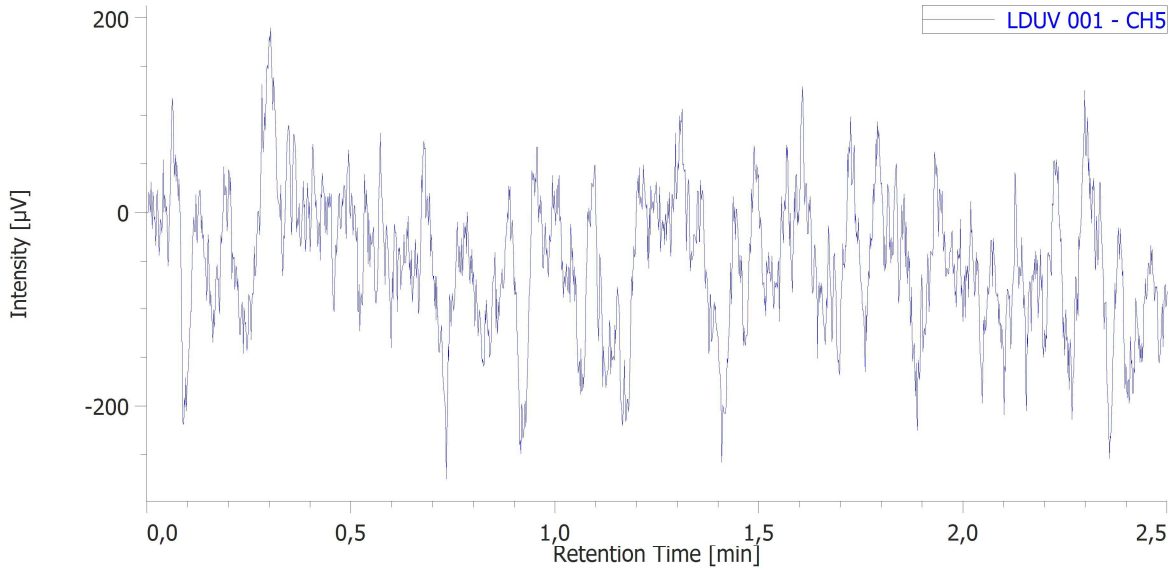


Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:32:58
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:30:25
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUVa
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	

Creator Jasco
Reviewer
Approver

Chromatogram

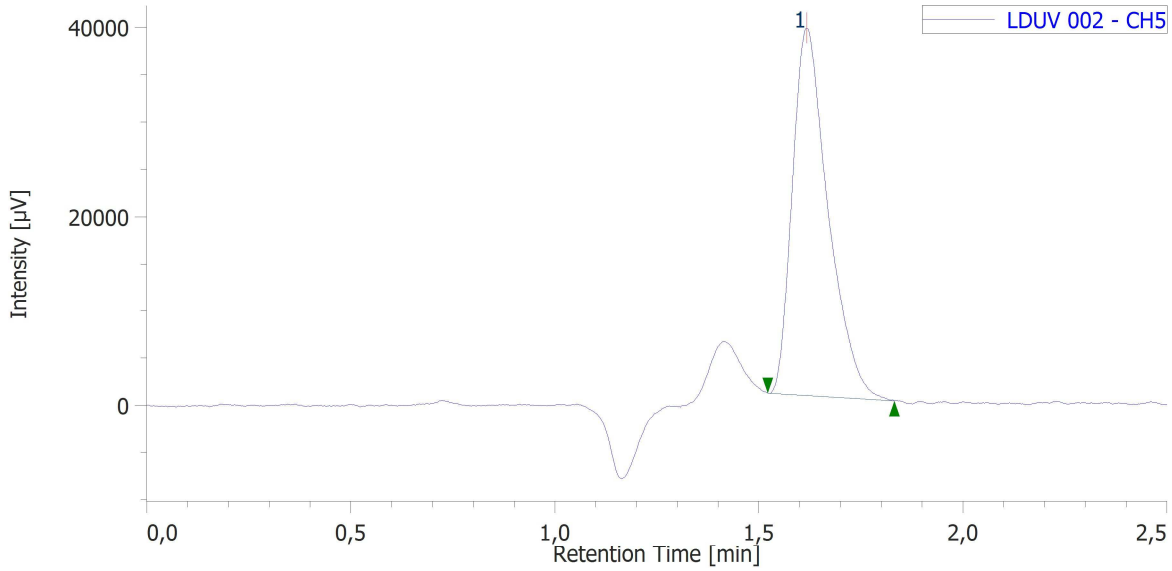

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:35:40
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:33:08
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUVa
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,617	237103	38864	100,000	100,000	N/A	1701	N/A	1,456	

Creator
Reviewer
Approver

Chromatogram

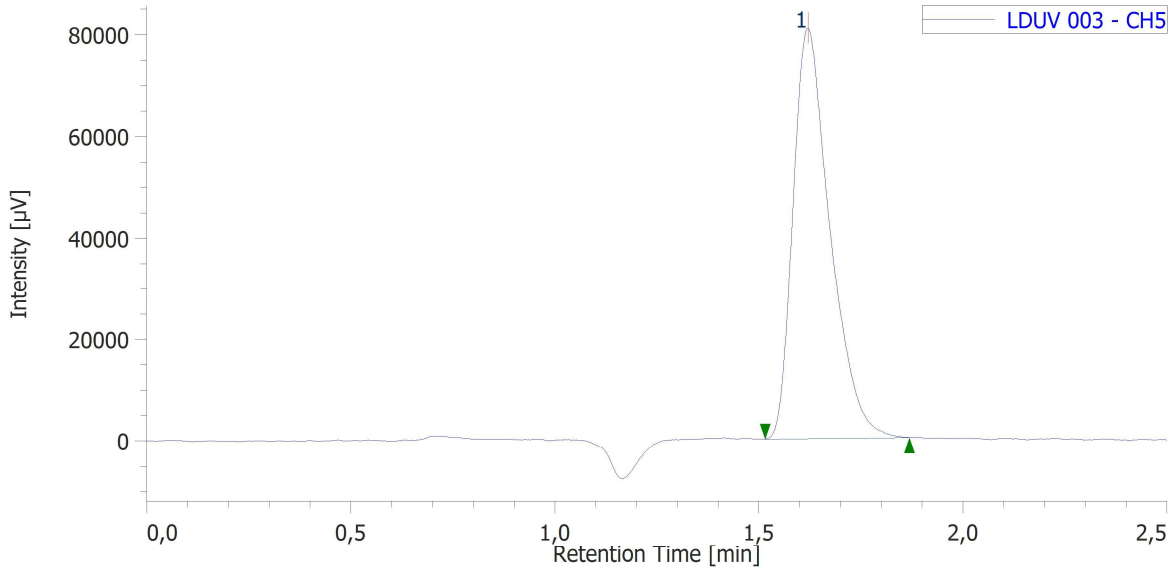

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:38:22
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:35:51
Volume	10,00 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUVa
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,620	510293	80781	100,000	100,000	N/A	1595	N/A	1,451	

Creator
Reviewer
Approver

Chromatogram

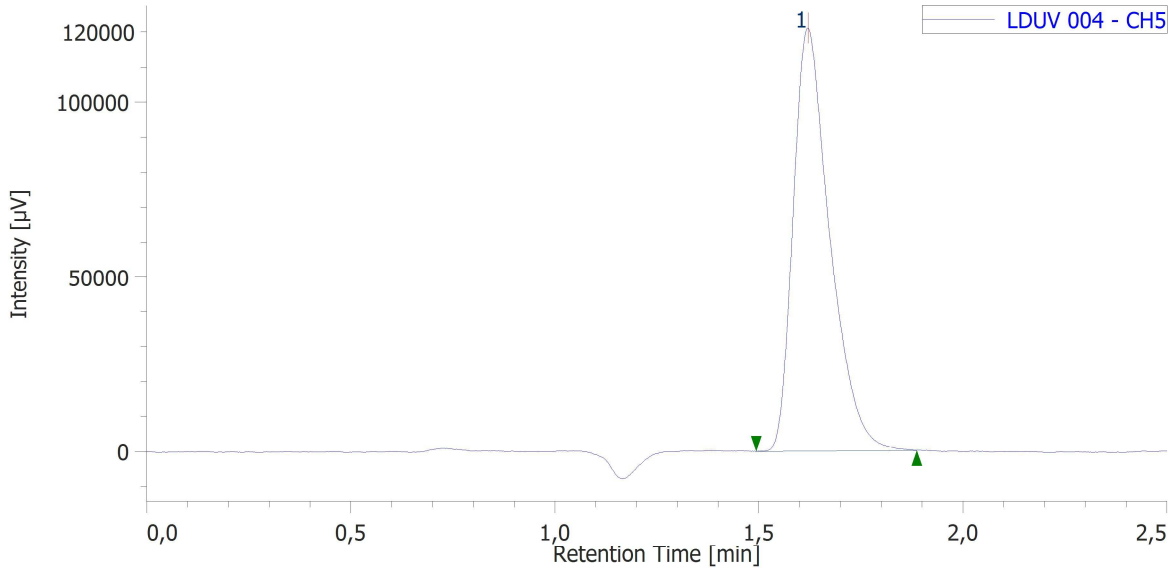

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:41:06
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:38:33
Volume	10,00 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUVa
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,620	754768	120837	100,000	100,000	N/A	1638	N/A	1,452	

Creator
Reviewer
Approver

Chromatogram

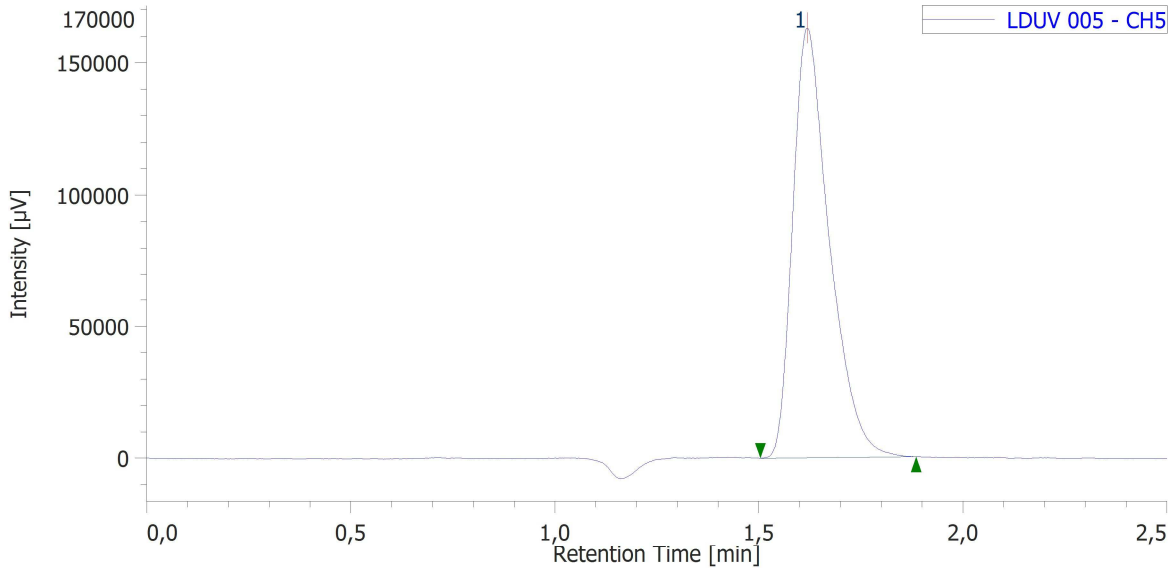

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:43:48
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:41:16
Volume	10,00 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUVa
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,618	1018486	162850	100,000	100,000	N/A	1645	N/A	1,474	

Creator
Reviewer
Approver

Chromatogram

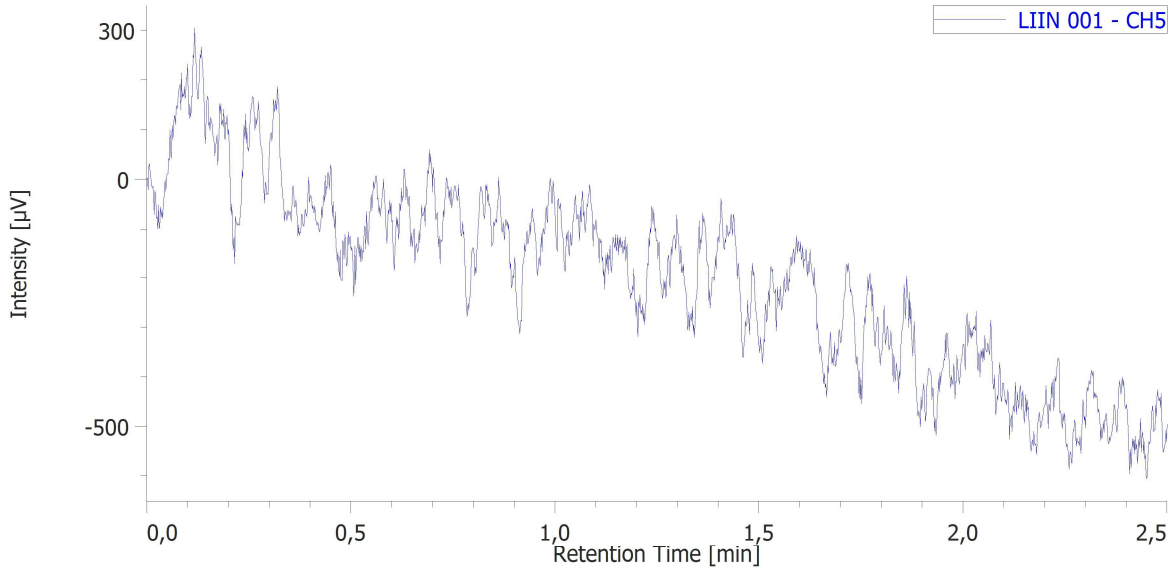


Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:48:58
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:46:27
Volume	0,10 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	

Creator Jasco
Reviewer
Approver

Chromatogram

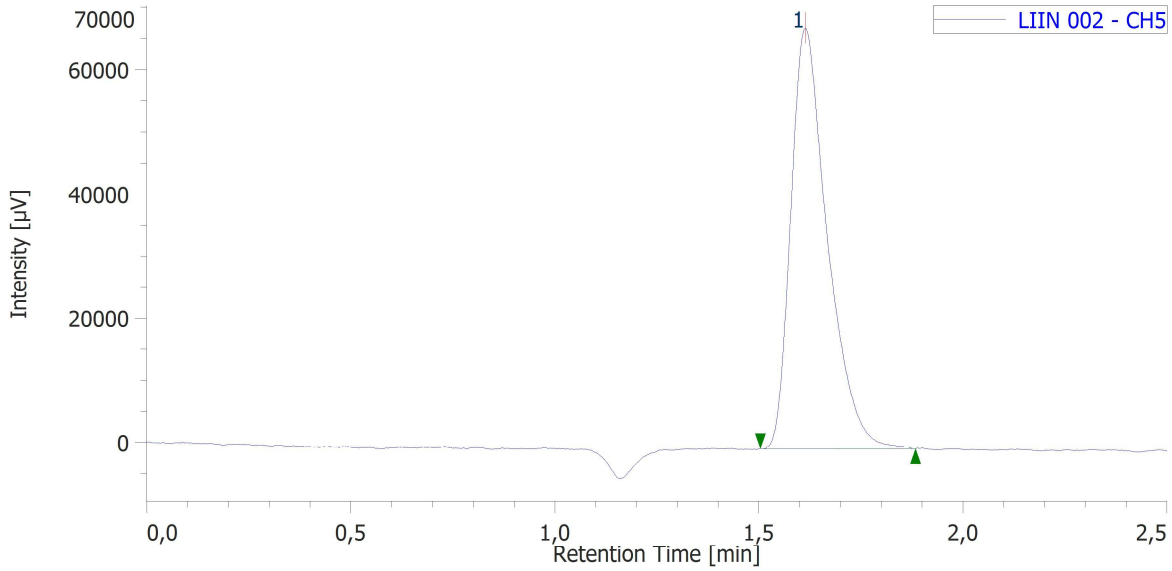

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:51:42
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:49:09
Volume	5,00 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	421447	67633	100,000	100,000	N/A	1658	N/A	1,473	

Creator
Reviewer
Approver

Chromatogram

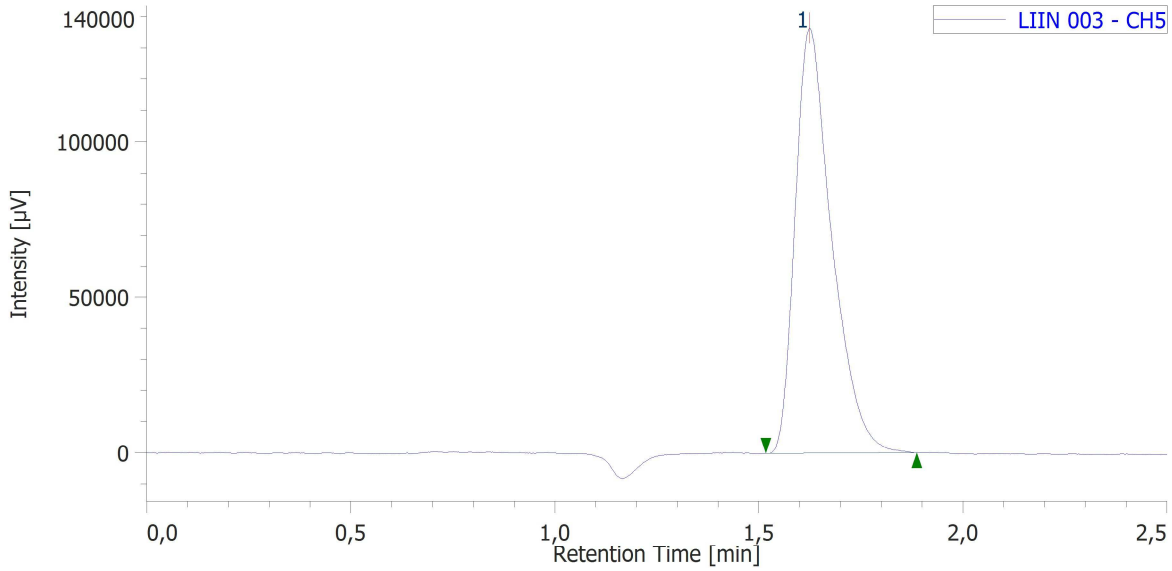

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:54:24
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:51:52
Volume	10,00 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,623	852271	136368	100,000	100,000	N/A	1657	N/A	1,494	

Creator
Reviewer
Approver

Chromatogram

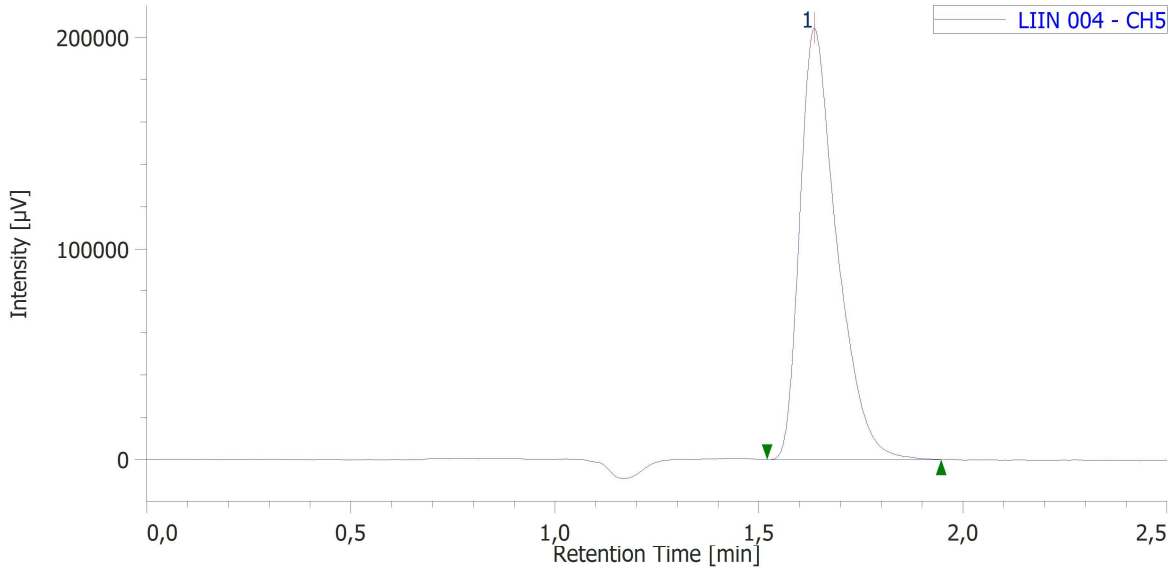

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:57:06
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:54:35
Volume	15,00 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,635	1290000	204366	100,000	100,000	N/A	1659	N/A	1,504	

Creator
Reviewer
Approver

Chromatogram

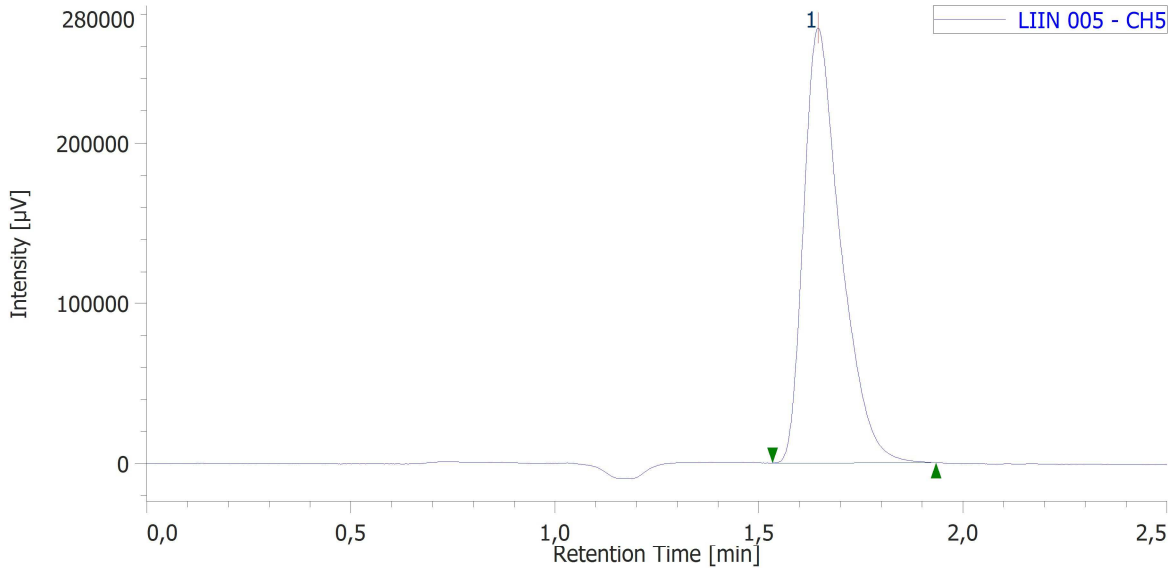

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 15:59:52
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 15:57:20
Volume	20,00 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,645	1712001	270966	100,000	100,000	N/A	1663	N/A	1,486	

Creator
Reviewer
Approver

Chromatogram

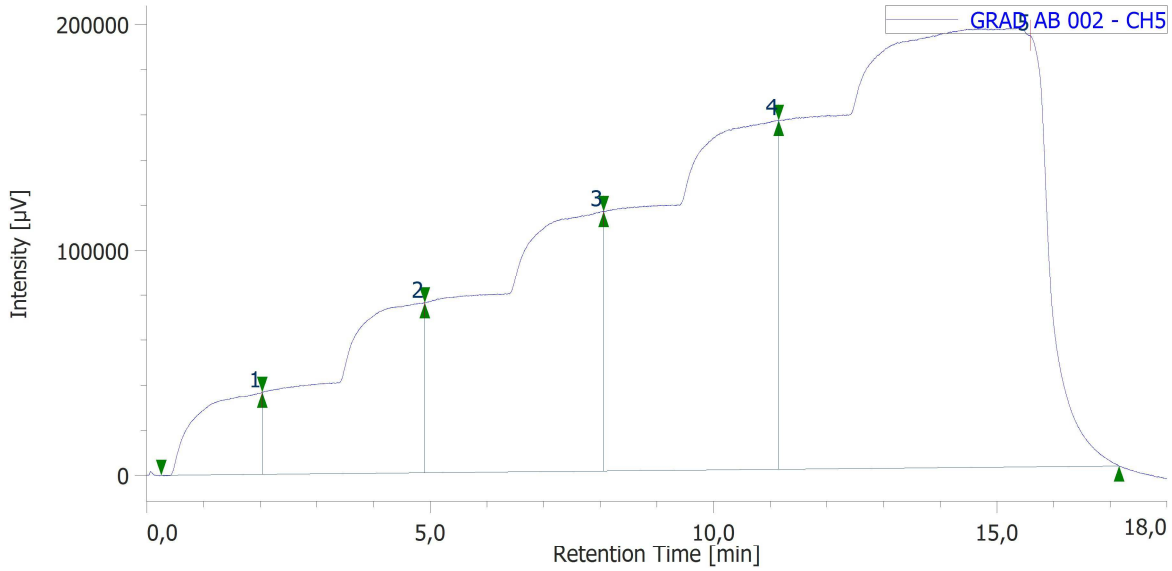

Chromatogram Information	
User Name	Jasco
Date Modified	11/09/2019 17:58:15
Description	
HPLC System Name	5CQ1HP03
Injection Date	11/09/2019 17:40:13
Volume	0,10 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	GRAD
Control Method	GRAD
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	2,032	2718065	36397	2,540	6,349	N/A	N/A	N/A	N/A	
2	Unknown	5	4,897	9296481	75415	8,688	13,155	N/A	N/A	N/A	N/A	
3	Unknown	5	8,052	17647968	115420	16,493	20,133	N/A	N/A	N/A	N/A	
4	Unknown	5	11,143	24774814	154877	23,153	27,016	N/A	N/A	N/A	N/A	
5	Unknown	5	15,585	52567109	191171	49,126	33,347	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

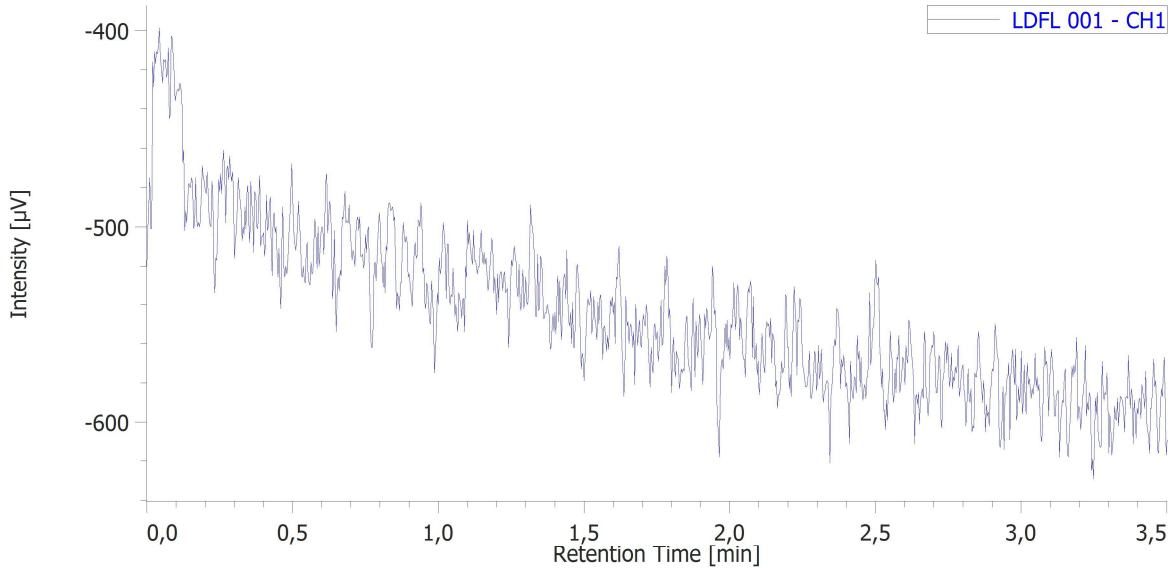


Chromatogram Information	
User Name	Jasco
Date Modified	12/09/2019 09:59:16
Description	
HPLC System Name	5CQ1HP03
Injection Date	12/09/2019 09:55:44
Volume	0,10 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDFL
Control Method	Qualificação FL
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDFL 001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	

Creator Jasco
Reviewer
Approver

Chromatogram

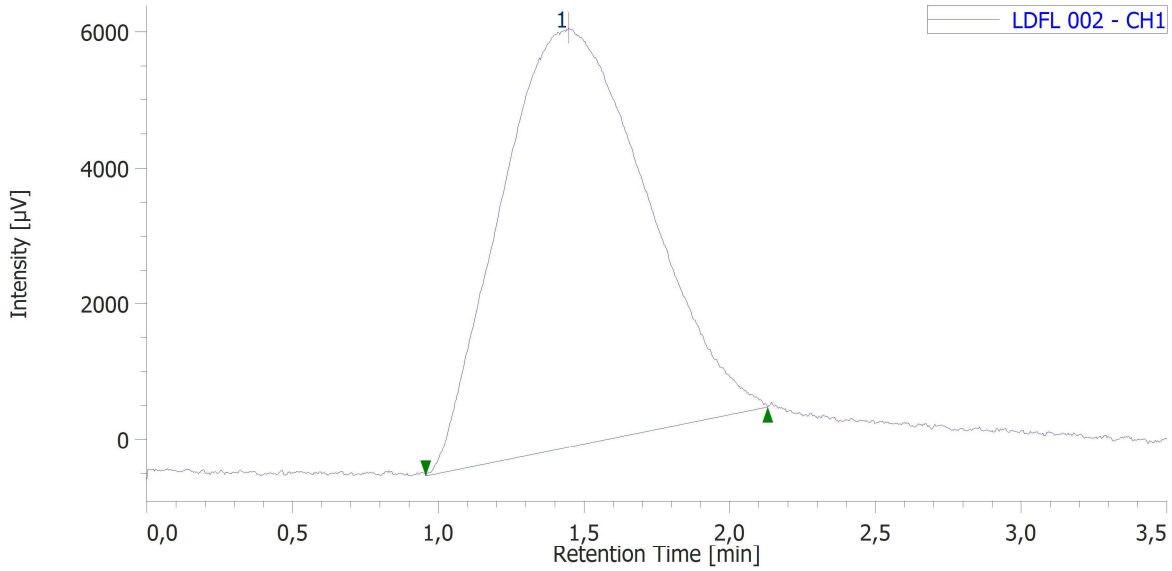

Chromatogram Information	
User Name	Jasco
Date Modified	12/09/2019 10:03:00
Description	
HPLC System Name	5CQ1HP03
Injection Date	12/09/2019 09:59:28
Volume	5,00 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDFL
Control Method	Qualificação FL
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDFL 002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Quinina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	1,447	214510	6160	100,000	100,000	N/A	36	N/A	1,196	

Creator
Reviewer
Approver

Chromatogram

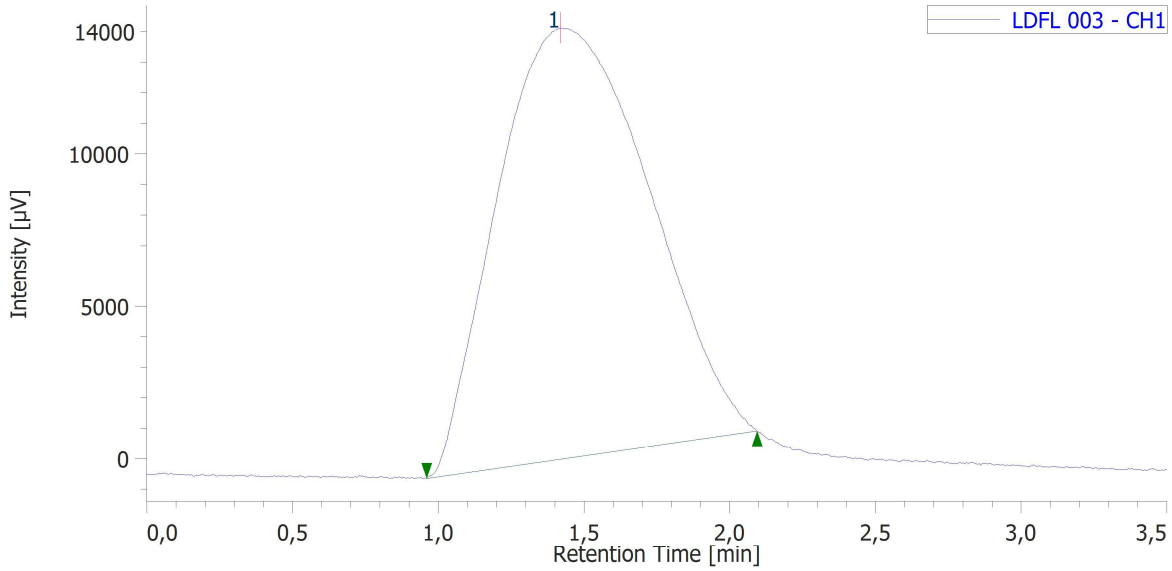

Chromatogram Information	
User Name	Jasco
Date Modified	12/09/2019 10:06:42
Description	
HPLC System Name	5CQ1HP03
Injection Date	12/09/2019 10:03:11
Volume	10,00 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDFL
Control Method	Qualificação FL
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDFL 003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Quinina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	1,420	511273	14112	100,000	100,000	N/A	30	N/A	1,248	

Creator
Reviewer
Approver

Chromatogram

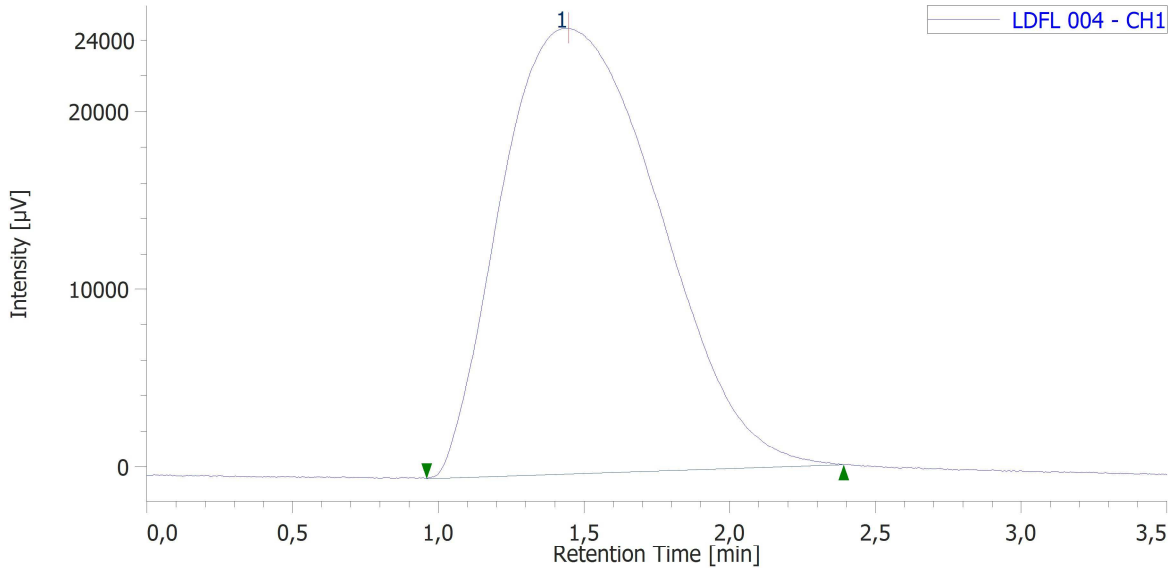

Chromatogram Information	
User Name	Jasco
Date Modified	12/09/2019 10:10:26
Description	
HPLC System Name	5CQ1HP03
Injection Date	12/09/2019 10:06:54
Volume	15,00 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDFL
Control Method	Qualificação FL
Peak ID Table	Quinina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDFL 004-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Quinina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	1,447	946508	25066	100,000	100,000	N/A	30	N/A	1,322	

Creator
Reviewer
Approver

Chromatogram

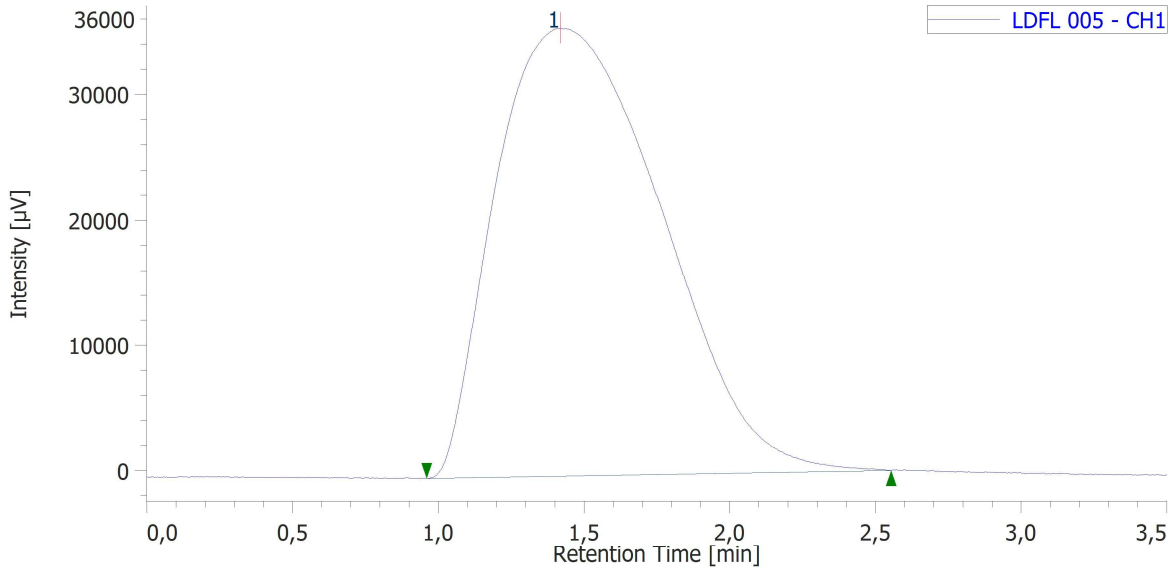

Chromatogram Information	
User Name	Jasco
Date Modified	12/09/2019 10:14:12
Description	
HPLC System Name	5CQ1HP03
Injection Date	12/09/2019 10:10:39
Volume	20,00 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDFL
Control Method	Qualificação FL
Peak ID Table	Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDFL 005-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Quinina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Quinina	1	1,420	1414215	35686	100,000	100,000	N/A	26	N/A	1,451	

Creator
Reviewer
Approver