
Peak Find - Qualificação do Comprimento de Onda_001 UV_tR1.83 D.jws

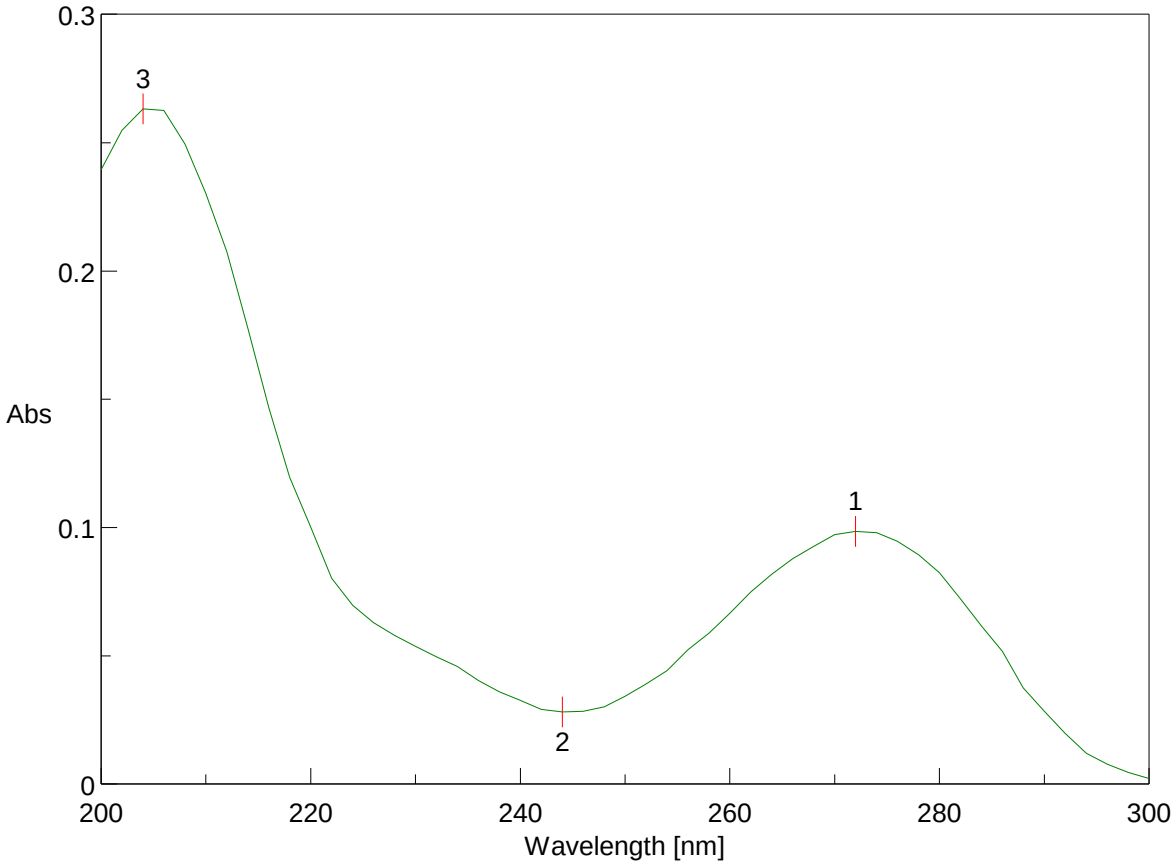

[Comments]

User	Administrator
Division	---
Company	TRB Pharma
Creation date	08/08/2017 12:15

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.0984474	2	244	0.028052
3	204	0.263103			

Chromatogram

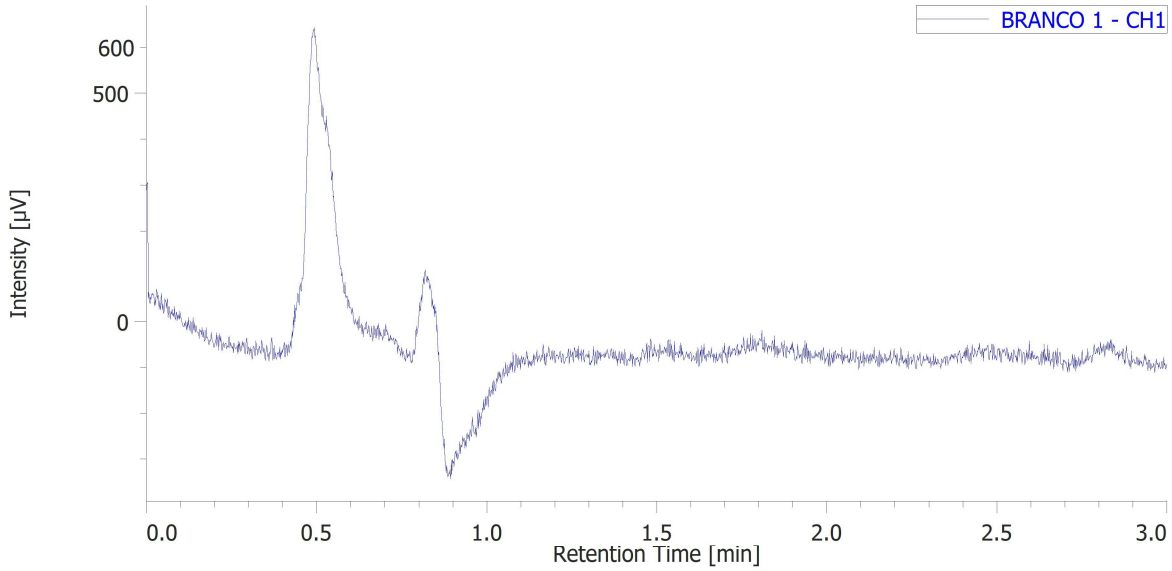


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 15:52:27
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 15:49:25
Volume	10.00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

Chromatogram

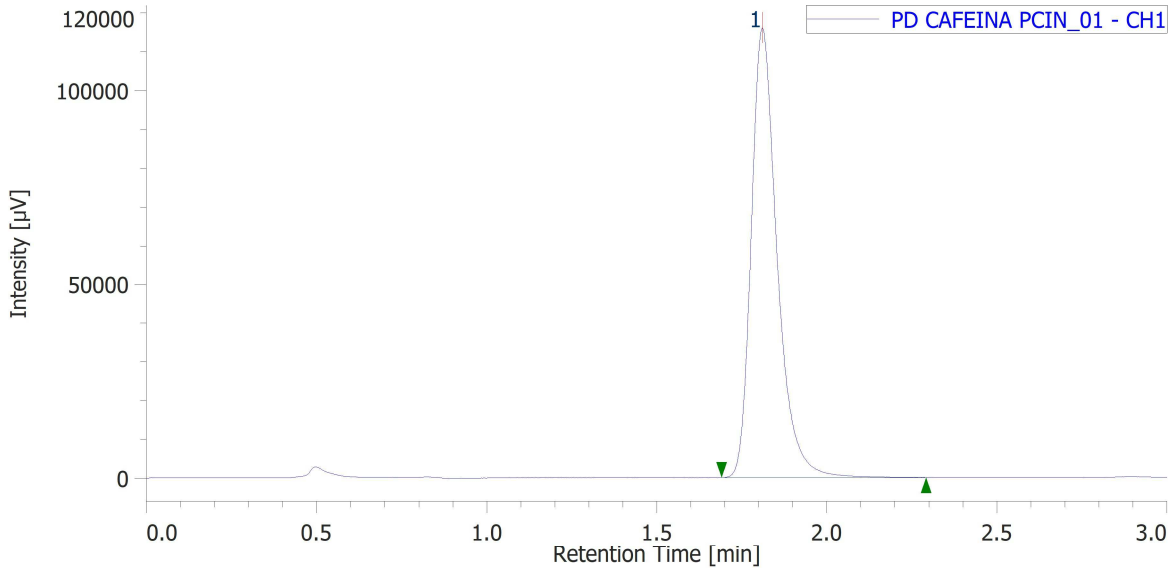


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 15:56:29
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 15:53:27
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PD CAFEINA PCIN_01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.810	613881	115963	100.000	100.000	N/A	2988	N/A	1.343	

Chromatogram

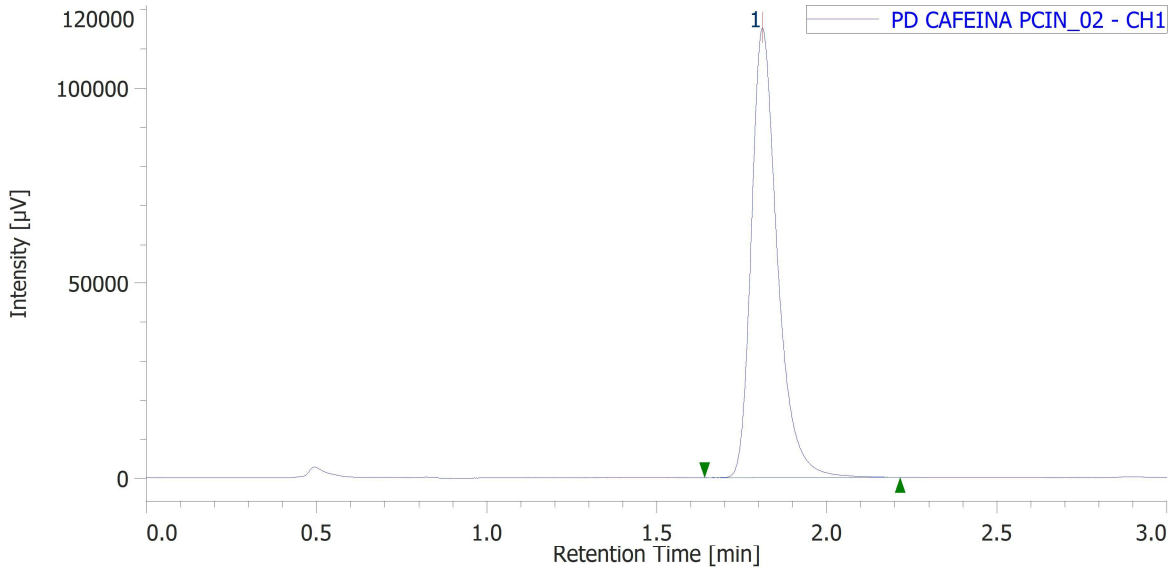


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:00:31
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 15:57:29
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PD CAFEINA PCIN_02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.810	612920	115176	100.000	100.000	N/A	2955	N/A	1.364	

Chromatogram

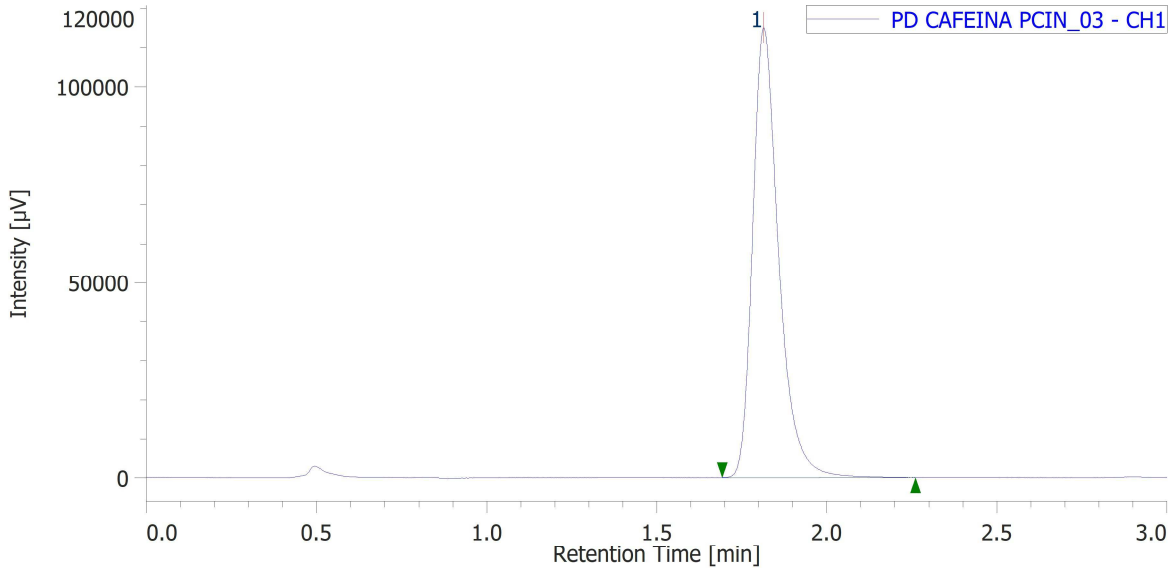


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:04:35
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:01:33
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PD CAFEINA PCIN_03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.813	613146	114863	100.000	100.000	N/A	2952	N/A	1.377	

Chromatogram

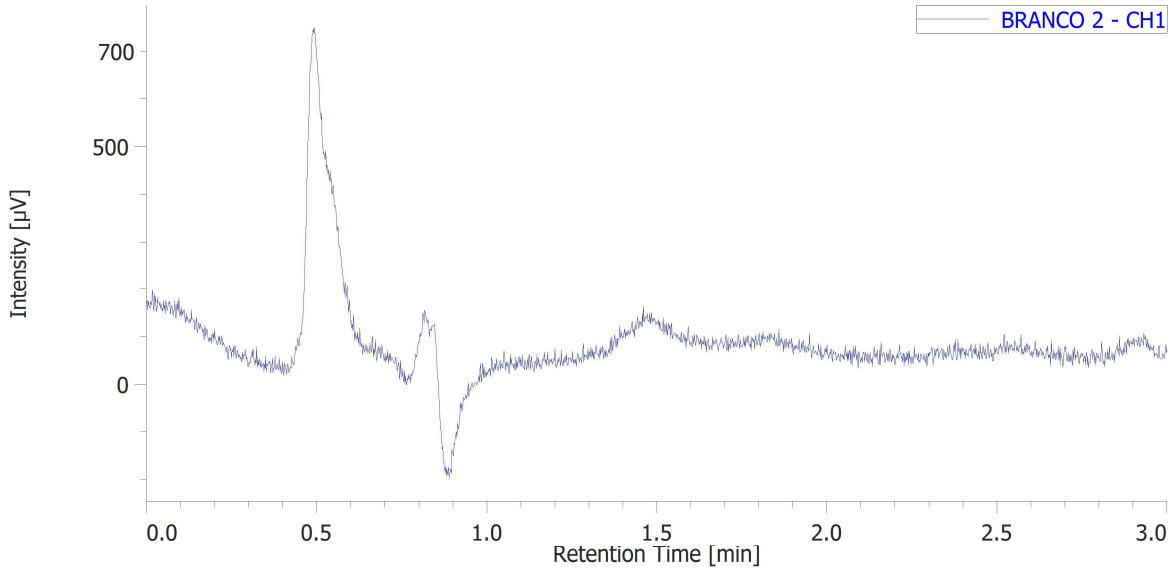


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:08:37
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:05:34
Volume	10.00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

Chromatogram

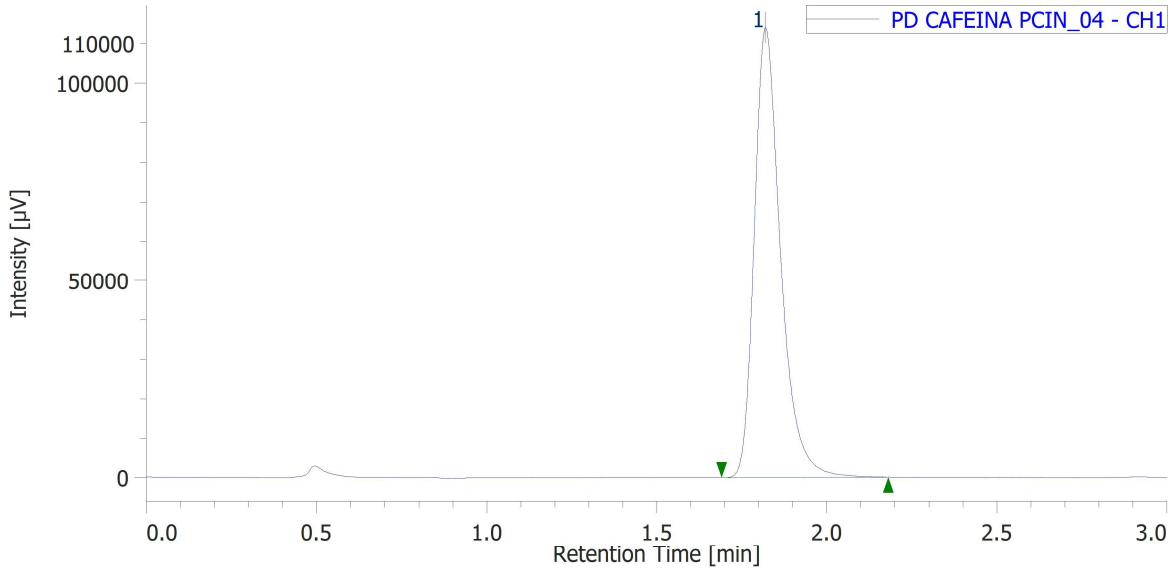


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:12:39
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:09:36
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PD CAFEINA PCIN_04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.818	612343	113801	100.000	100.000	N/A	2904	N/A	1.379	

Chromatogram

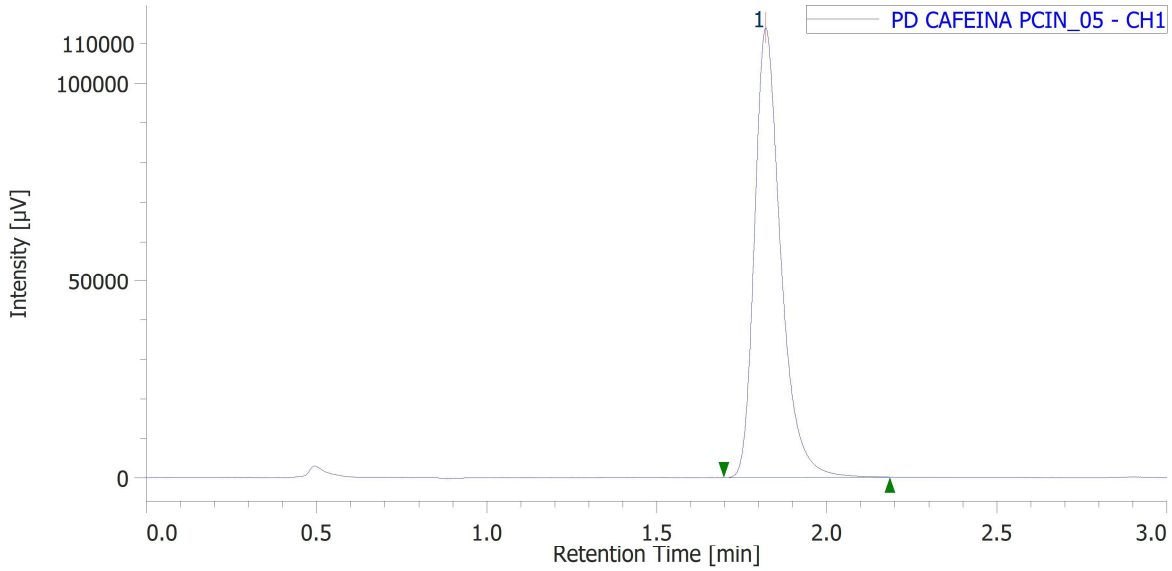


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:16:43
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:13:40
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PD CAFEINA PCIN_05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.820	611475	113785	100.000	100.000	N/A	2917	N/A	1.358	

Chromatogram

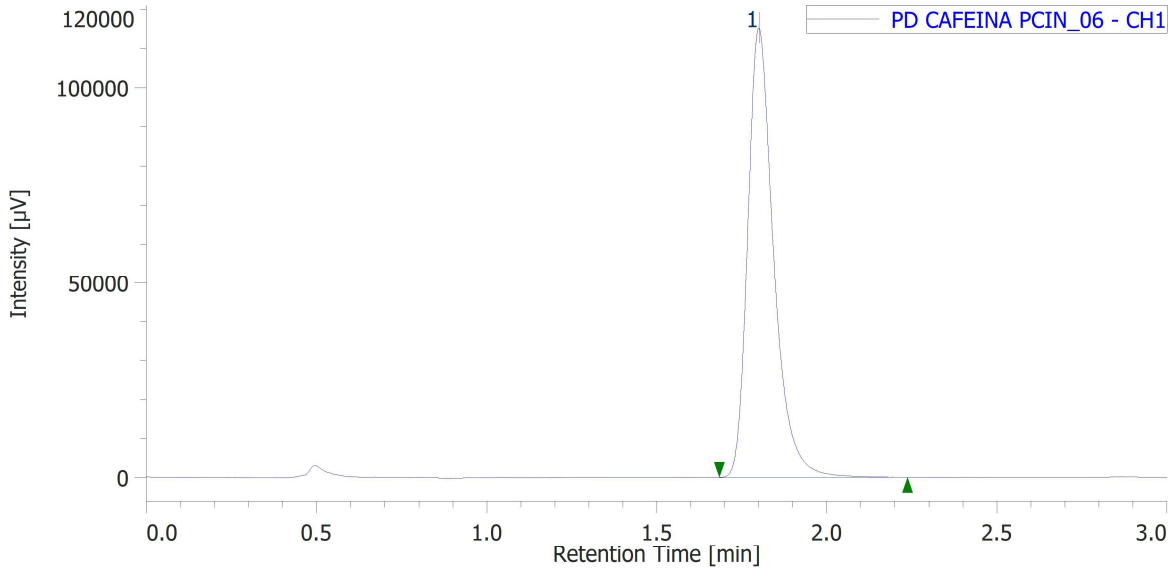


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:20:47
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:17:44
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PD CAFEINA PCIN_06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.800	611763	115197	100.000	100.000	N/A	2931	N/A	1.353	

Chromatogram

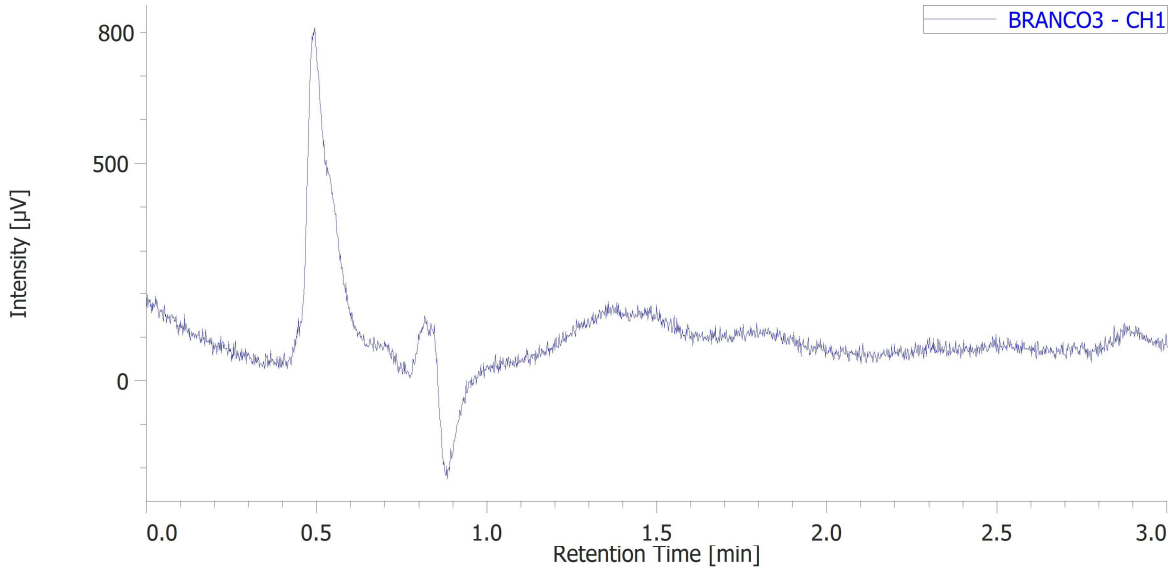


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:24:48
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:21:46
Volume	10.00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

Chromatogram

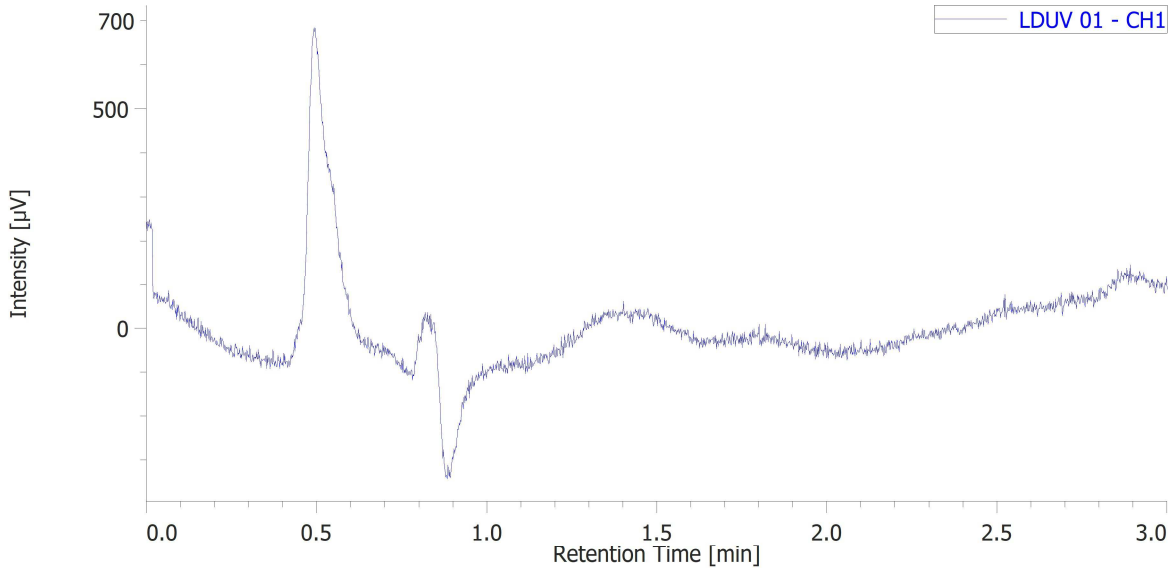


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:28:50
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:25:48
Volume	10.00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

Chromatogram

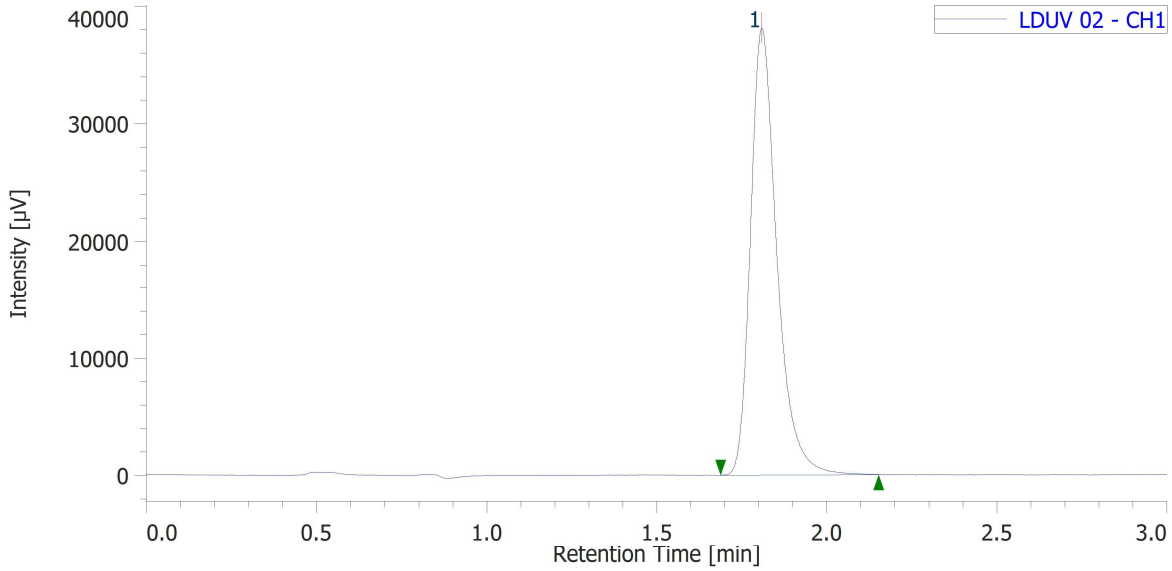


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:32:52
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:29:49
Volume	10.00 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.808	205607	38104	100.000	100.000	33.5636	2865	N/A	1.354	

Chromatogram

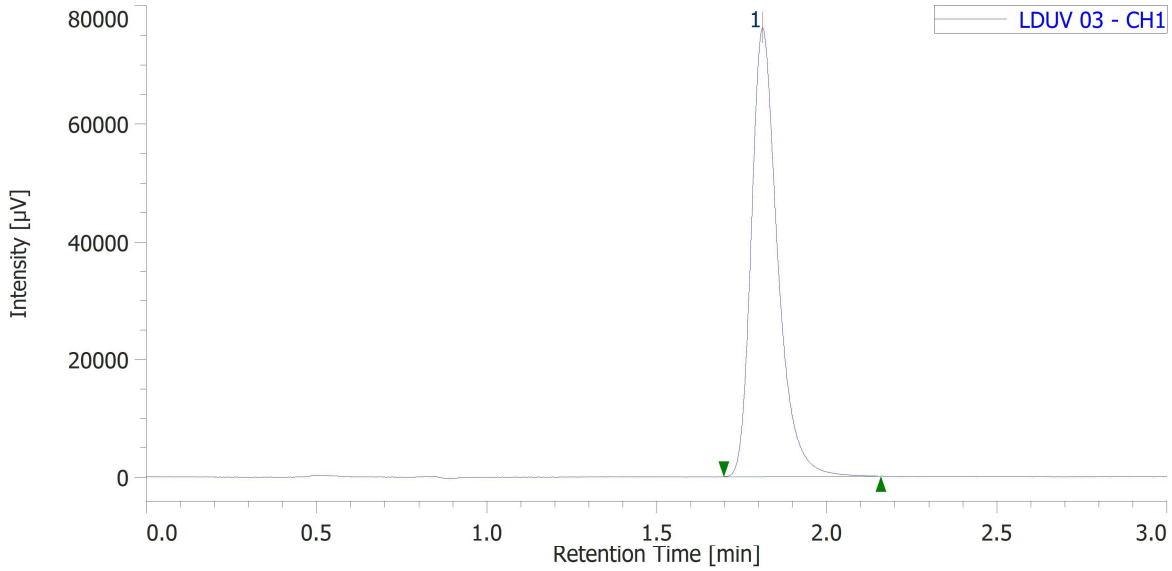


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:36:54
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:33:51
Volume	10.00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.810	409353	76133	100.000	100.000	66.8236	2879	N/A	1.365	

Chromatogram

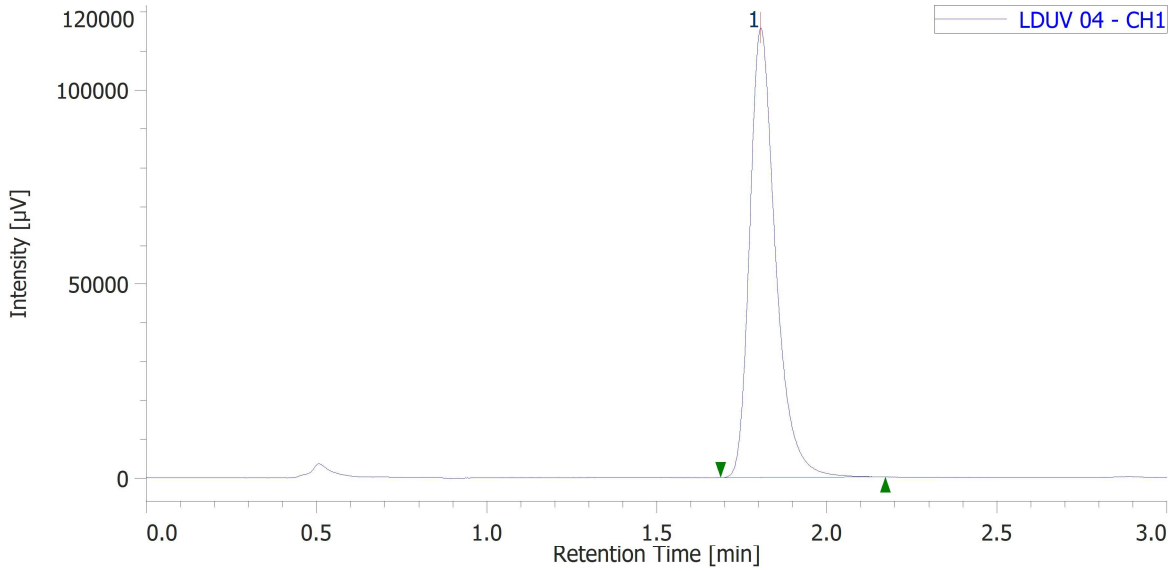


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:40:56
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:37:53
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.805	613056	115727	100.000	100.000	100.076	2949	N/A	1.363	Extrapolation

Chromatogram

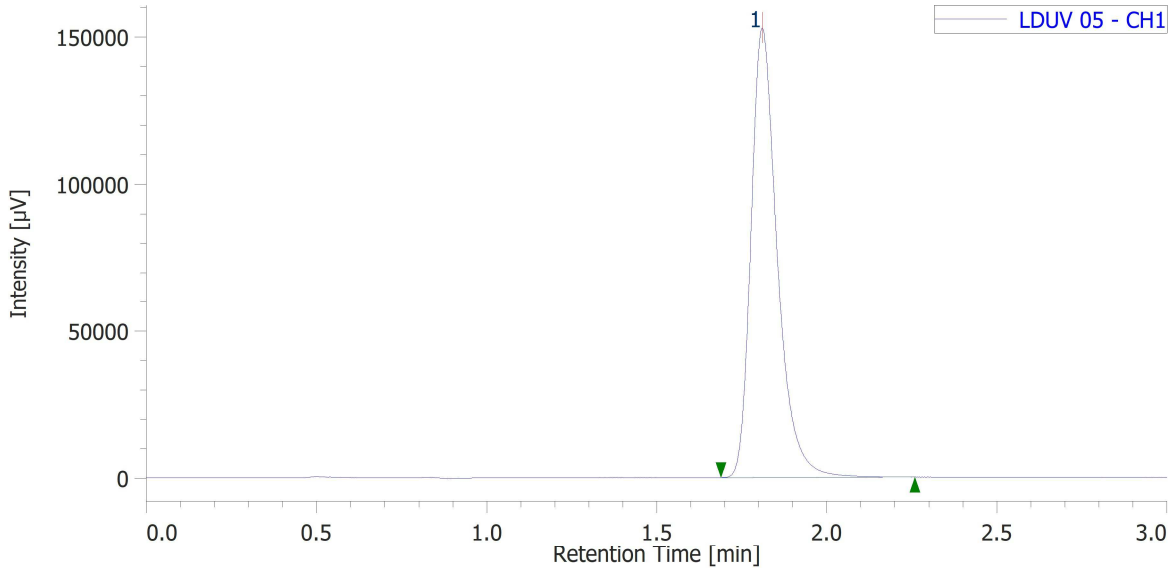


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:45:00
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:41:57
Volume	10.00 [µL]
Sample #	5
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.810	821704	152808	100.000	100.000	134.137	2883	N/A	1.352	Extrapolation

Chromatogram

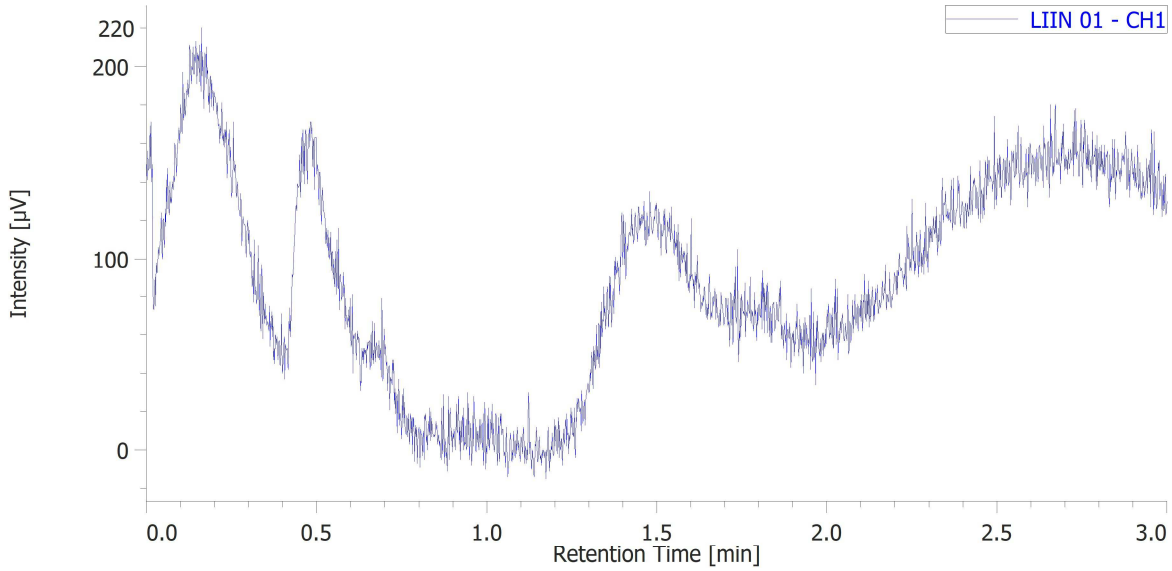


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:48:50
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:45:47
Volume	0.10 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

Chromatogram

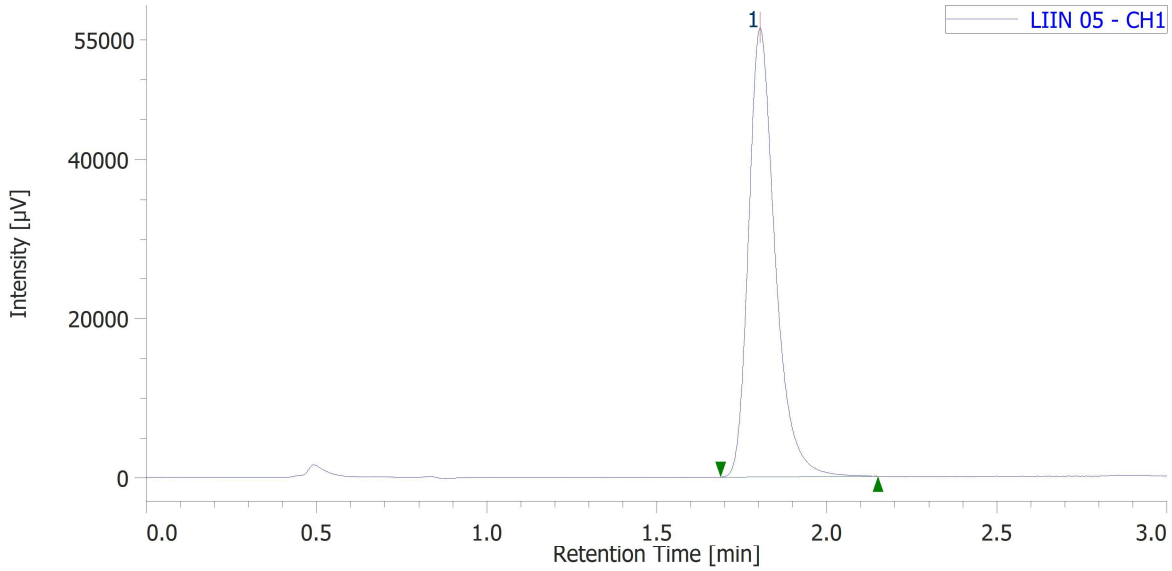


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:52:44
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:49:42
Volume	5.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.803	306323	56357	100.000	100.000	50.0047	2792	N/A	1.338	

Chromatogram

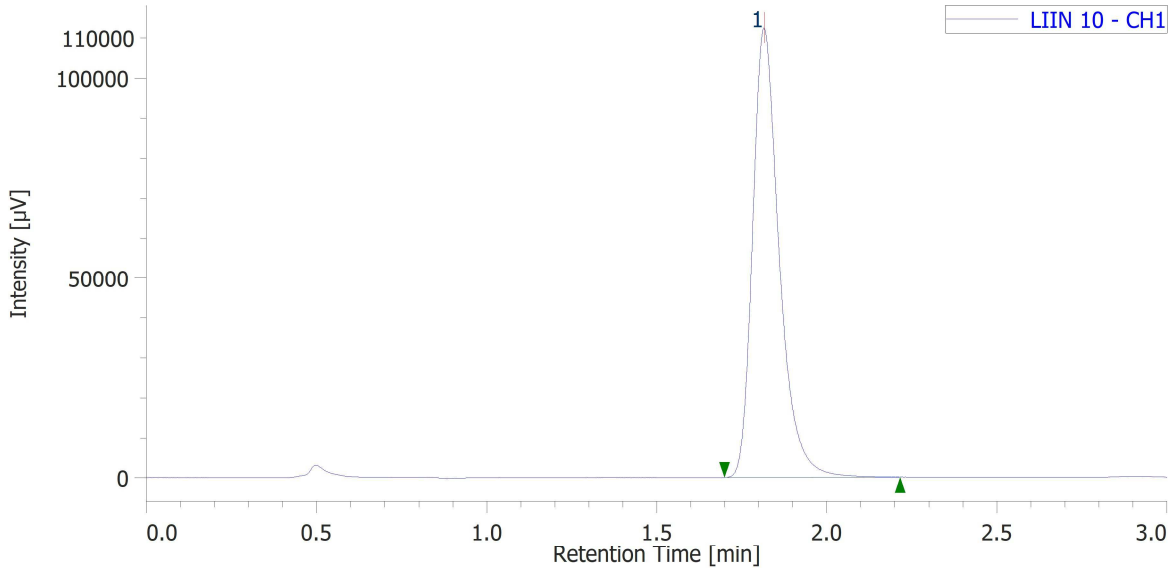


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 16:56:46
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:53:44
Volume	10.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 10-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.815	611191	112342	100.000	100.000	99.7720	2823	N/A	1.352	

Chromatogram

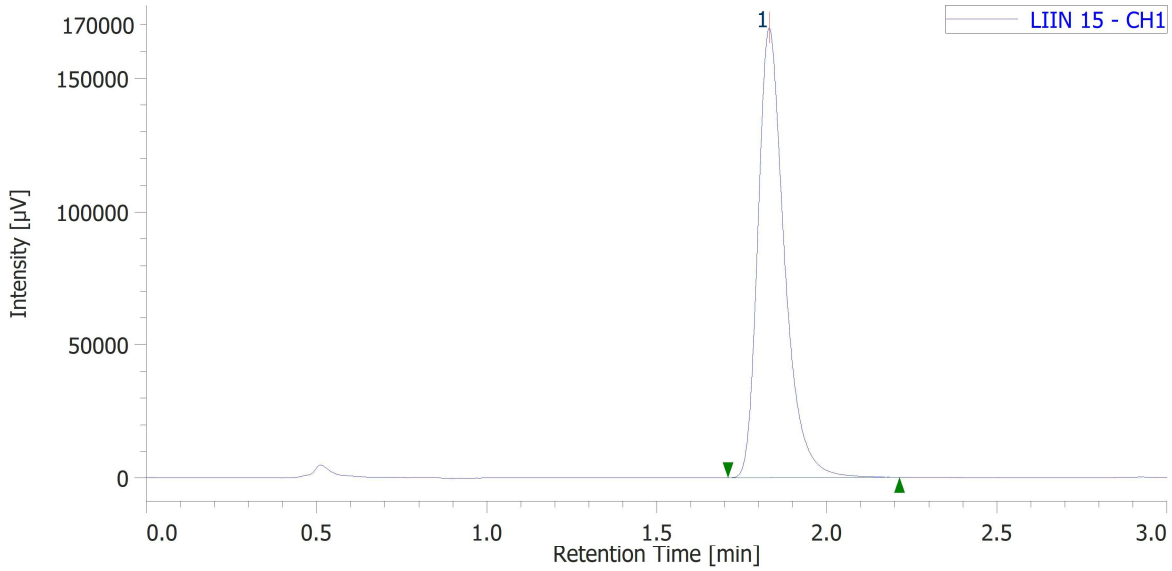


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 17:00:54
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 16:57:53
Volume	15.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 15-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.830	915816	168693	100.000	100.000	149.500	2885	N/A	1.373	Extrapolation

Chromatogram

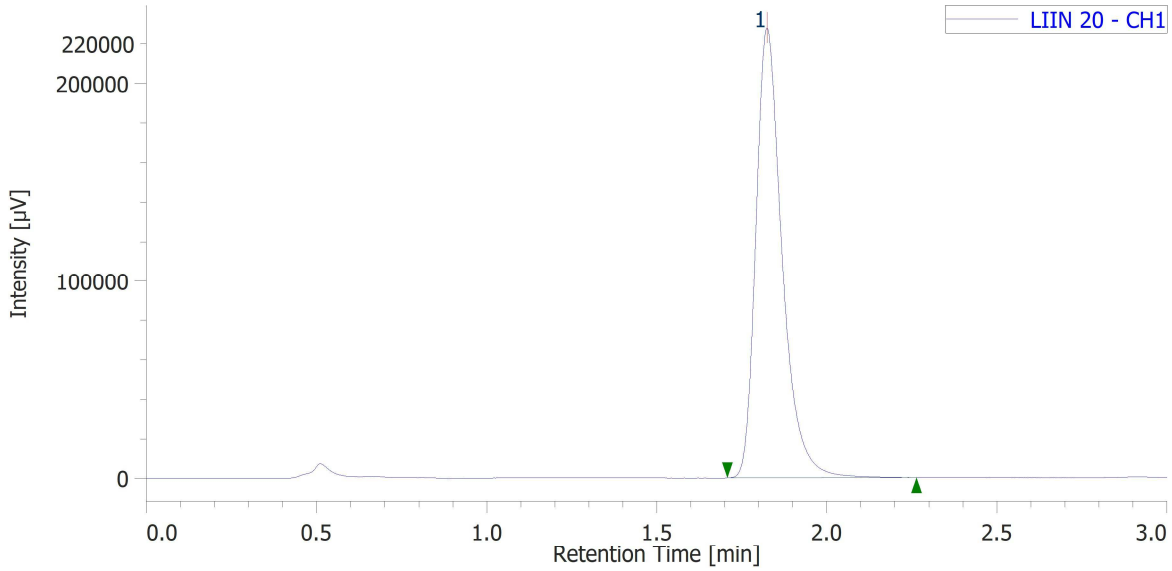


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2017 17:05:10
Description	
HPLC System Name	HPLC-0001
Injection Date	08/08/2017 17:02:08
Volume	20.00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação_HPLC_0001
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	Cafeina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 20-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.823	1222490	227742	100.000	100.000	199.562	2940	N/A	1.382	Extrapolation

Chromatogram

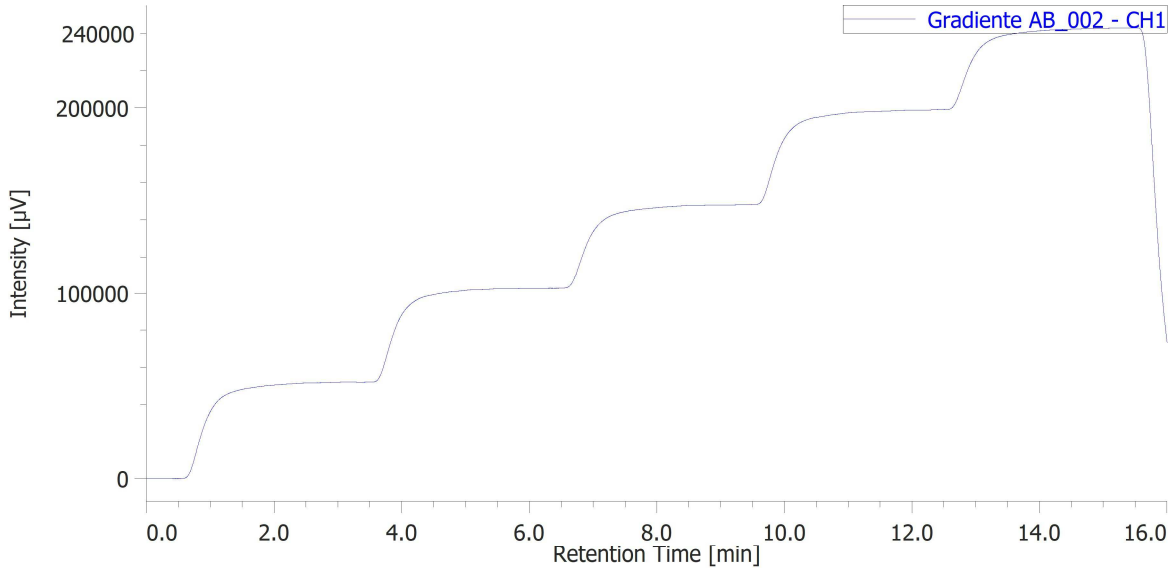


Chromatogram Information	
User Name	Administrator
Date Modified	09/08/2017 14:51:09
Description	
HPLC System Name	HPLC-0001
Injection Date	09/08/2017 14:35:06
Volume	0.00 [µL]
Sample #	-
Project Name	QUALIFICAÇÃO
Acquisition Time	16.0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	

Chromatogram

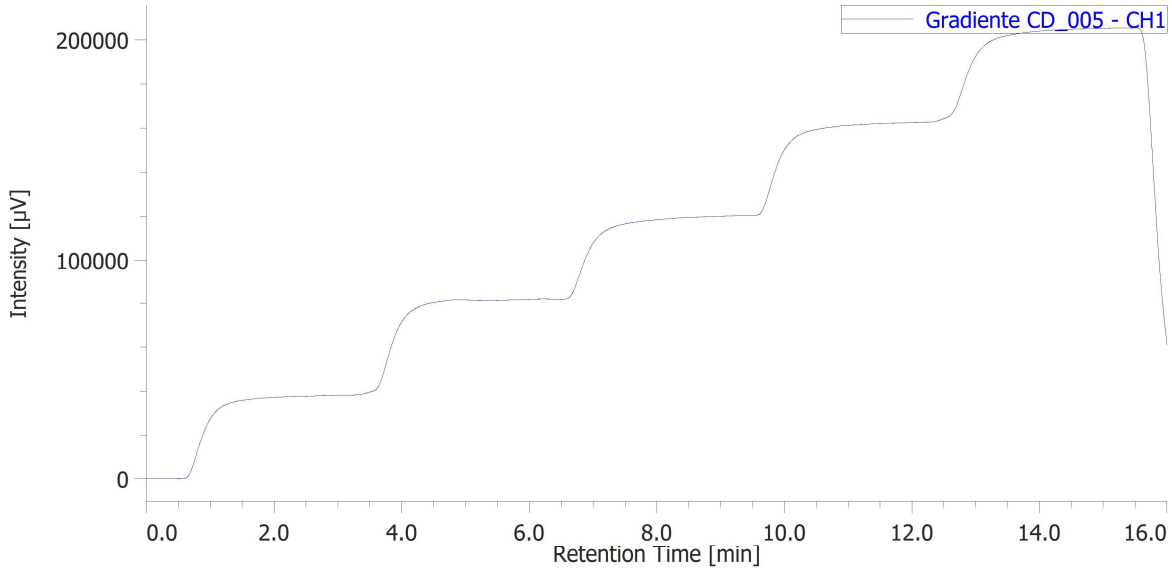

Chromatogram Information	
User Name	Administrator
Date Modified	09/08/2017 15:40:15
Description	
HPLC System Name	HPLC-0001
Injection Date	09/08/2017 15:24:13
Volume	0.00 [µL]
Sample #	-
Project Name	QUALIFICAÇÃO
Acquisition Time	16.0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_005-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	