
Peak Find - 5CQ1HP01 UV_20180824T100236-0300.jws

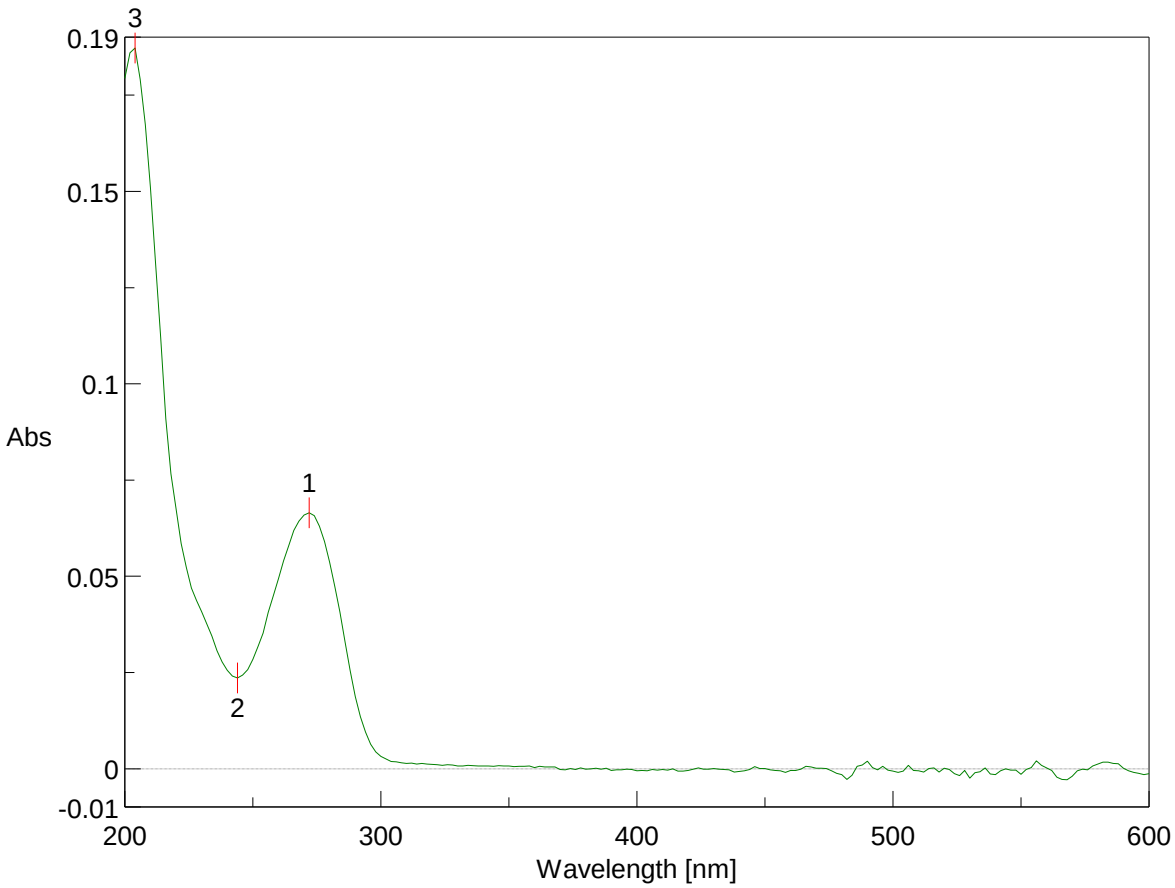

[Comments]

User	Administrator
Division	---
Company	Jasco
Creation date	8/24/2018 10:02 AM

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	201


[Measurement Information]

Instrument Name	UV-1575
Model Name	UV-1575
Serial No.	XXXXX
ROM version	V1.20

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.0664071	2	244	0.0234969
3	204	0.187186			

Chromatogram

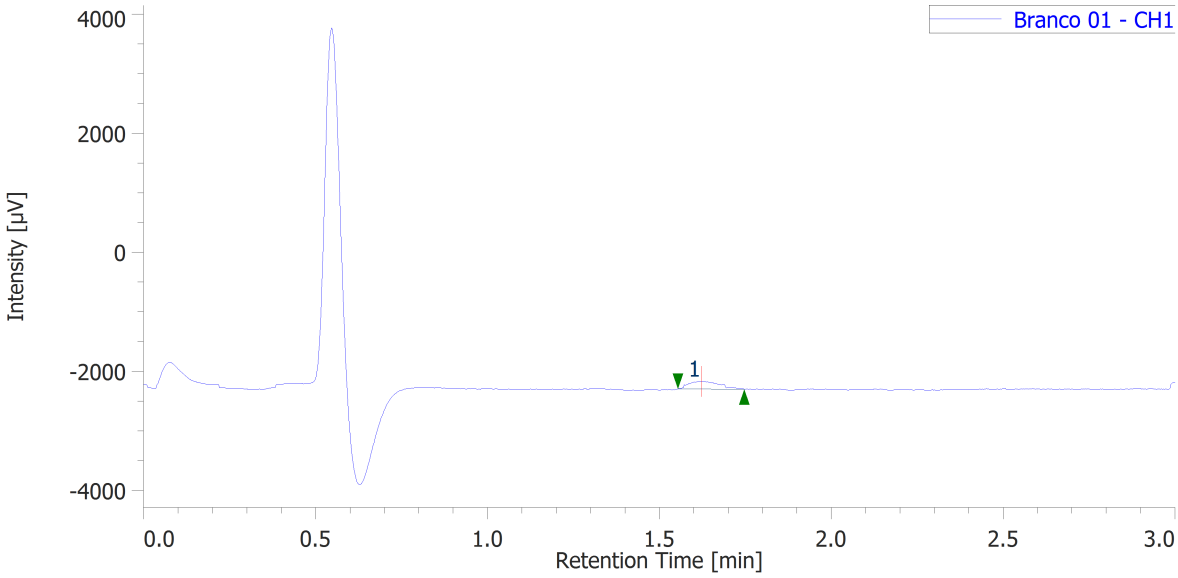


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:23:52 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 10:54:22 AM
Volume	10.00 [µL]
Sample #	46
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.622	794	126	100.000	100.000	N/A	1027	N/A	1.497	

Chromatogram

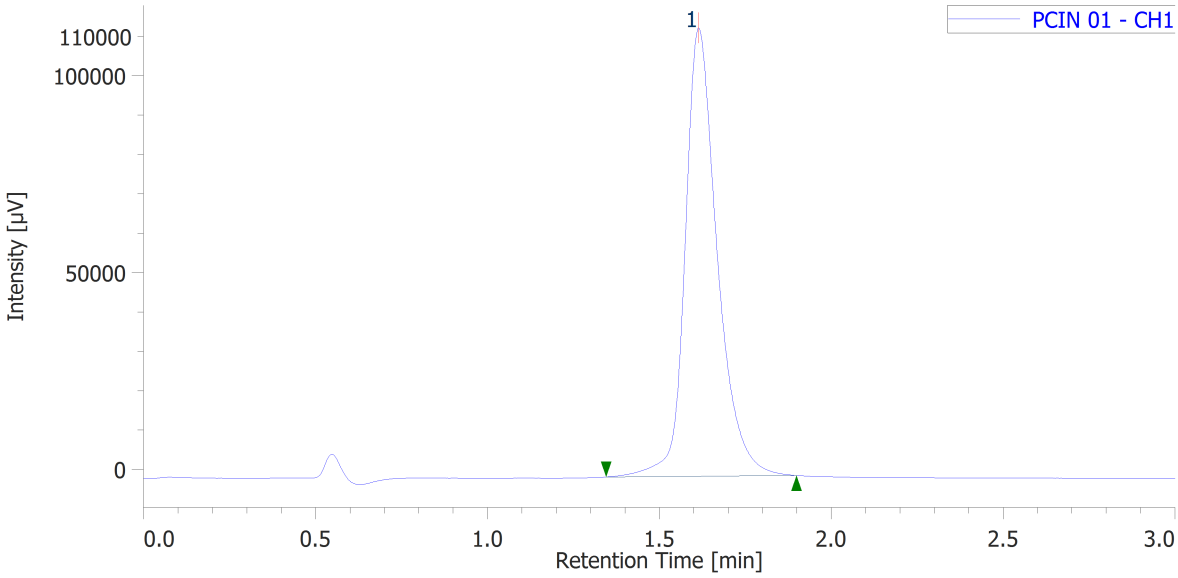


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:20:15 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 10:57:38 AM
Volume	10.00 [µL]
Sample #	47
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.613	739555	113791	100.000	100.000	N/A	1633	N/A	1.321	

Chromatogram

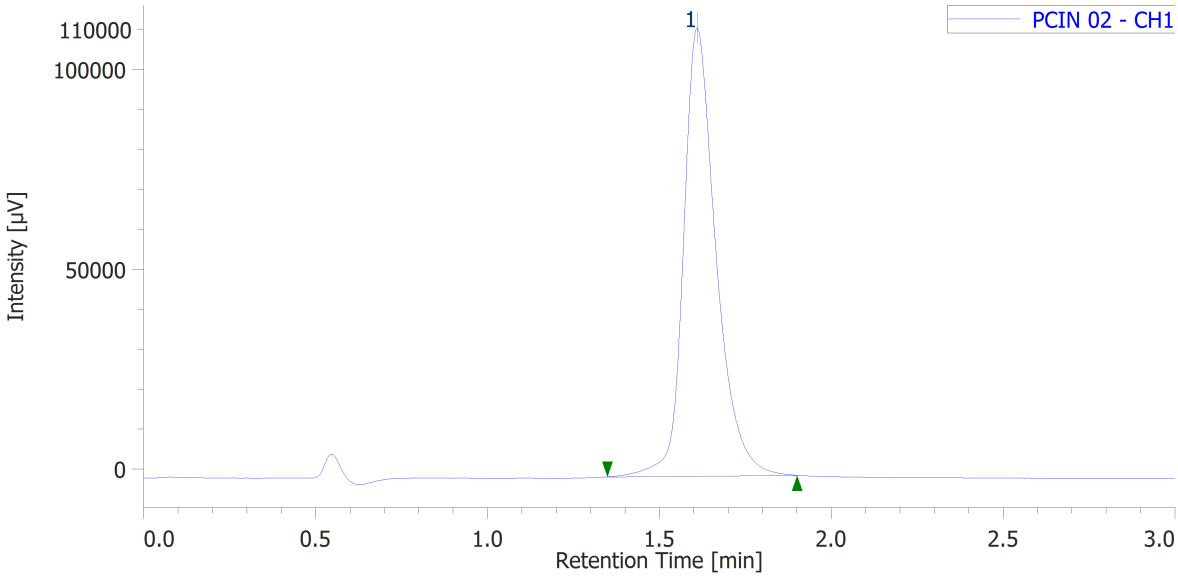


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:20:15 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:00:56 AM
Volume	10.00 [µL]
Sample #	47
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.610	738214	112085	100.000	100.000	N/A	1572	N/A	1.317	

Chromatogram

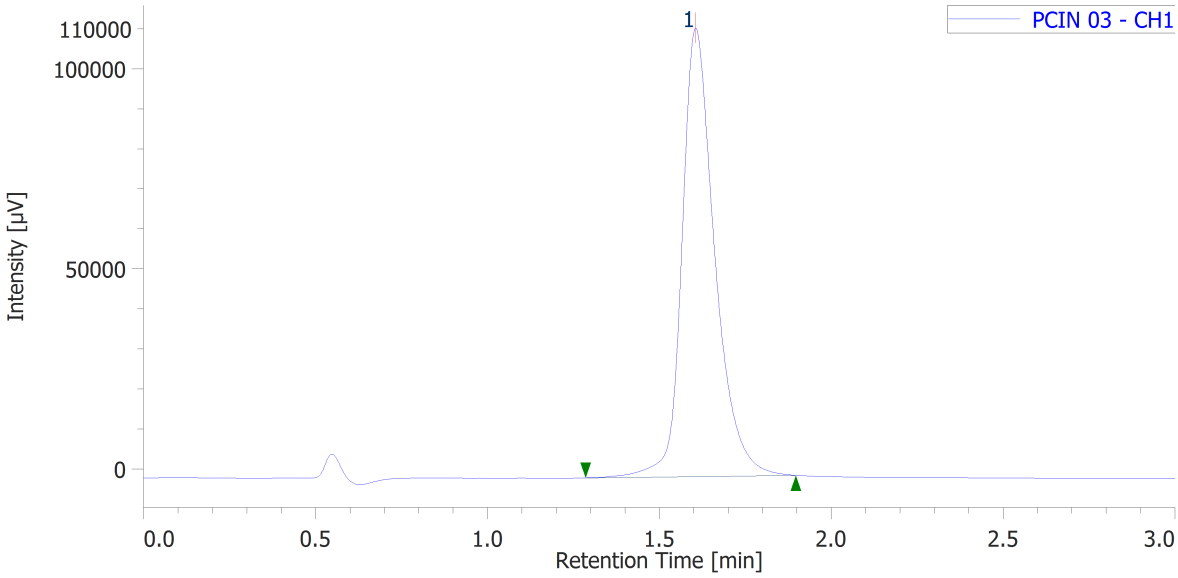


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:20:15 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:04:15 AM
Volume	10.00 [µL]
Sample #	47
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.605	743268	112063	100.000	100.000	N/A	1543	N/A	1.335	

Chromatogram

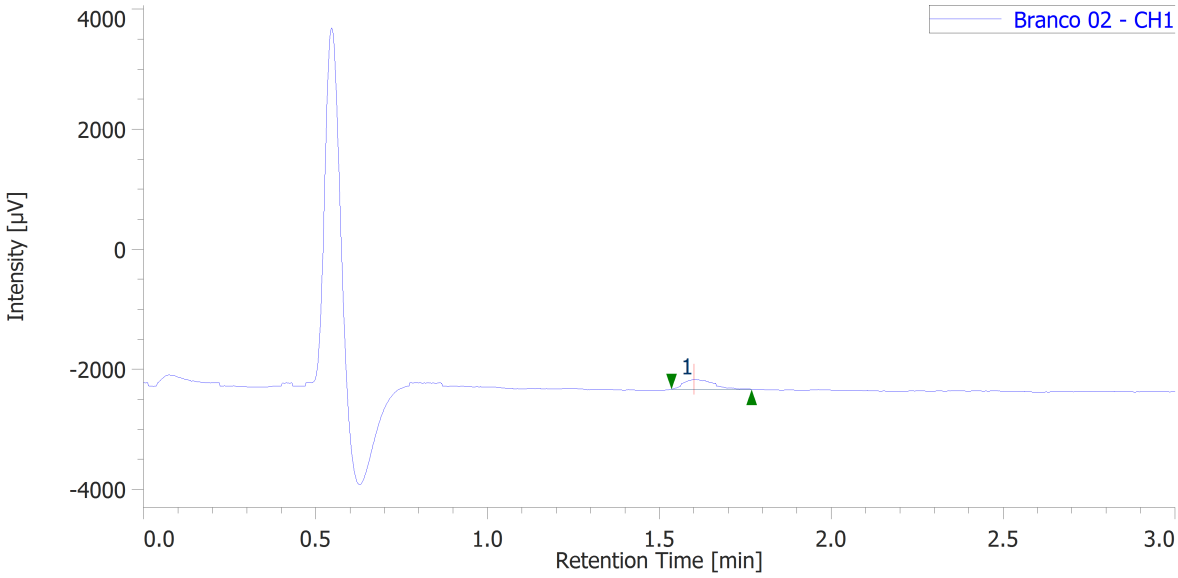


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:24:19 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:07:30 AM
Volume	10.00 [µL]
Sample #	46
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.600	1011	168	100.000	100.000	N/A	1385	N/A	1.873	

Chromatogram

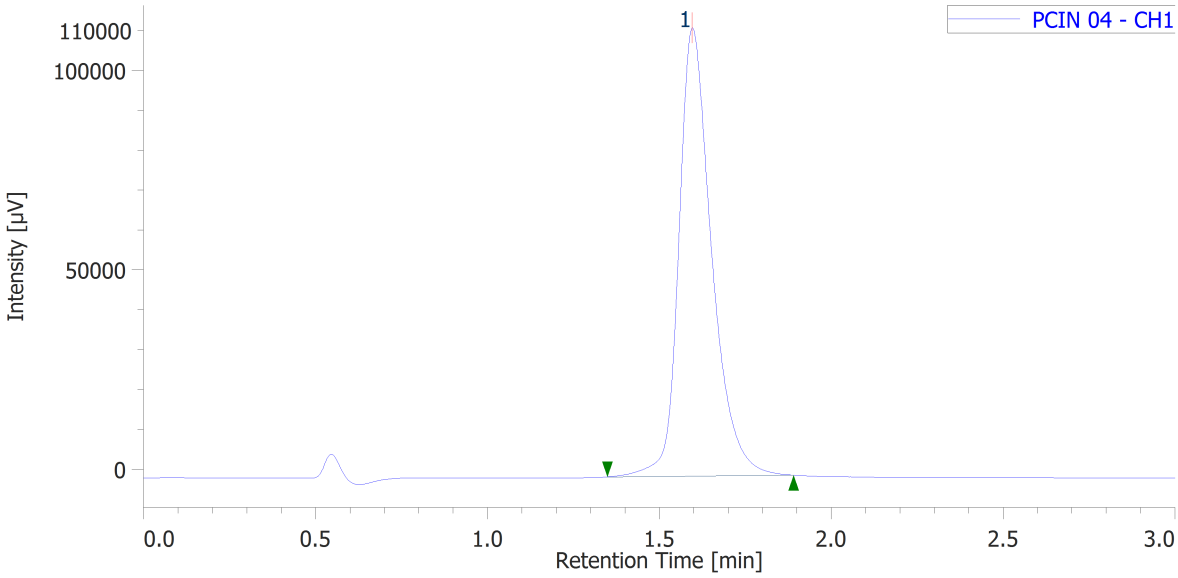


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:20:15 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:10:49 AM
Volume	10.00 [µL]
Sample #	47
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.595	745216	112306	100.000	100.000	N/A	1500	N/A	1.359	

Chromatogram

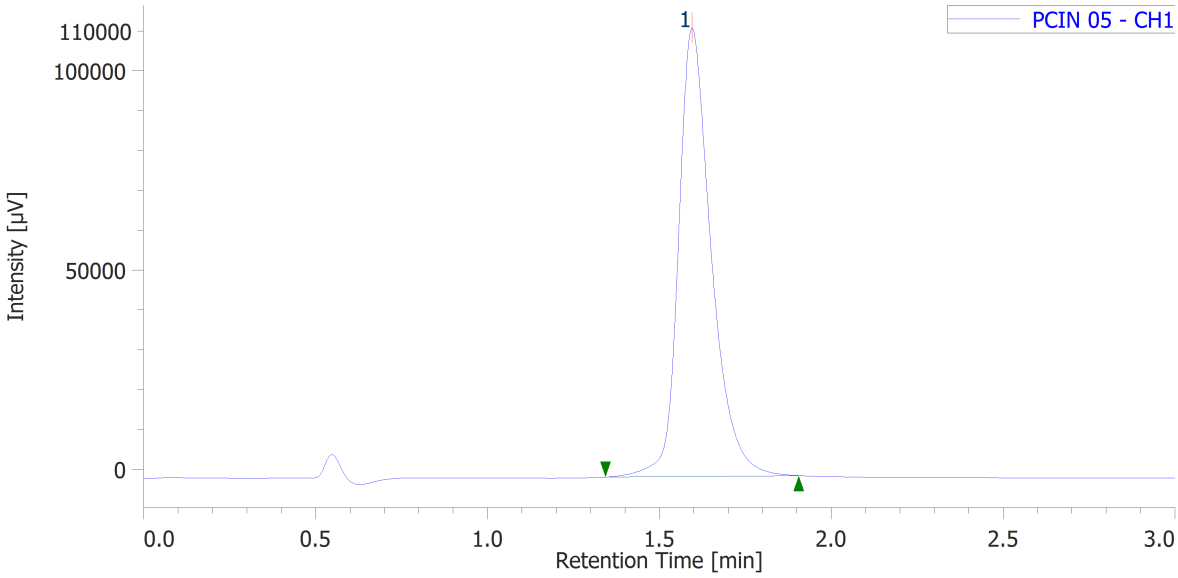


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:20:15 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:14:07 AM
Volume	10.00 [µL]
Sample #	47
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.595	745706	112510	100.000	100.000	N/A	1508	N/A	1.341	

Chromatogram

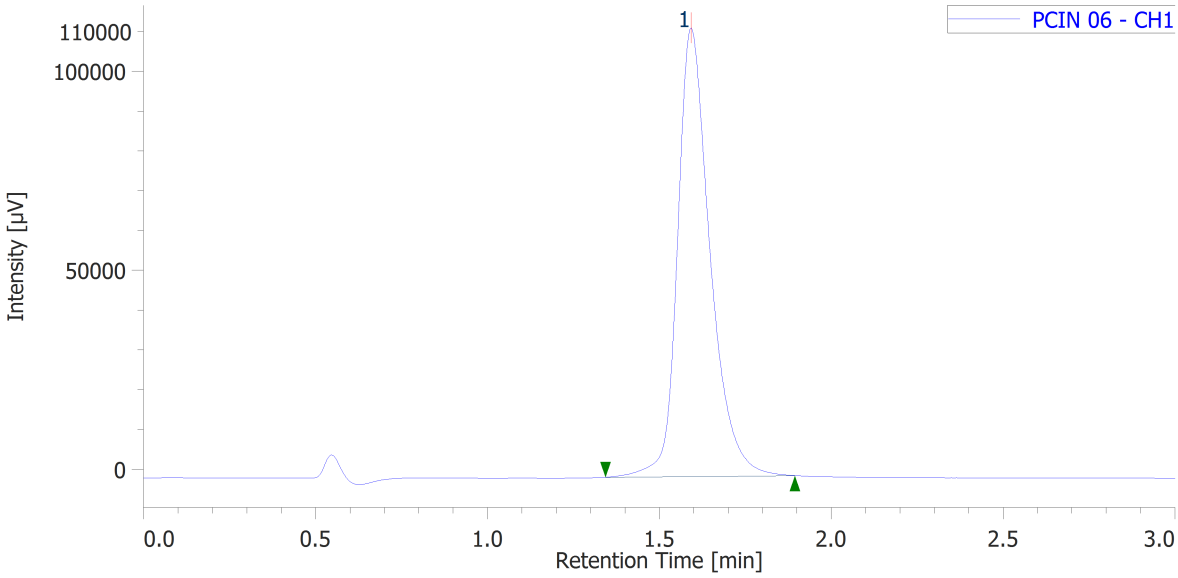


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:20:56 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:17:24 AM
Volume	10.00 [µL]
Sample #	47
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.592	740940	112646	100.000	100.000	N/A	1525	N/A	1.340	

Chromatogram

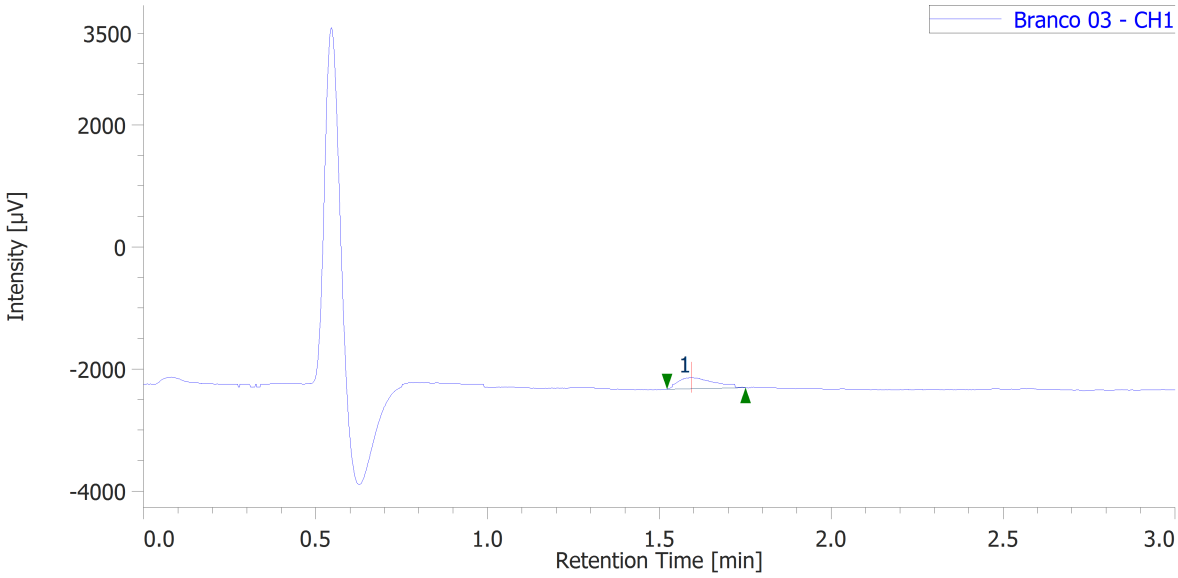


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:25:23 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:20:43 AM
Volume	10.00 [µL]
Sample #	46
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.593	1328	185	100.000	100.000	N/A	1062	N/A	1.460	

Chromatogram

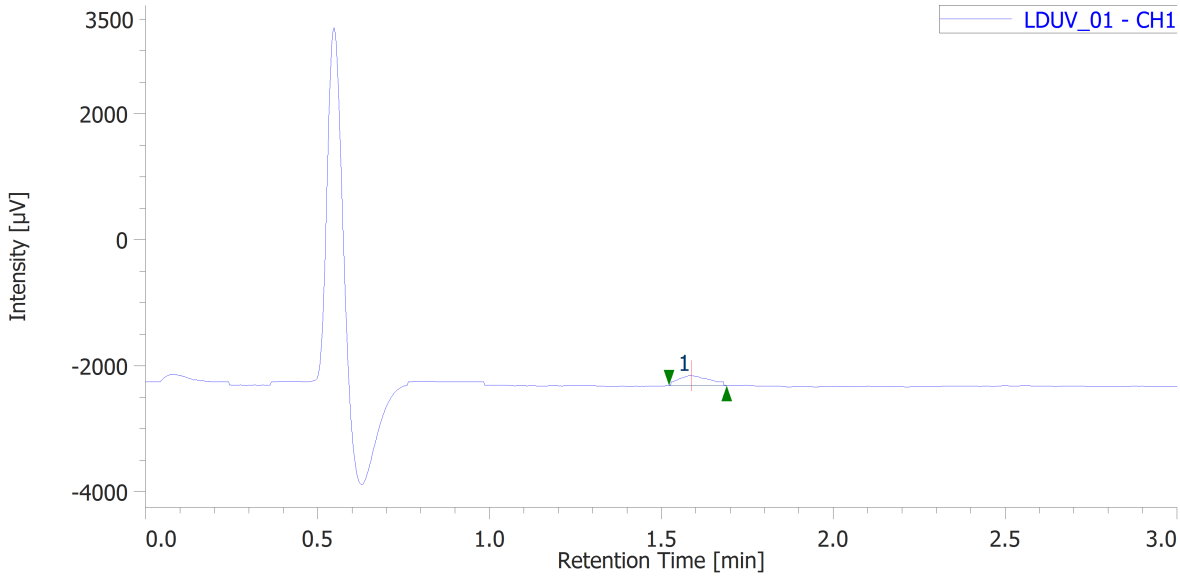


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:46:14 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:30:43 AM
Volume	10.00 [µL]
Sample #	46
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.587	974	153	100.000	100.000	N/A	1147	N/A	1.324	

Chromatogram

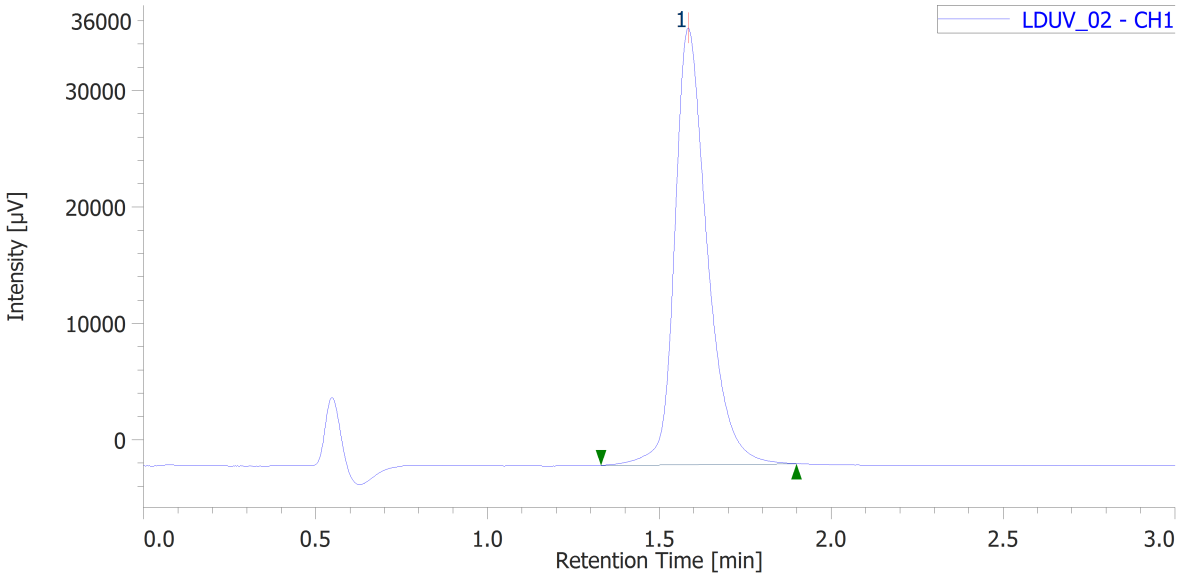


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:53:12 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:34:01 AM
Volume	10.00 [µL]
Sample #	47
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.583	246193	37491	100.000	100.000	N/A	1514	N/A	1.334	

Chromatogram

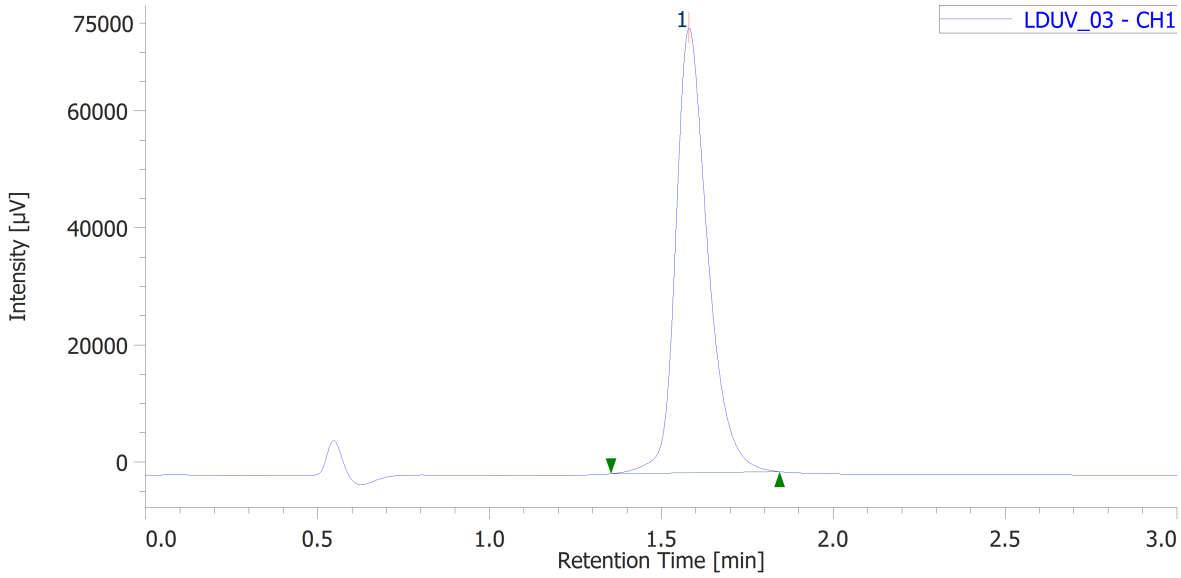


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:46:44 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:37:19 AM
Volume	10.00 [µL]
Sample #	48
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.580	492008	76010	100.000	100.000	N/A	1527	N/A	1.322	

Chromatogram

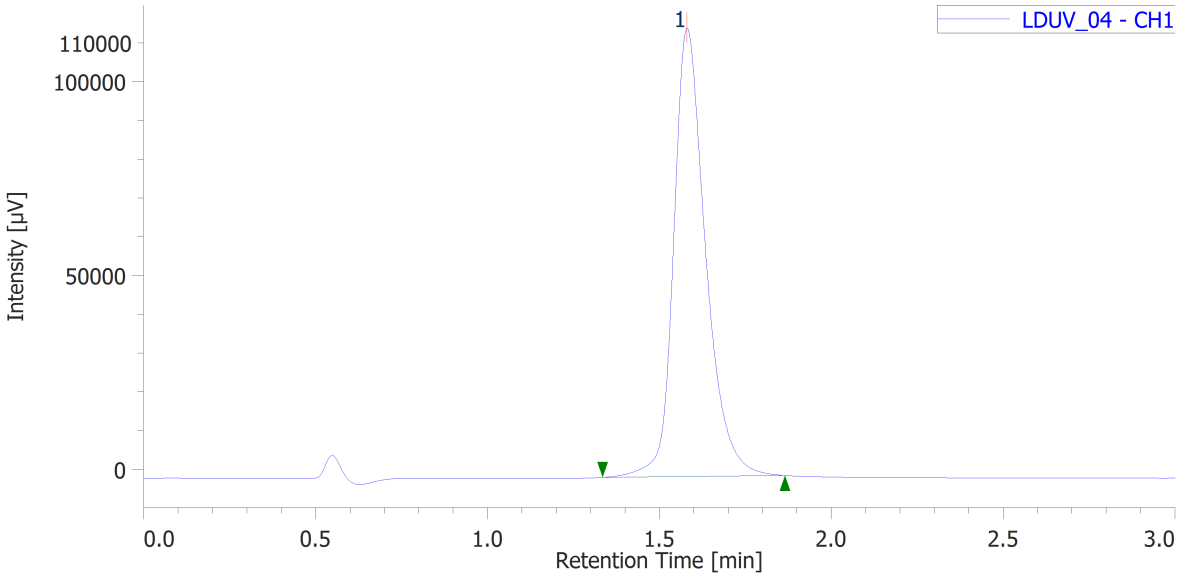


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:46:44 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:40:39 AM
Volume	10.00 [µL]
Sample #	49
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.580	747209	115600	100.000	100.000	N/A	1546	N/A	1.315	

Chromatogram

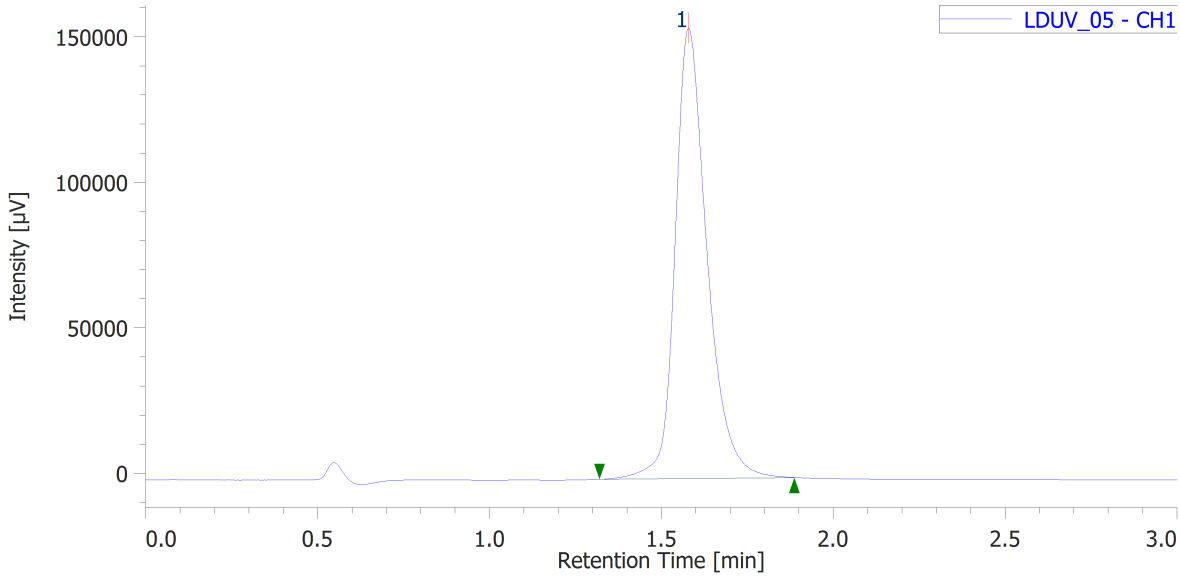


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:50:37 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:43:58 AM
Volume	10.00 [µL]
Sample #	50
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.578	1000515	154718	100.000	100.000	N/A	1552	N/A	1.313	

Chromatogram

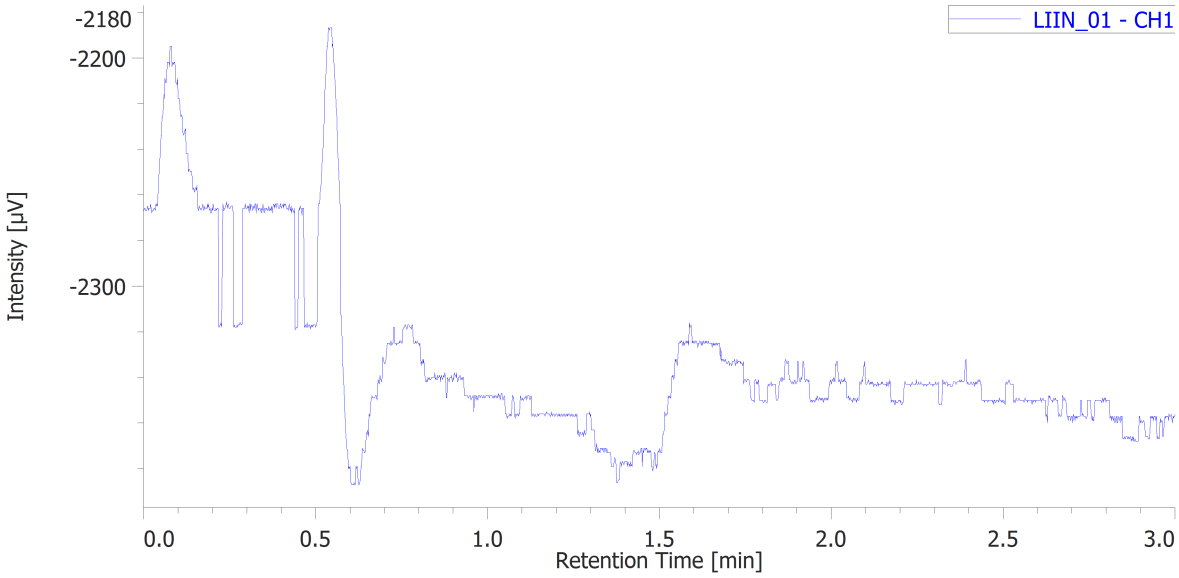


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:50:15 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:47:10 AM
Volume	0.10 [µL]
Sample #	46
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	

Chromatogram

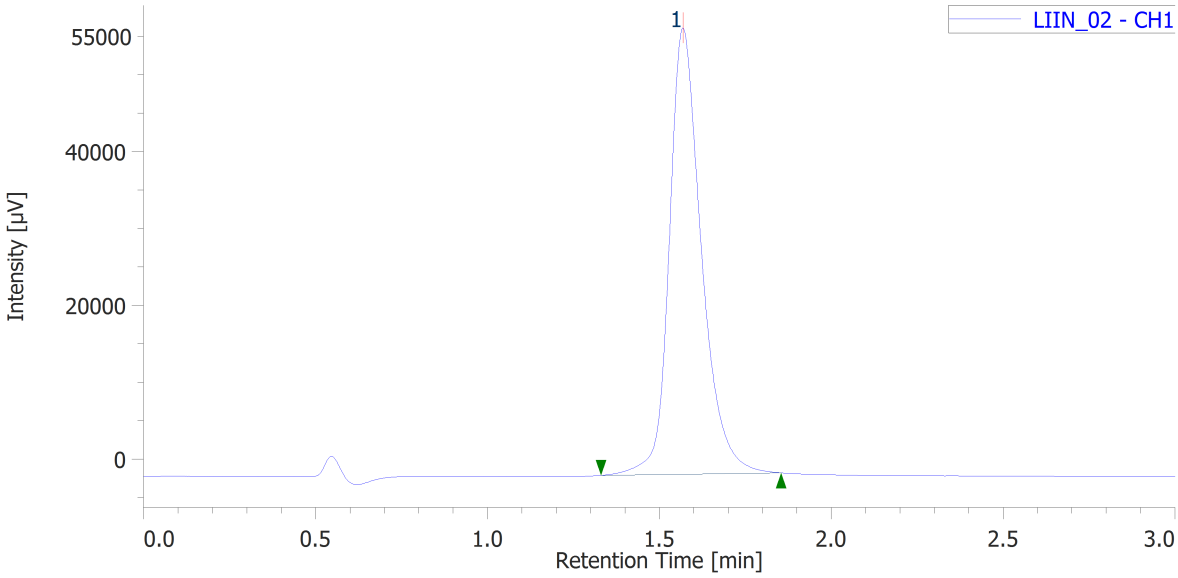


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 12:05:21 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:50:26 AM
Volume	5.00 [µL]
Sample #	49
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.568	376914	58005	100.000	100.000	N/A	1502	N/A	1.294	

Chromatogram

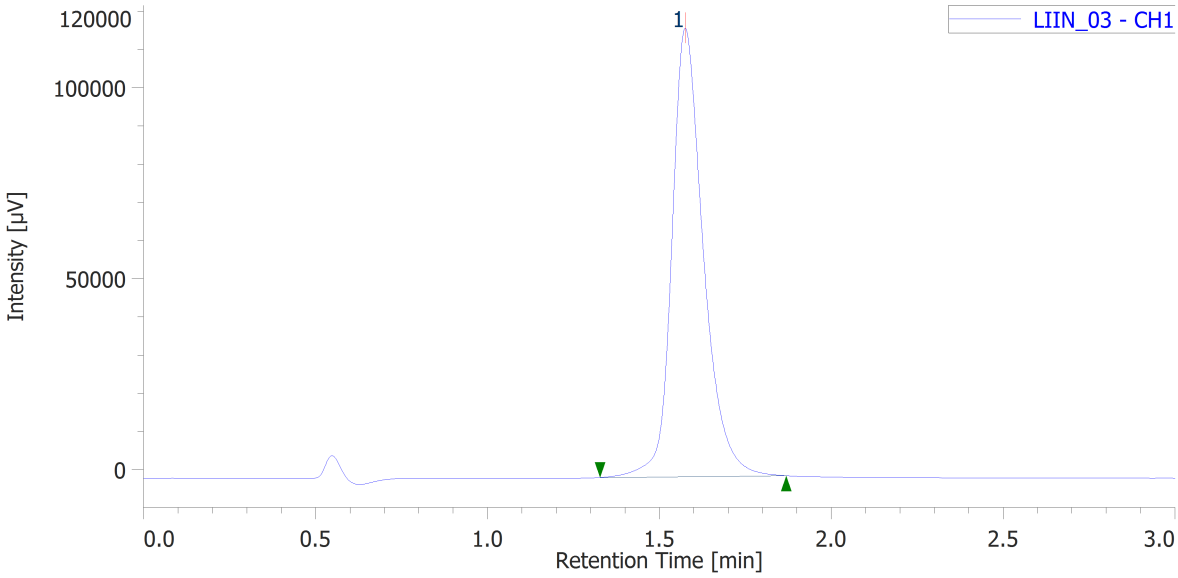


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 11:58:40 AM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:53:44 AM
Volume	10.00 [µL]
Sample #	49
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.575	749300	117446	100.000	100.000	N/A	1591	N/A	1.284	

Chromatogram

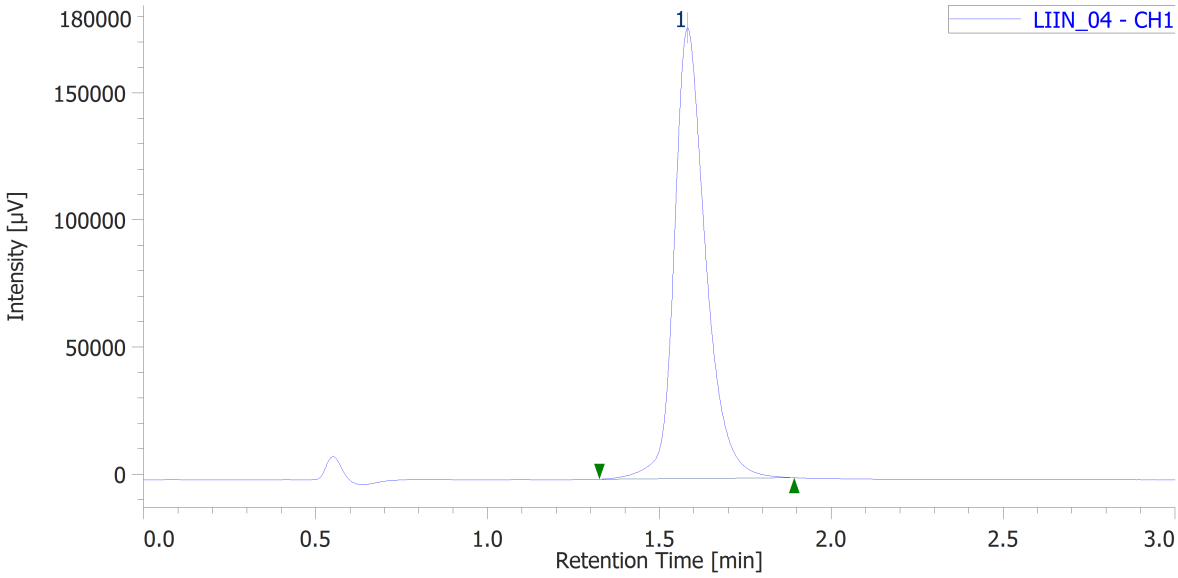


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 12:00:58 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 11:57:08 AM
Volume	15.00 [µL]
Sample #	49
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.582	1123916	177120	100.000	100.000	N/A	1627	N/A	1.289	

Chromatogram

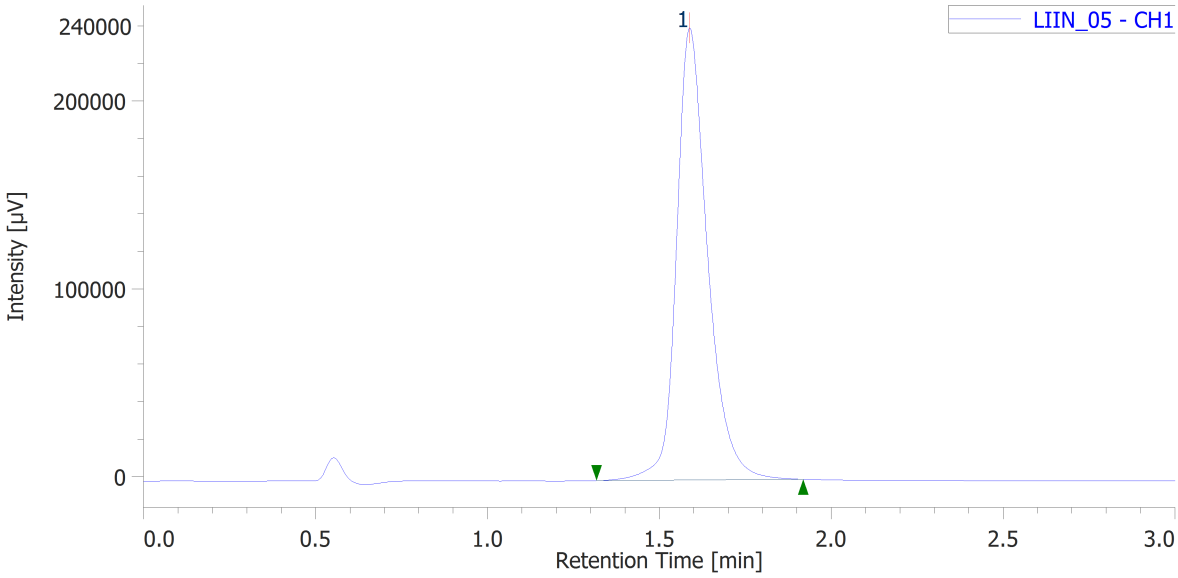


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 12:04:05 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 12:00:37 PM
Volume	20.00 [µL]
Sample #	49
Project Name	Qualificação HP01 – DLA
Acquisition Time	3.0 [min]
Acquisition Sequence	Linearidade
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1.588	1515492	240470	100.000	100.000	N/A	1670	N/A	1.288	

Chromatogram

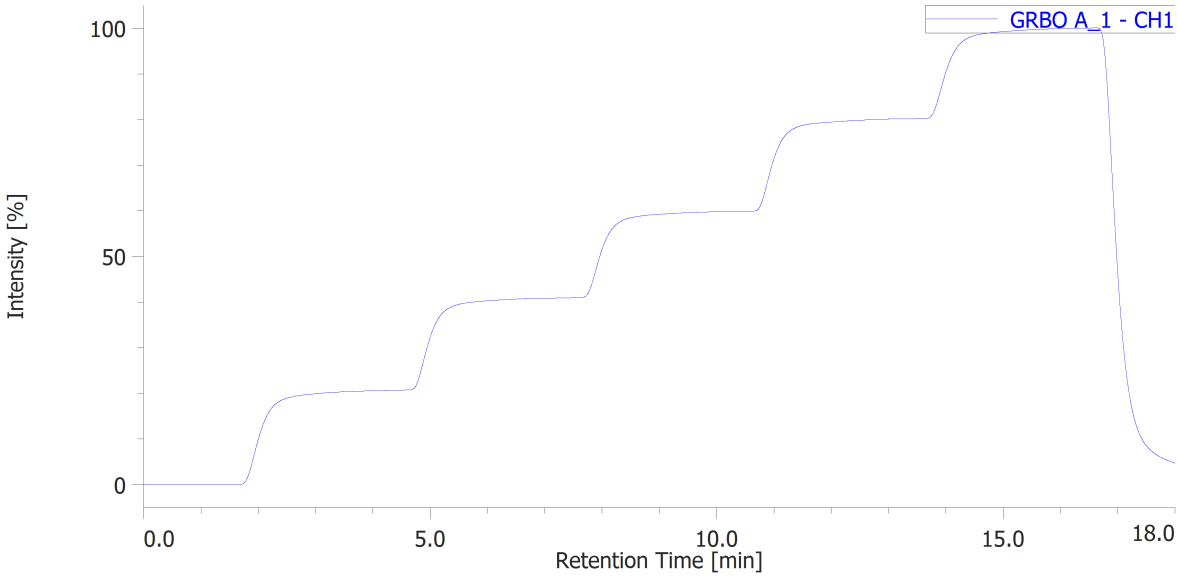


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 3:23:01 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 3:04:59 PM
Volume	0.00 [µL]
Sample #	–
Project Name	Qualificação HP01 – DLA
Acquisition Time	18.0 [min]
Acquisition Sequence	
Control Method	GRBO A
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRBO A_1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	

Chromatogram

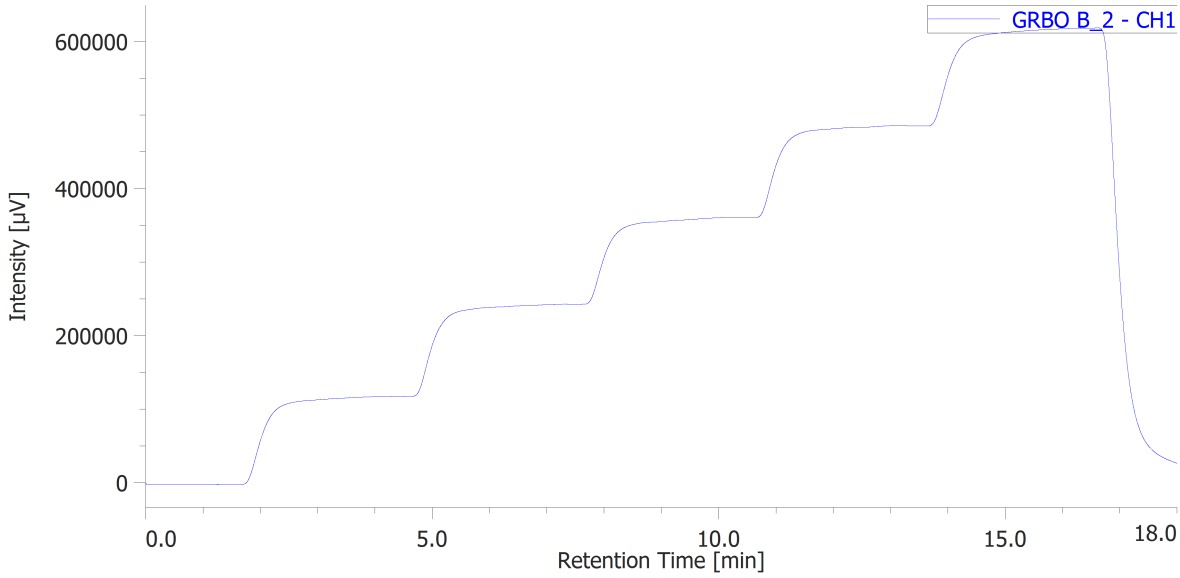


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 3:48:45 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 3:30:43 PM
Volume	0.00 [µL]
Sample #	–
Project Name	Qualificação HP01 – DLA
Acquisition Time	18.0 [min]
Acquisition Sequence	
Control Method	GRBO B
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRBO B_2–CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	

Peak Find - Comprimento de Onda_004 FPEm_tR0.54 D.jws

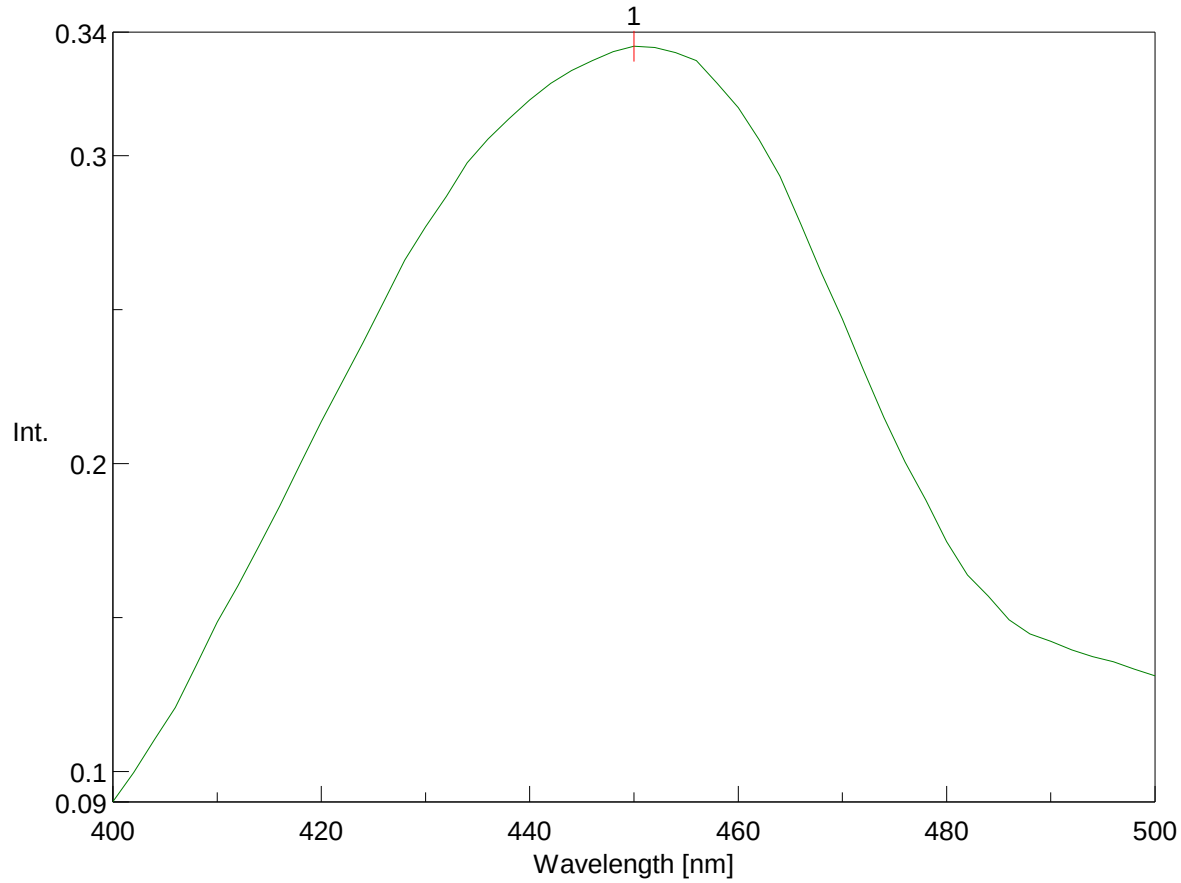

[Comments]

User	Administrator
Division	---
Company	Jasco
Creation date	8/24/2018 9:53 AM


[Detailed Information]		[Measurement Information]	
Data array type	Linear data array	Instrument Name	FP-1520
Horizontal axis	Wavelength [nm]	Model Name	FP-1520
Vertical axis	Int.	Serial No.	XXXXX
Start	360 nm	ROM version	V1.42
End	700 nm		
Data interval	2 nm	Measurement mode	Emission
Data points	171	Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	450	0.335434			

Chromatogram


Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 1:23:27 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 1:21:53 PM
Sample #	46
Project Name	Qualificação HP01 – DLA
Chromatogram Name	LDFL_01
Sample Name	
Acquisition Time	1.5 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

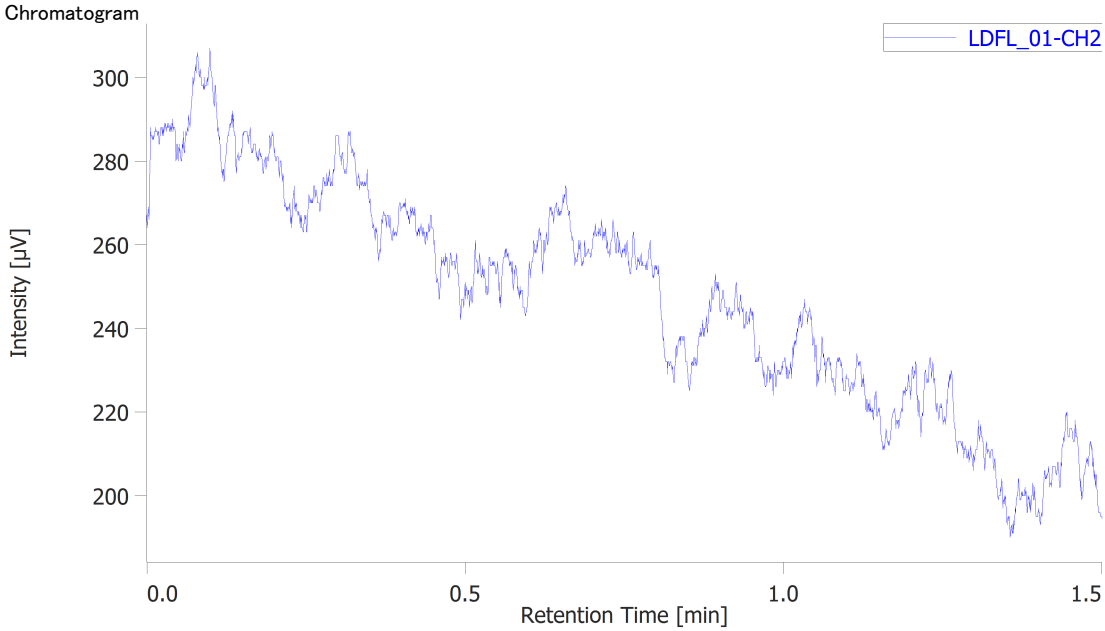

Peak Information – No data.

Chromatogram

Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 2:49:21 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 1:31:46 PM
Sample #	47
Project Name	Qualificação HP01 – DLA
Chromatogram Name	LDFL_02
Sample Name	
Acquisition Time	1.5 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	Identificação FL
Calibration Method	
Additional Information	
Column Info	

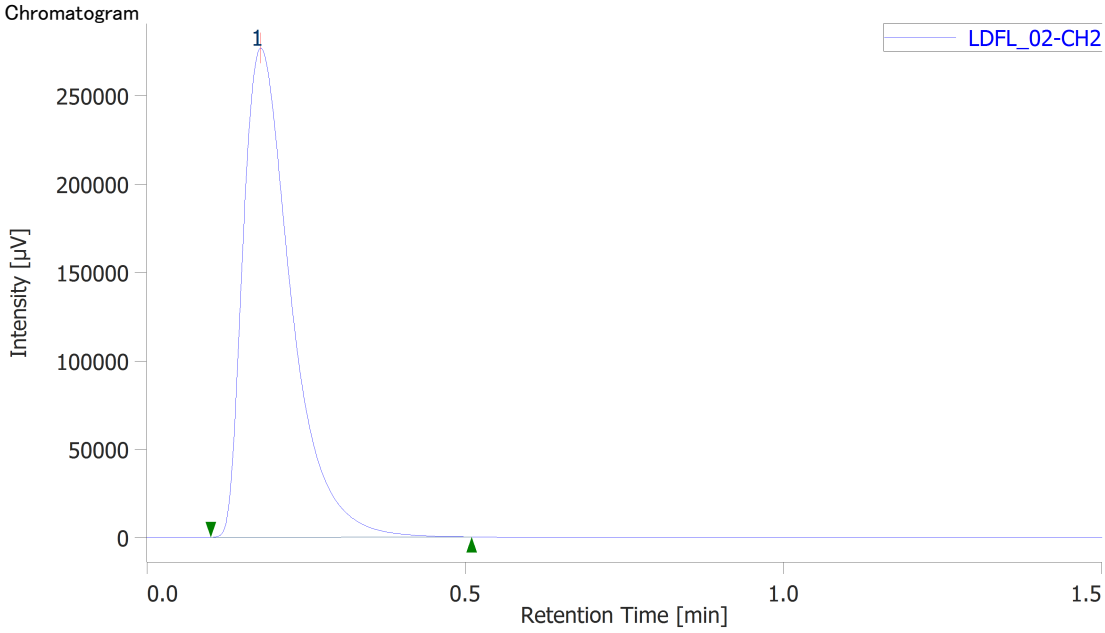


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Warning
1	PD Quinina	2	0.179	1450971	

Chromatogram

Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 1:54:14 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 1:49:17 PM
Sample #	48
Project Name	Qualificação HP01 – DLA
Chromatogram Name	LDFL_03
Sample Name	
Acquisition Time	1.5 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	Identificação FL
Calibration Method	
Additional Information	
Column Info	

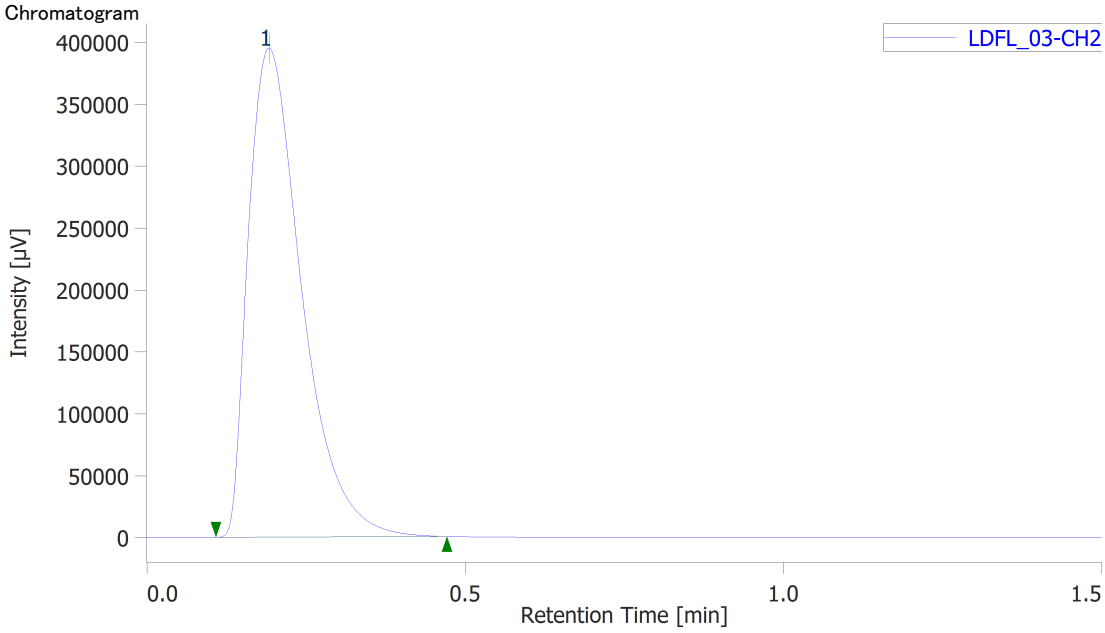


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Warning
1	PD Quinina	2	0.192	2299188	

Chromatogram

Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 2:29:42 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 2:24:29 PM
Sample #	49
Project Name	Qualificação HP01 – DLA
Chromatogram Name	LDFL_04
Sample Name	
Acquisition Time	1.5 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	Identificação FL
Calibration Method	
Additional Information	
Column Info	

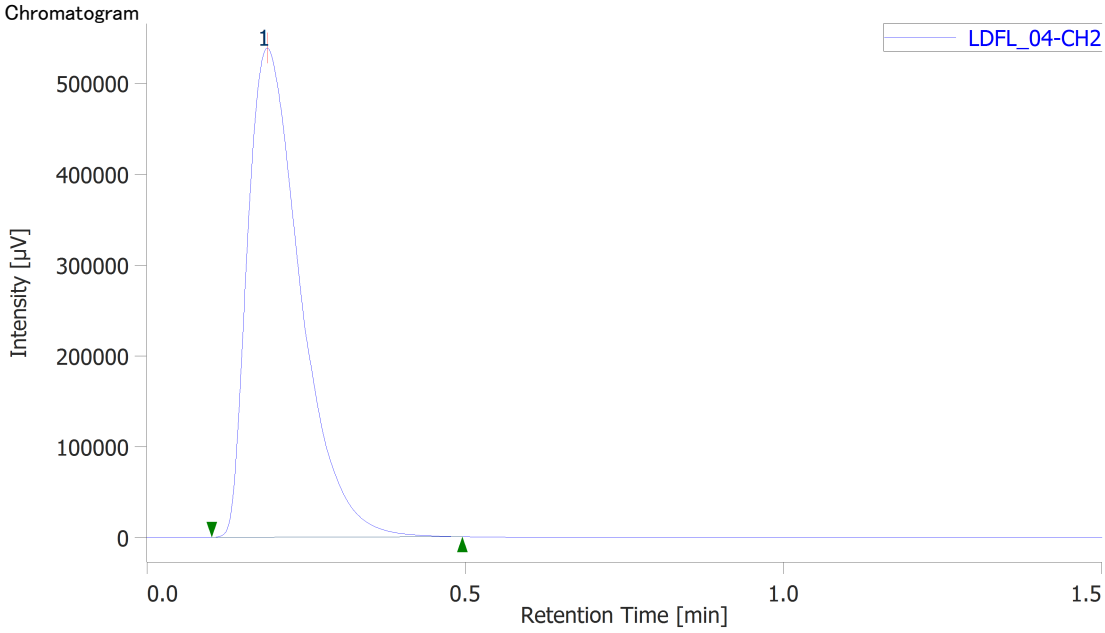


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Warning
1	PD Quinina	2	0.189	3114710	

Chromatogram

Chromatogram Information	
User Name	Administrator
Date Modified	8/24/2018 2:48:21 PM
Description	
HPLC System Name	5CQ1HP01
Injection Date	8/24/2018 2:44:37 PM
Sample #	50
Project Name	Qualificação HP01 – DLA
Chromatogram Name	LDFL_05
Sample Name	
Acquisition Time	1.5 [min]
Acquisition Sequence	
Control Method	Qualificação FL
Peak ID Table	Identificação FL
Calibration Method	
Additional Information	
Column Info	

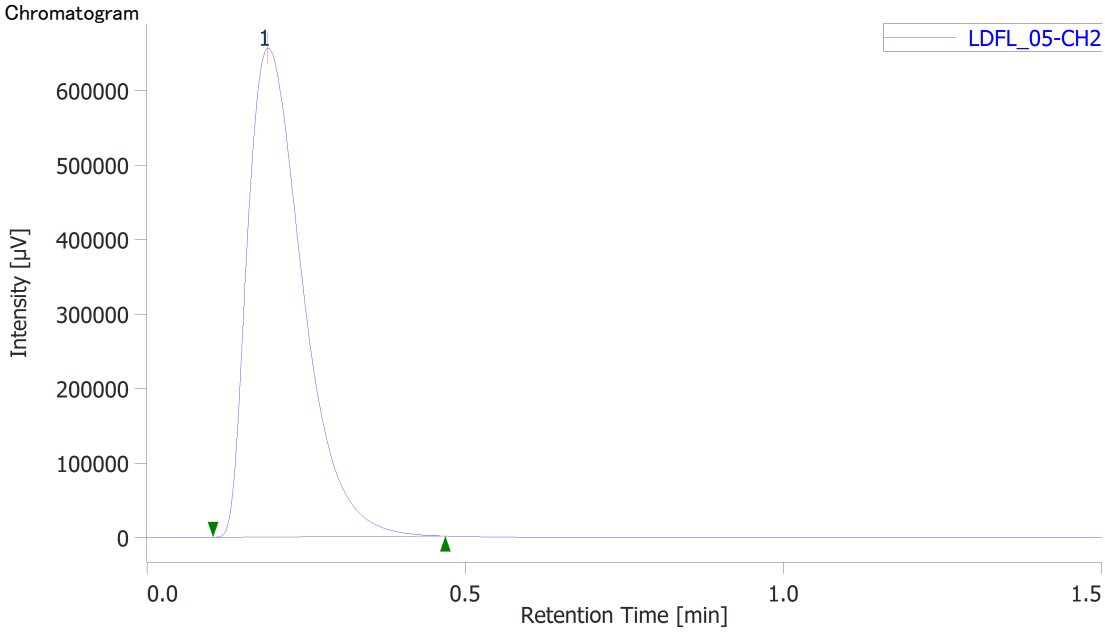

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Warning
1	PD Quinina	2	0.190	3945261	