

Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:36:23
Volume	10.00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

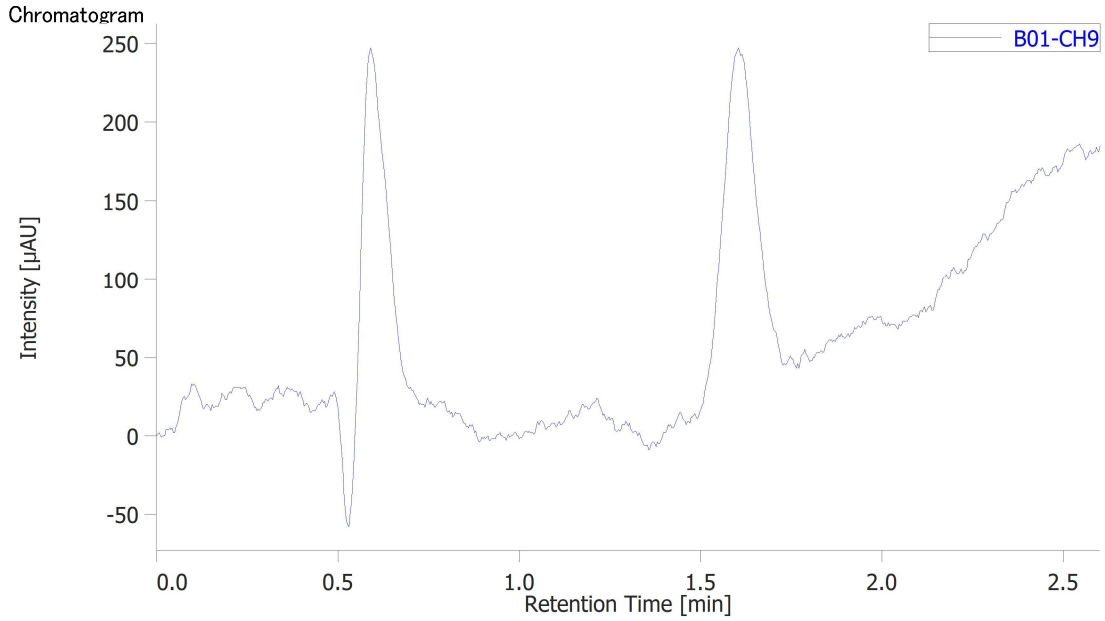


Peak Information – No data.

Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:47:35
Volume	10.00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

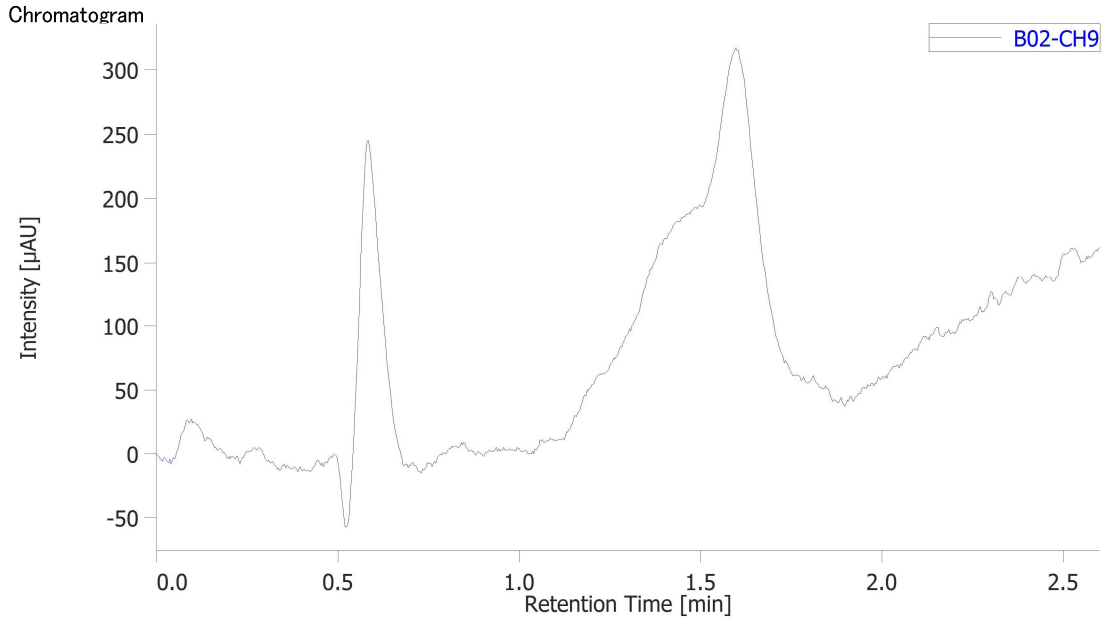


Peak Information – No data.

Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:58:47
Volume	10.00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

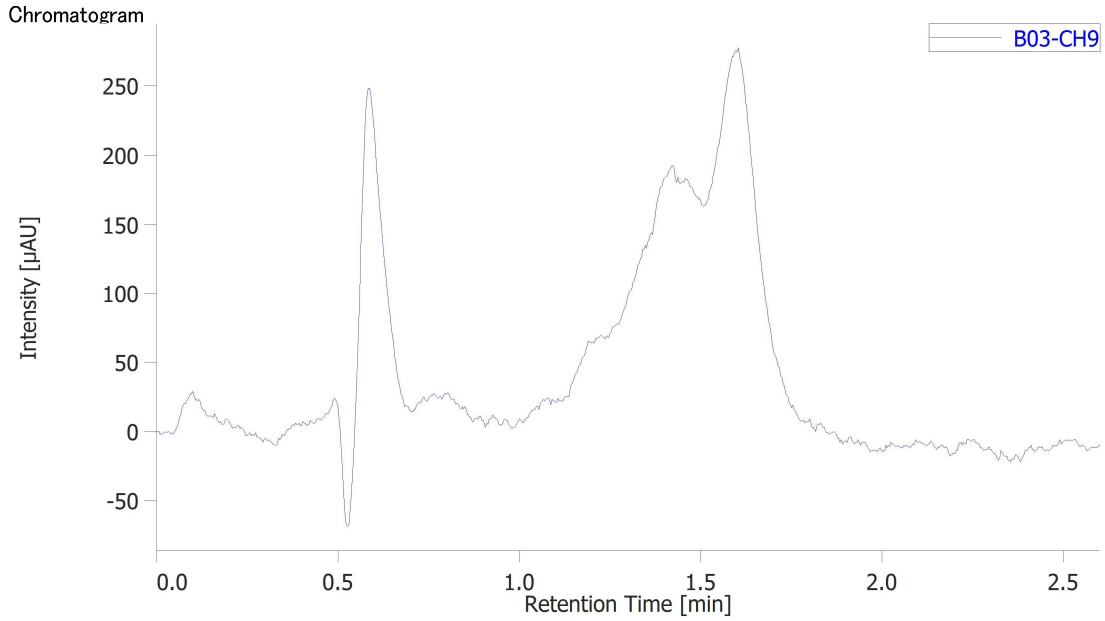

Peak Information – No data.

Peak Find - EDUV_001 PDA_1.6100.JWS

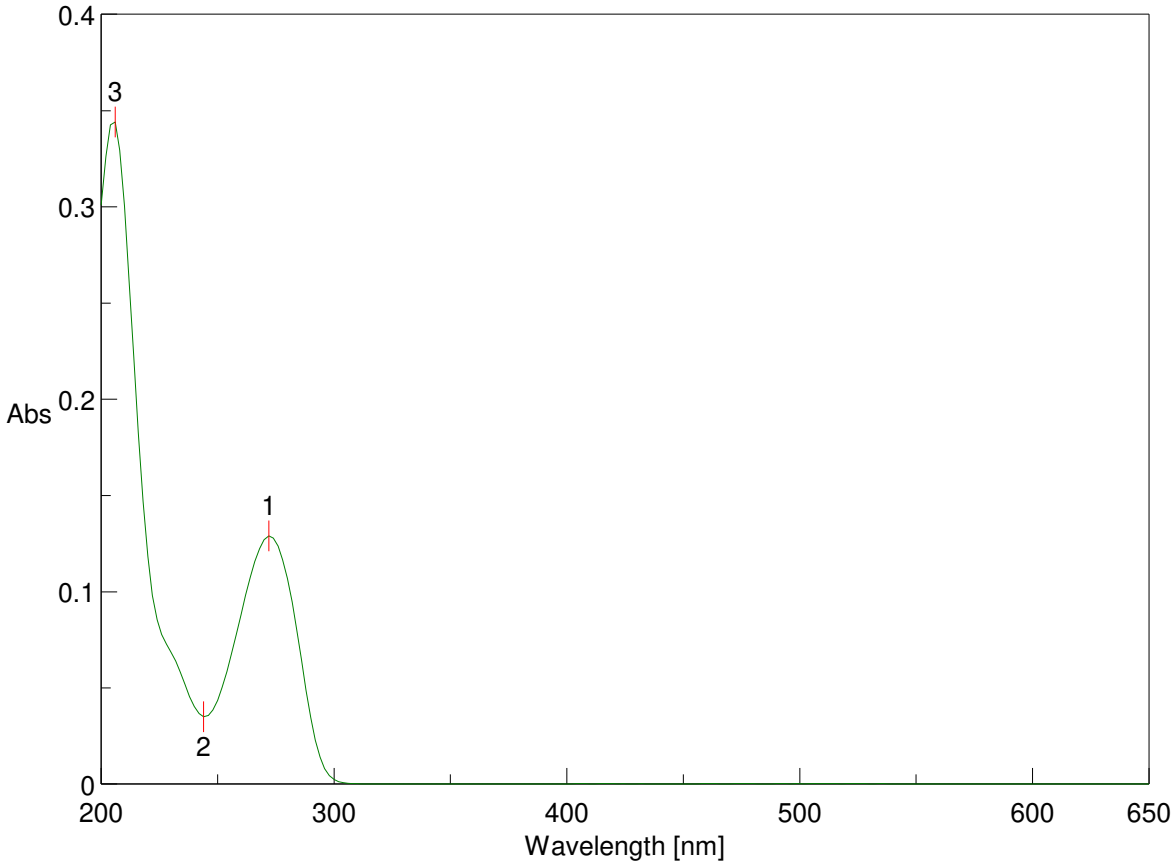

[Comments]

User	Administrator
Division	---
Company	Jasco
Creation date	02/10/2018 10:44
Date modified	02/10/2018 11:43

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	650 nm
Data interval	2 nm
Data points	226


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A025161665
ROM version	V1.02.02

[Result of Peak Picking]


No.	Position	Intensity	No.	Position	Intensity
1	272	0.128823	2	244	0.034921
3	206	0.343962			

Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 14:17:50
Volume	0.00 [µL]
Sample #	–
Project Name	Jasco
Acquisition Time	36.0 [min]
Acquisition Sequence	
Control Method	Qualificação Gradiente 2018
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

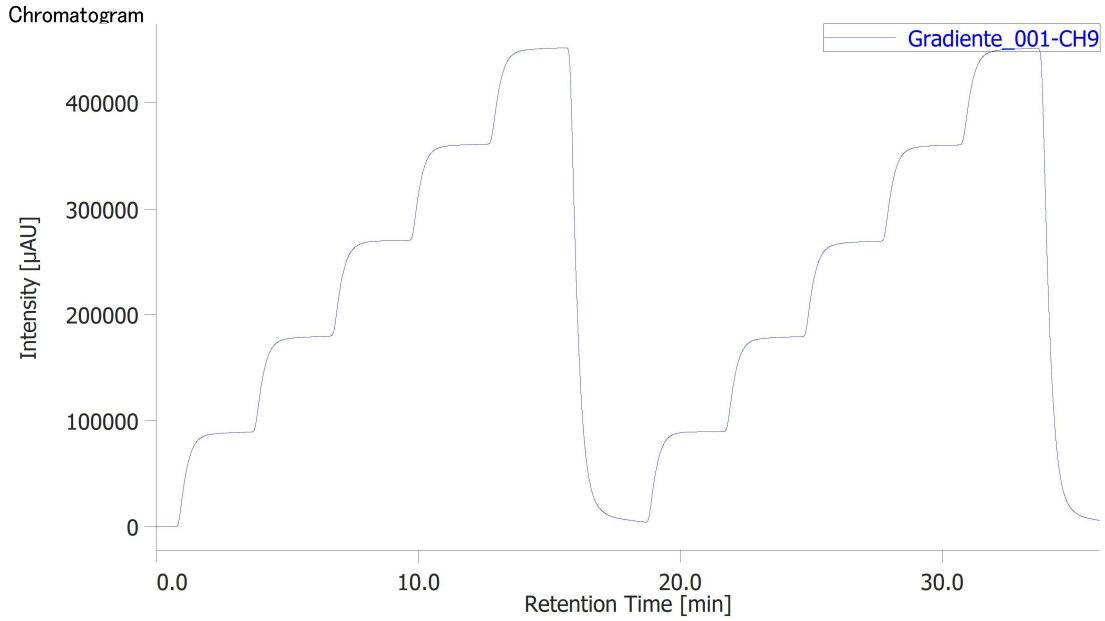


Peak Information – No data.

Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 12:01:35
Volume	10.00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva
Additional Information	
Column Info	

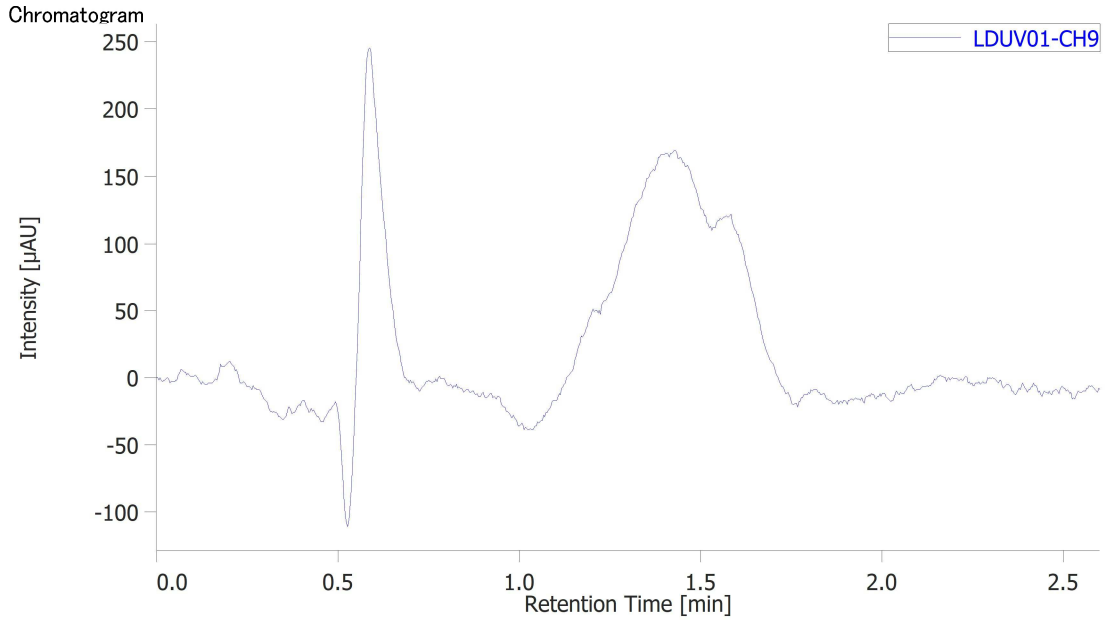

Peak Information – No data.


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 12:04:23
Volume	10.00 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva
Additional Information	
Column Info	

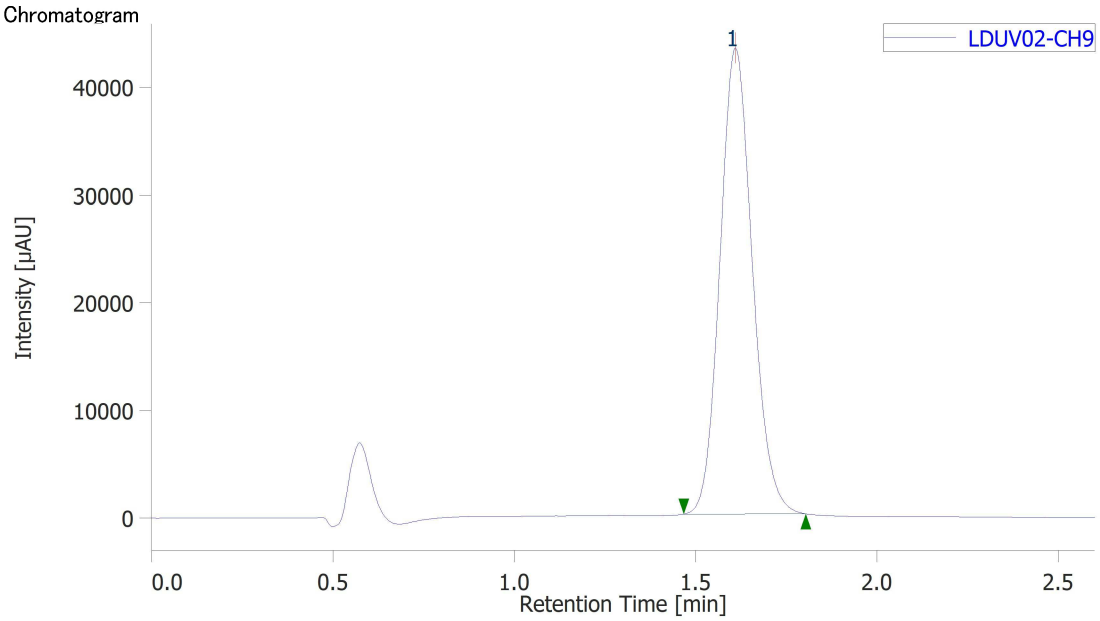

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.610	268315	43240


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 12:07:11
Volume	10.00 [µL]
Sample #	4
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva
Additional Information	
Column Info	

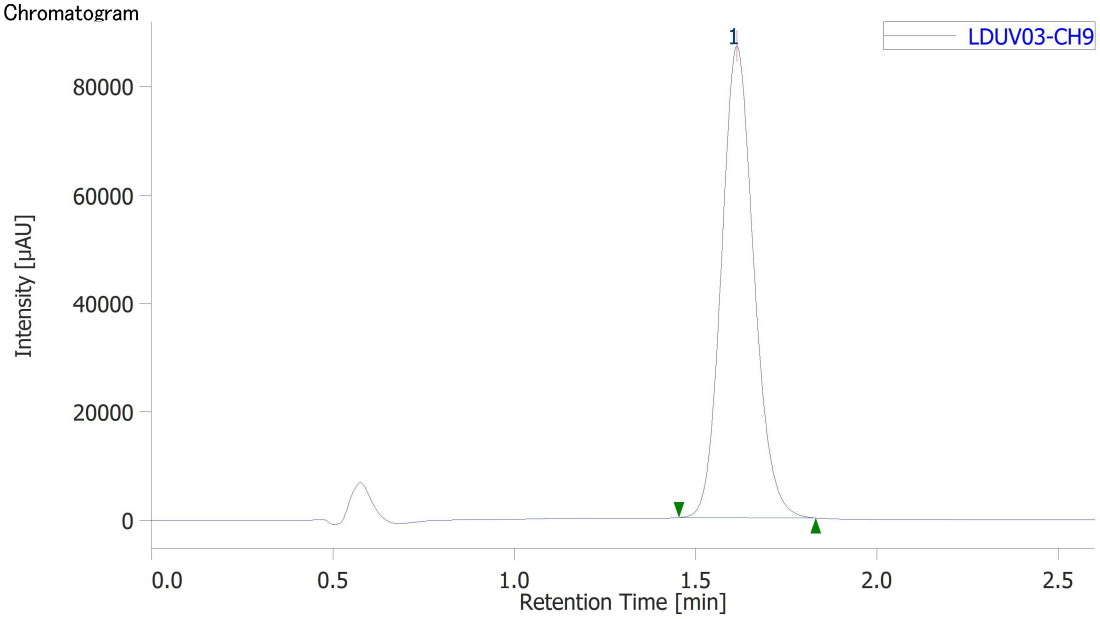

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.613	540580	86934


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 12:09:59
Volume	10.00 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva
Additional Information	
Column Info	

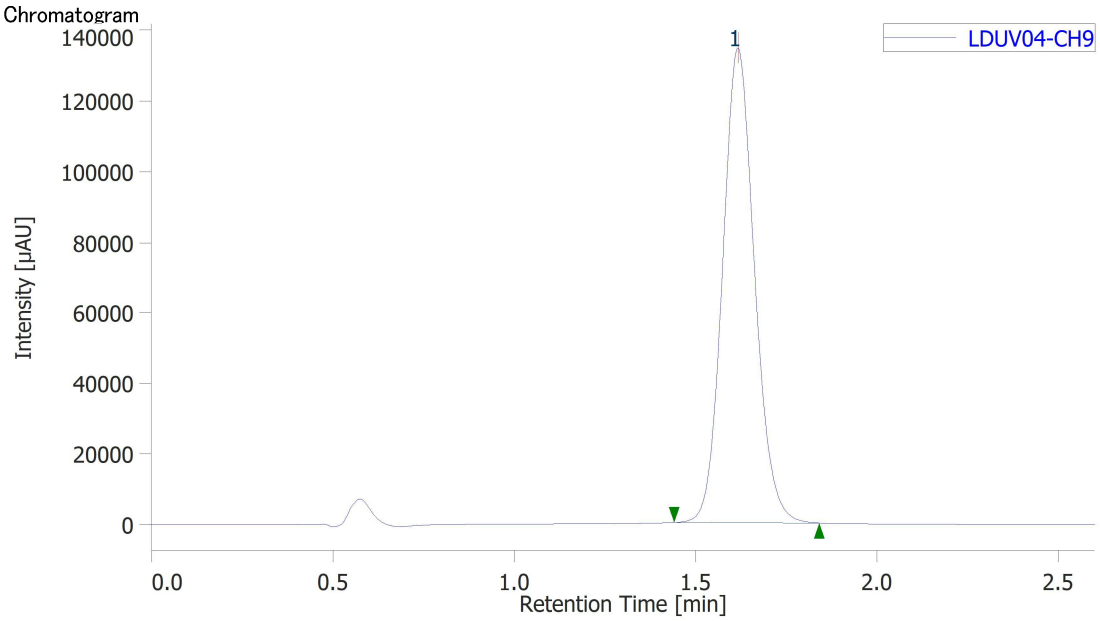

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.617	821278	134368


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 12:12:47
Volume	10.00 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva
Additional Information	
Column Info	

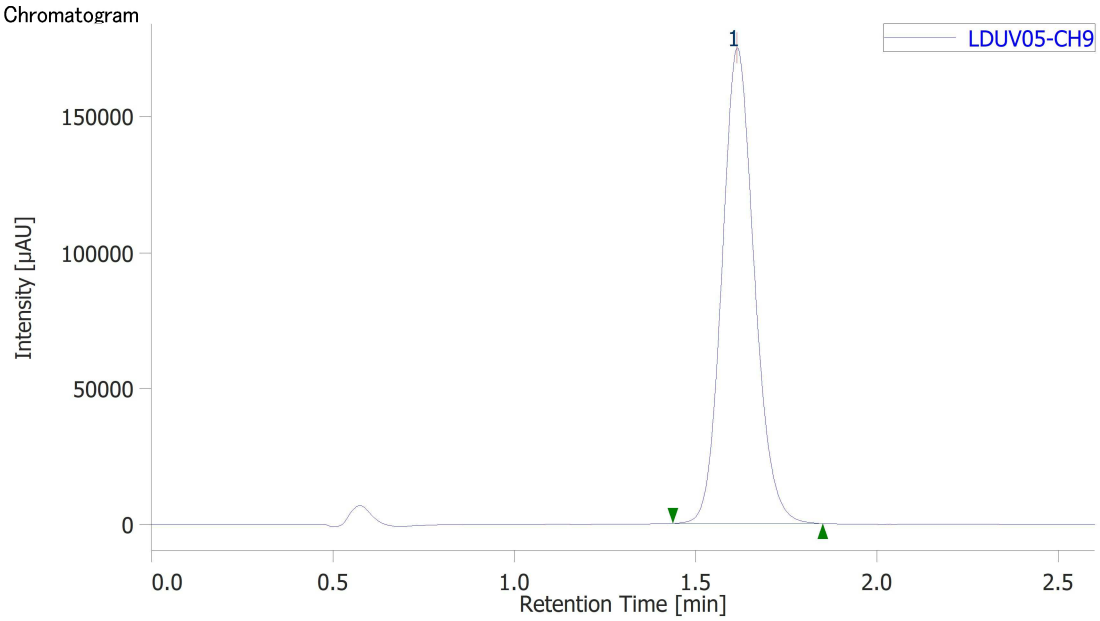

Peak Information


#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.613	1080734	174523

Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 13:16:47
Volume	0.10 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação LIIN
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva LIIN
Additional Information	
Column Info	

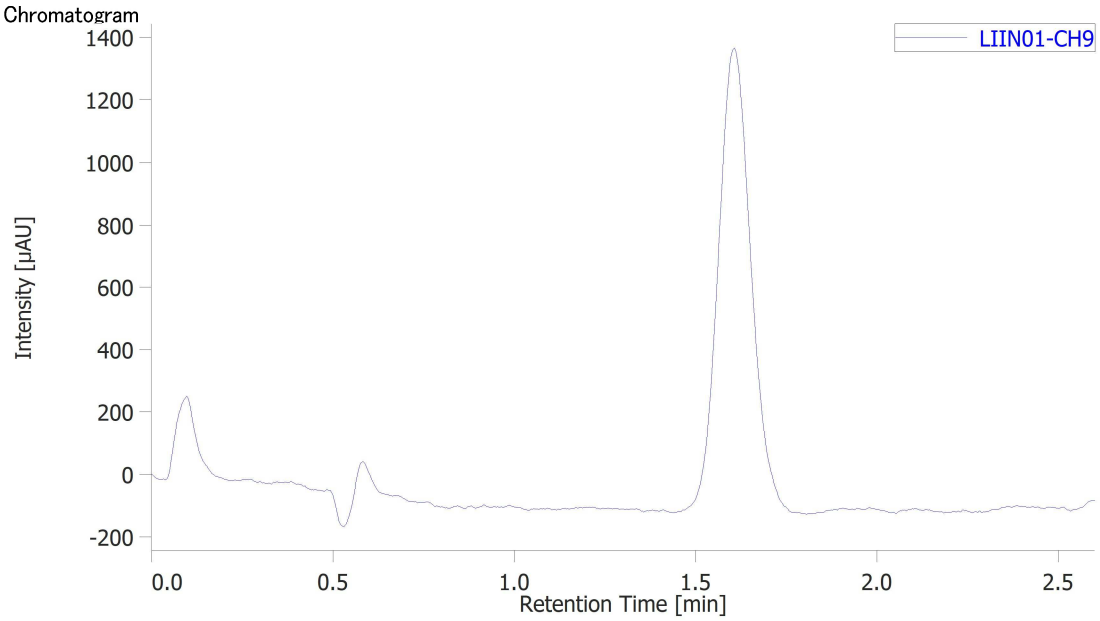

Peak Information – No data.


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 13:19:35
Volume	5.00 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação LIIN
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva LIIN
Additional Information	
Column Info	

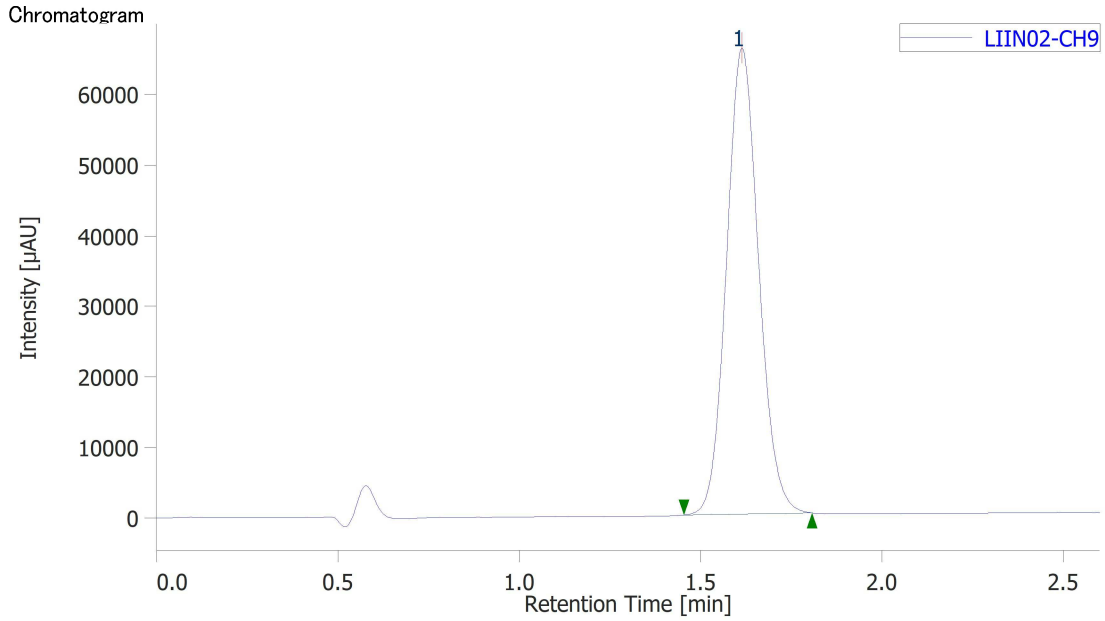

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.613	406217	65982


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 13:22:23
Volume	10.00 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação LIIN
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva LIIN
Additional Information	
Column Info	

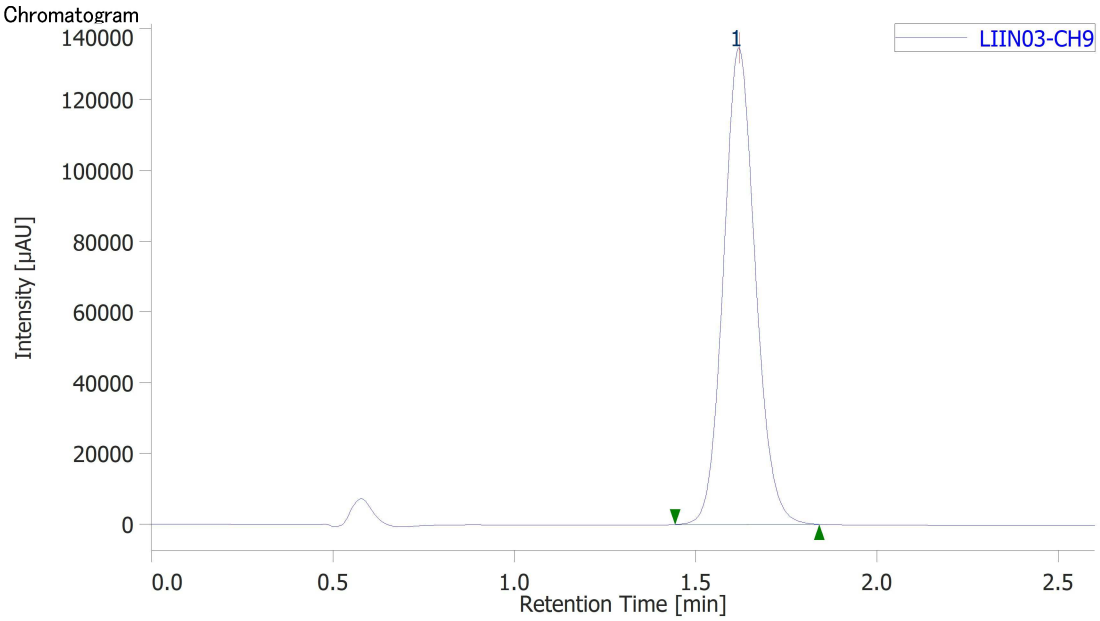

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.620	822097	134573


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 13:25:11
Volume	15.00 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação LIIN
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva LIIN
Additional Information	
Column Info	

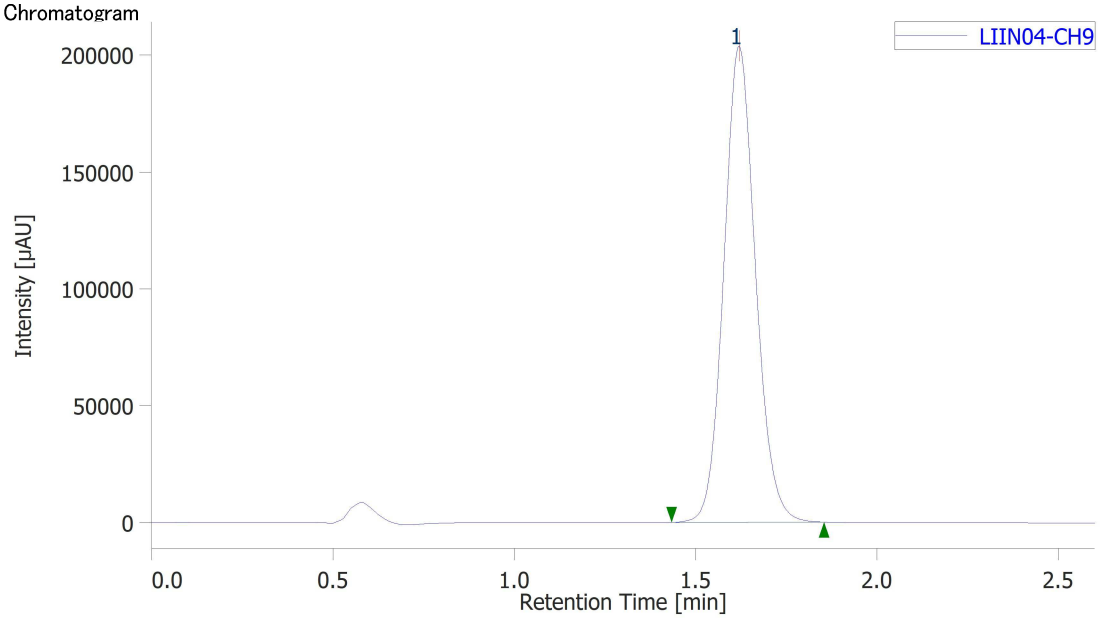

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.620	1235263	203675


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 13:28:01
Volume	20.00 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação LIIN
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	Curva LIIN
Additional Information	
Column Info	

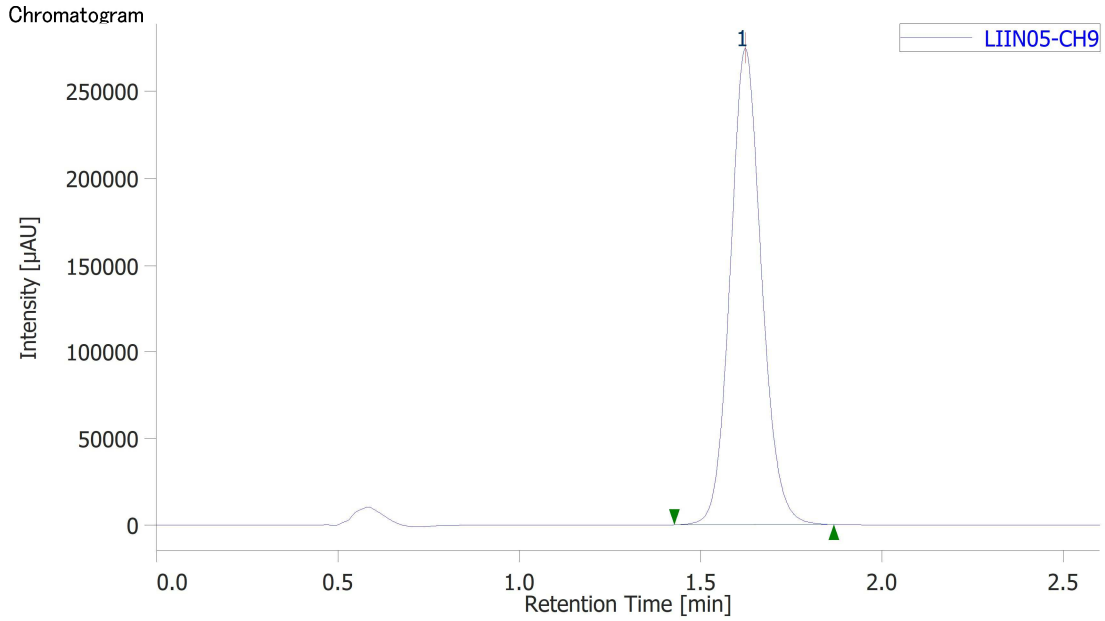

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.623	1646540	274488


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:39:11
Volume	10.00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

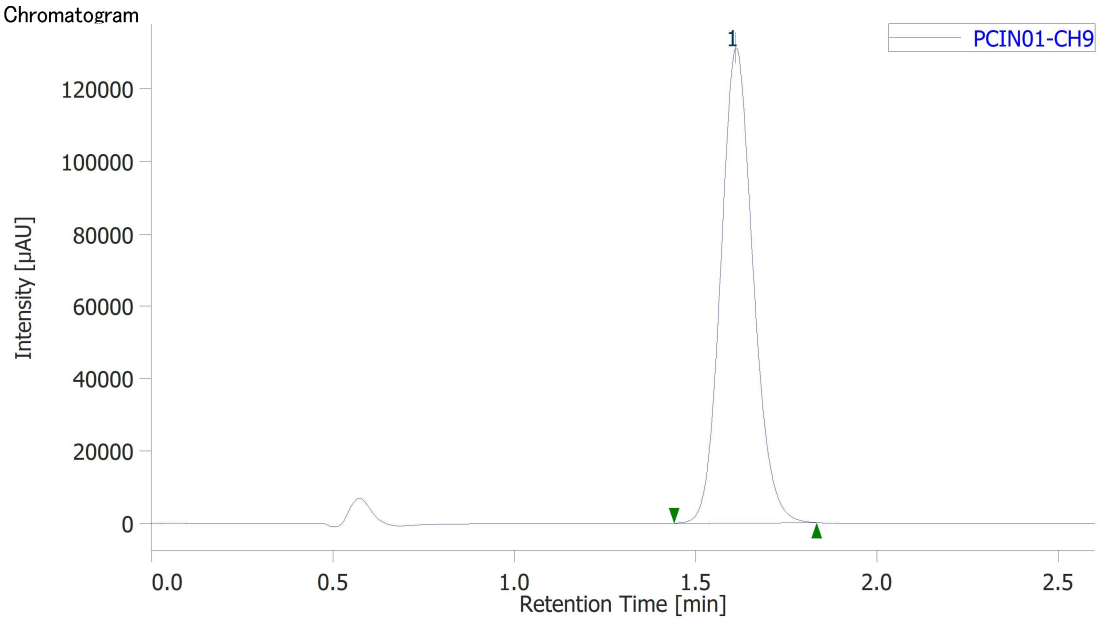

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.610	811689	131150


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:42:03
Volume	10.00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

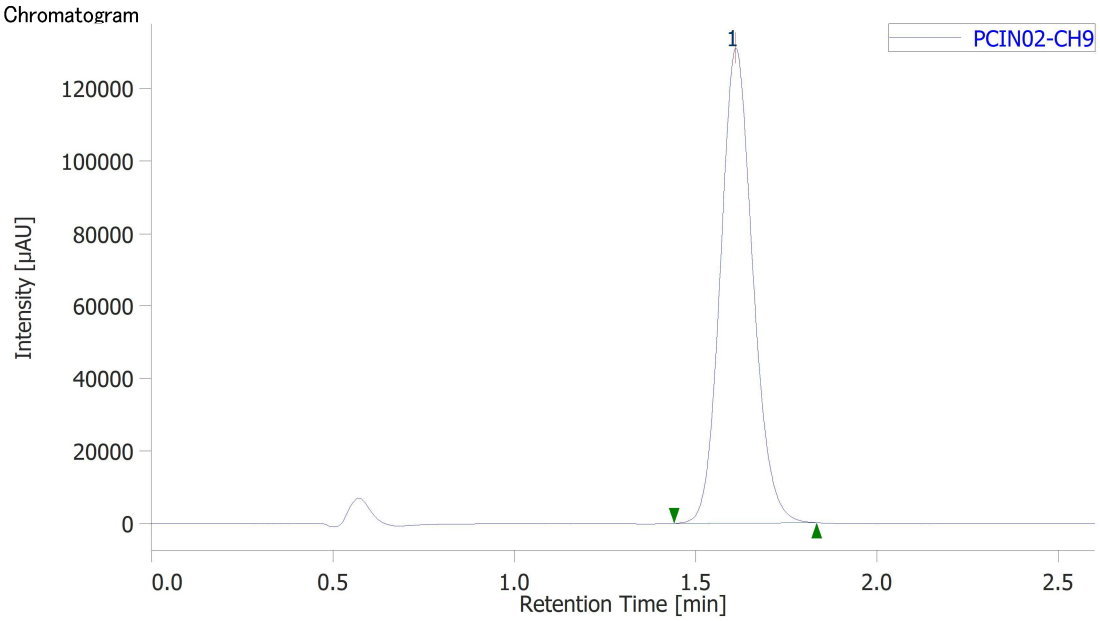

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.610	810293	130880


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:44:48
Volume	10.00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

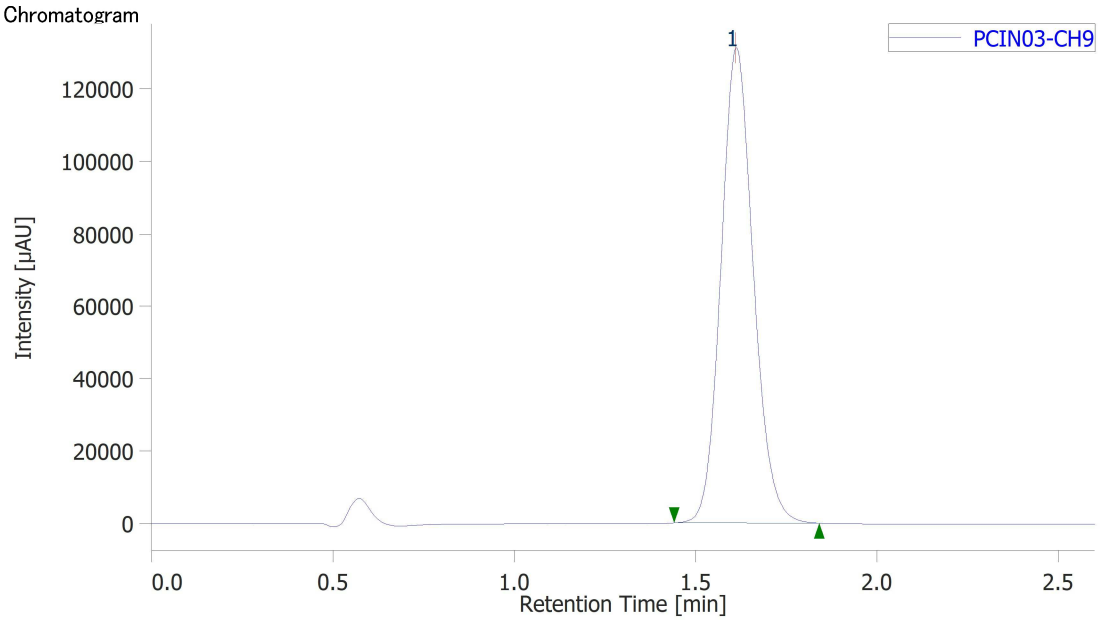

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.610	813711	131033


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:50:23
Volume	10.00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

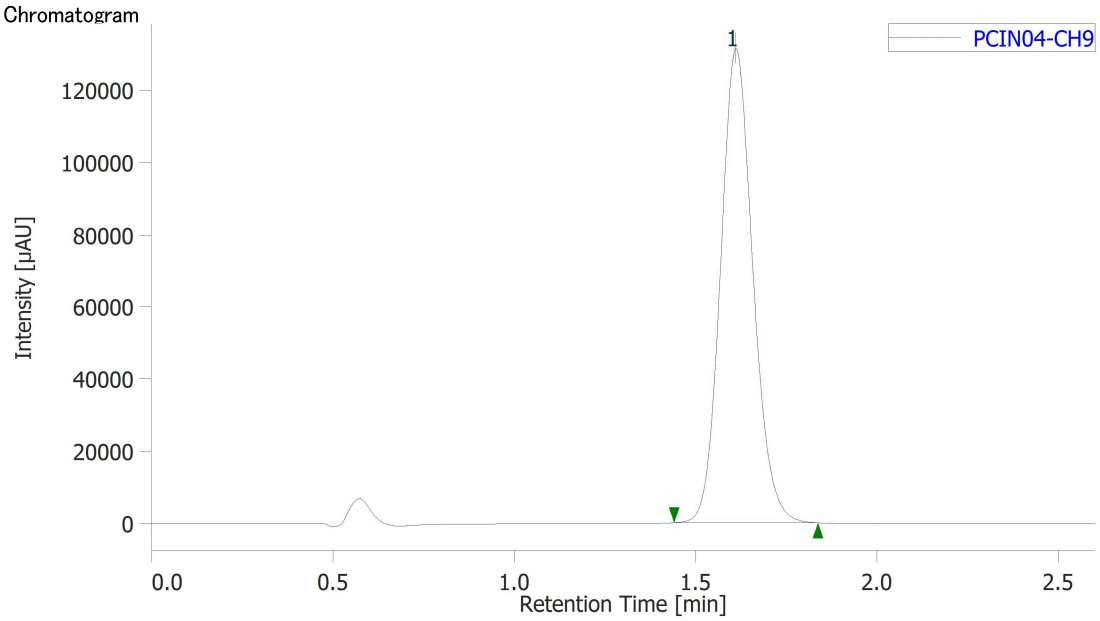

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.610	813032	131397


Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:53:11
Volume	10.00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

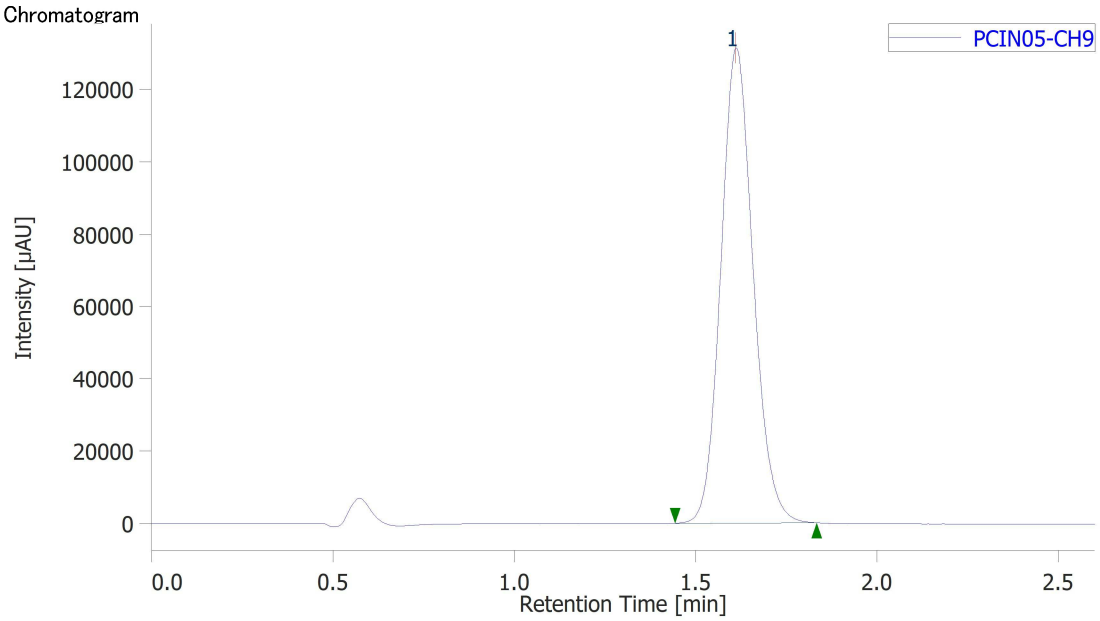

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.610	812132	131248

Chromatogram Information	
User Name	Administrator
HPLC System Name	HPLC012
Injection Date	02/10/2018 11:55:59
Volume	10.00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	2.6 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 2018
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

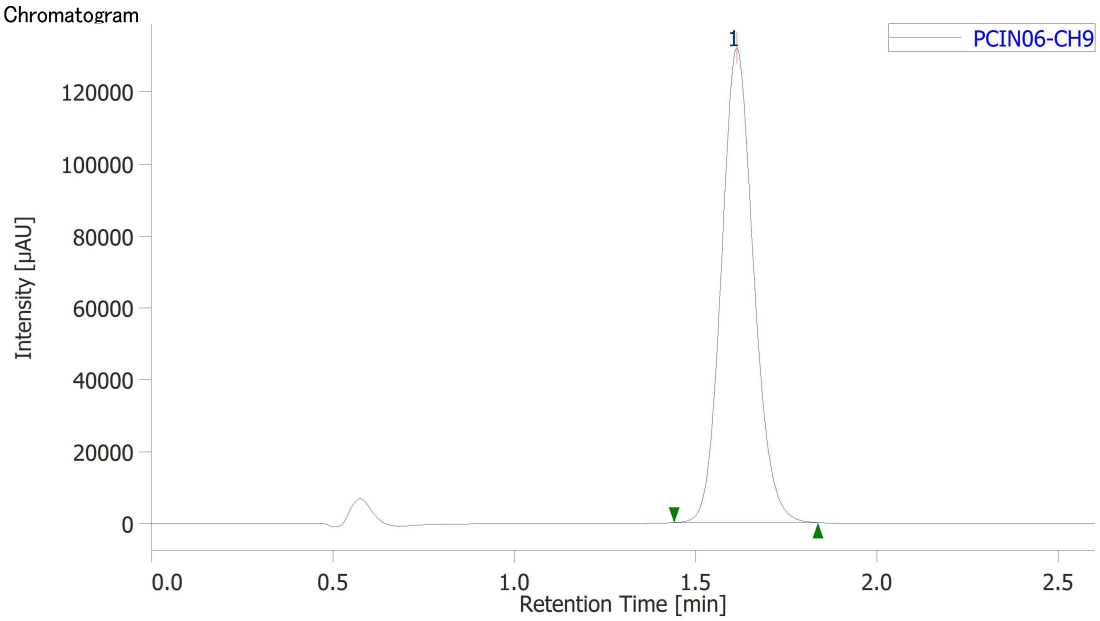

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1.613	814899	131757