
Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:08:44
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:32:48
Volume	10,00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

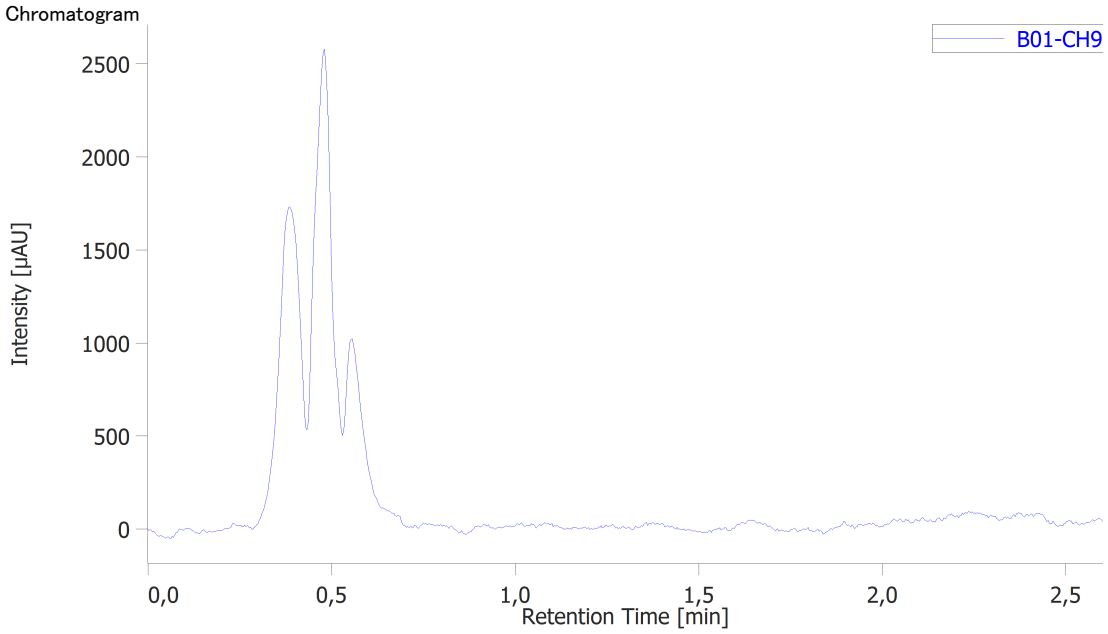


Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:10
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:44:00
Volume	10,00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

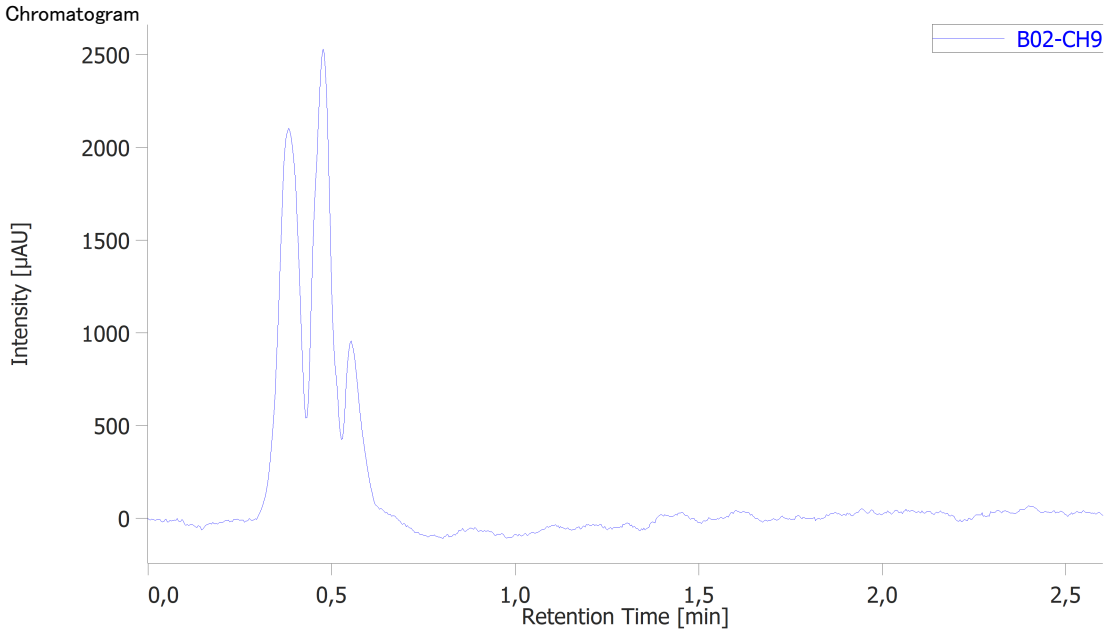


Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information


User Name	Administrator
Date Modified	10/10/2018 10:09:36
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:55:11
Volume	10,00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

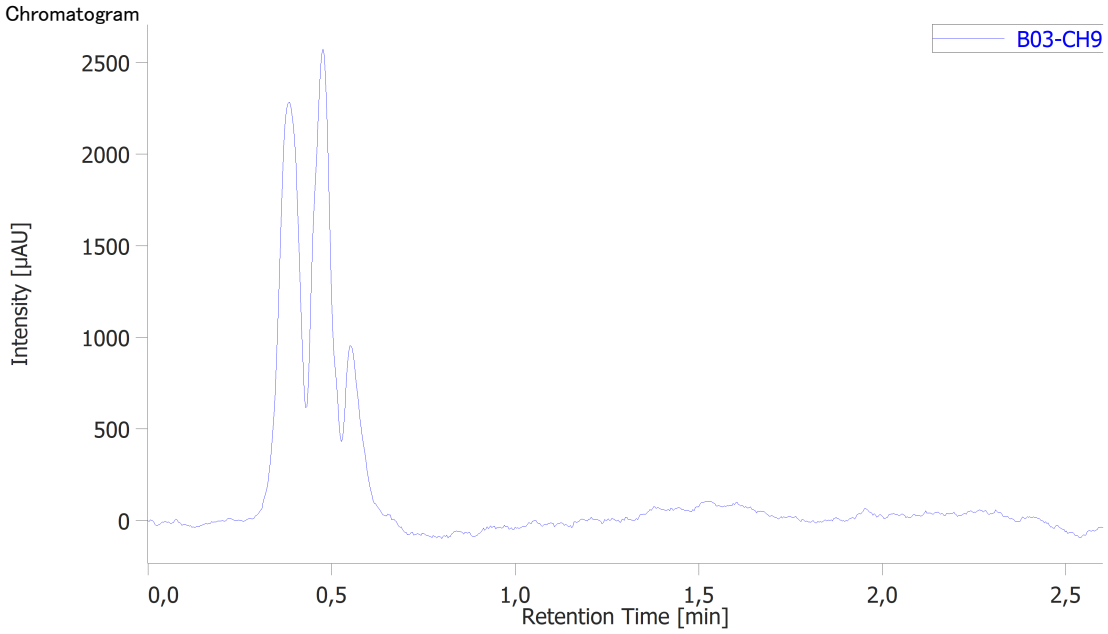

Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Peak Find - EDUV_001 PDA_2,1267.JWS

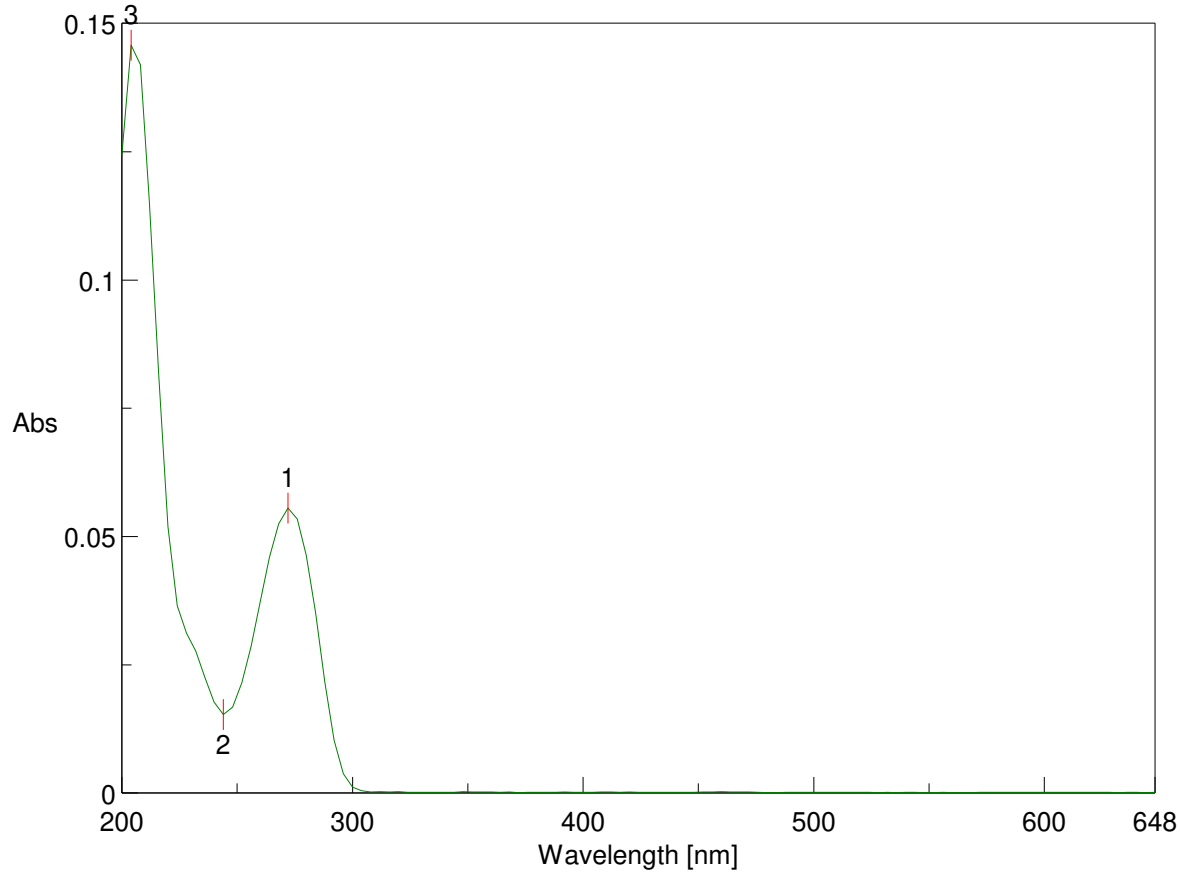

[Comments]

User	Administrator
Division	---
Company	Cristalia
Creation date	09/10/2018 13:13
Date modified	09/10/2018 14:08

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	648 nm
Data interval	4 nm
Data points	113


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A024761665
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.055503	2	244	0.015274
3	204	0.145672			

Chromatogram

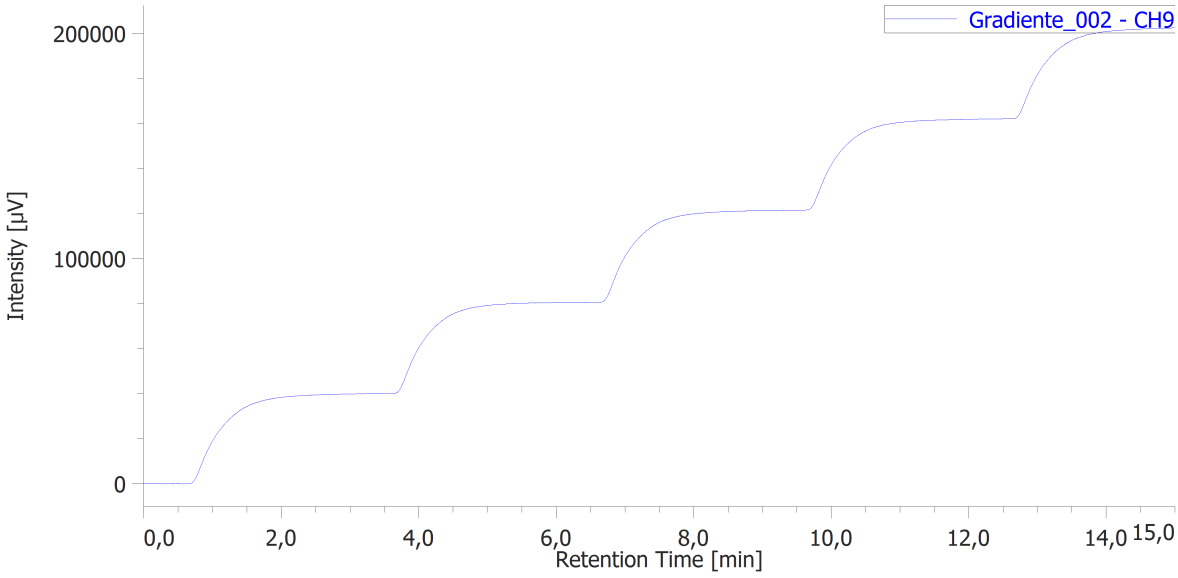


Chromatogram Information	
User Name	Administrator
Date Modified	10/10/2018 10:52:18
Description	
HPLC System Name	JASCO
Injection Date	10/10/2018 10:37:17
Volume	0,00 [µL]
Sample #	–
Project Name	JASCO
Acquisition Time	15,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_002-CH9
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

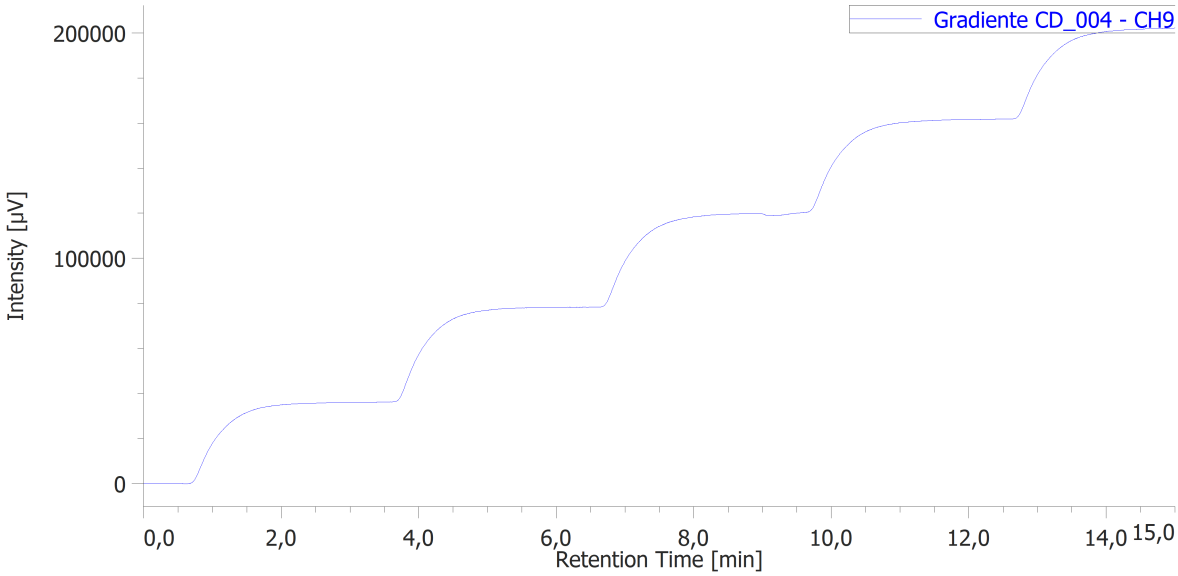

Chromatogram Information	
User Name	Administrator
Date Modified	10/10/2018 11:32:22
Description	
HPLC System Name	JASCO
Injection Date	10/10/2018 11:17:20
Volume	0,00 [µL]
Sample #	–
Project Name	JASCO
Acquisition Time	15,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente CD_004-CH9
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:42
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:57:59
Volume	10,00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

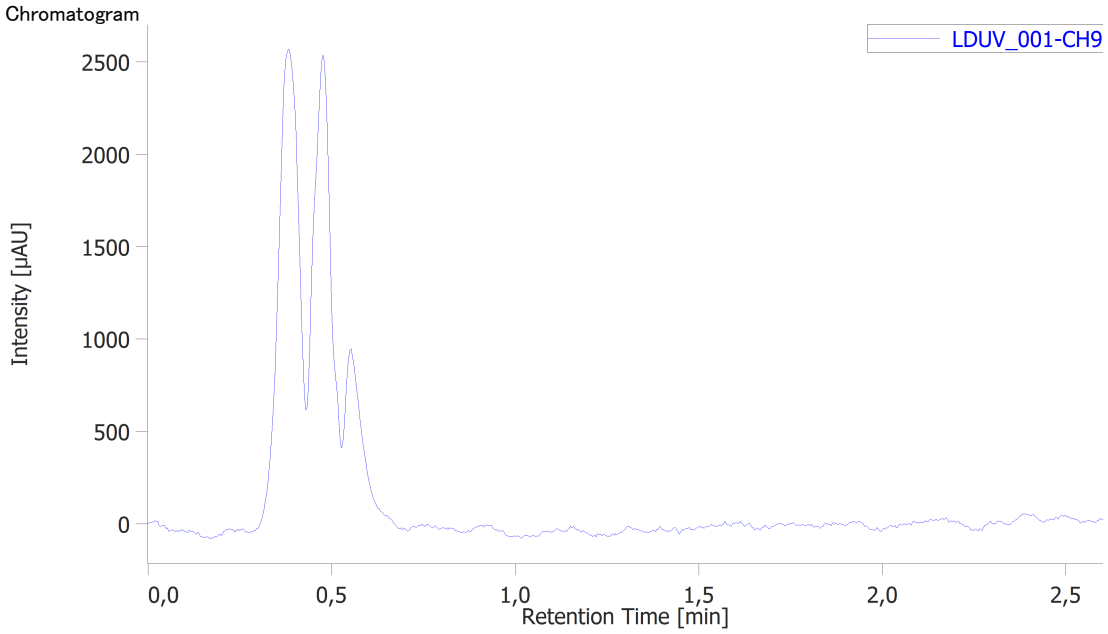


Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:47
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:00:47
Volume	10,00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

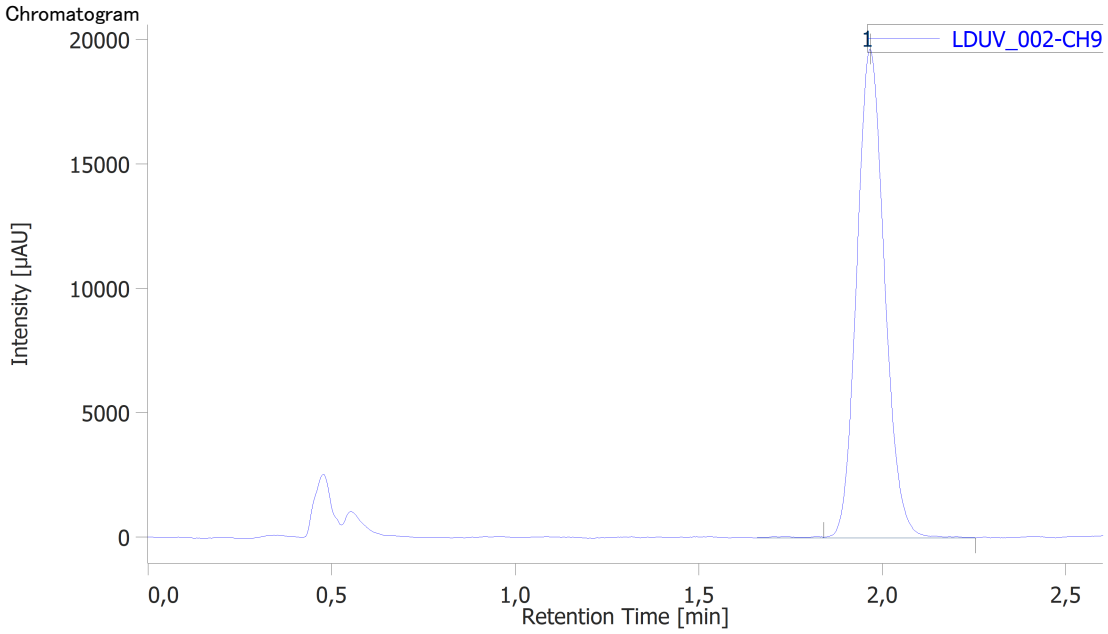


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,967	103282	19646

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:54
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:03:35
Volume	10,00 [µL]
Sample #	4
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

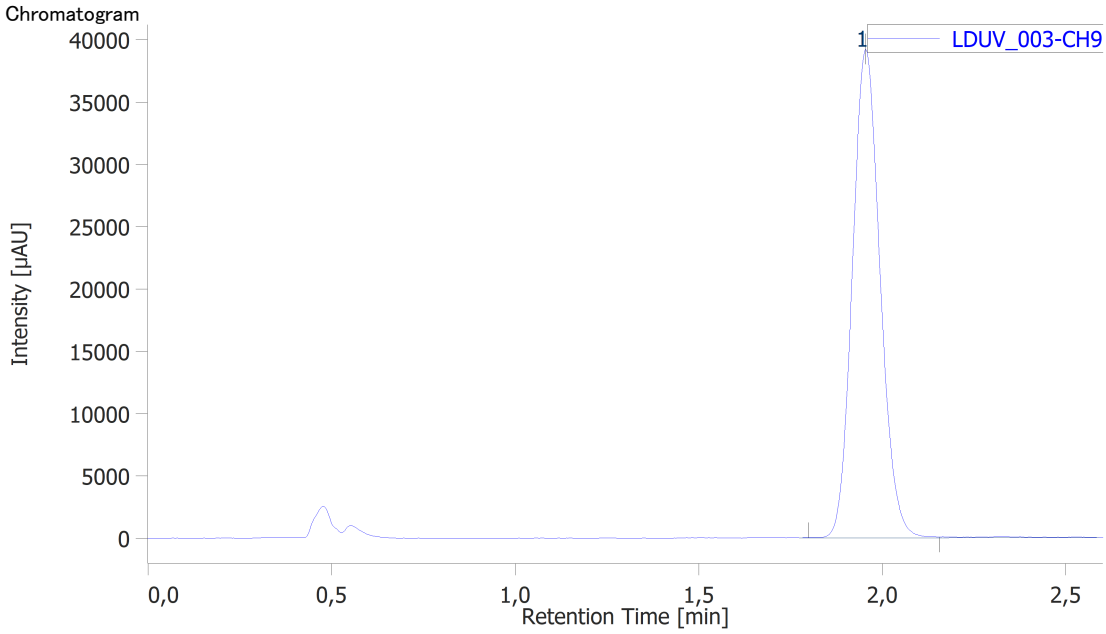


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,953	205028	39204

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:10:02
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:06:23
Volume	10,00 [µL]
Sample #	5
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

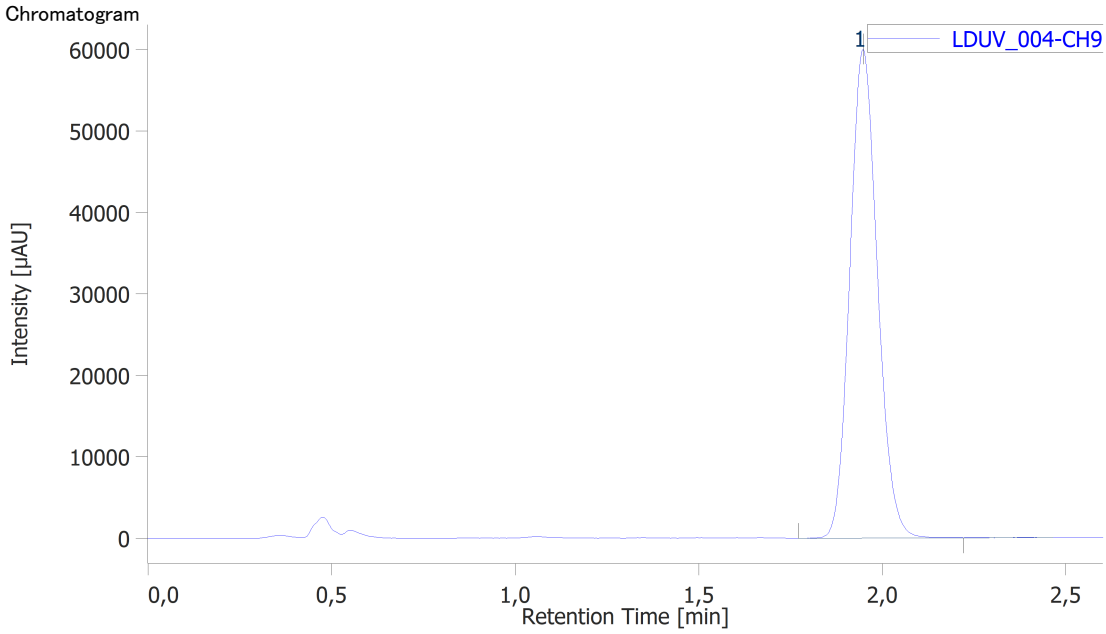


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,947	313793	60050

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:10:09
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:09:11
Volume	10,00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

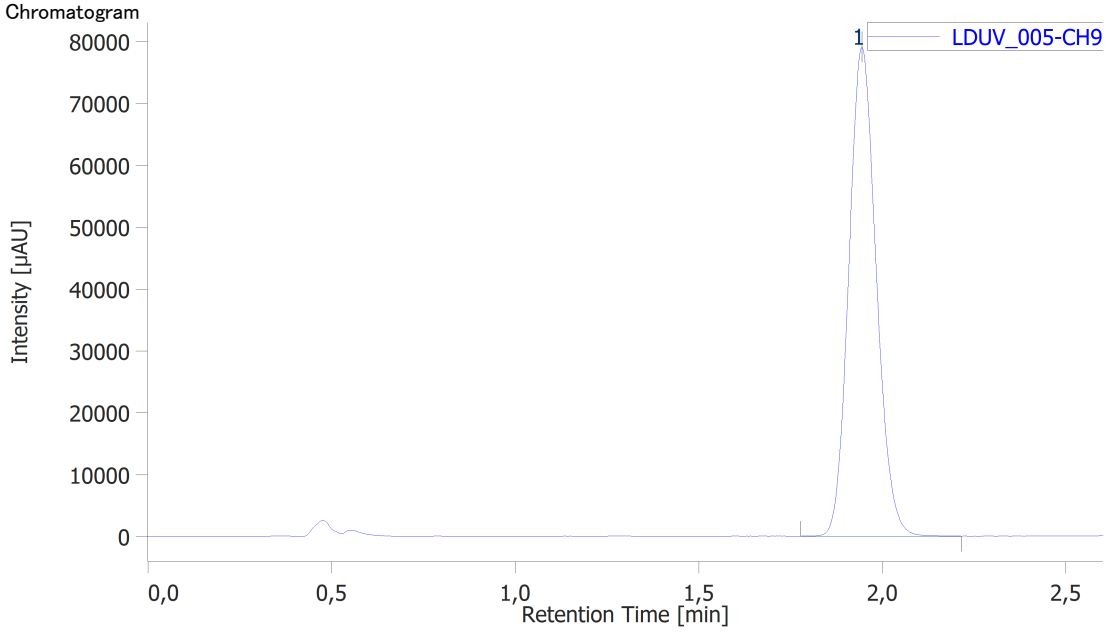


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,943	409683	79026

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:10:16
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:11:59
Volume	0,10 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

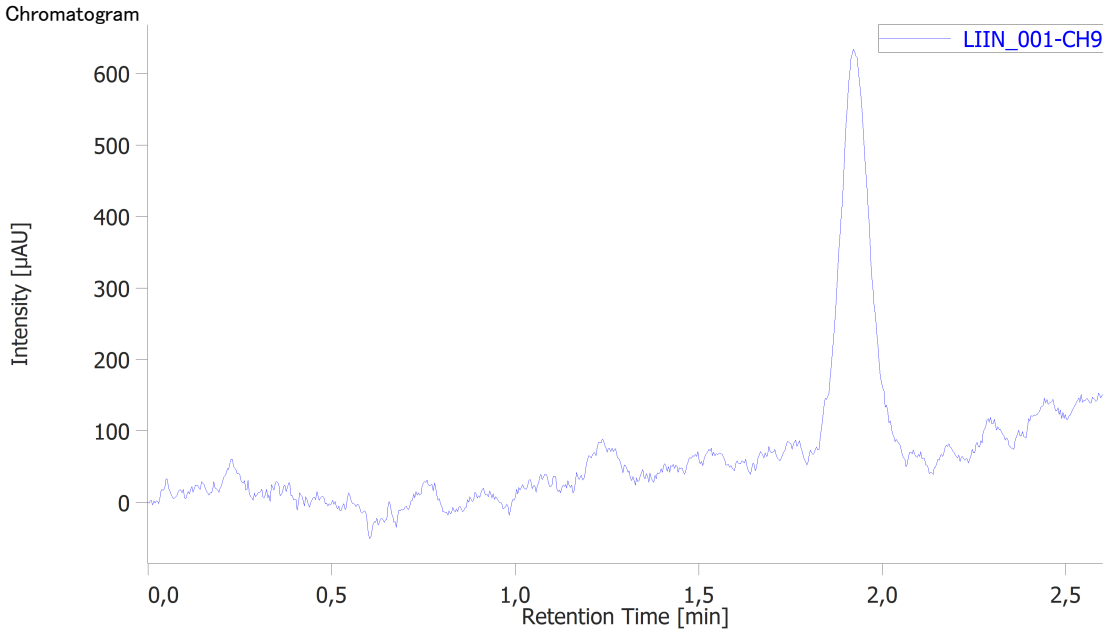


Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:10:22
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:14:47
Volume	5,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

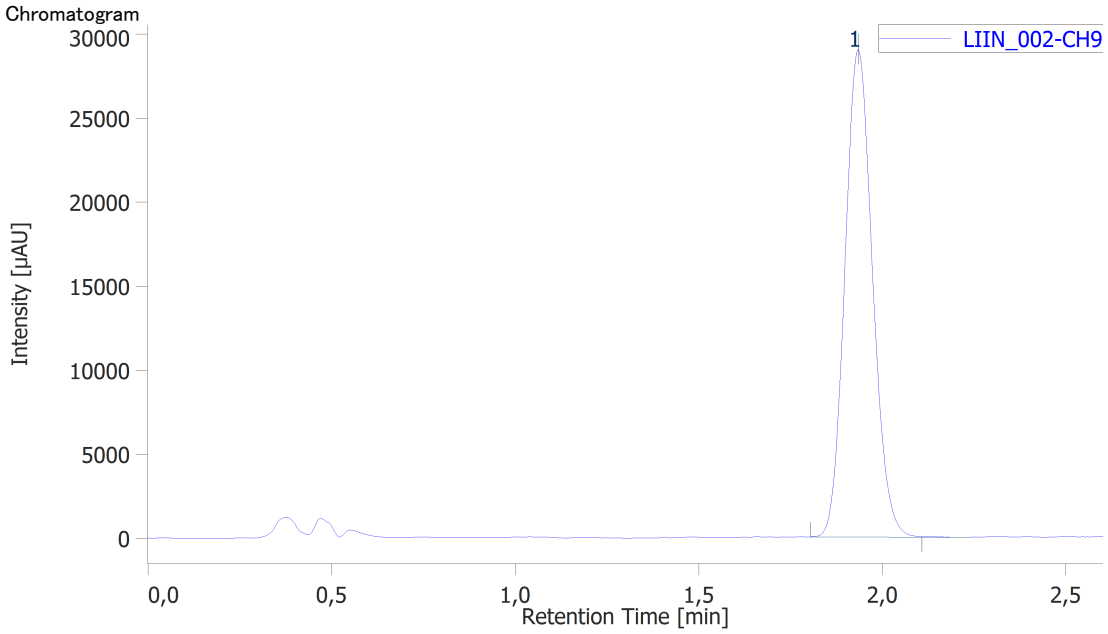


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,933	151366	29025

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:10:28
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:17:35
Volume	10,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

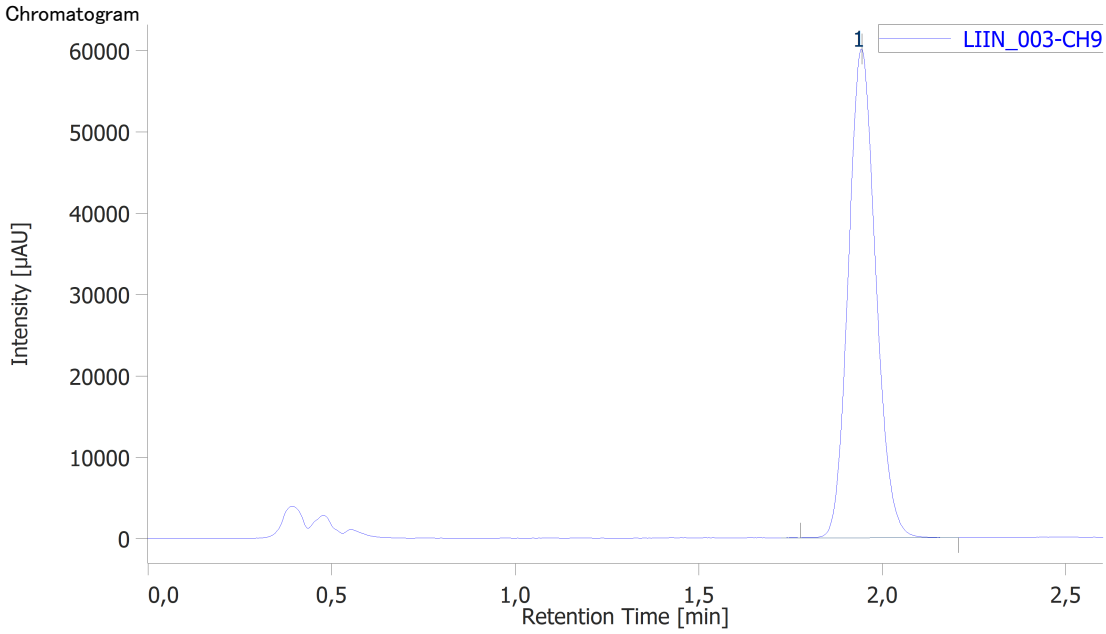


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,943	311199	60068

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:10:36
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:20:23
Volume	15,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

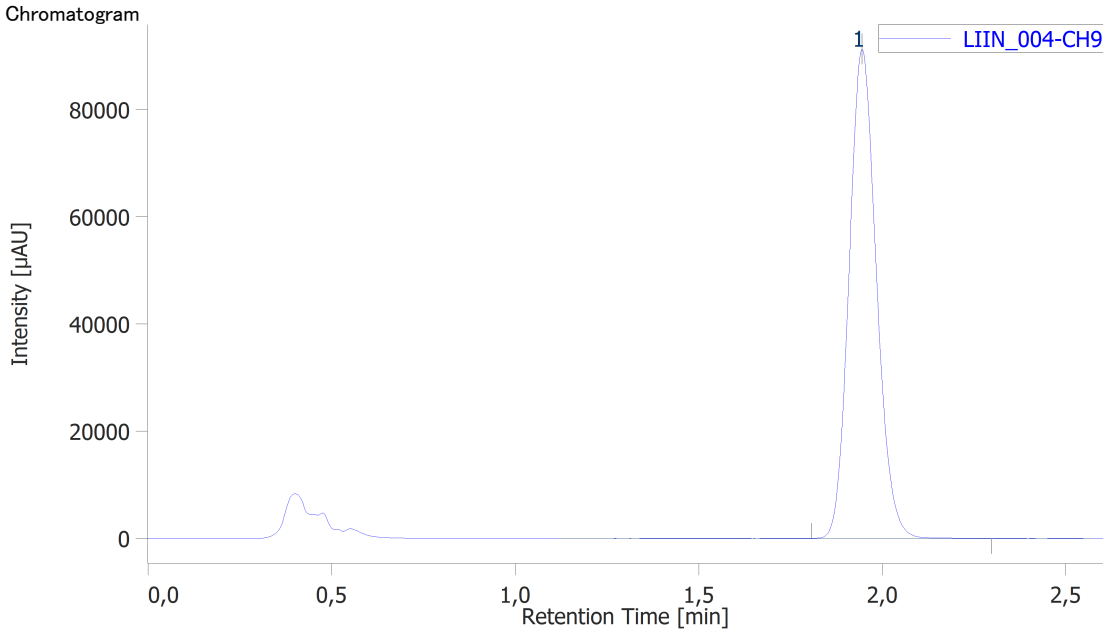


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,943	472252	91314

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:10:43
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 16:23:11
Volume	20,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

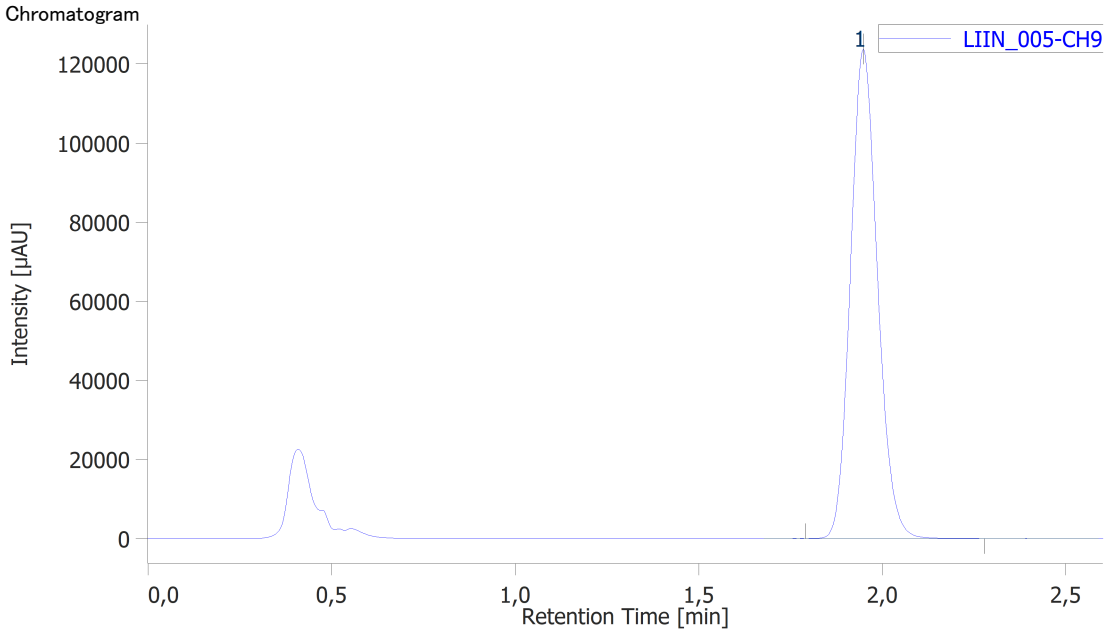


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,947	632287	123753

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:08:49
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:35:36
Volume	10,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

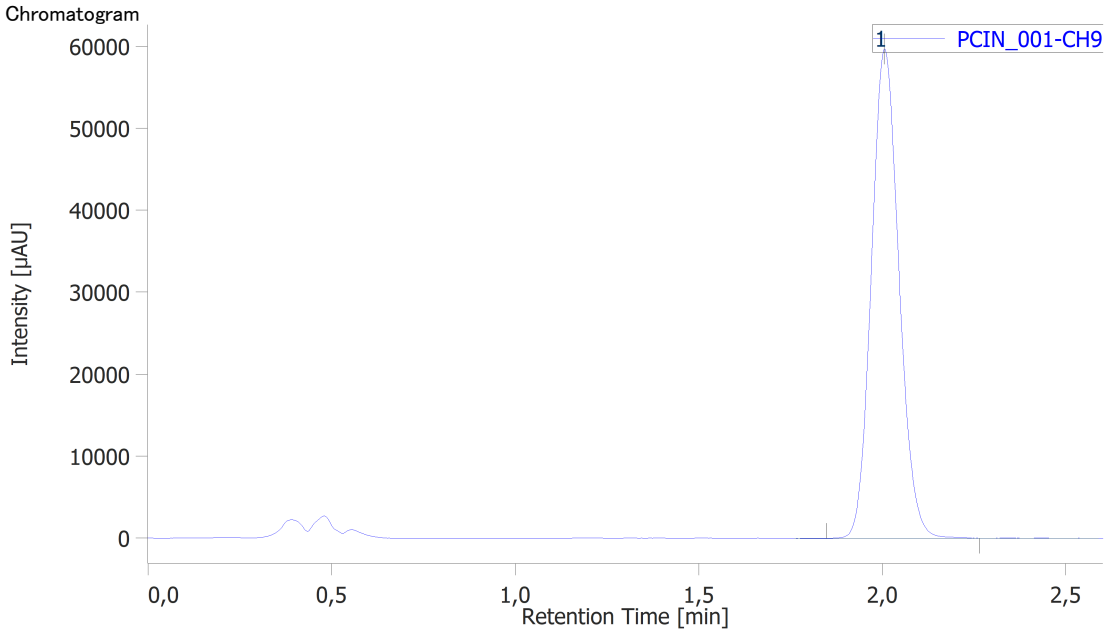


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	2,003	312332	59679

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:08:56
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:38:24
Volume	10,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

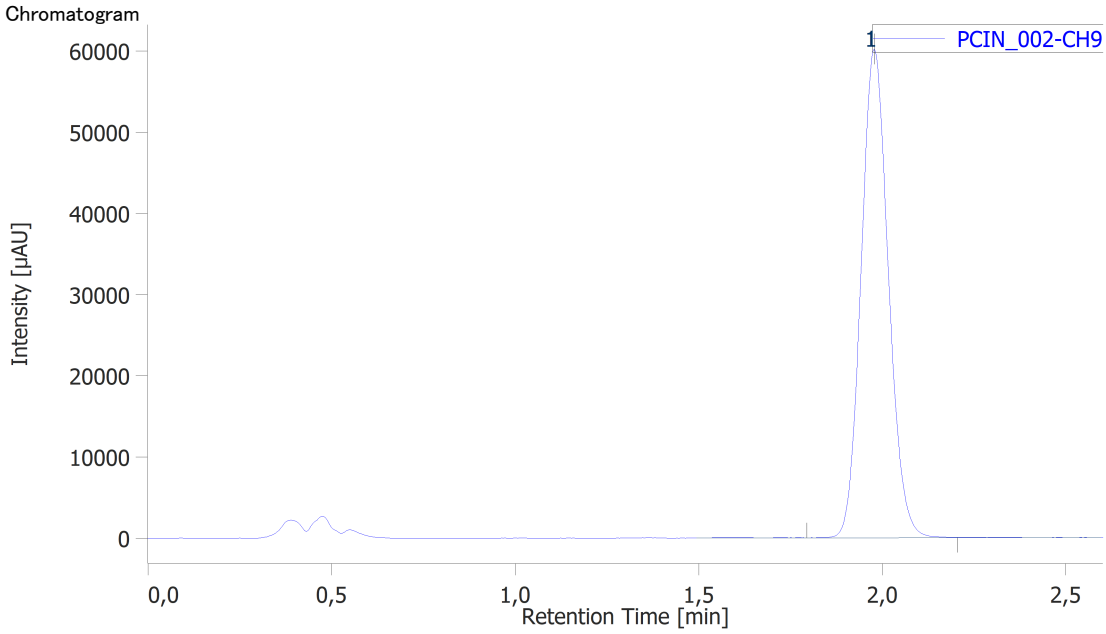


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,977	311269	60181

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:03
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:41:12
Volume	10,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

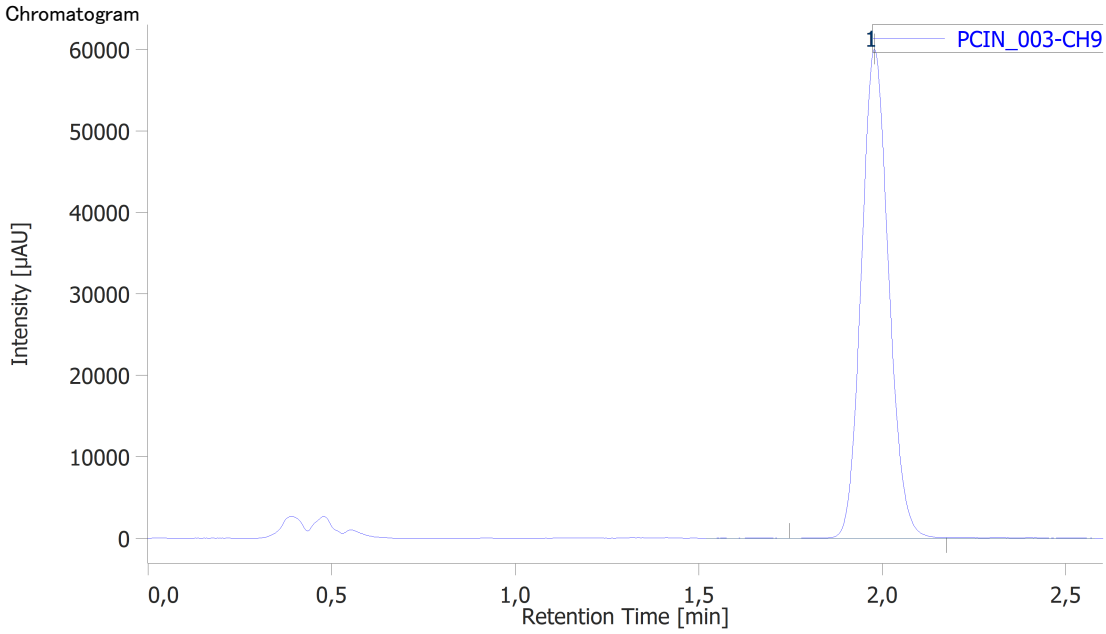


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,977	310814	60042

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:15
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:46:47
Volume	10,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

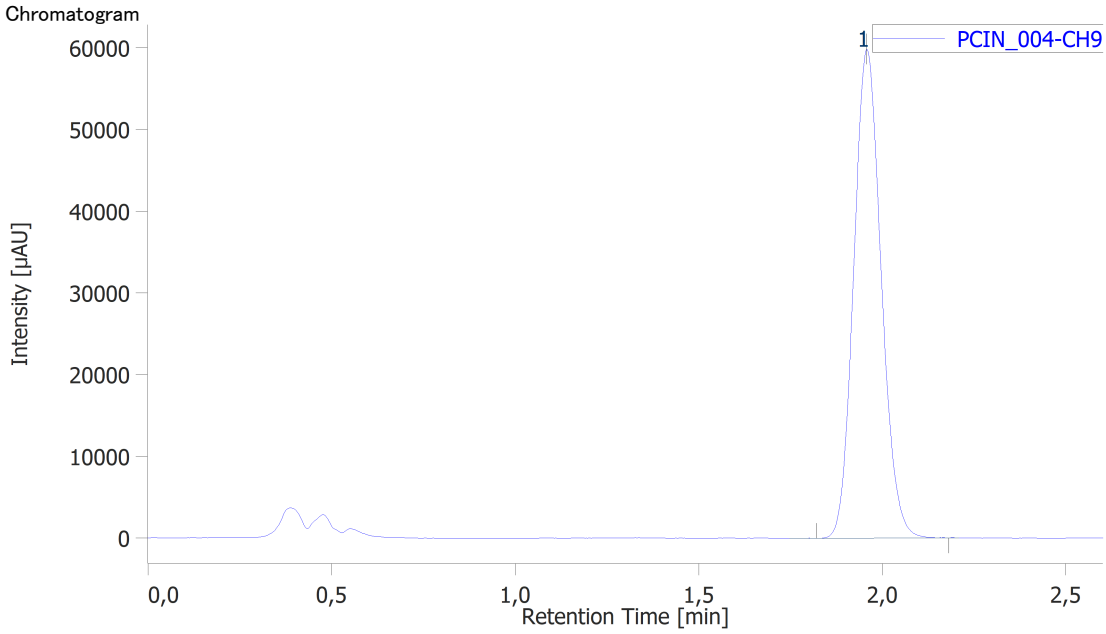


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,957	310789	59852

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:22
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:49:35
Volume	10,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

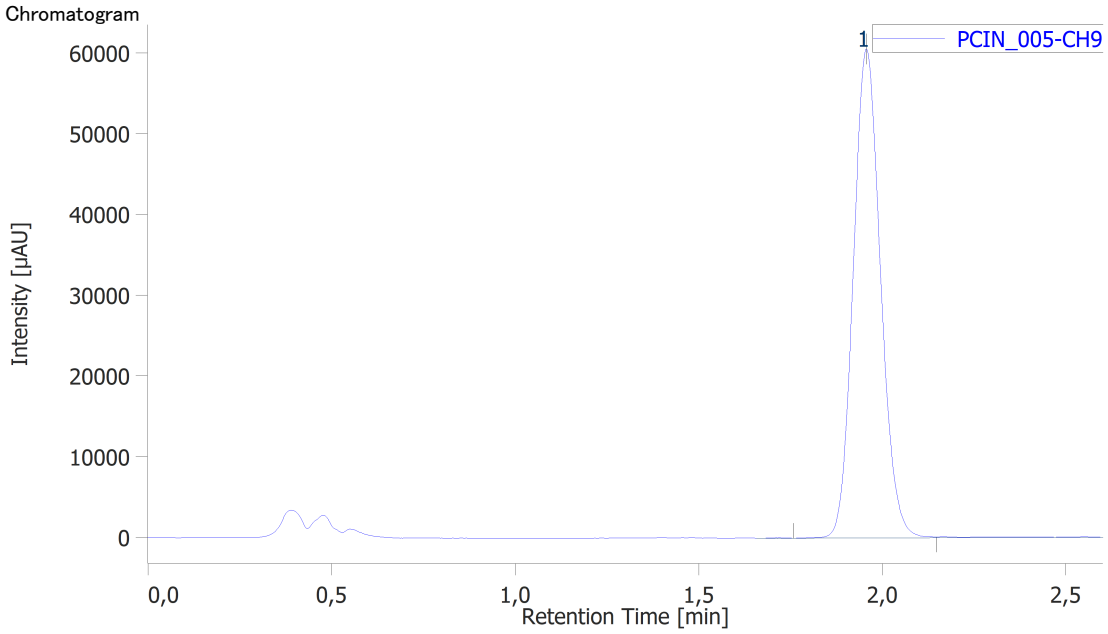


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,957	311954	60519

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	10/10/2018 10:09:29
Description	
HPLC System Name	JASCO
Injection Date	09/10/2018 15:52:23
Volume	10,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	2,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 01
Peak ID Table	Identificação
Calibration Method	
Additional Information	
Column Info	

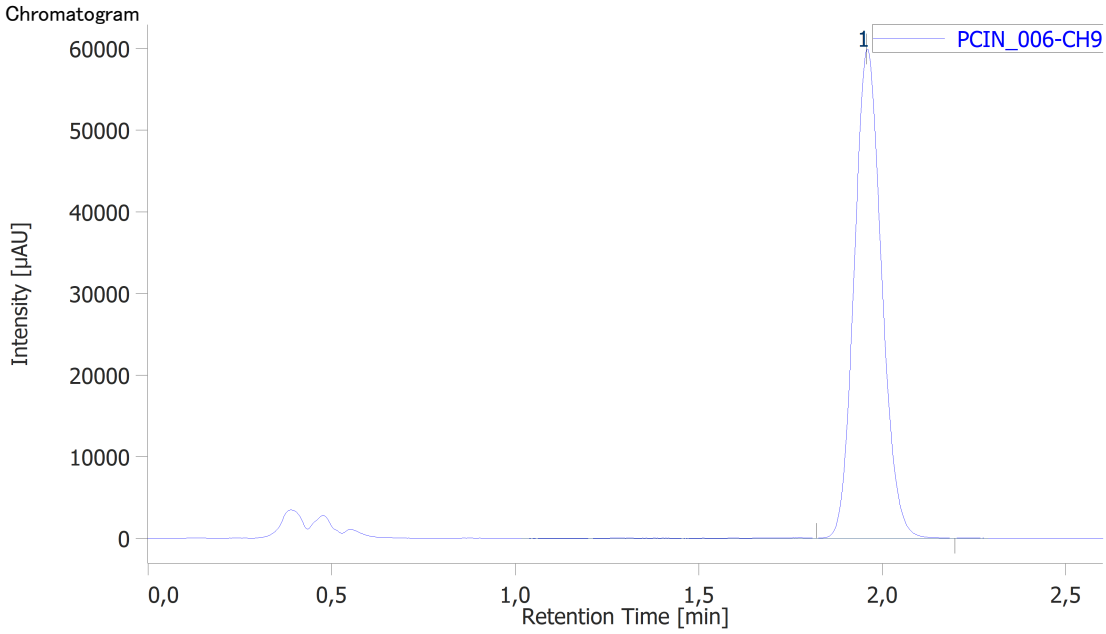

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	9	1,957	311065	59903

Creator *Administrator*
Reviewer
Approver