
EDUV_003 PDA_1,9267.JWS

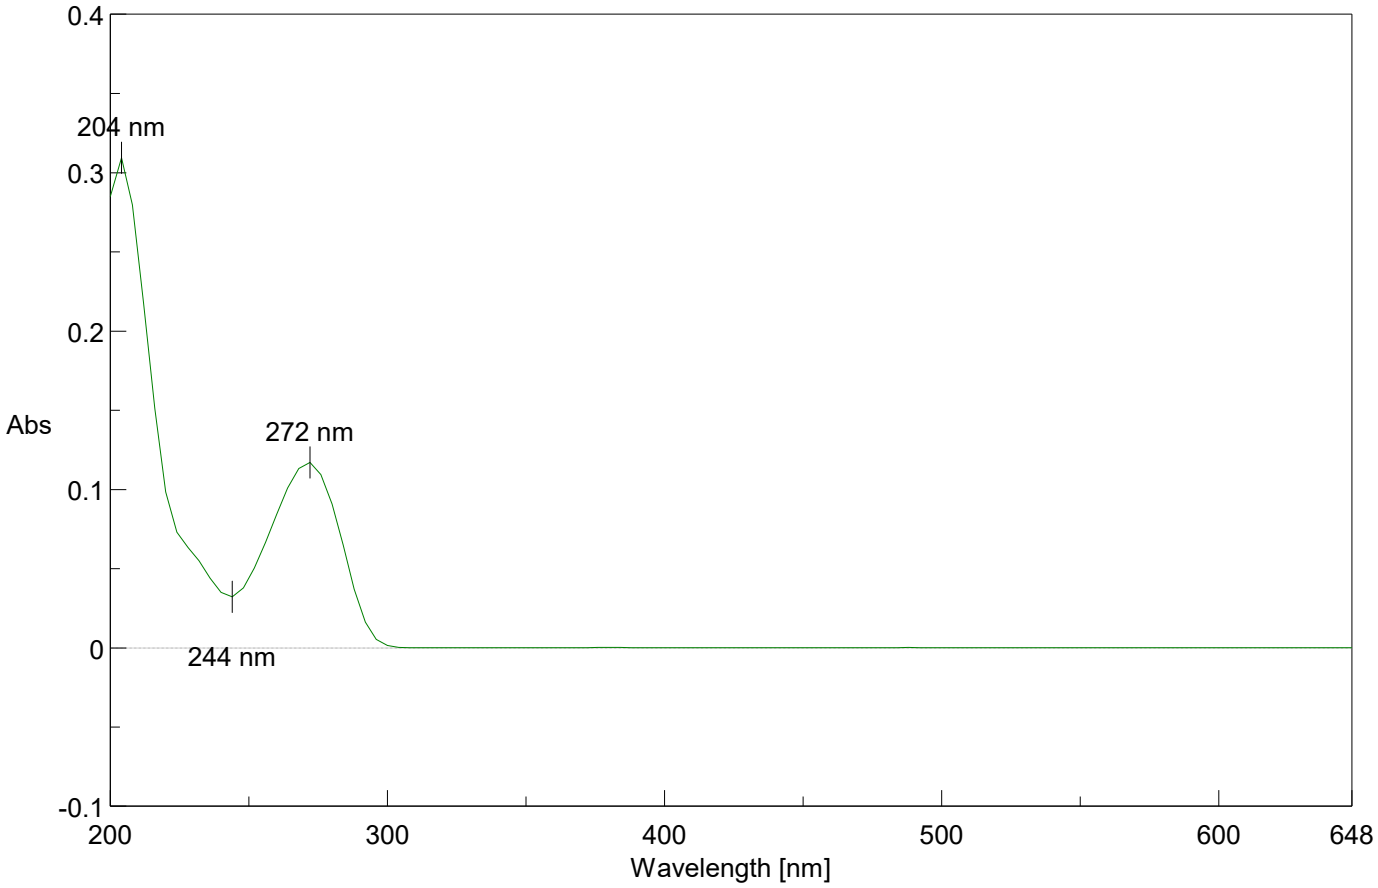

[Comments]

User	Administrator
Division	---
Company	Jasco
Creation date	14/11/2018 11:17
Date modified	14/11/2018 11:56

EDUV_003 PDA_1,9267.JWS

[Detailed Information]


Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	648 nm
Data interval	4 nm
Data points	113

[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A029161665
ROM version	V1.02.03

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 13:12:12
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:27:32
Volume	10,00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

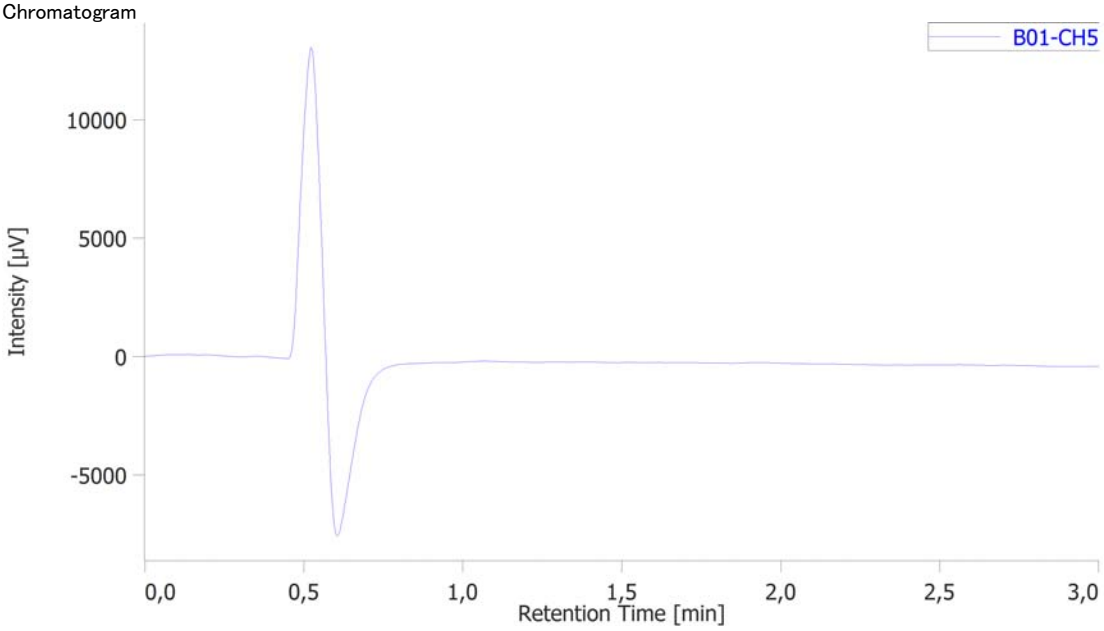


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:12:17
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:30:44
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

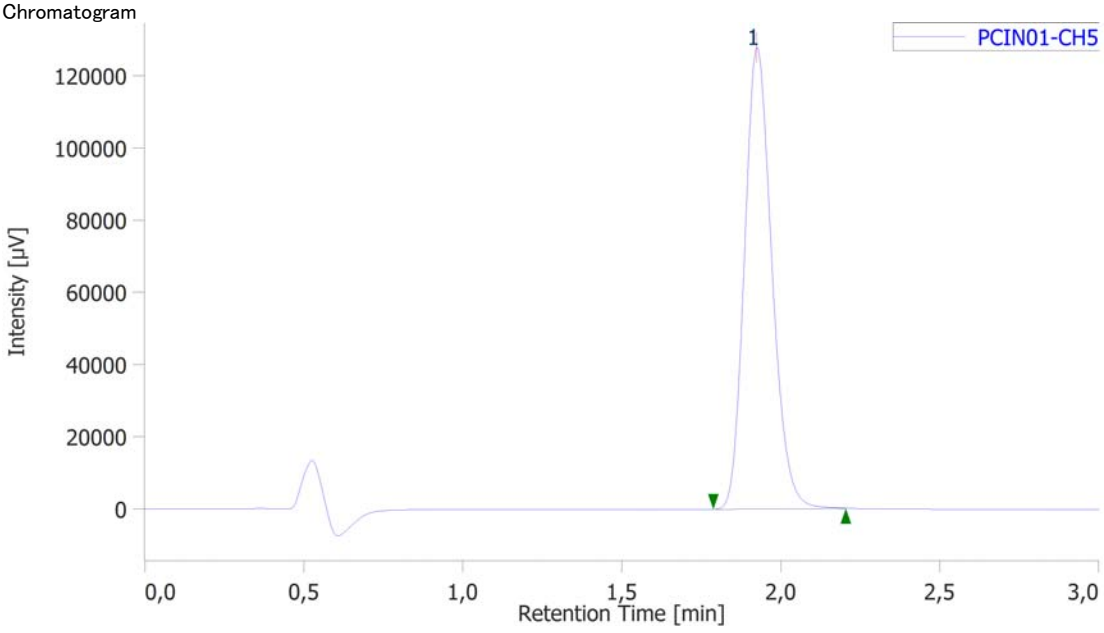


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,923	764185	127852

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:12:26
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:33:56
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

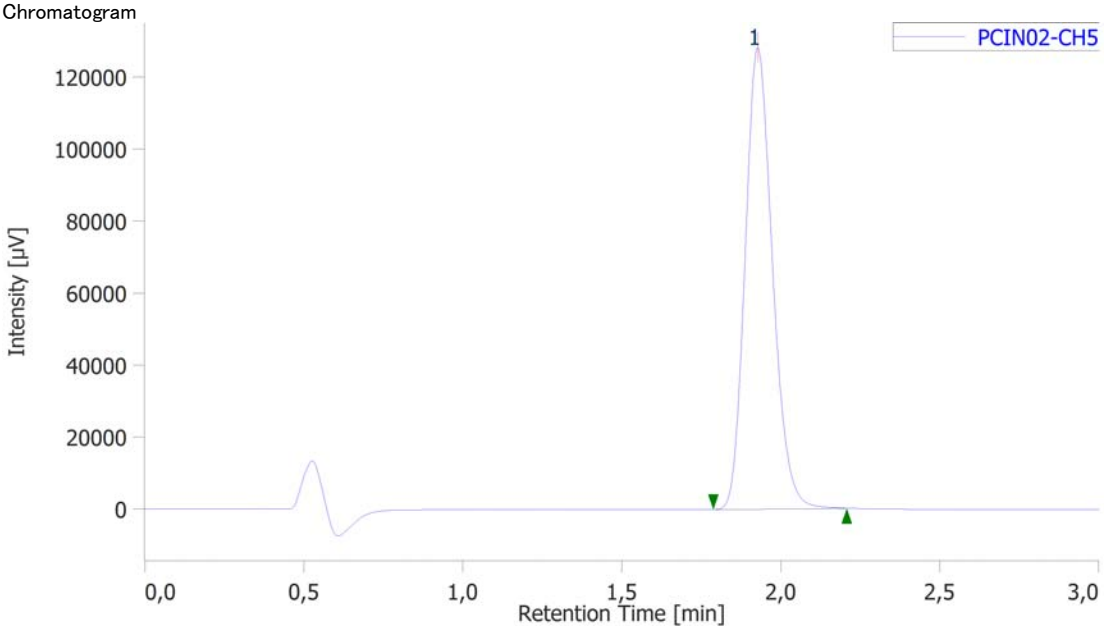


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,927	763734	128212

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:12:35
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:37:08
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

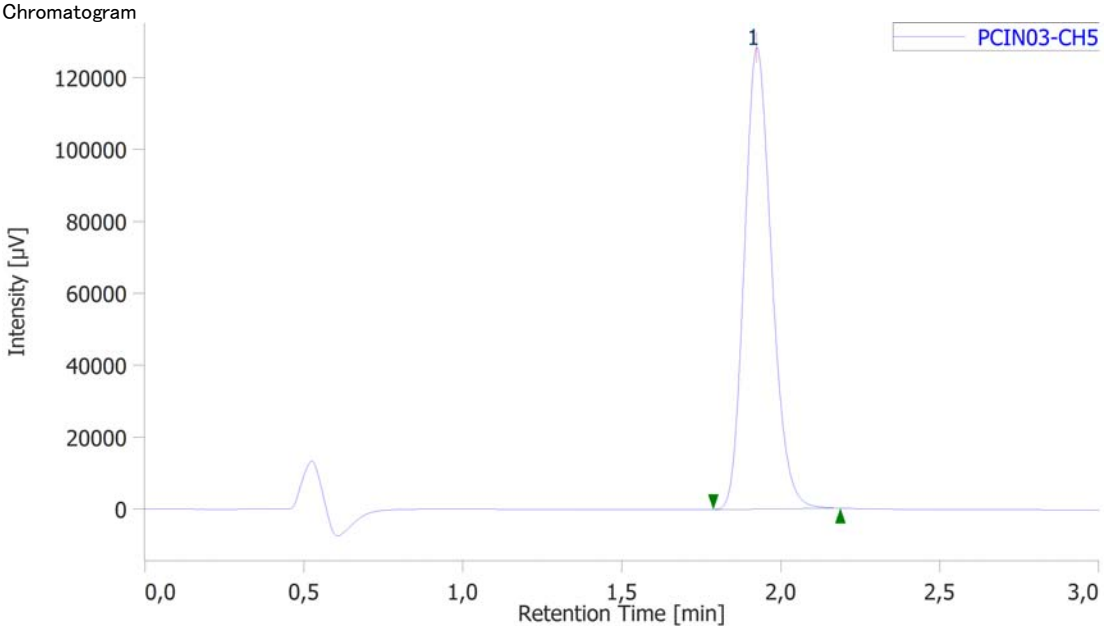


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,923	764275	128317

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 13:12:43
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:40:20
Volume	10,00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

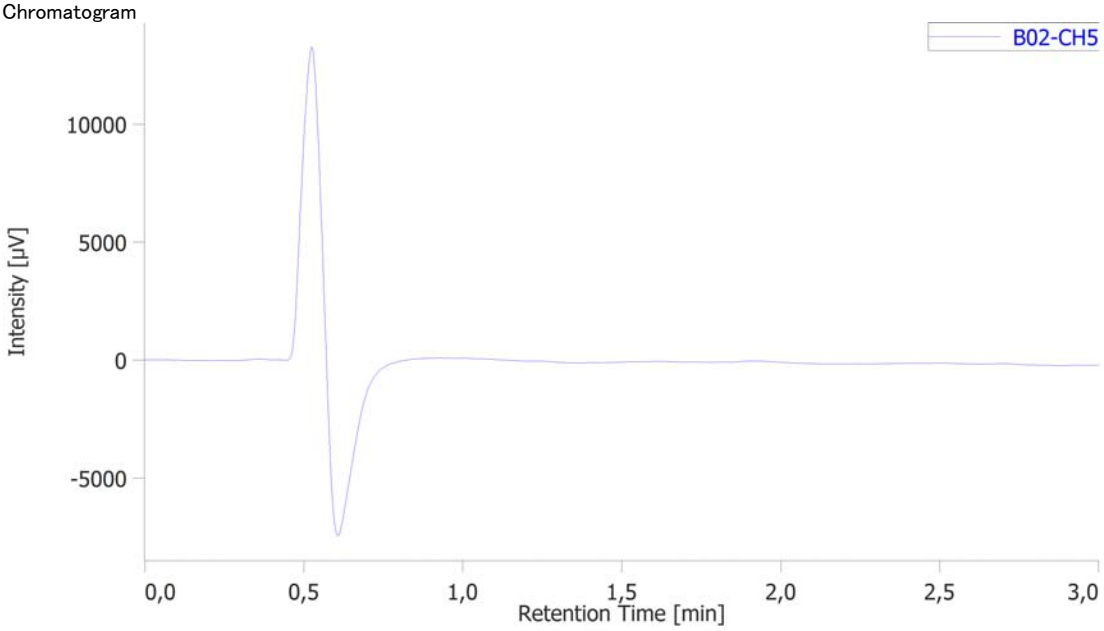


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:12:49
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:43:32
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

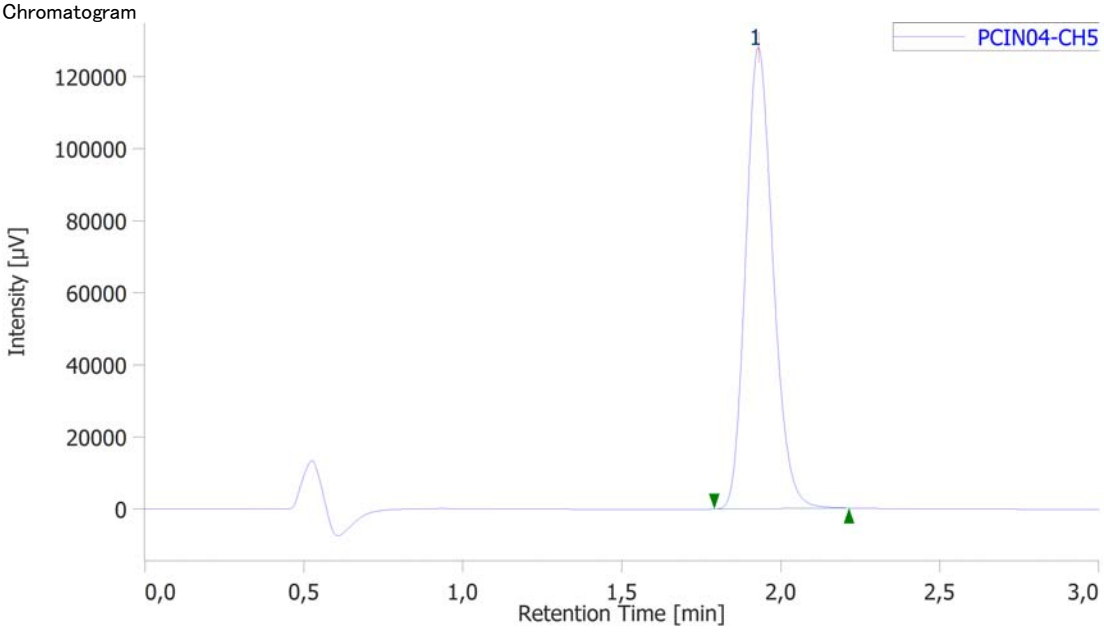


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,930	763901	128014

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:12:58
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:46:44
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

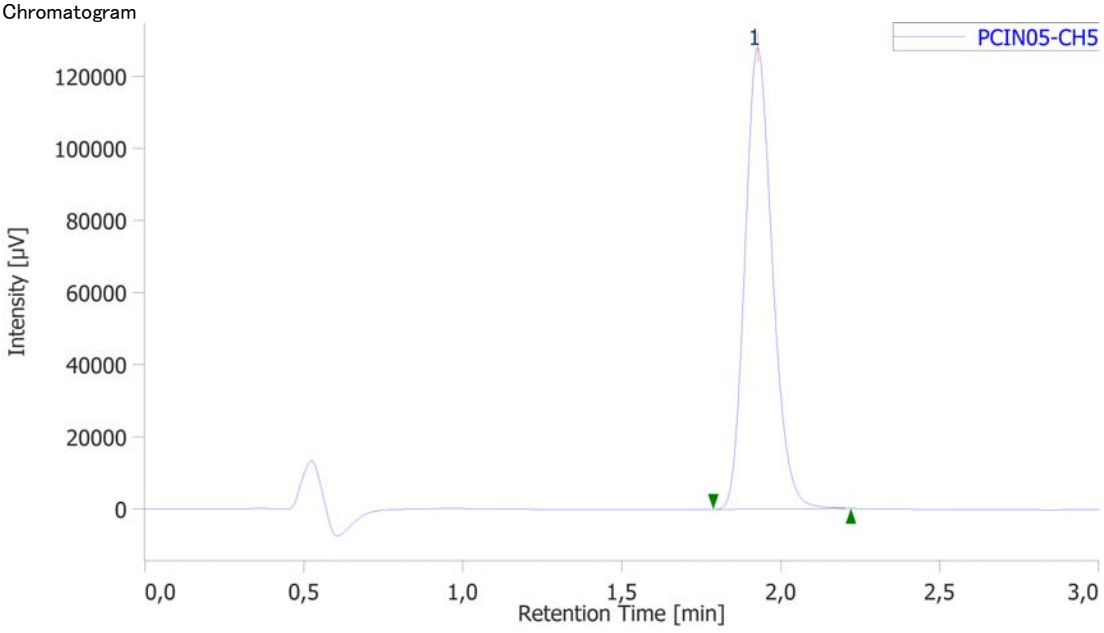


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,927	766693	128051

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:13:06
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:49:56
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

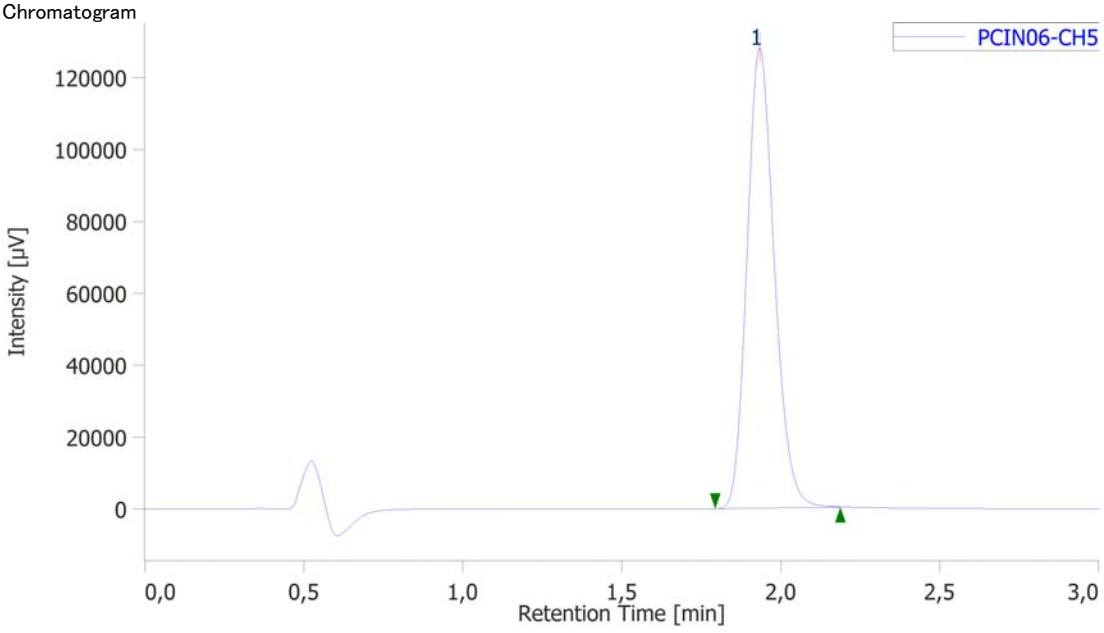


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,933	763268	128153

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 13:13:15
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:53:08
Volume	10,00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	


Chromatogram

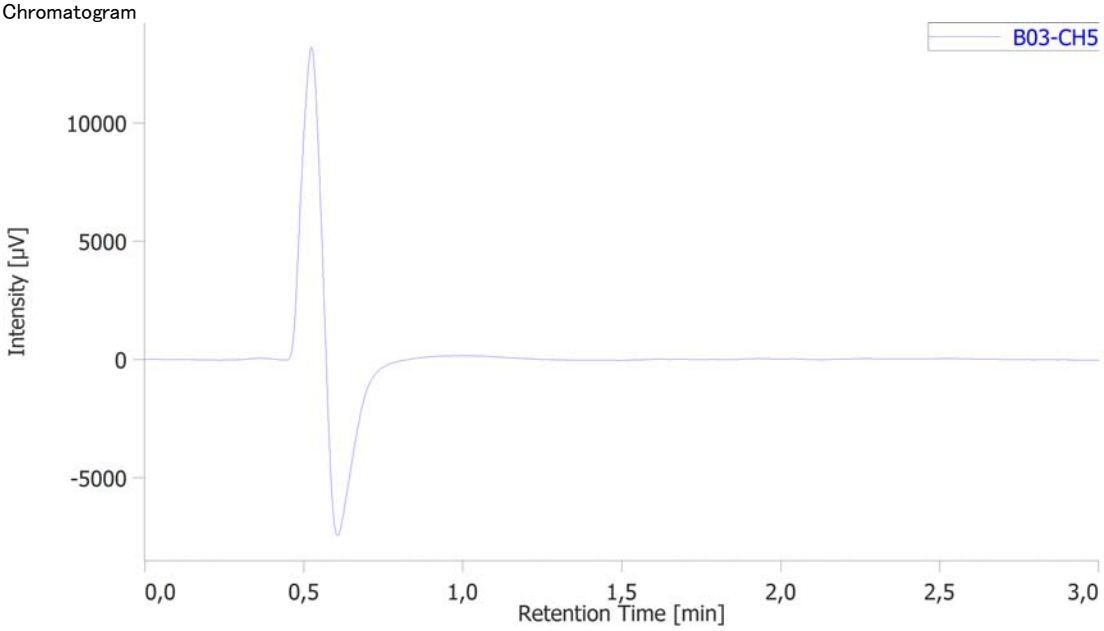

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 13:13:21
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:56:20
Volume	10,00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

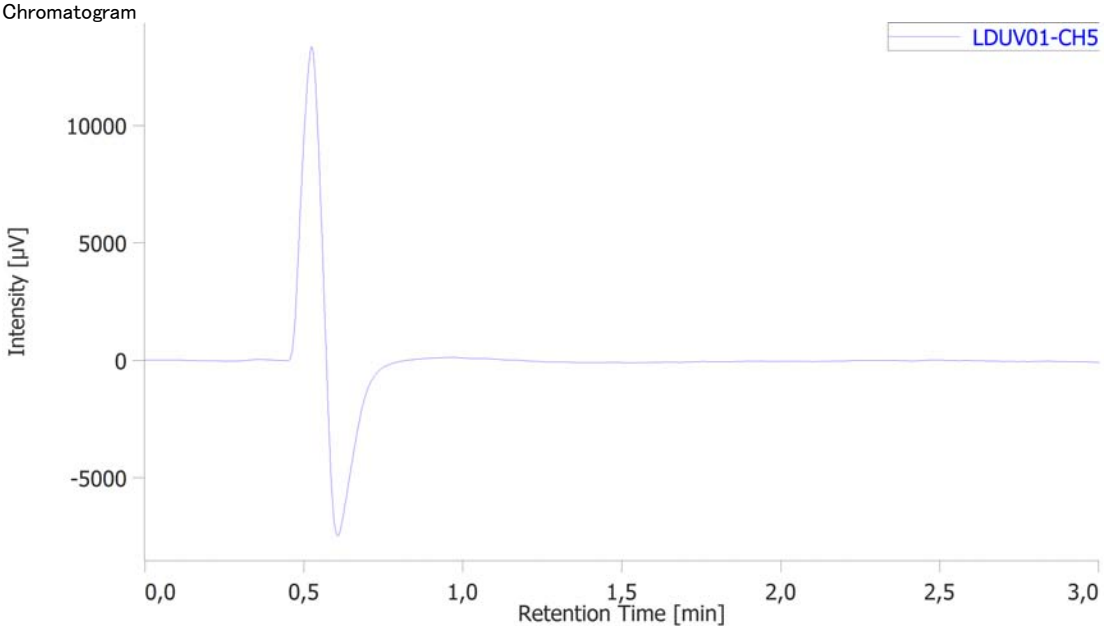


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:13:28
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 11:59:32
Volume	10,00 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

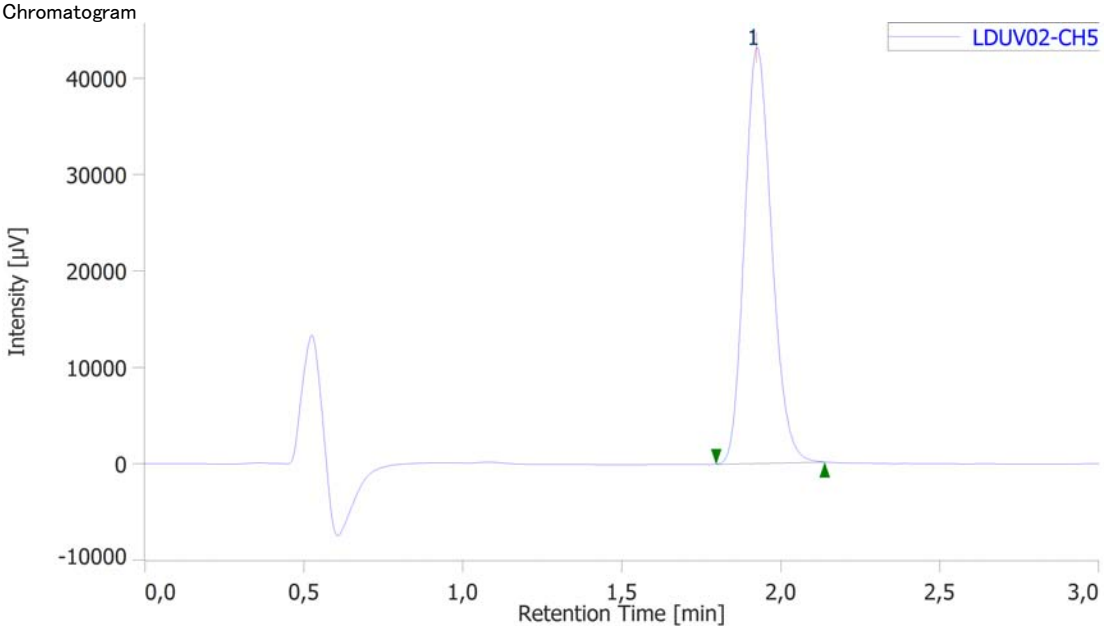


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,923	256512	43162

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:13:37
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:02:44
Volume	10,00 [µL]
Sample #	4
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

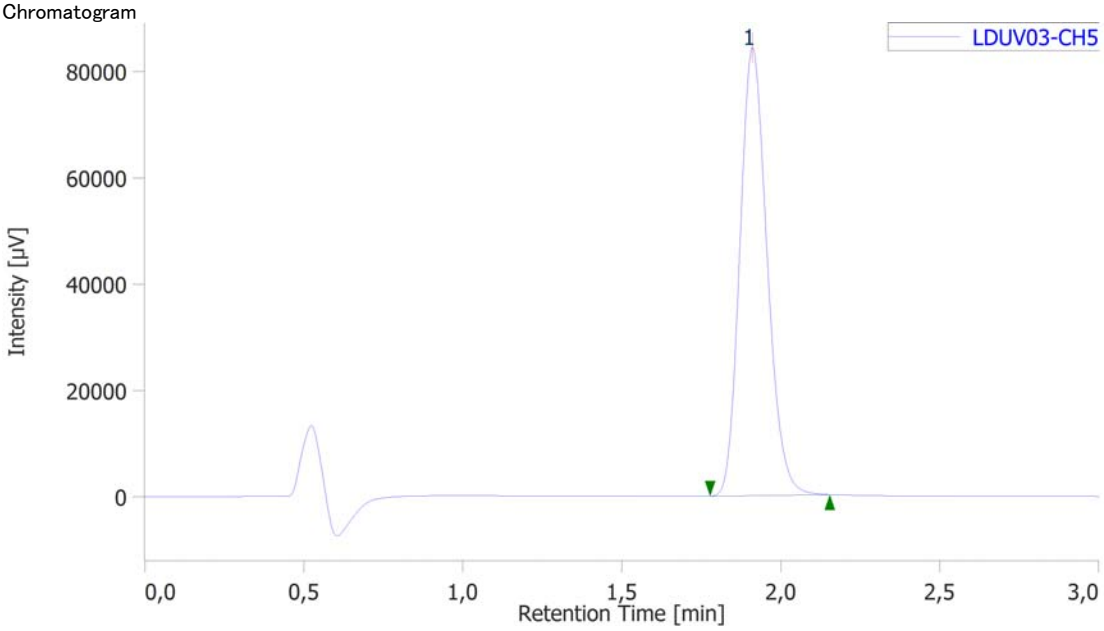


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,910	501049	84269

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:13:46
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:05:56
Volume	10,00 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

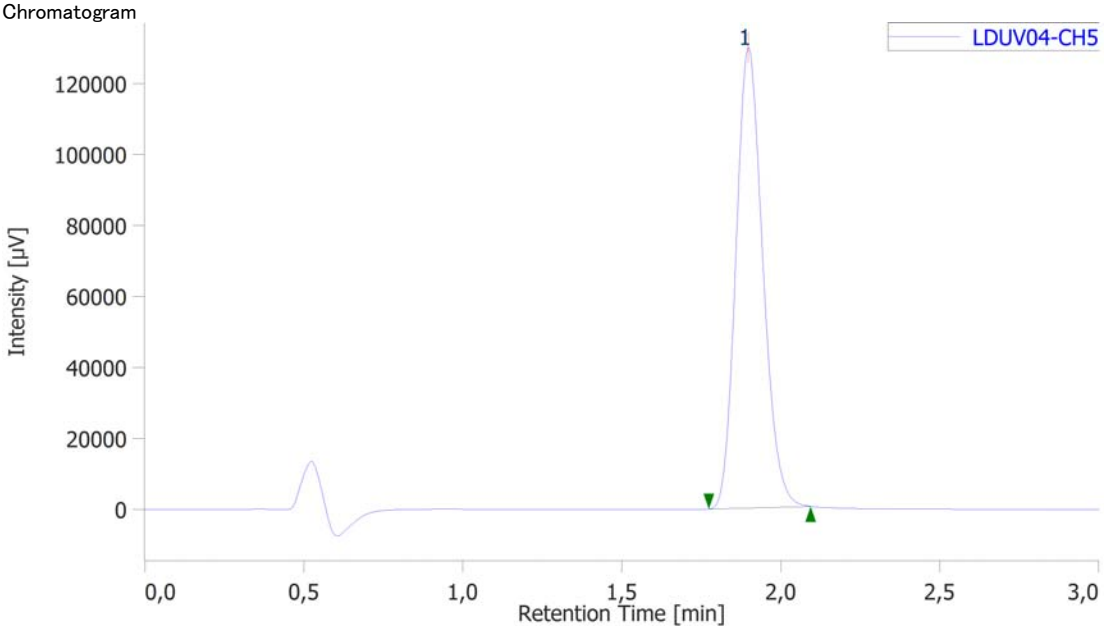


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,897	760641	129742

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 13:13:56
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:09:08
Volume	10,00 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

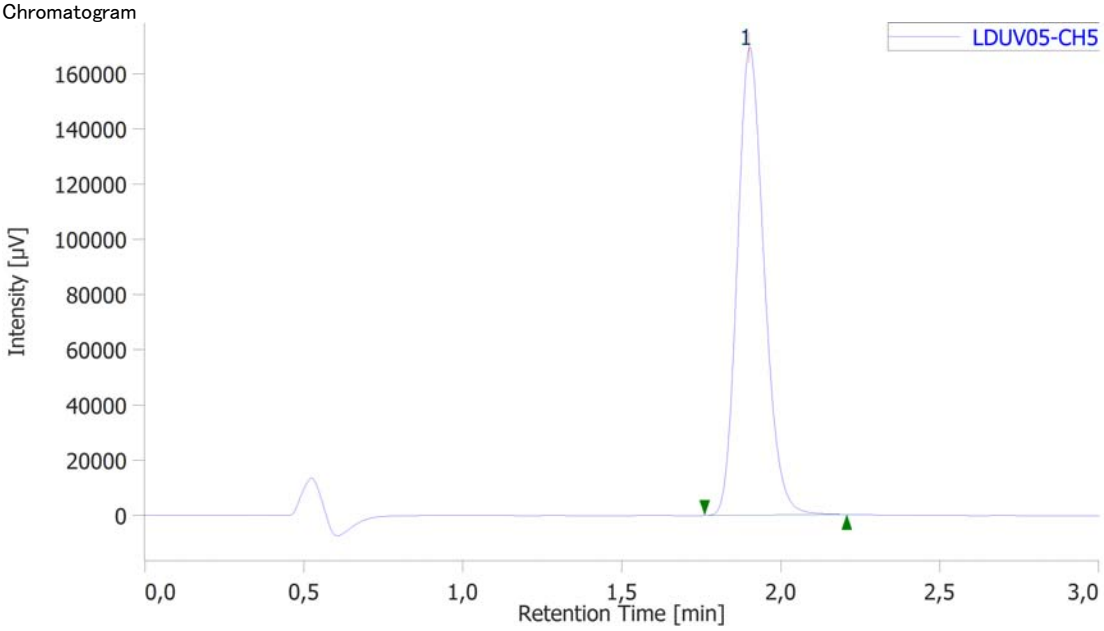


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,900	993328	169456

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 13:14:05
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:12:20
Volume	0,10 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

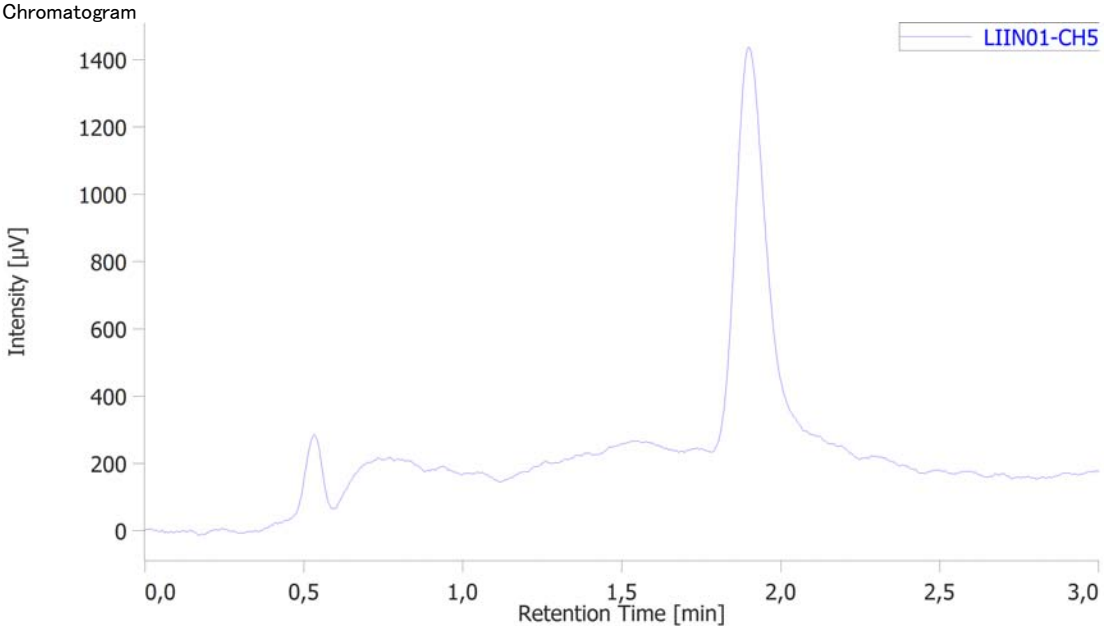


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:14:12
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:15:32
Volume	5,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

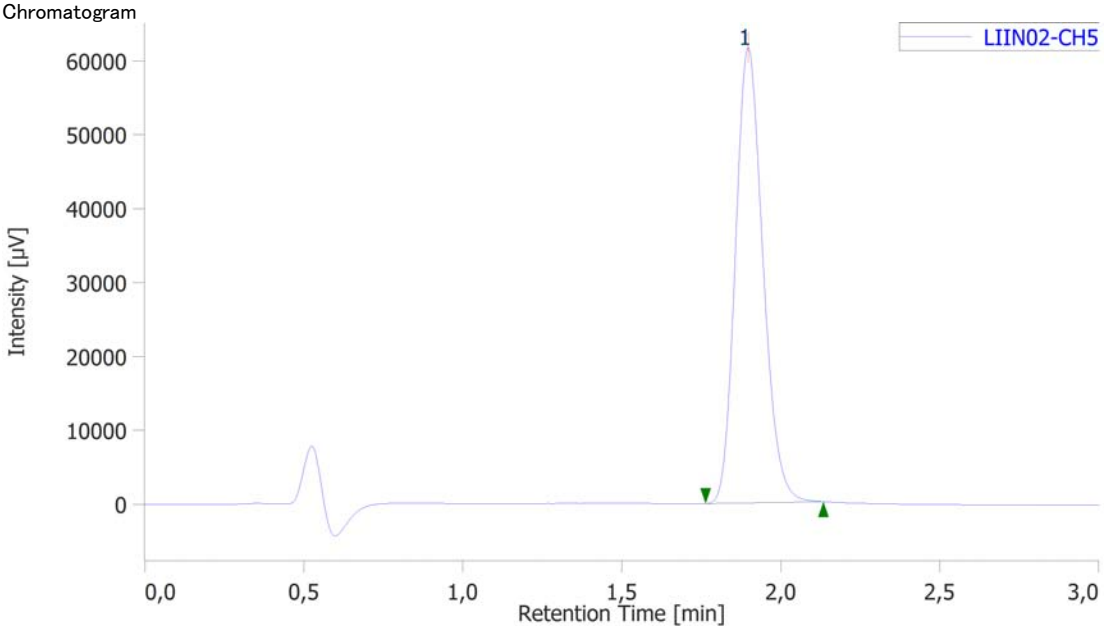


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,897	369854	61627

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:14:21
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:18:44
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

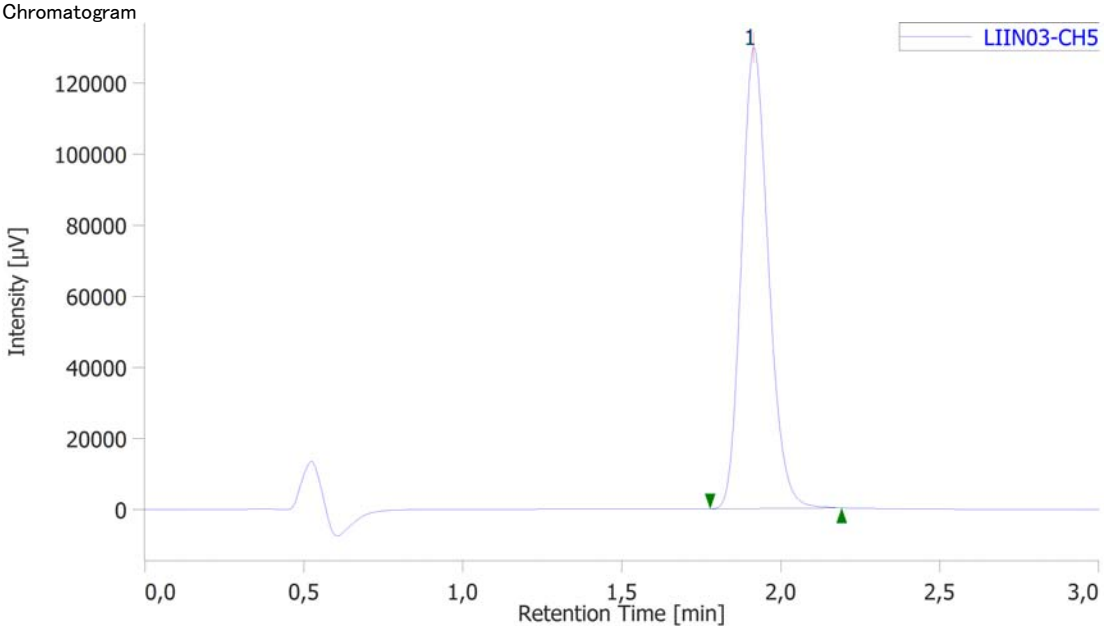


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,913	765217	129750

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 13:14:31
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:21:56
Volume	15,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

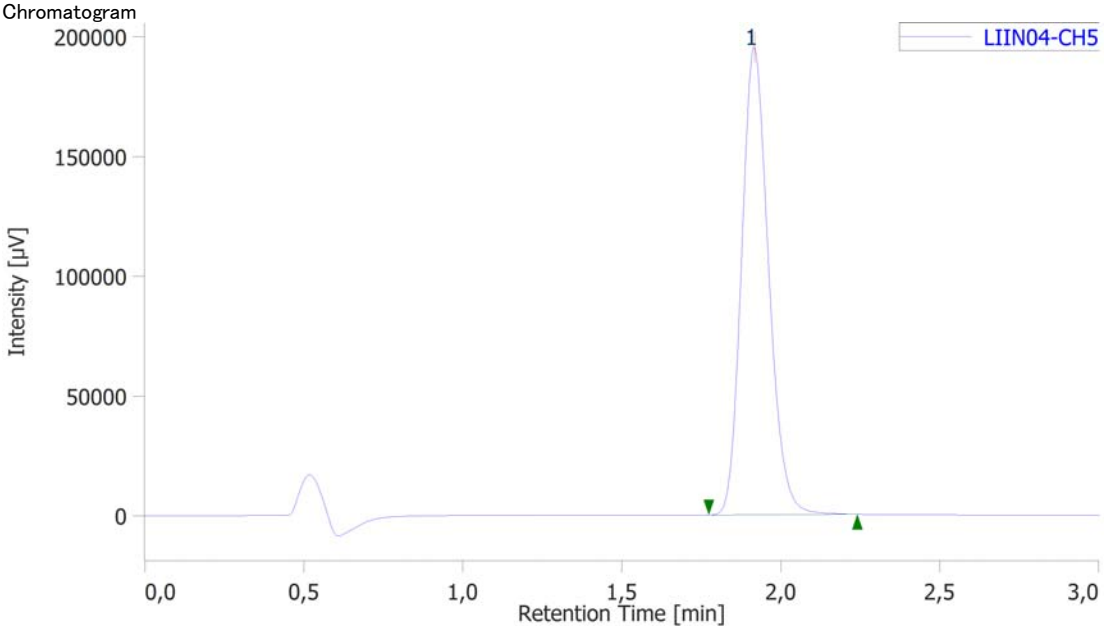


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,917	1151192	195169

Chromatogram Information

User Name	Administrator
Date Modified	14/11/2018 13:14:39
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 12:25:08
Volume	20,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICACAO
Control Method	Qualificacao
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

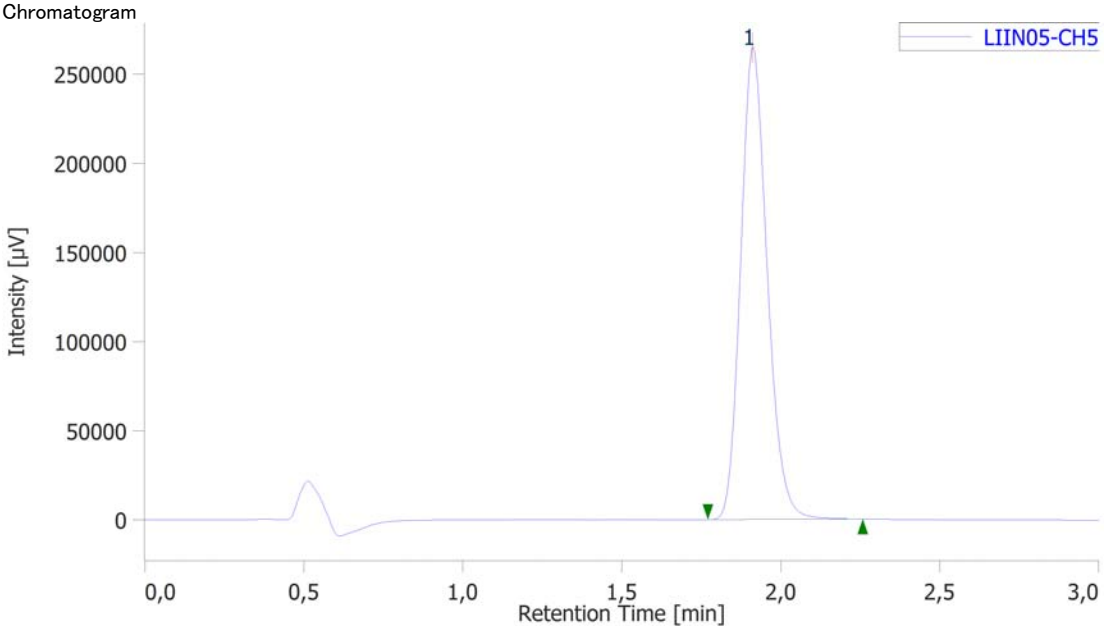


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,910	1535024	264687

Chromatogram Information	
User Name	Administrator
Date Modified	14/11/2018 16:16:38
Description	
HPLC System Name	HPLC
Injection Date	14/11/2018 15:43:19
Volume	0,10 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	33,3 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente02
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

Chromatogram

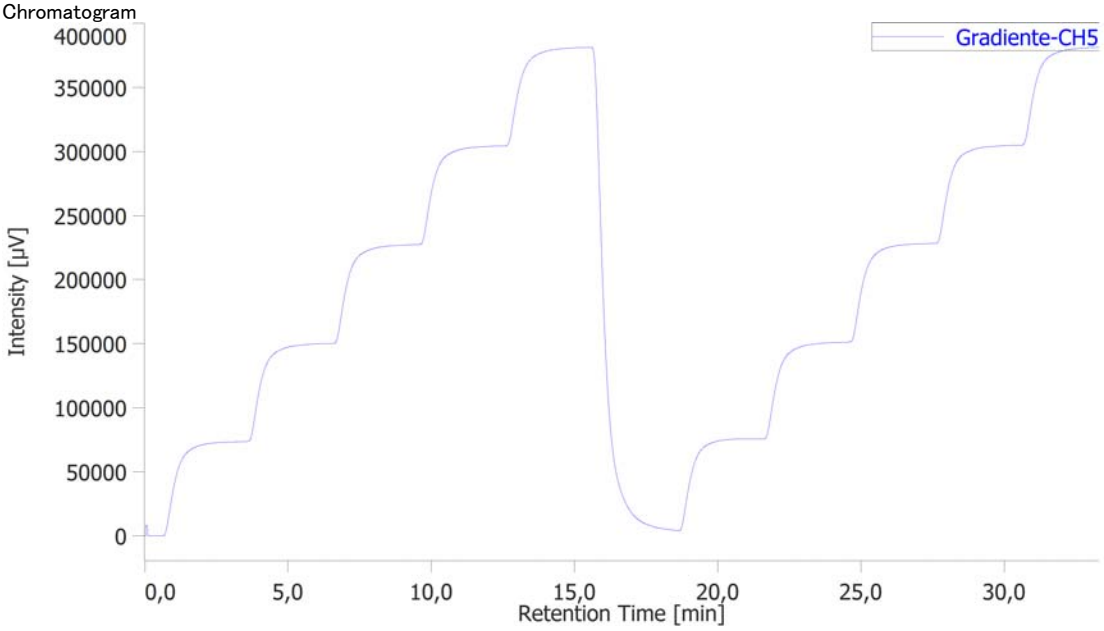

Peak Information – No data.