
Peak Find - EDUV.jws

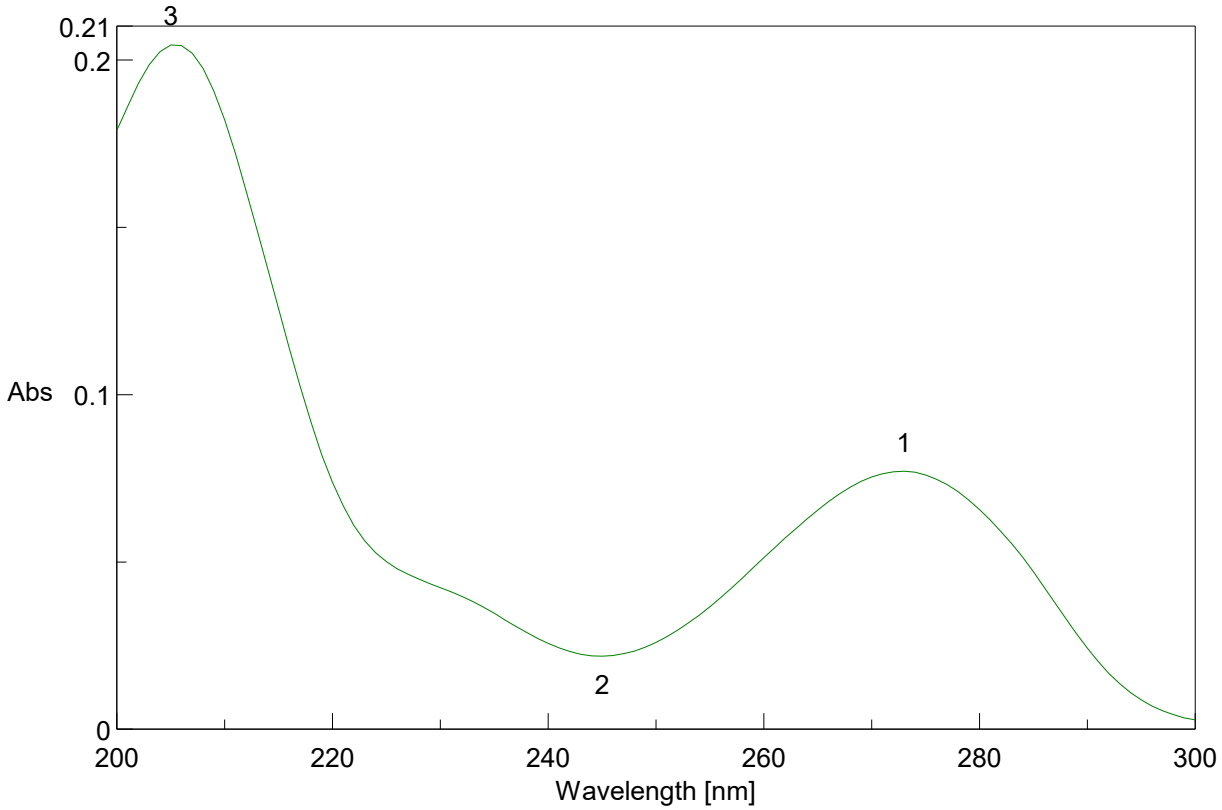

[Comments]

User	Administrator
Division	---
Company	HP Inc.
Creation date	12/11/2018 15:13

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4015
Model Name	MD-4015
Serial No.	A006861663
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.077033	2	245	0.021799
3	205	0.204359			

Chromatogram

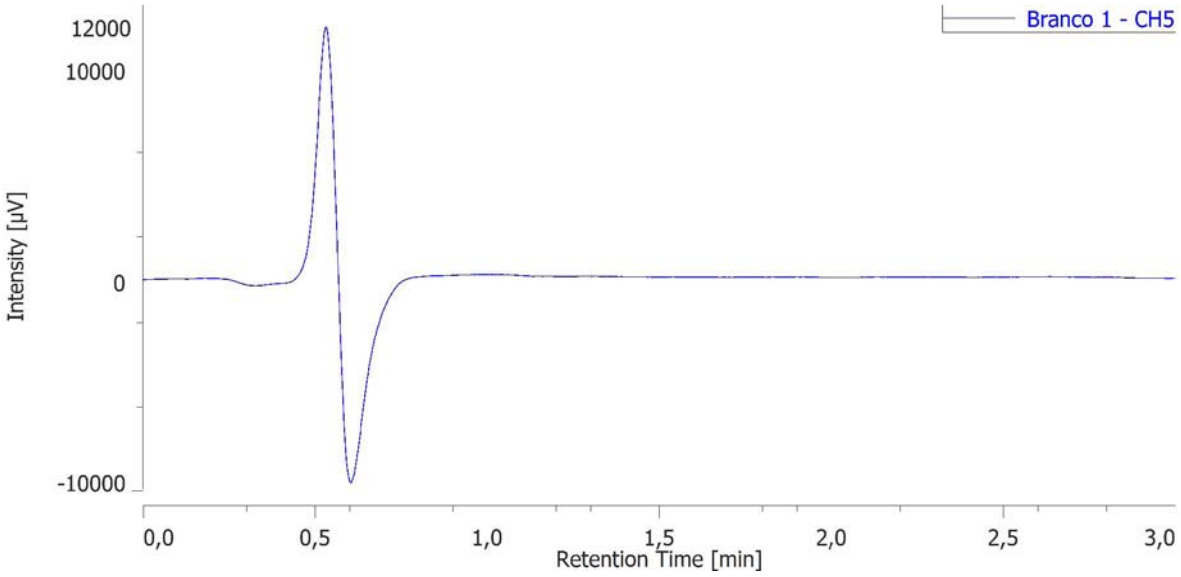


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 09:38:13
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:33:51
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	Branco 1
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

Chromatogram

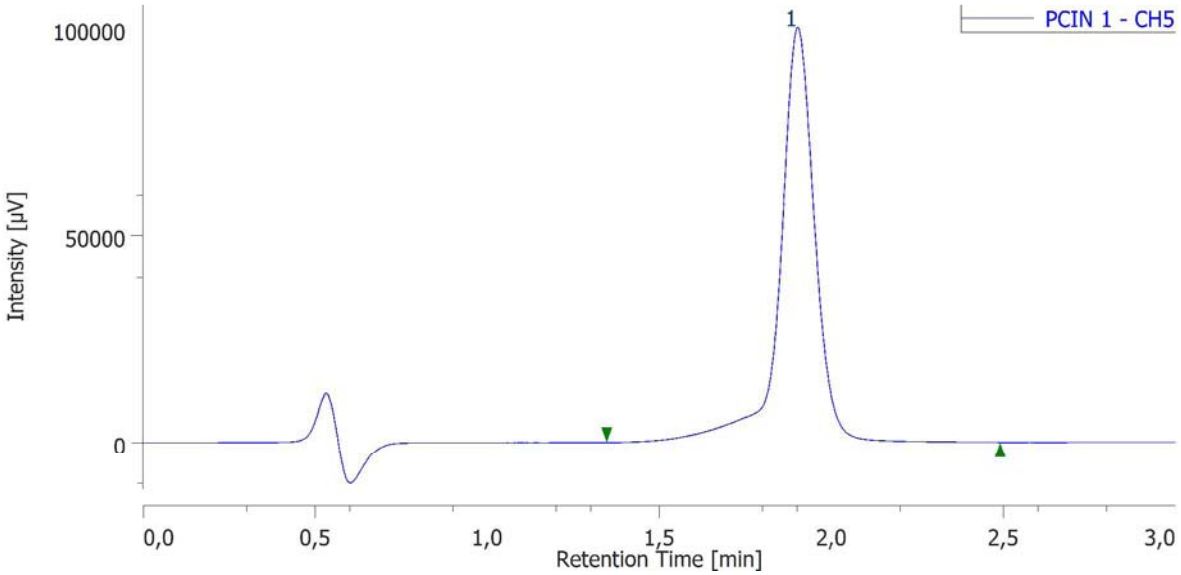


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 09:42:08
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:37:03
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	PCIN 1
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,903	708960	100215

Chromatogram

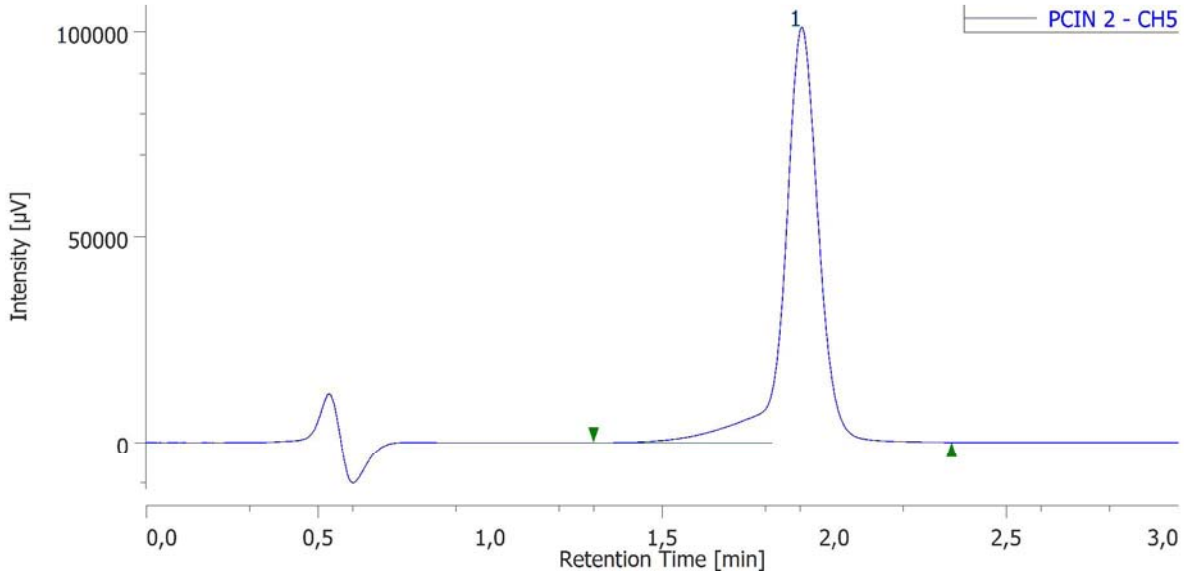


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 09:43:55
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:40:15
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	PCIN 2
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,907	705267	100958

Chromatogram

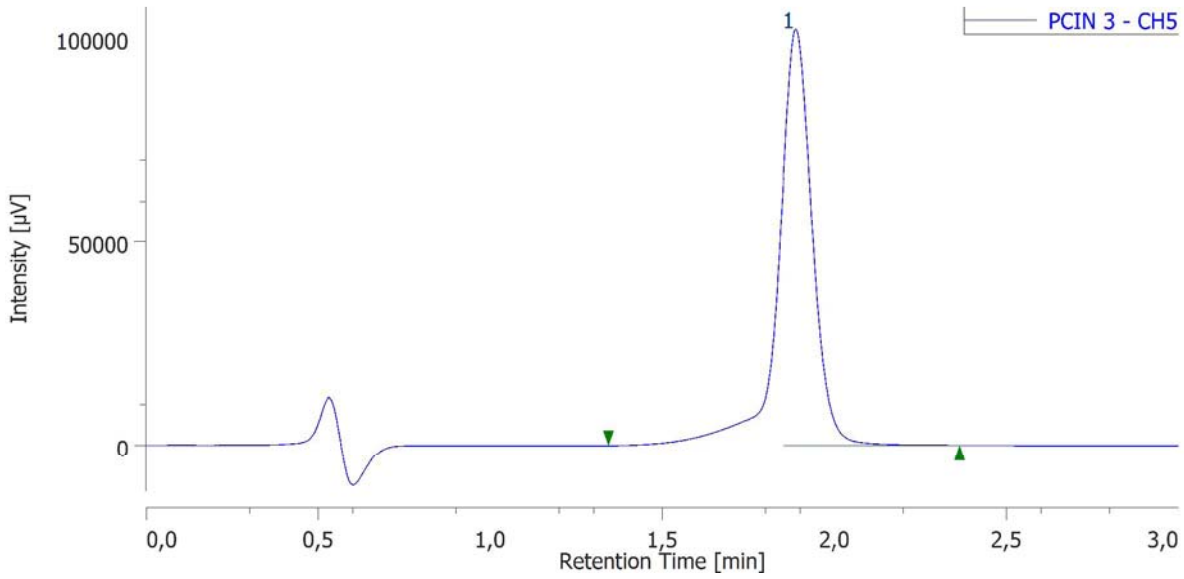


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 09:49:40
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:43:27
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	PCIN 3
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,887	706092	102119

Chromatogram

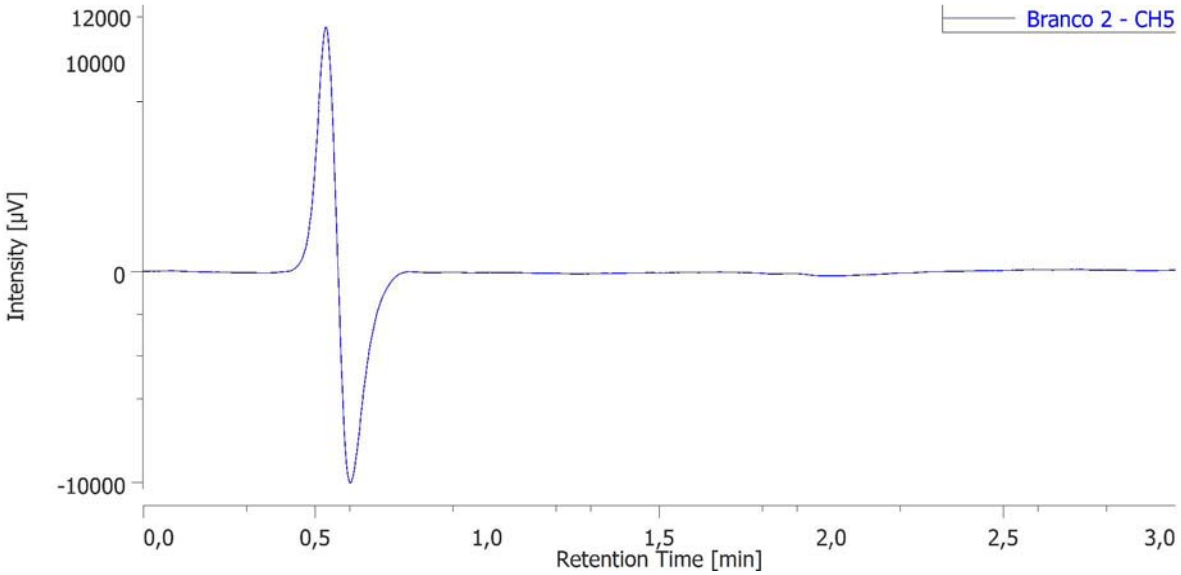


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 09:52:17
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:46:39
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	Branco 2
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

Chromatogram

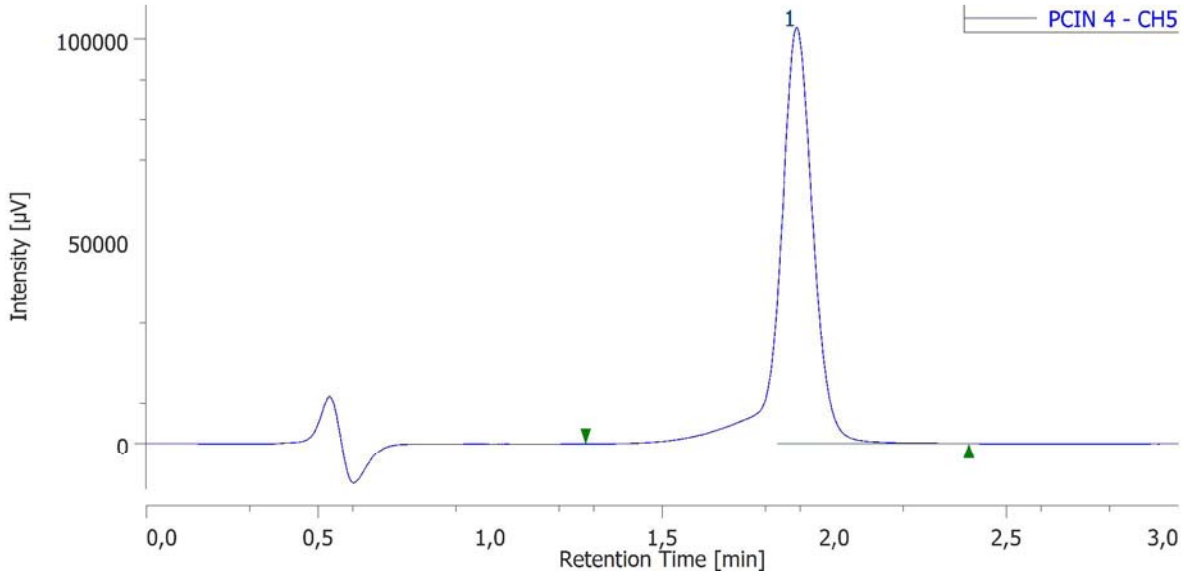


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:02:20
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:49:51
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	PCIN 4
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,890	708169	102787

Chromatogram

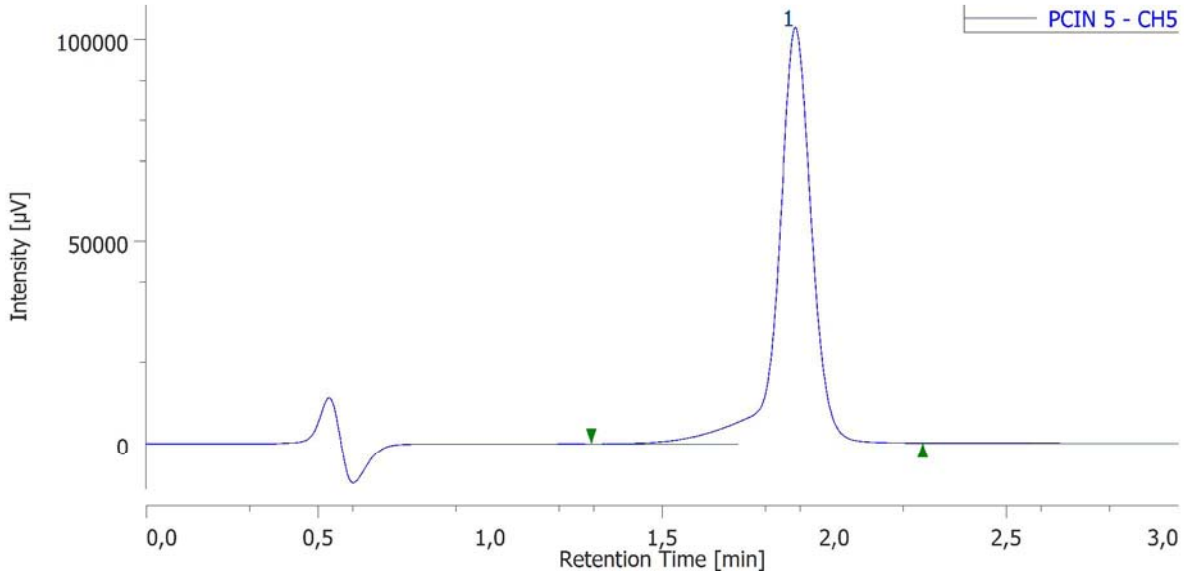


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:04:23
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:53:03
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	PCIN 5
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,887	704311	102922

Chromatogram

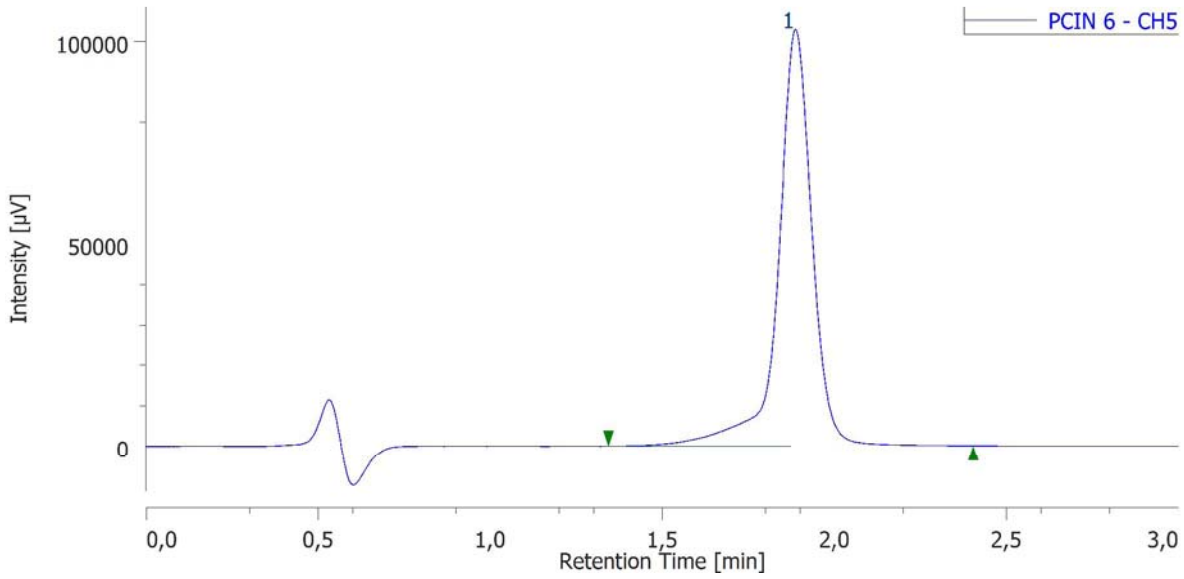


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:05:37
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:56:15
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	PCIN 6
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,887	707326	102846

Chromatogram

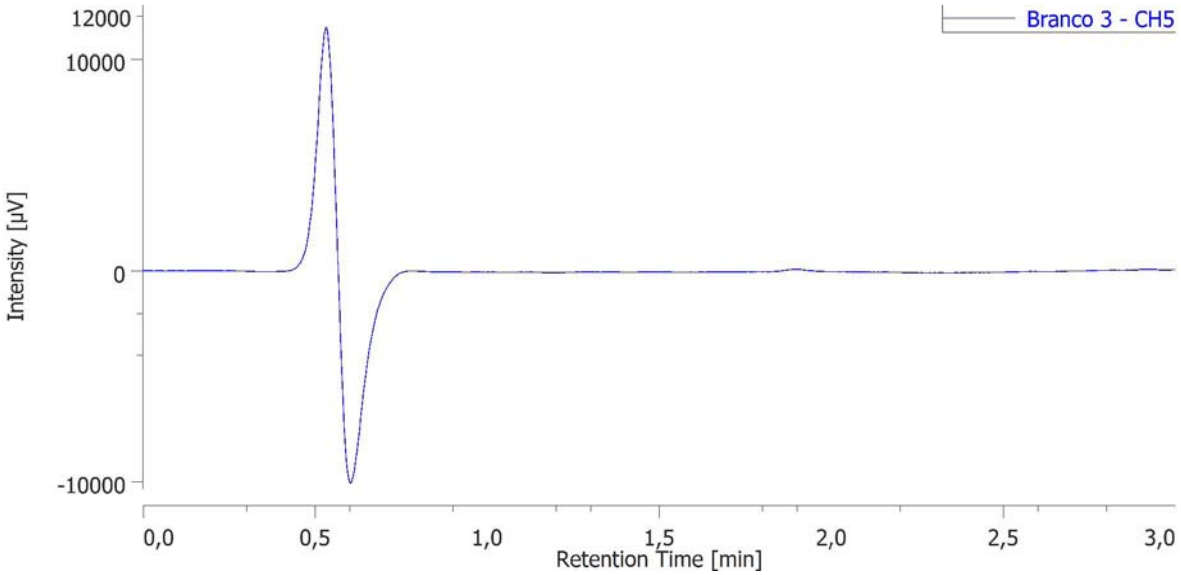


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:06:22
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 09:59:27
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	Branco 3
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

Chromatogram

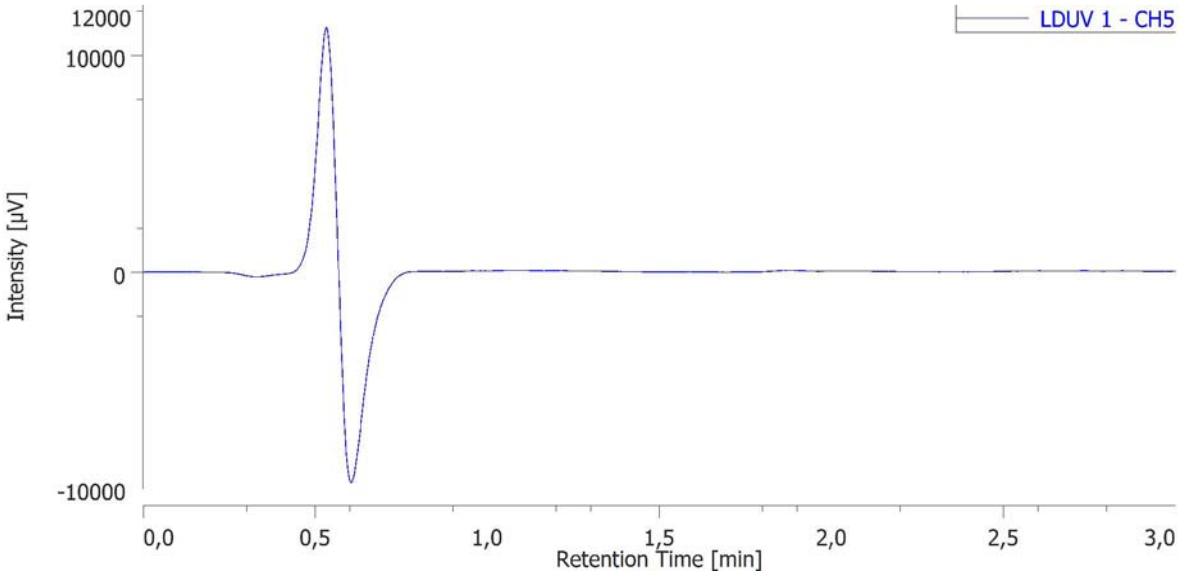


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:15:33
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:10:29
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	LDUV 1
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

Chromatogram

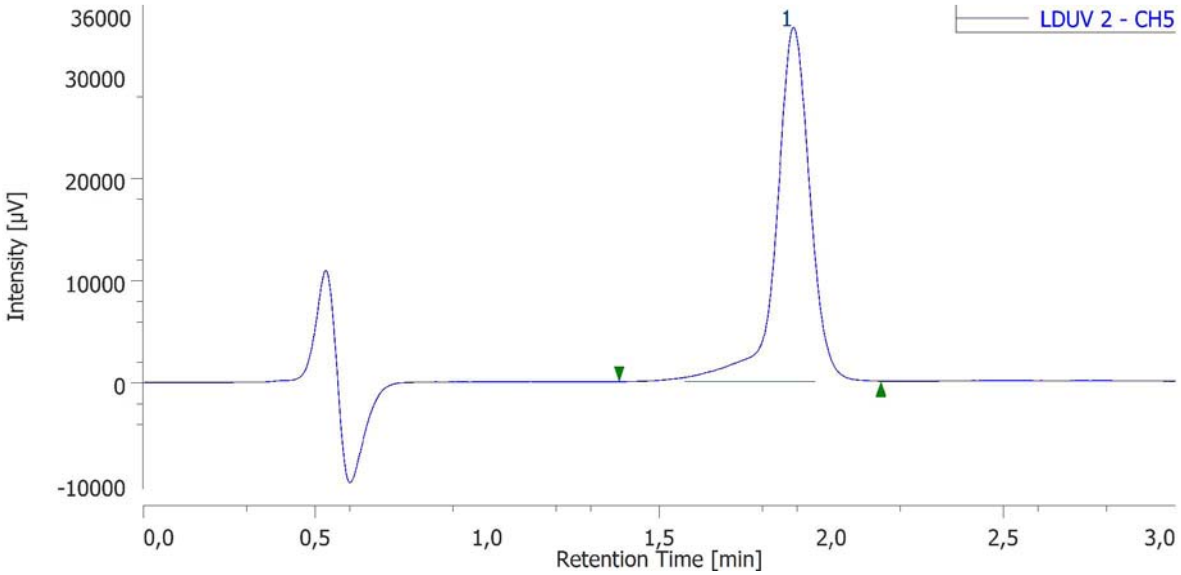


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:17:06
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:13:41
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	LDUV 2
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,890	238216	34486

Chromatogram

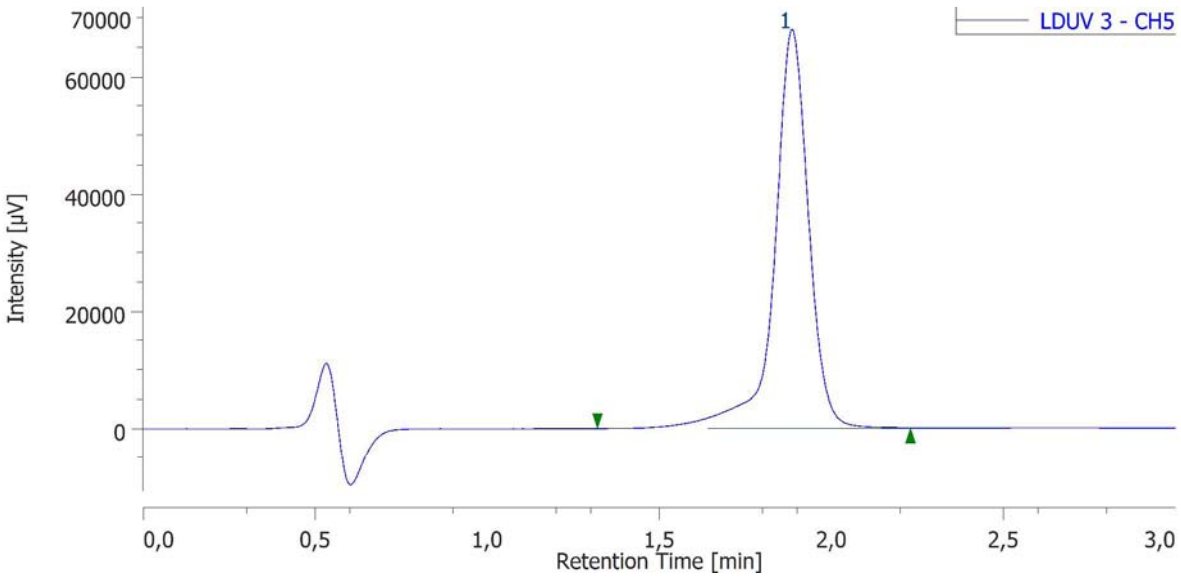


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:28:27
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:16:53
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	LDUV 3
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,887	473674	67907

Chromatogram

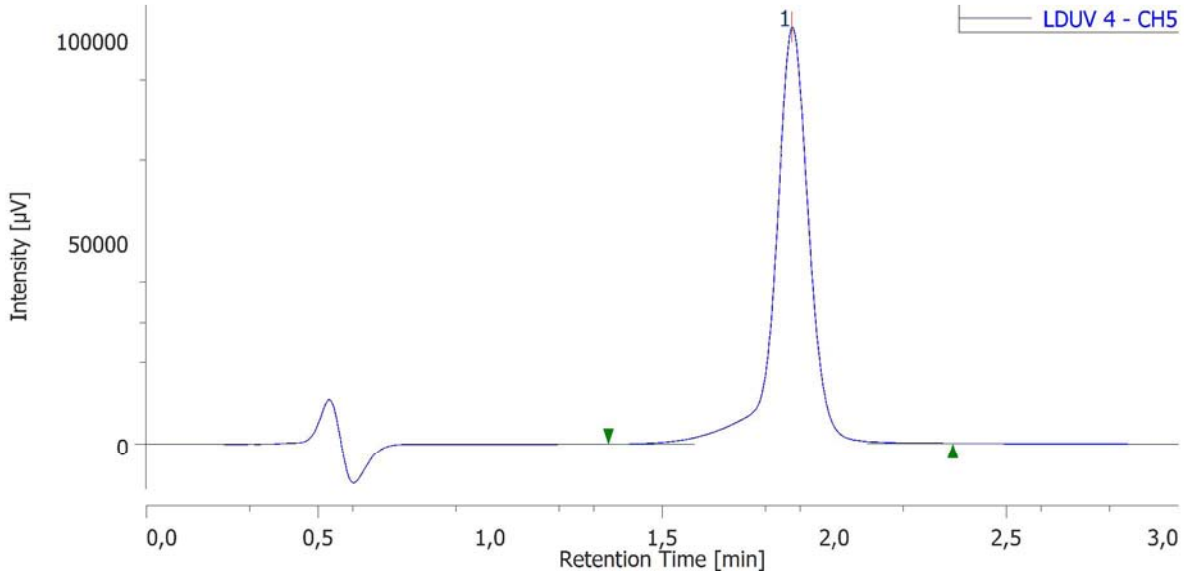


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:30:05
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:20:05
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	LDUV 4
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,877	706173	102562

Chromatogram

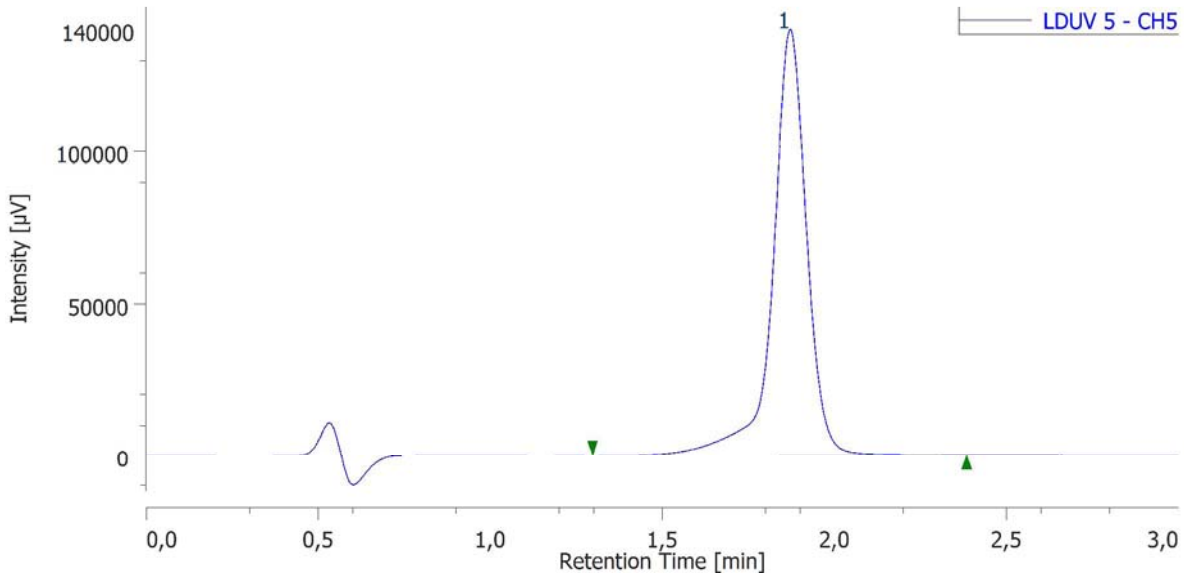


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:30:32
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:23:17
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	LDUV 5
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,873	963796	139852

Chromatogram

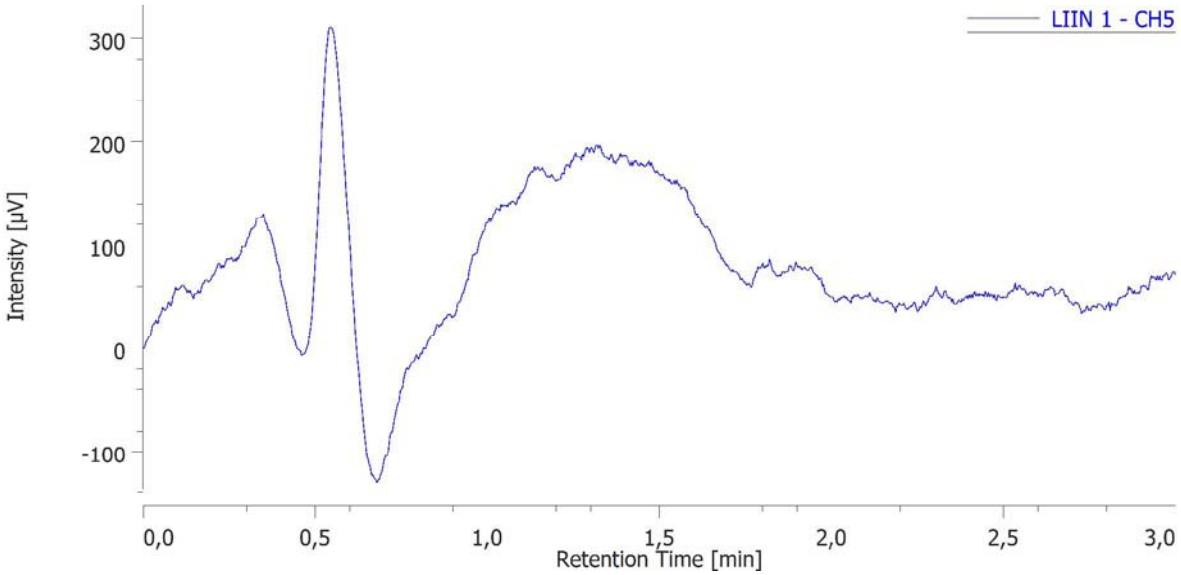


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:38:02
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:34:21
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	LIIN 1
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

Chromatogram

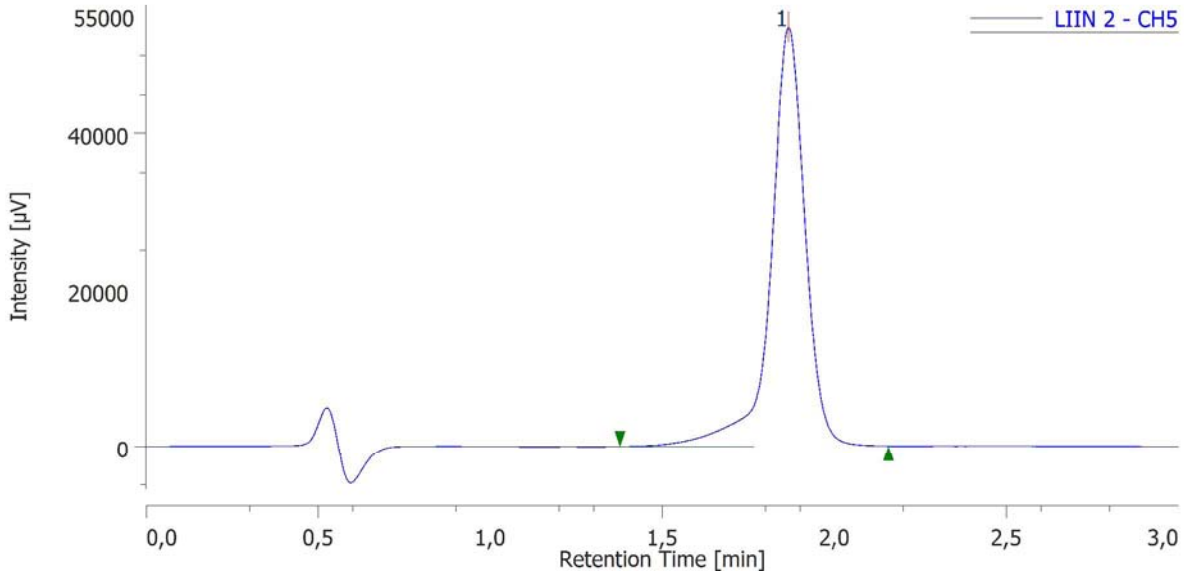


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:41:50
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:37:33
Volume	5,00 [μL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	LIIN 2
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]
1	Cafeina	5	1,867	371036	53436

Chromatogram

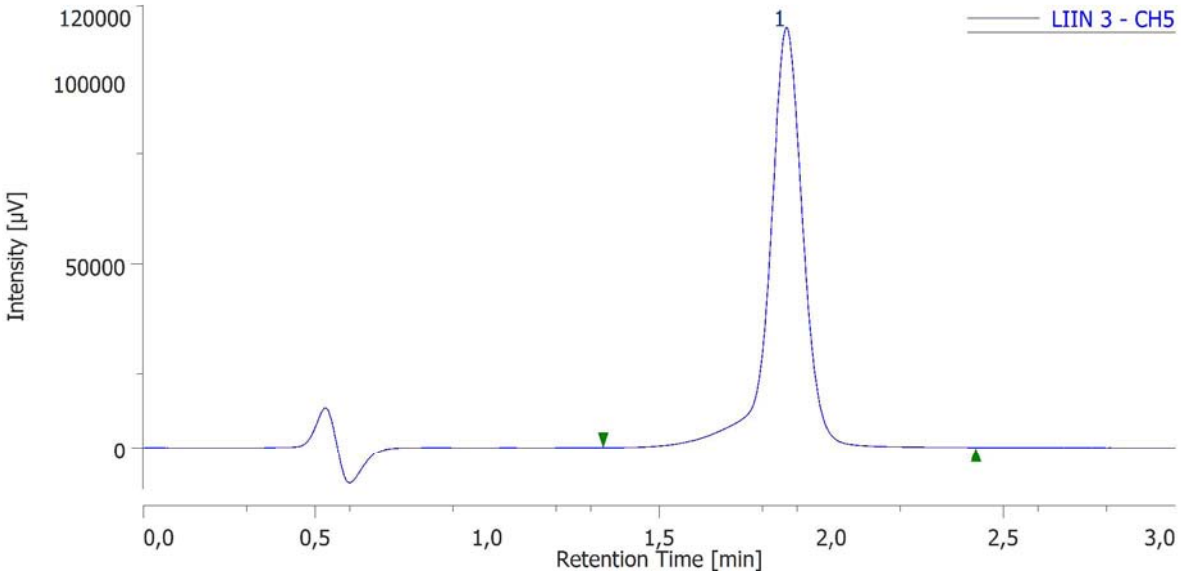


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:48:01
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:40:45
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	LIIN 3
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,870	787246	114151

Chromatogram

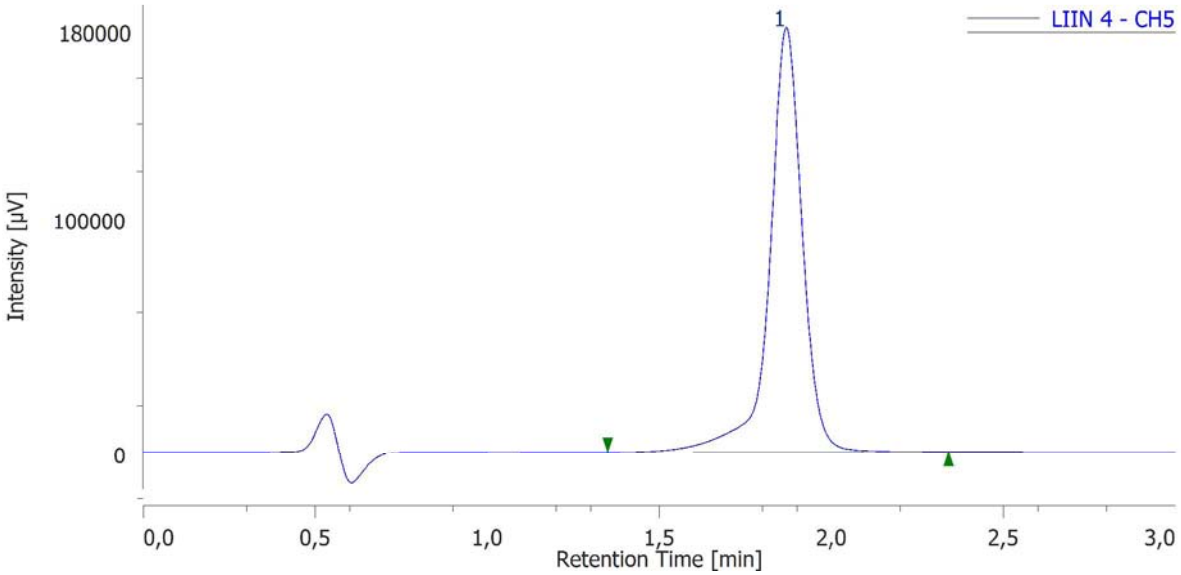


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:48:30
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:43:57
Volume	15,00 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	LIIN 4
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,870	1210732	180932

Chromatogram

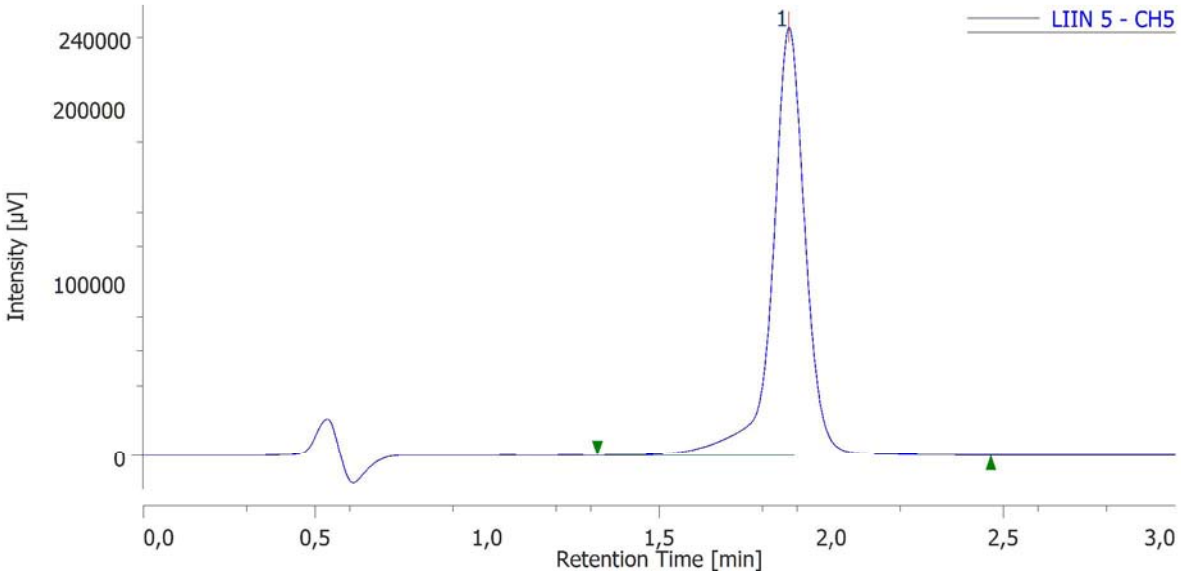


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 10:50:45
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 10:47:09
Volume	20,00 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificacao
Peak ID Table	Qualificacao
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	LIIN 5
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificacao

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,877	1646617	245521

Chromatogram

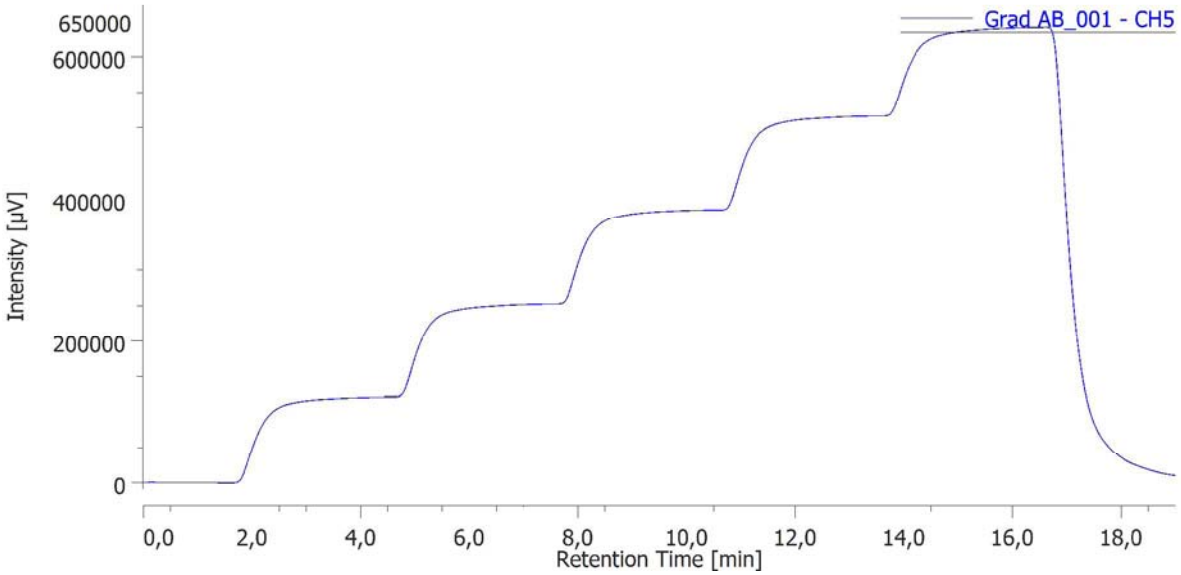


Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 11:32:10
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 11:13:08
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Chromatogram

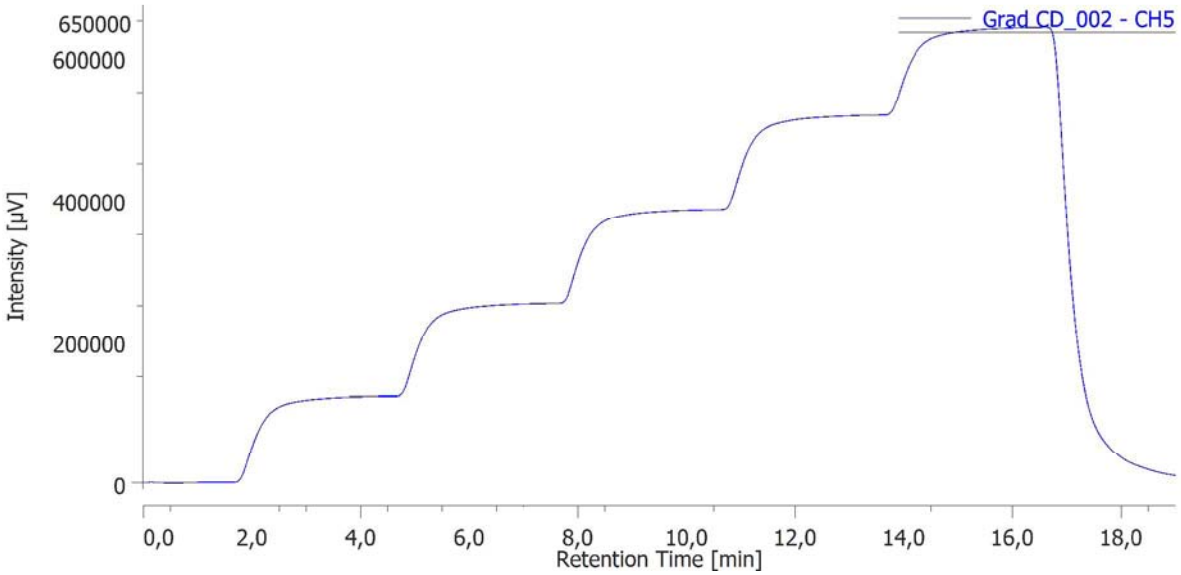

Chromatogram Information	
User Name	Administrator
Date Modified	13/11/2018 11:54:46
Description	
HPLC System Name	JASCO HPLC
Injection Date	13/11/2018 11:35:45
Volume	0,10 [μL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	