
Peak Find - EDUV_003 PDA_2,0200

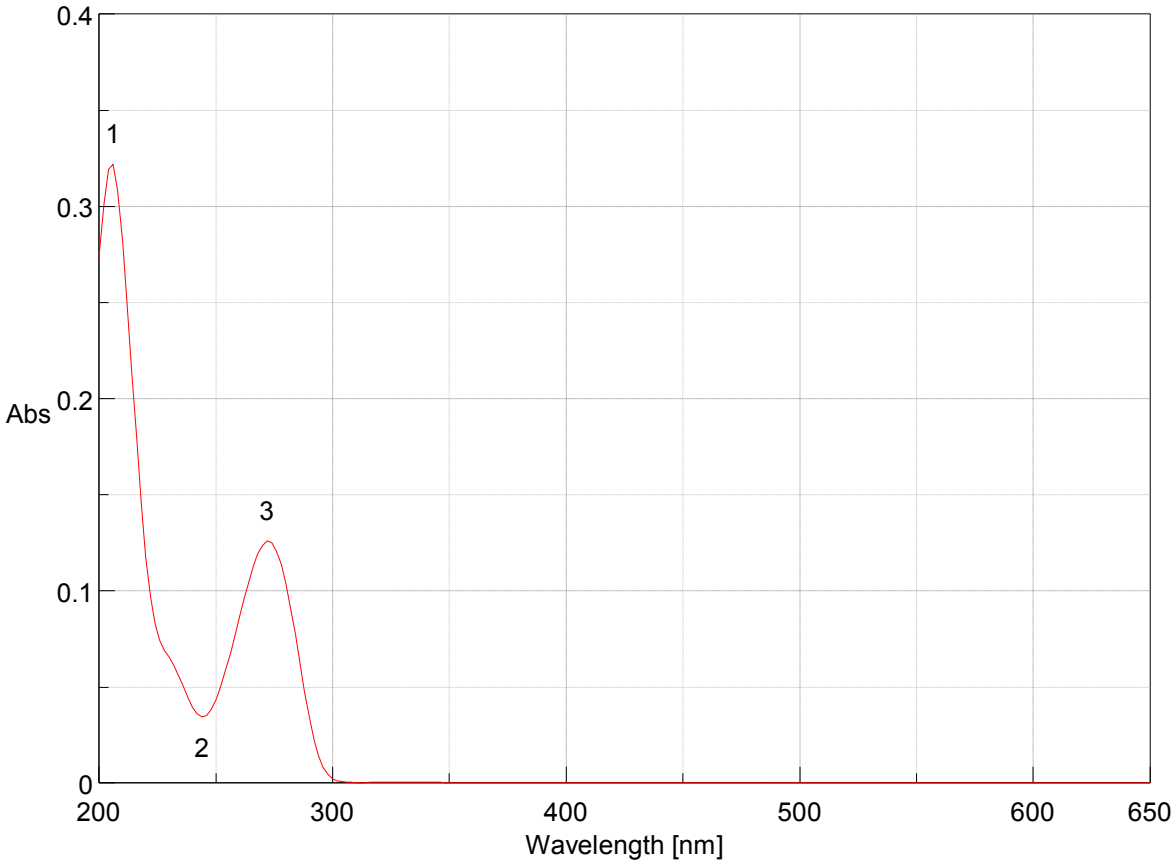

[Comments]

User	Administrator
Division	---
Company	M
Creation date	15/11/2018 11:29
Date modified	15/11/2018 11:34

[Detailed Information]


Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	650 nm
Data interval	2 nm
Data points	226

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	206	0.321746	2	244	0.034323
3	272	0.125885			

Chromatogram Information	
User Name	Administrator
Date Modified	15/11/2018 12:15:06
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 11:41:35
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

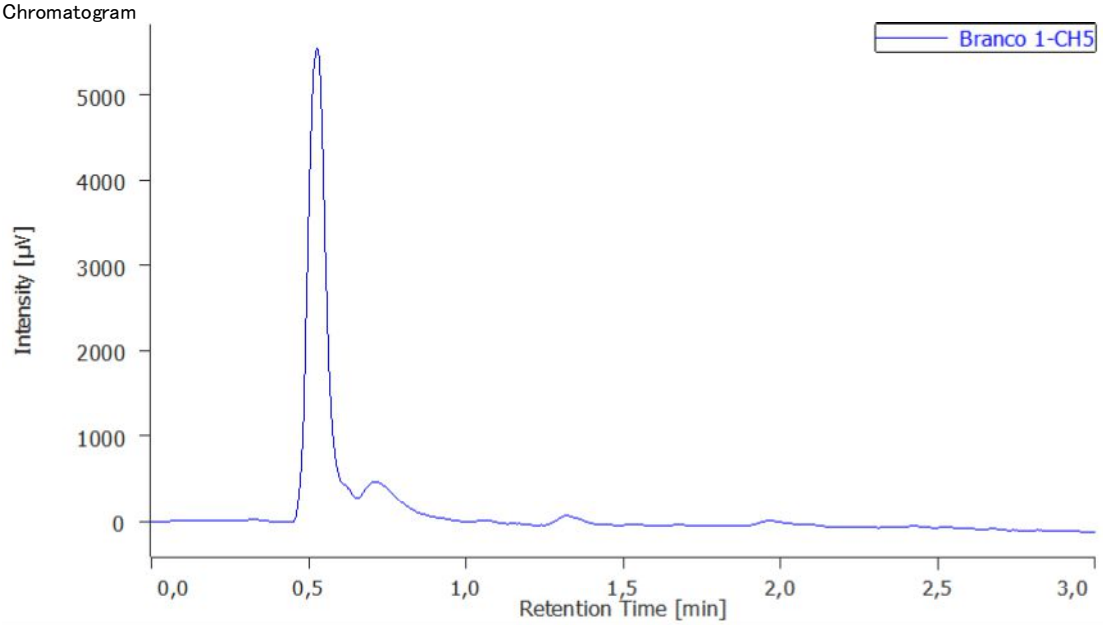


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 12:15:11
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 11:44:47
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

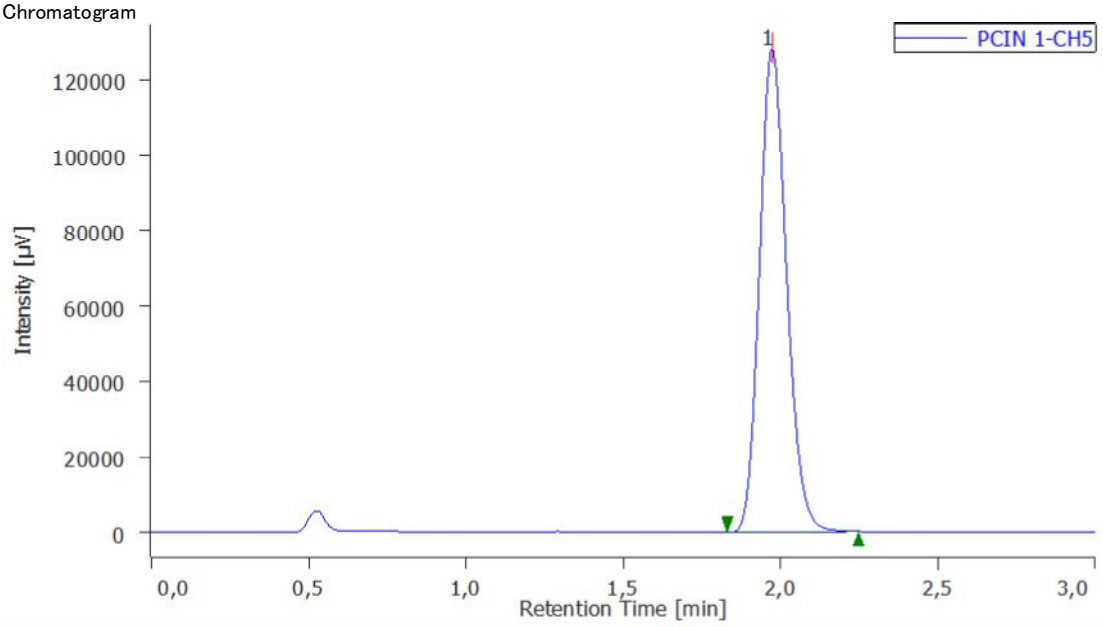


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,973	765098	128175

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 12:20:10
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 11:47:59
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

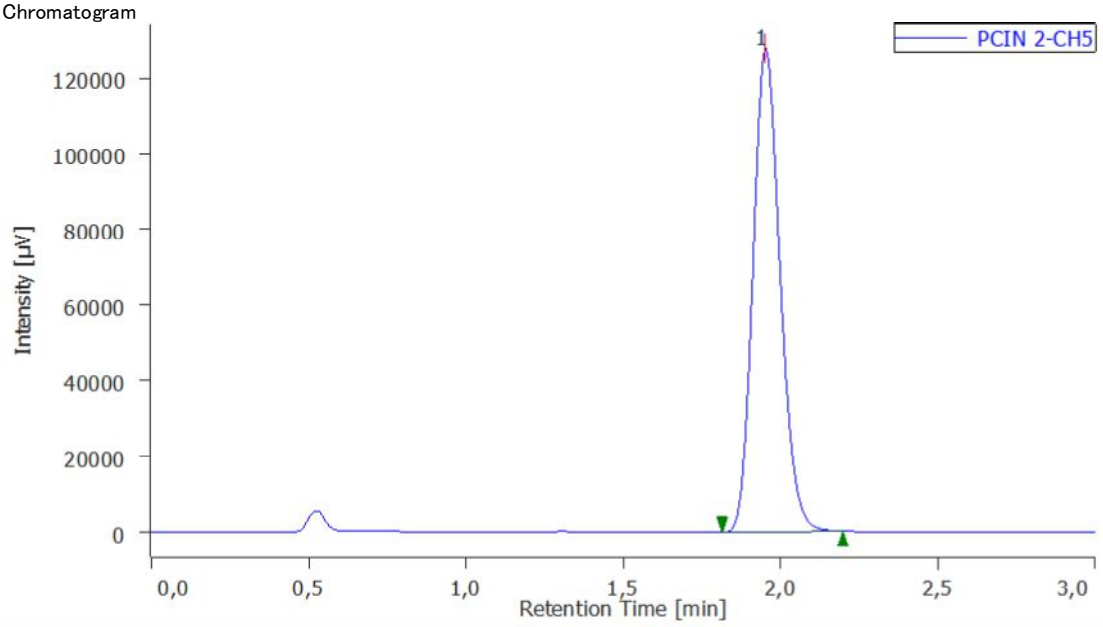


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,950	762931	127799

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 12:20:16
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 11:51:11
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

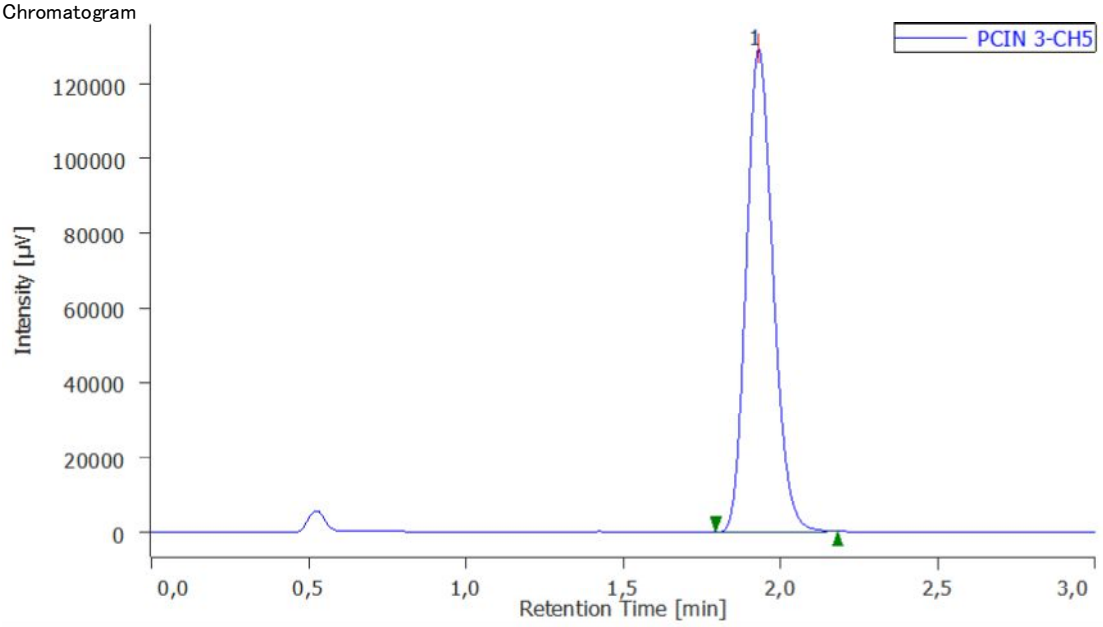


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,930	763012	129446

Chromatogram Information	
User Name	Administrator
Date Modified	15/11/2018 12:15:31
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 11:54:23
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

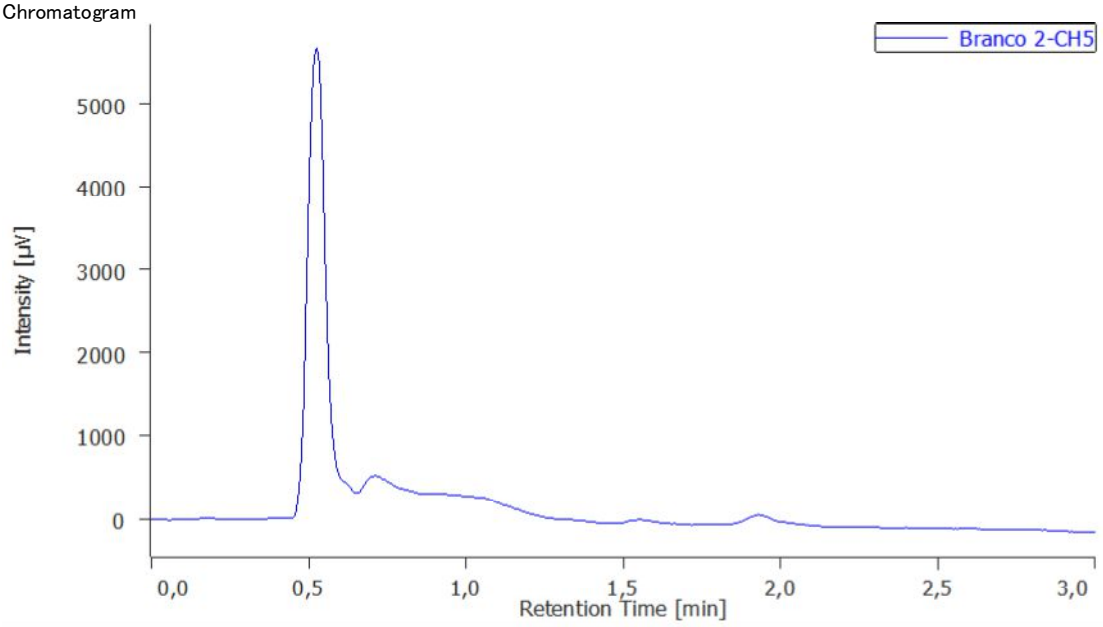


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 12:15:36
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 11:57:35
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

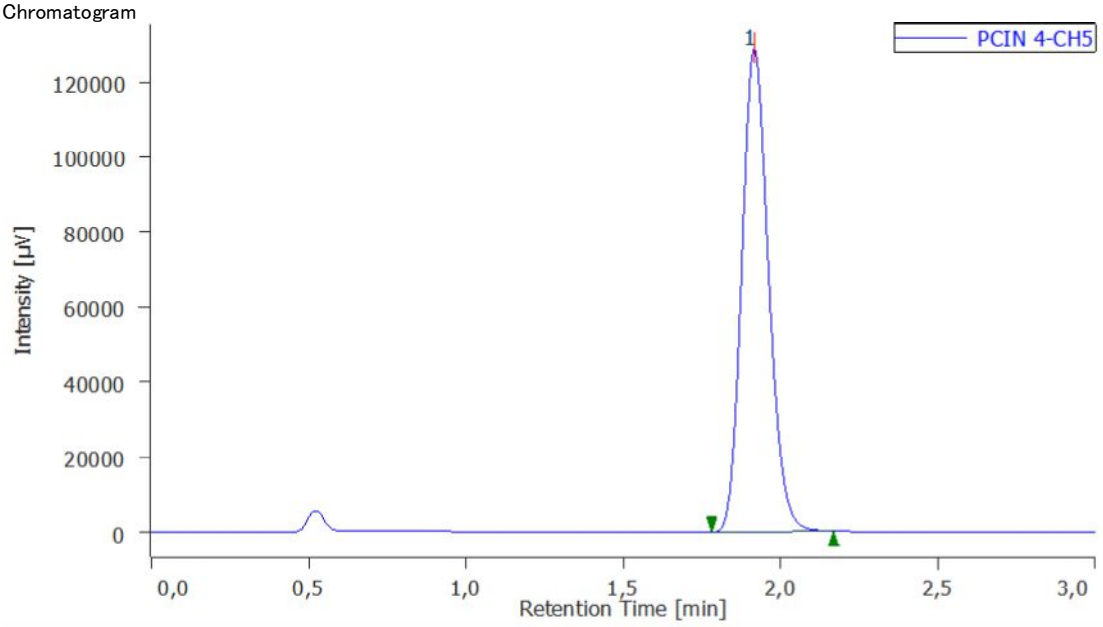


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,917	760829	128786

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 12:15:42
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 12:00:47
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

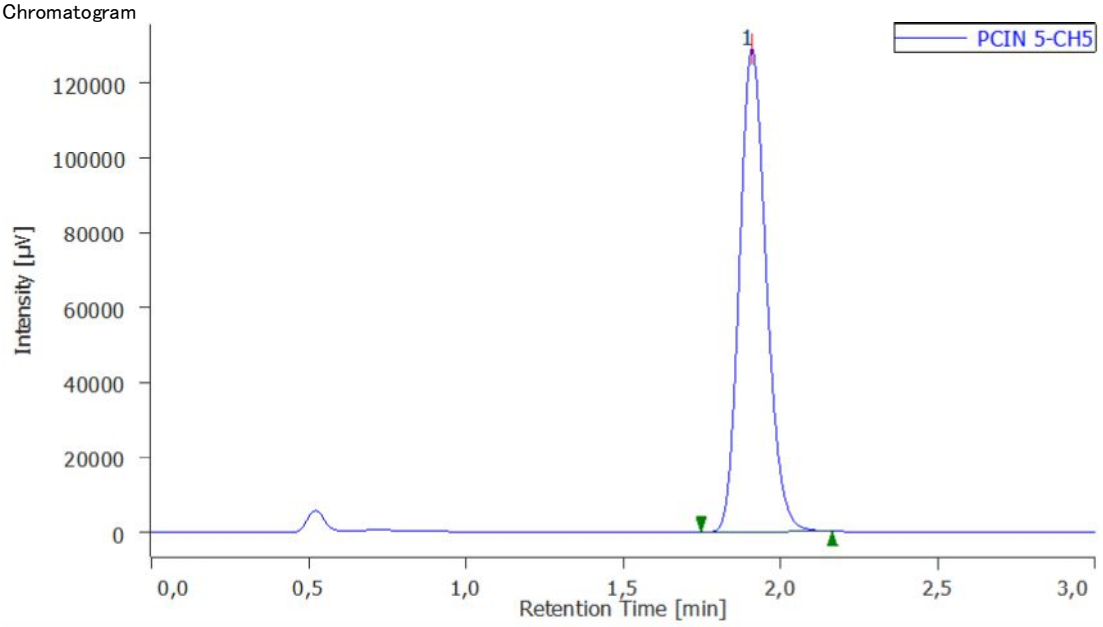


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,907	762402	129134

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 12:15:49
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 12:03:59
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

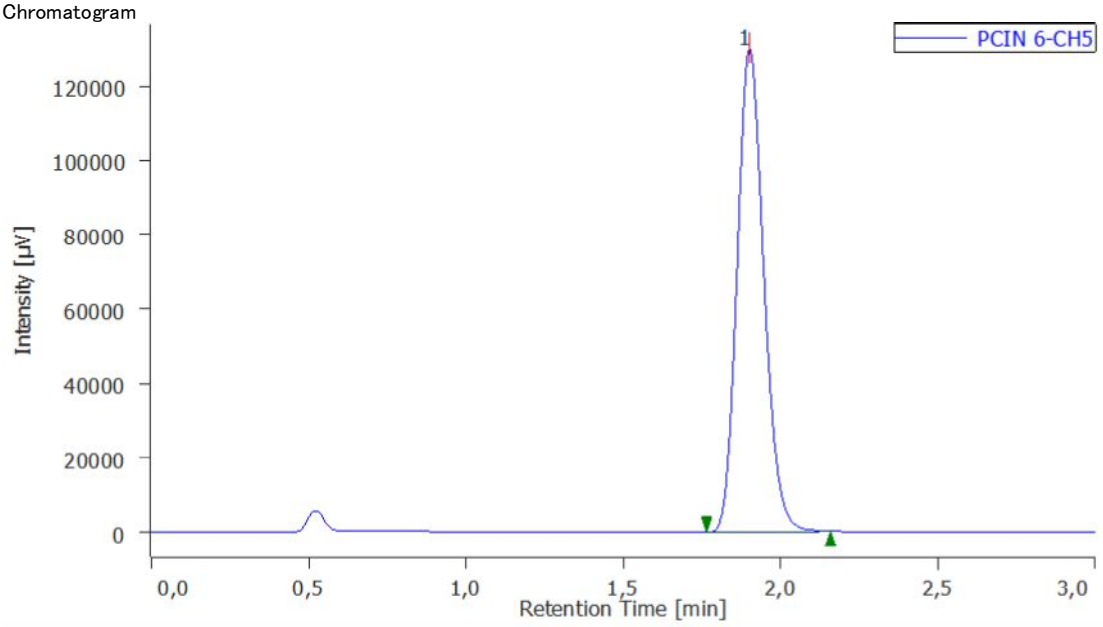


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,900	762397	129893

Chromatogram Information	
User Name	Administrator
Date Modified	15/11/2018 12:15:56
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 12:07:10
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificacao
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	


Chromatogram

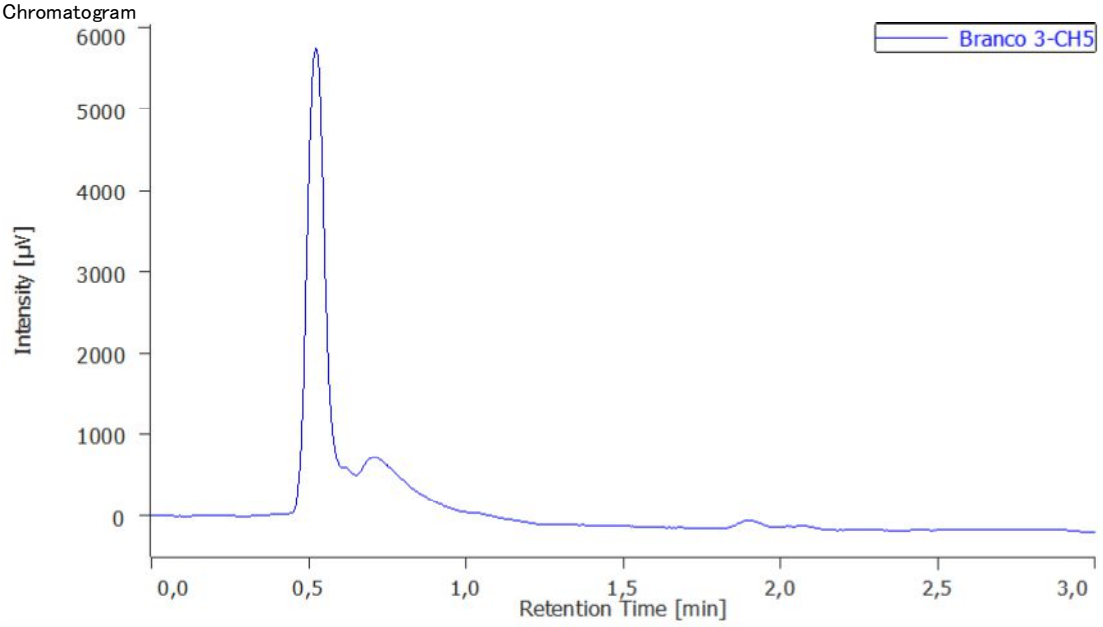

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	15/11/2018 14:06:34
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 13:47:35
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

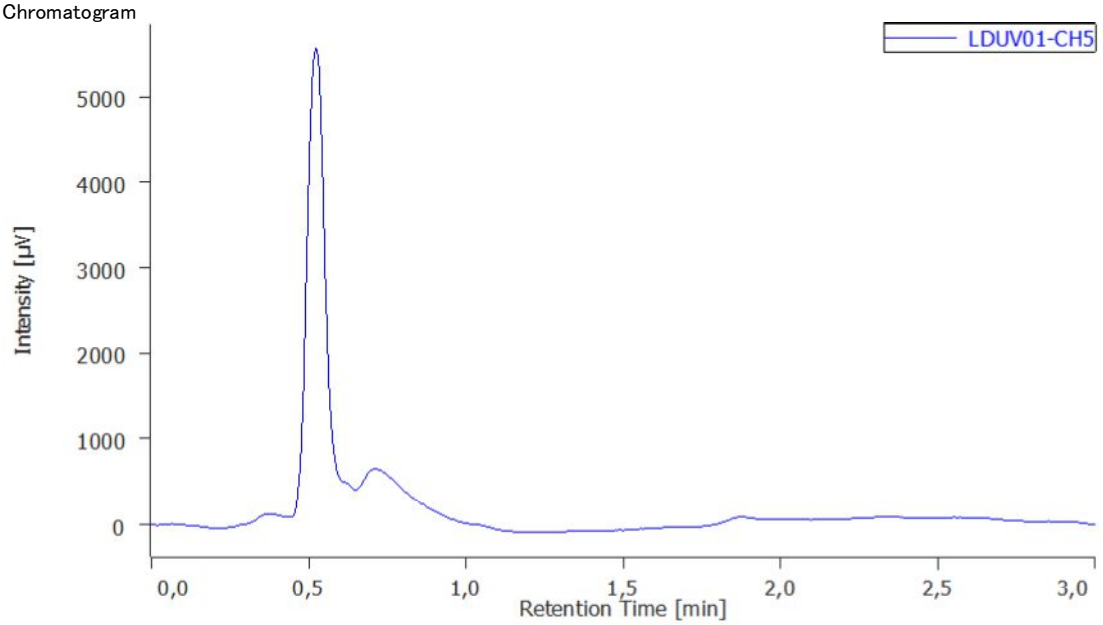


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:06:39
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 13:50:47
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

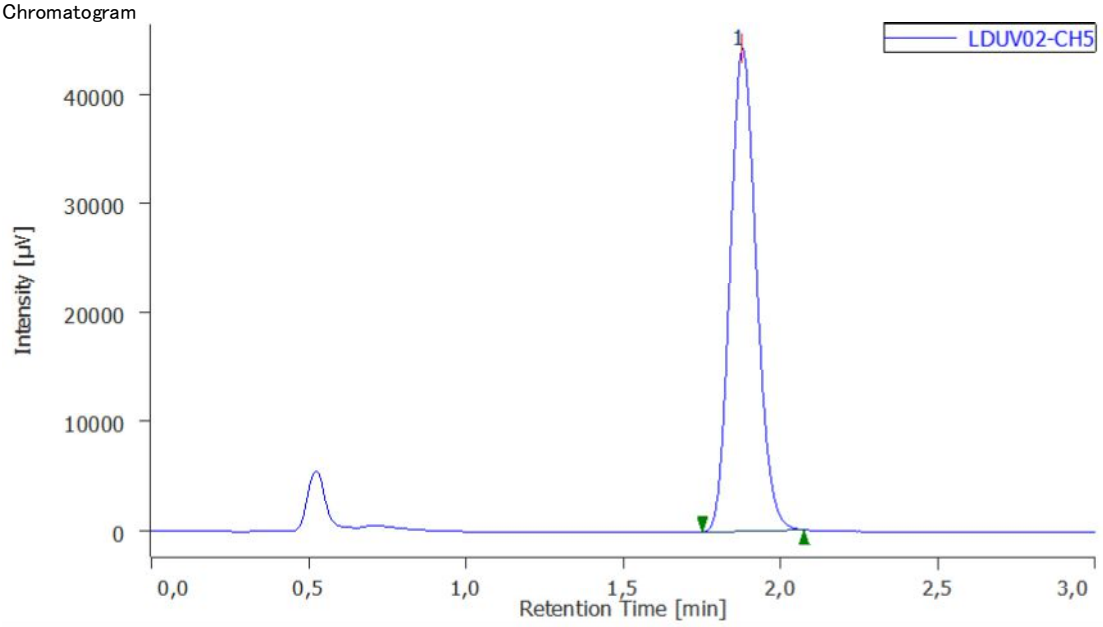


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,877	256030	44257

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:06:45
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 13:53:59
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

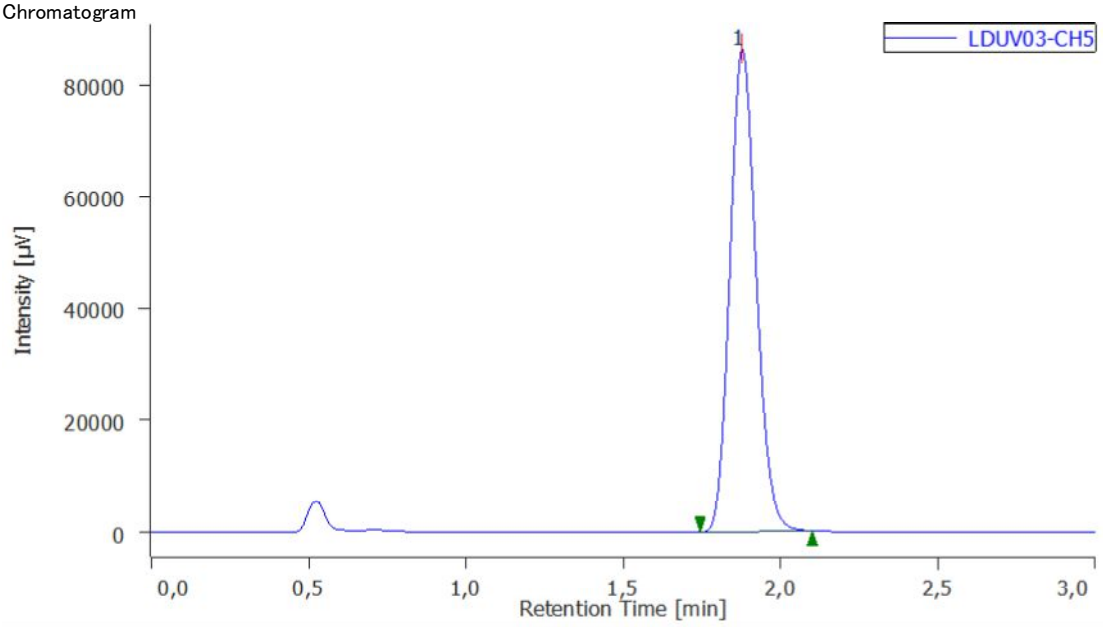


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,877	499235	86400

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:06:52
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 13:57:11
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

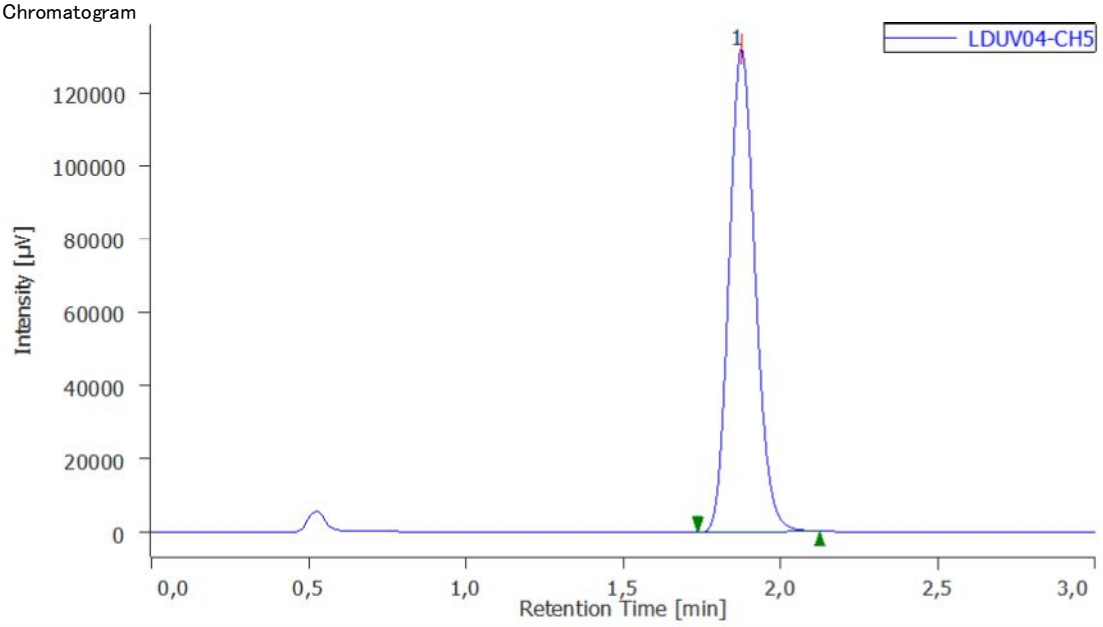


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,873	758126	131982

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:06:58
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:00:23
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LDUV
Additional Information	
Column Info	

Chromatogram

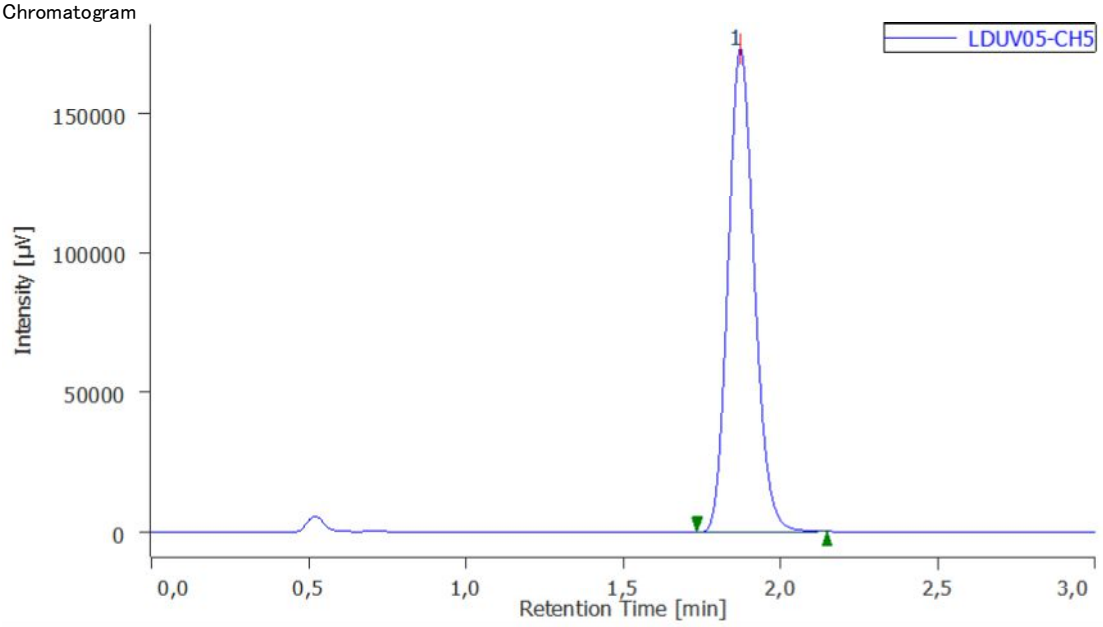


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,870	999673	173097

Chromatogram Information	
User Name	Administrator
Date Modified	15/11/2018 14:33:03
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:03:35
Volume	0,10 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

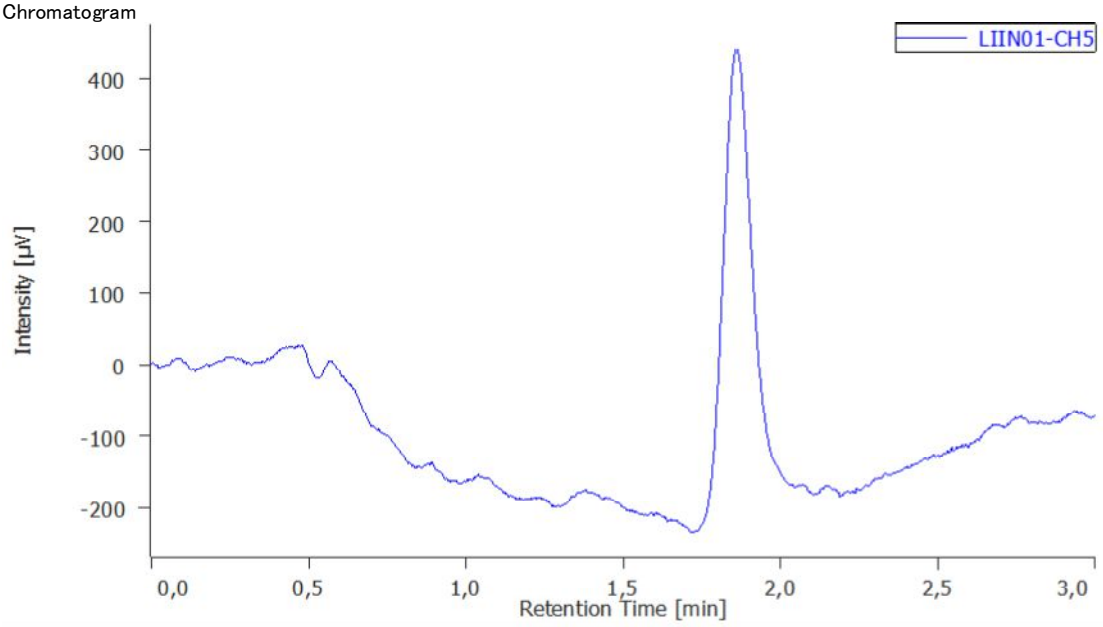


Peak Information – No data.

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:33:08
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:06:47
Volume	5,00 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

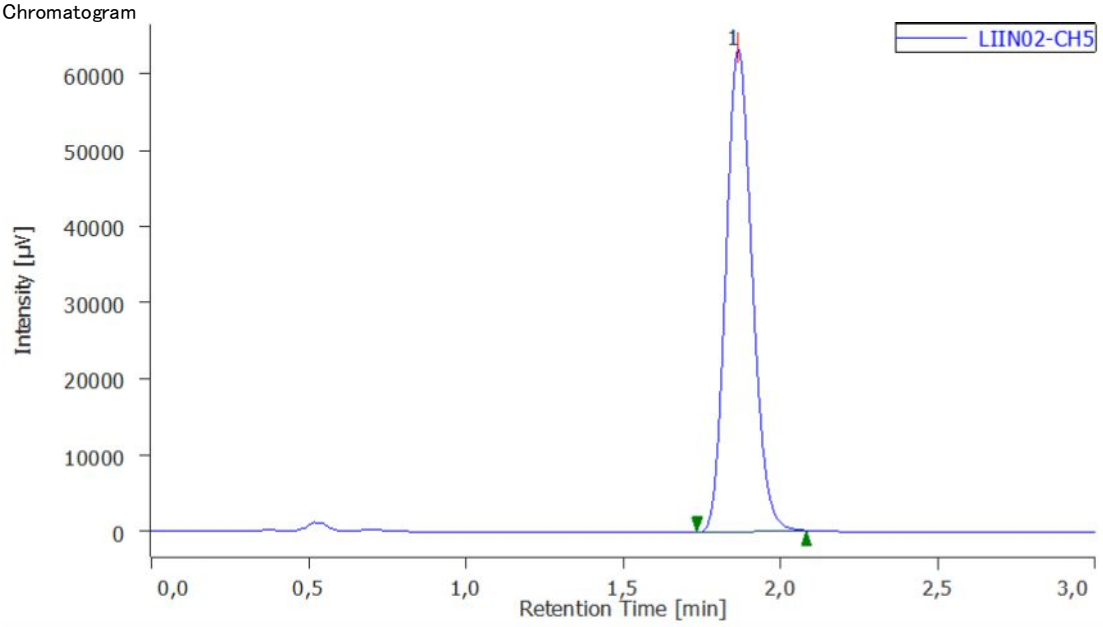


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,863	367088	63425

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:33:14
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:09:59
Volume	10,00 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

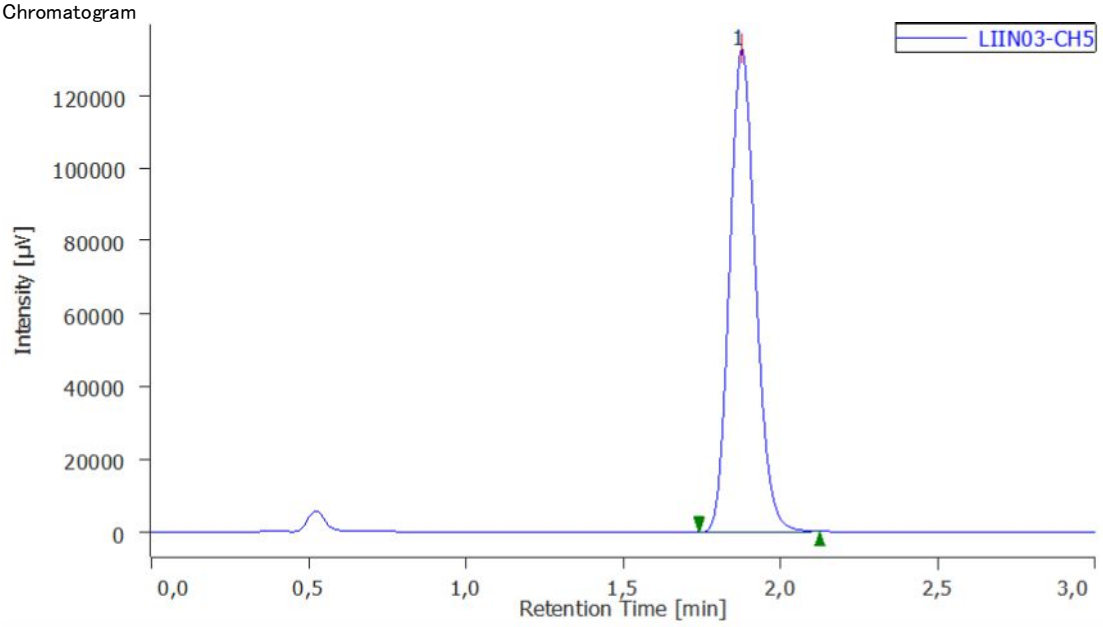


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,877	759340	132884

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:33:20
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:13:11
Volume	15,00 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

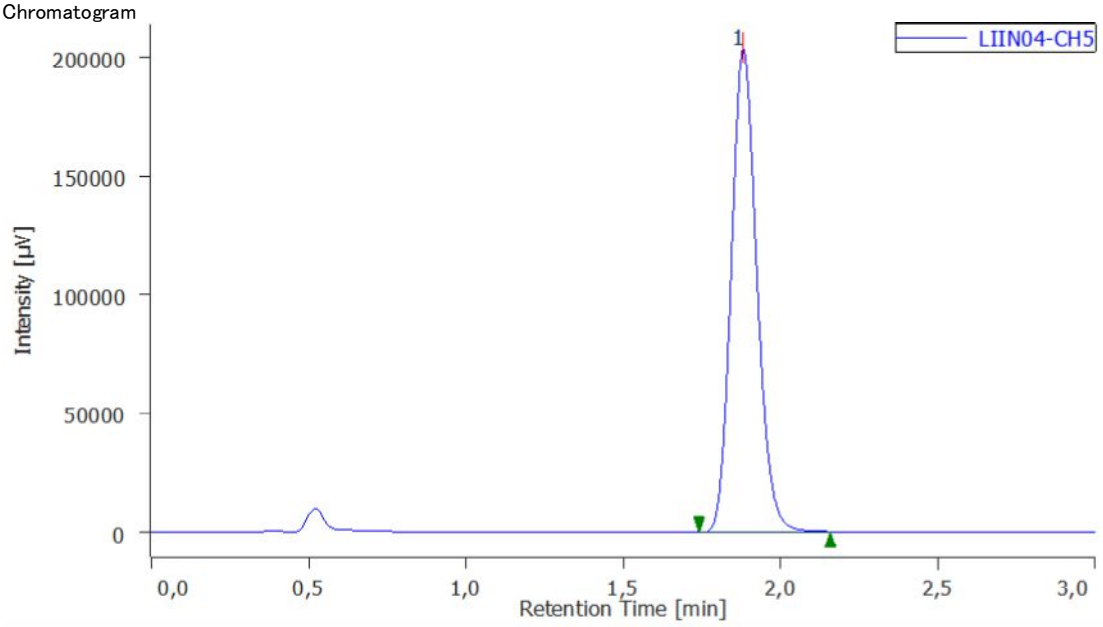


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,880	1149484	203672

Chromatogram Information

User Name	Administrator
Date Modified	15/11/2018 14:33:27
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:16:23
Volume	20,00 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV LIIN
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	LIIN
Additional Information	
Column Info	

Chromatogram

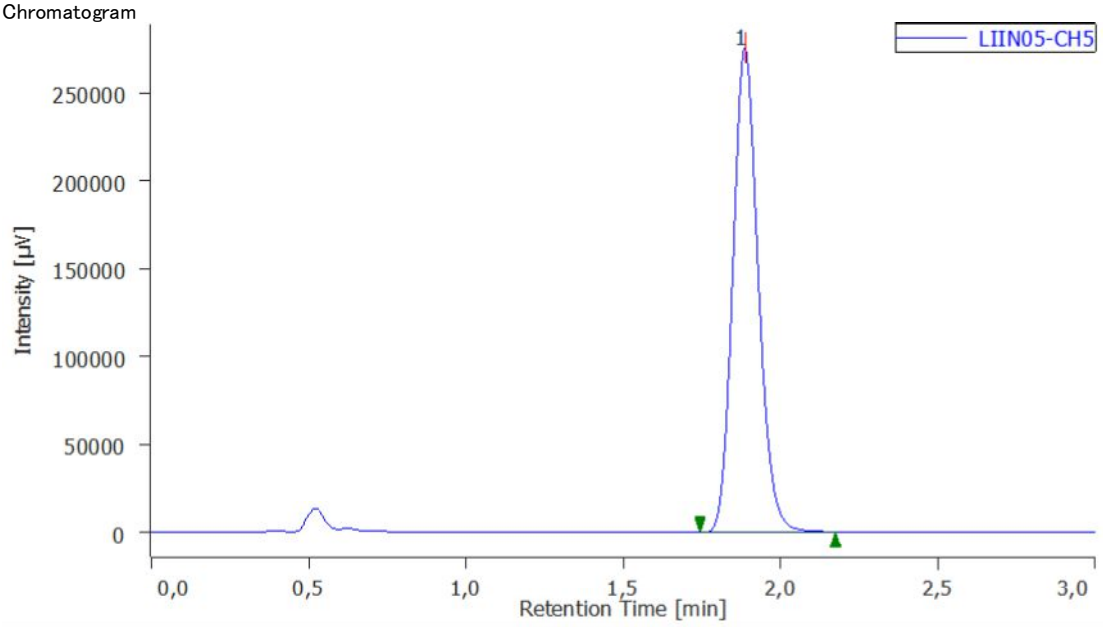


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	5	1,887	1537864	275002

Chromatogram Information	
User Name	Administrator
Date Modified	15/11/2018 14:59:22
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:41:21
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	Gradiente
Control Method	Grad AB
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	


Chromatogram

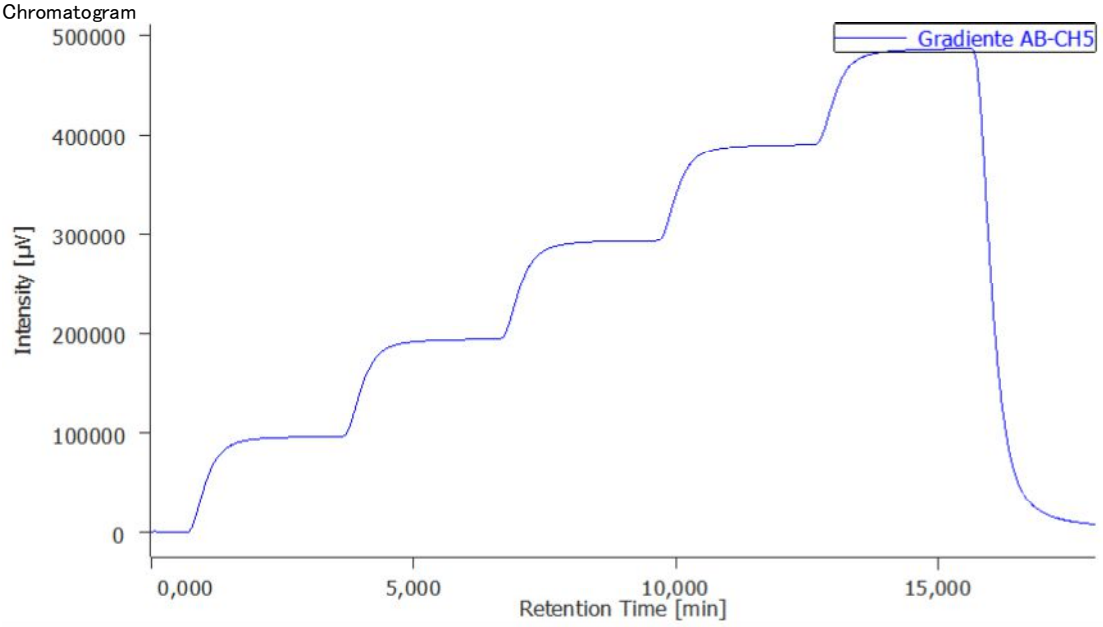

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	15/11/2018 15:14:34
Description	
HPLC System Name	JASCO HPLC
Injection Date	15/11/2018 14:59:33
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	15,0 [min]
Acquisition Sequence	Gradiente
Control Method	Grad CD
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

Chromatogram

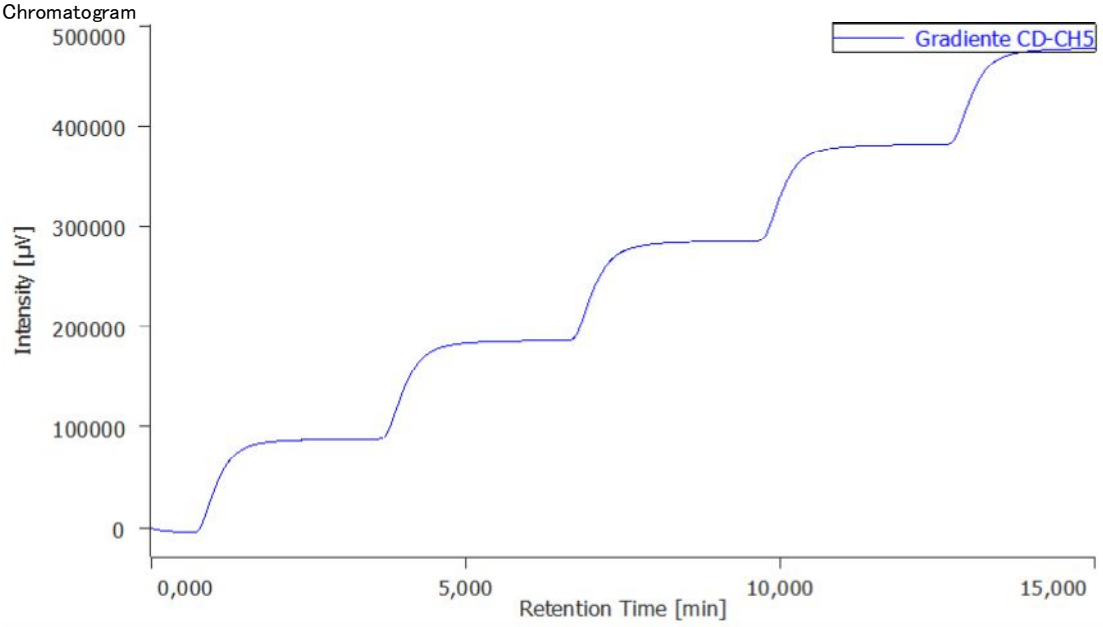

Peak Information – No data.