
Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:09:05
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:49:38
Volume	40,00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

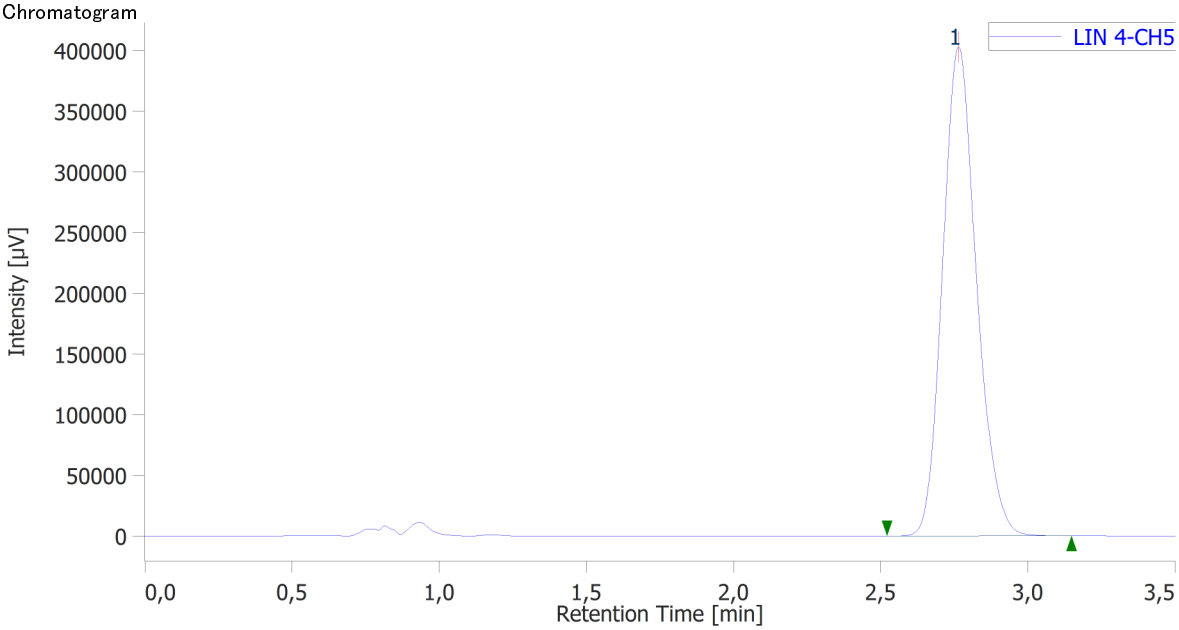

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,763	3215616	402822	2851	N/A	1,164

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:19:04
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 16:09:39
Volume	30.00 [µL]
Sample #	7
Project Name	JASCO
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LDUV_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

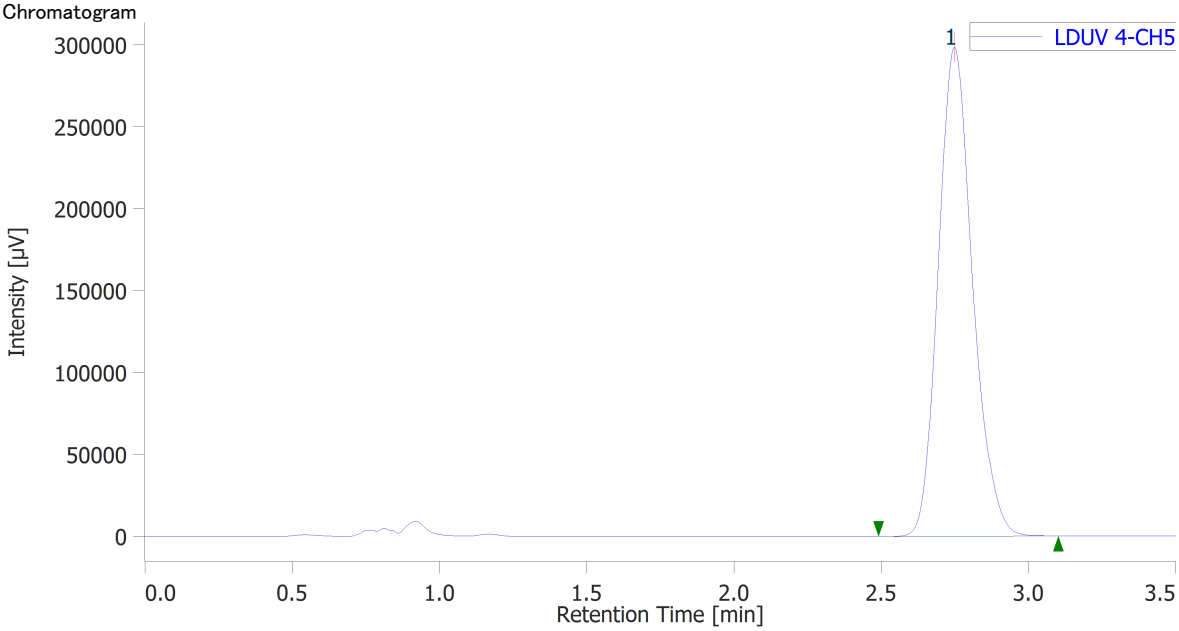

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2.747	2415286	298592	2761	N/A	1.184

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:19:03
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 16:05:47
Volume	30.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LDUV_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

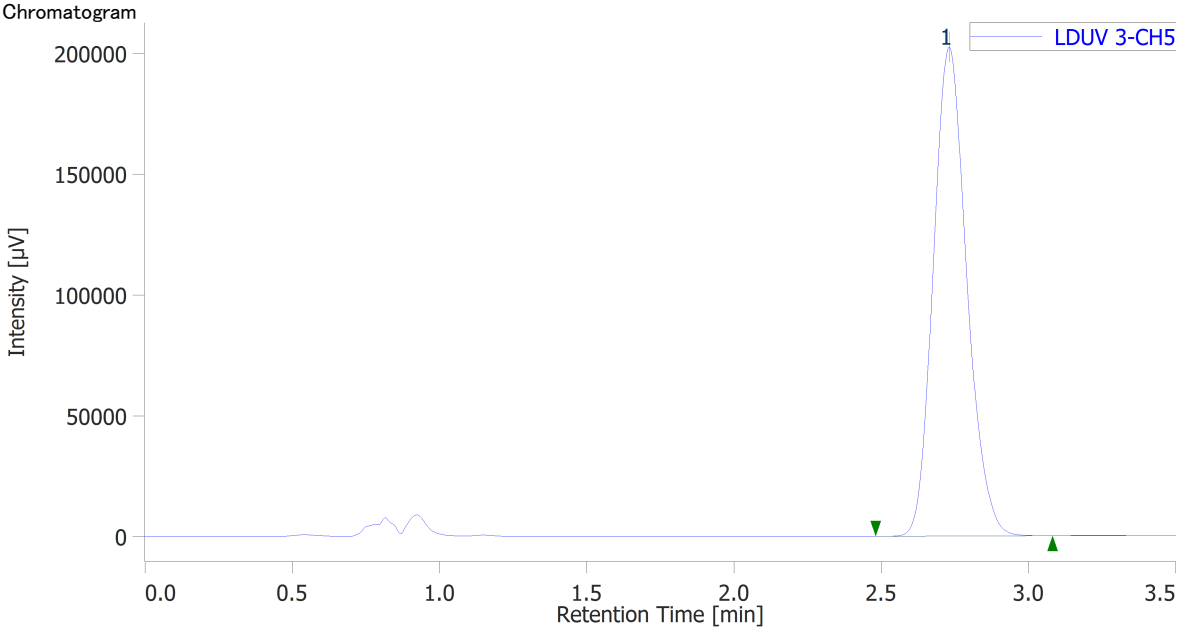

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2.730	1598717	202317	2810	N/A	1.155

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:22:10
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:18:38
Volume	30,00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

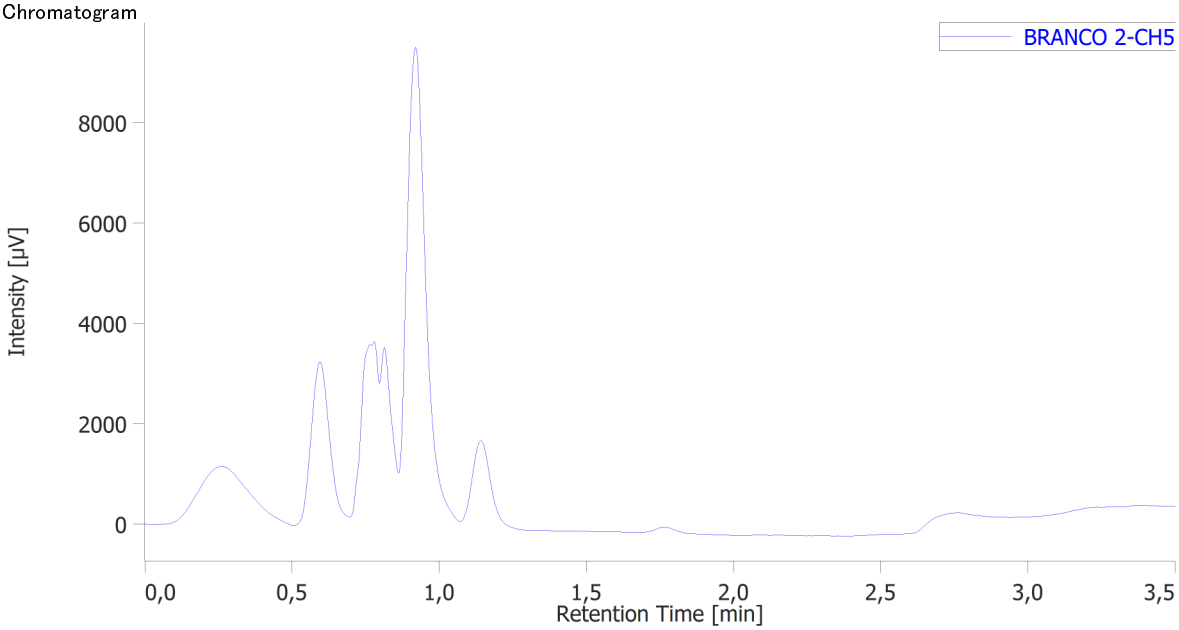


Peak Information - No data.

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:26:02
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:22:30
Volume	30,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

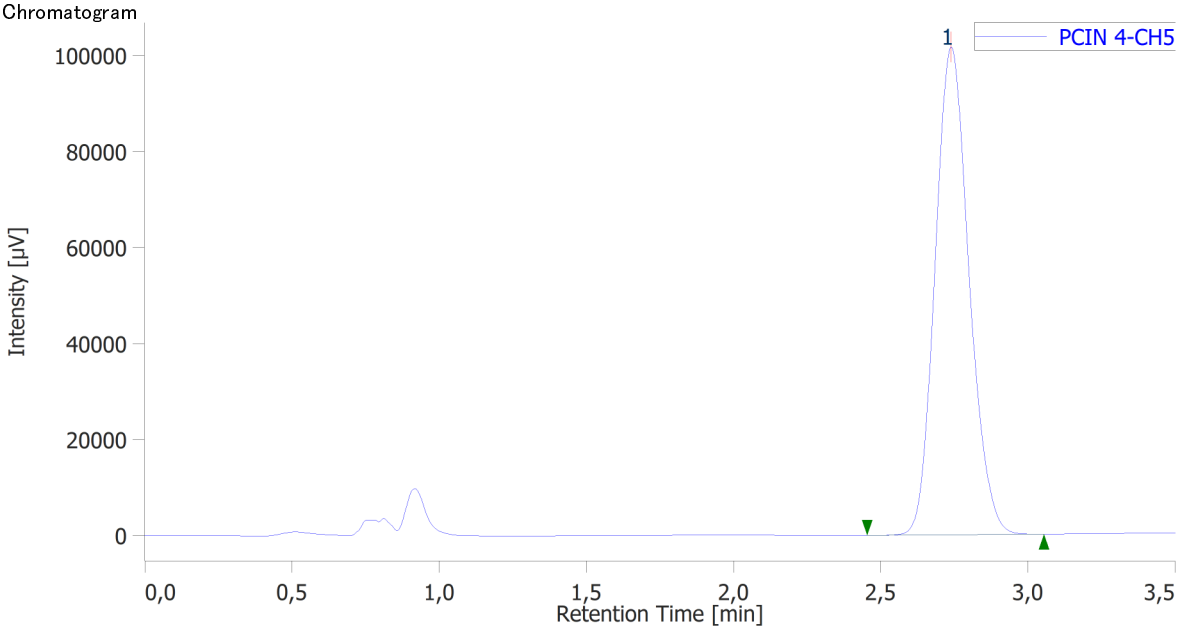

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,737	814422	101588	2717	N/A	1,157

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:19:03
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 16:01:55
Volume	30.00 [µL]
Sample #	5
Project Name	JASCO
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LDUV_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

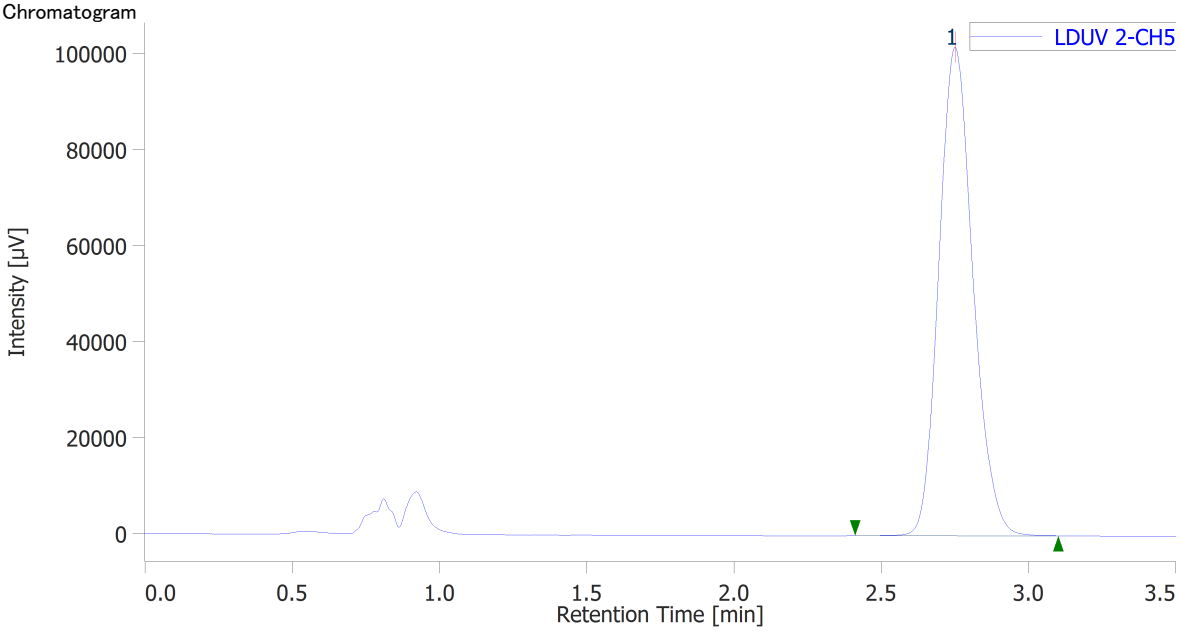

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2.750	817795	101752	2755	N/A	1.148

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:10:30
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:06:59
Volume	30,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

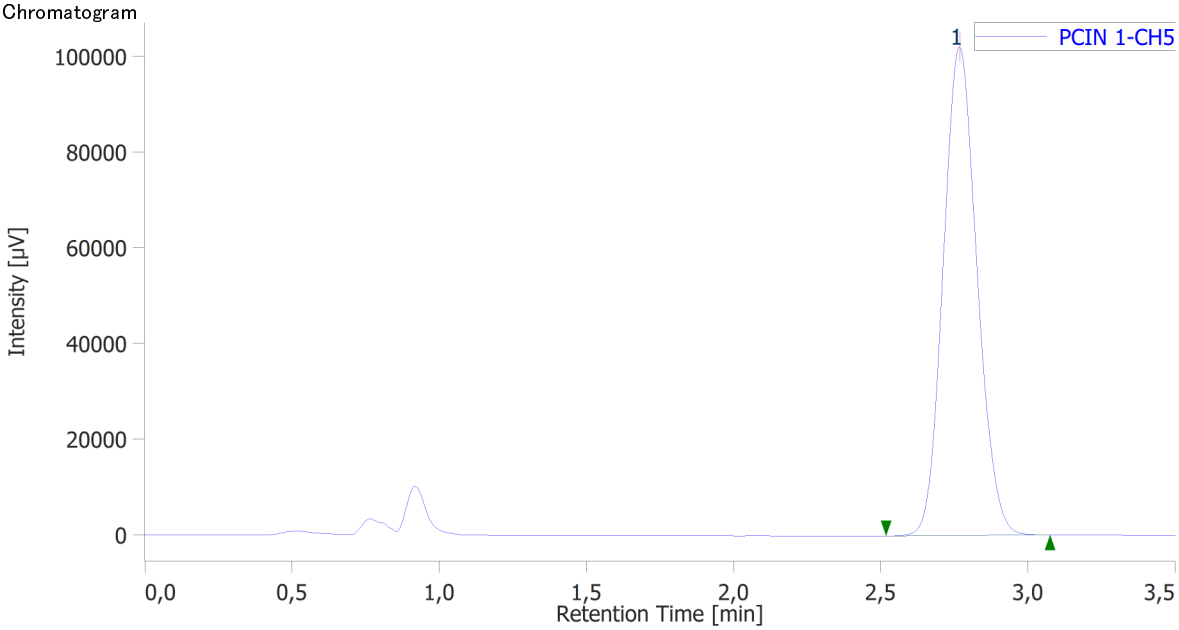

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,767	814533	102049	2775	N/A	1,108

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:09:03
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:41:31
Volume	20,00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

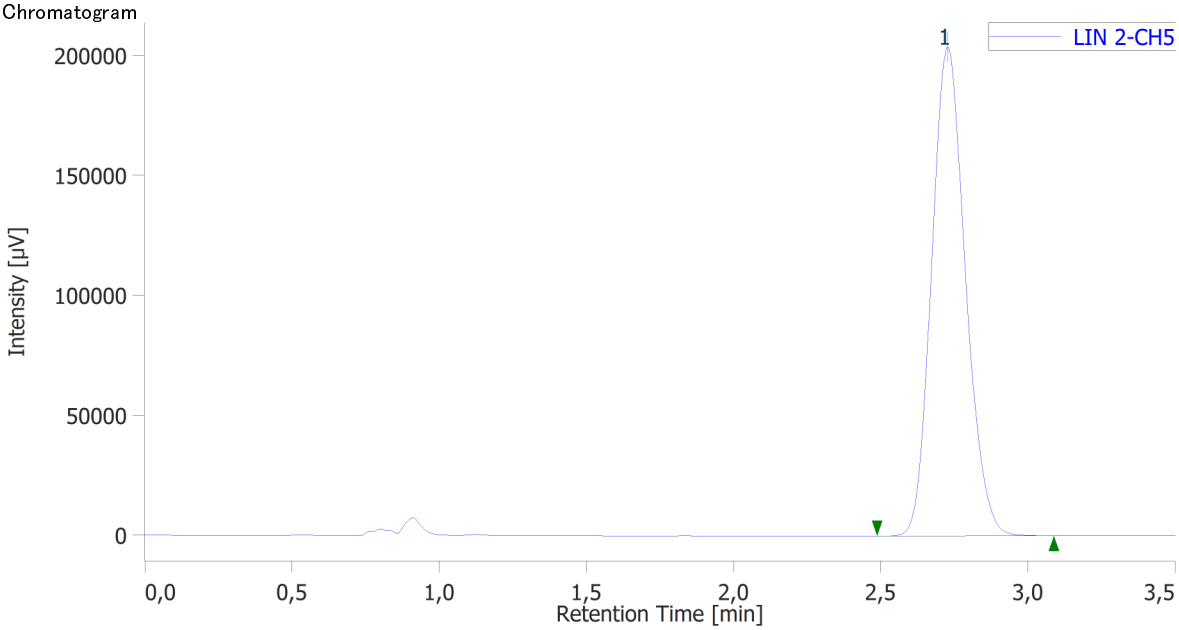


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,727	1625017	203824	2724	N/A	1,140

Creator Administrator
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	06/02/2018 18:33:19
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 18:14:30
Volume	0,00 [µL]
Sample #	-
Project Name	JASCO
Acquisition Time	18,8 [min]
Acquisition Sequence	
Control Method	Qualificação GRO A-B_20180206
Peak ID Table	

Chromatogram

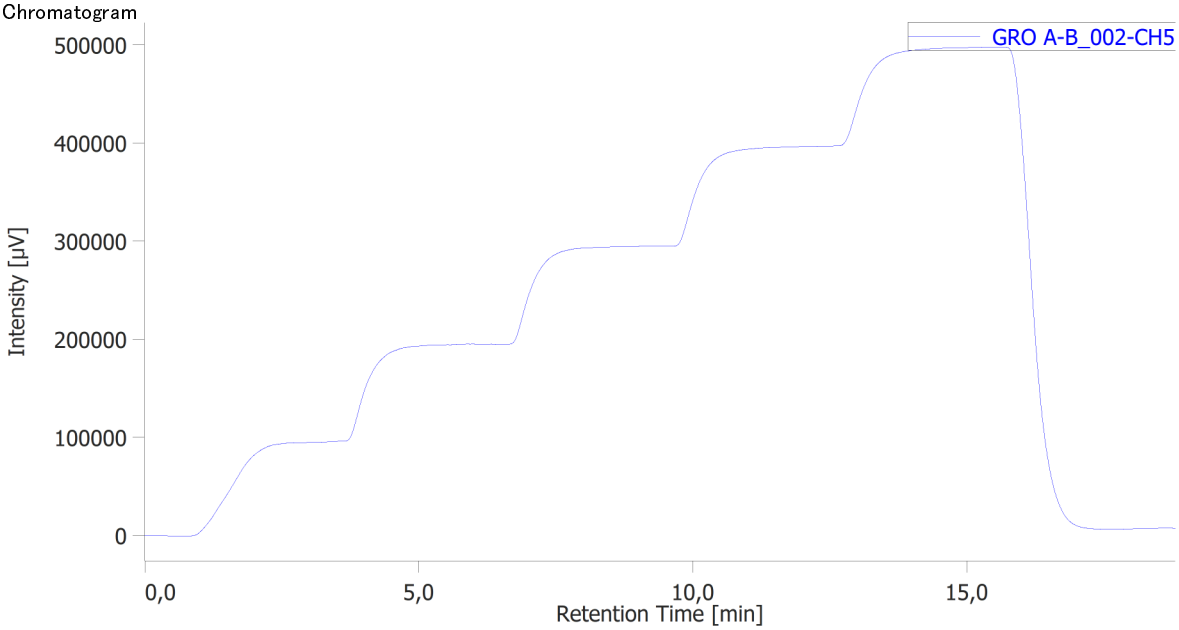


Peak Information - No data.

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:37:38
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:34:07
Volume	30,00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

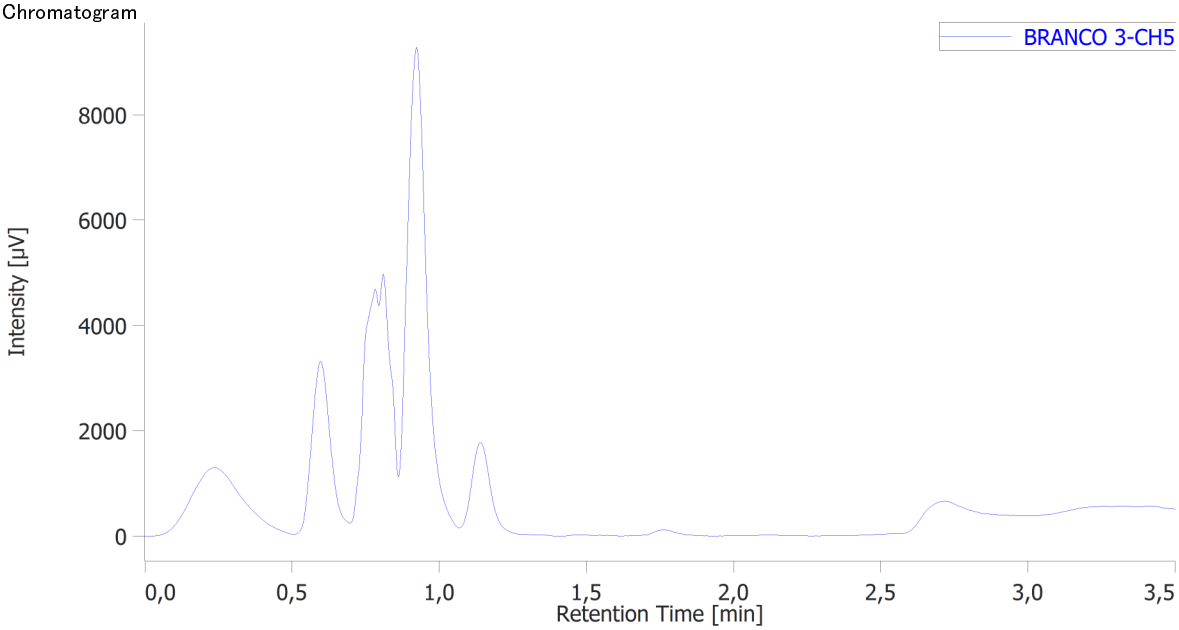


Peak Information - No data.

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:09:05
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:49:38
Volume	40,00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

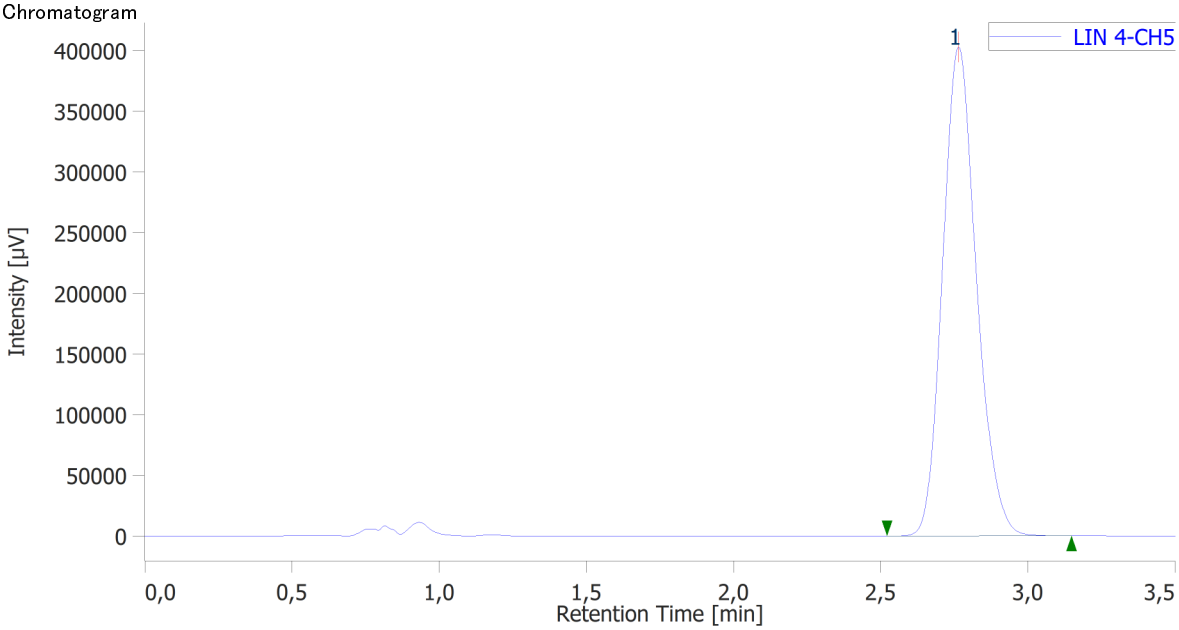

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,763	3215616	402822	2851	N/A	1,164

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:19:04
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 16:13:30
Volume	30.00 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LDUV_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

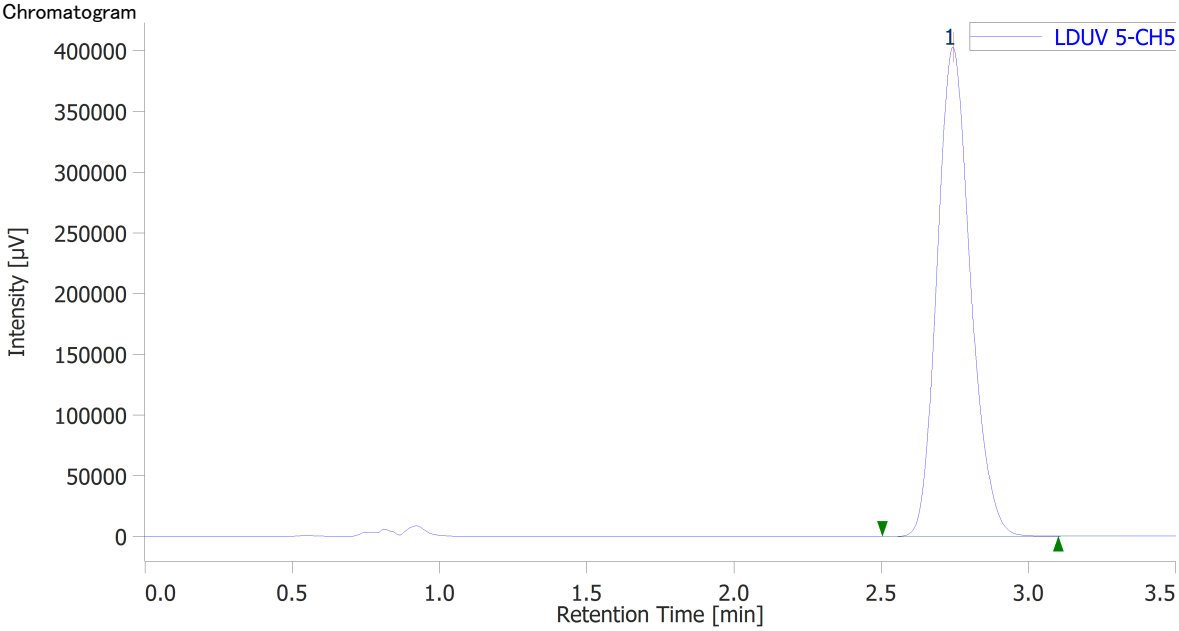

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2.743	3176306	402975	2874	N/A	1.153

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:09:04
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:45:24
Volume	30,00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

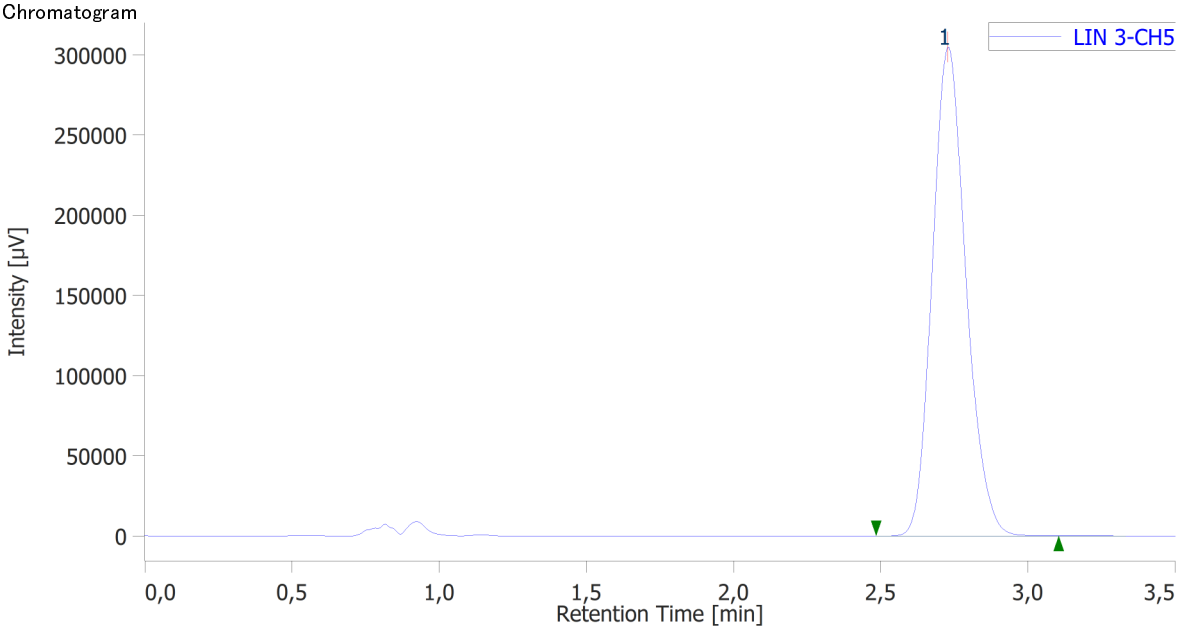

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,727	2425013	304942	2788	N/A	1,178

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:06:38
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:03:06
Volume	30,00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206


Chromatogram

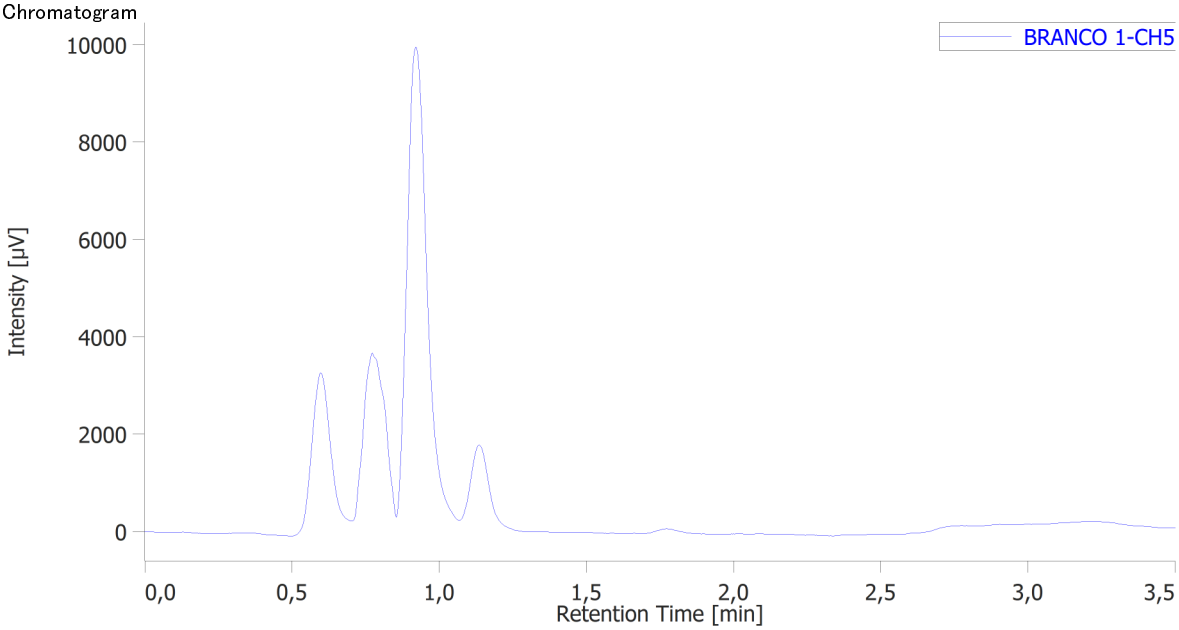

Peak Information - No data.

Creator
Reviewer
Approver

Peak Find - EDUV PDA_tR2,81 D.jws

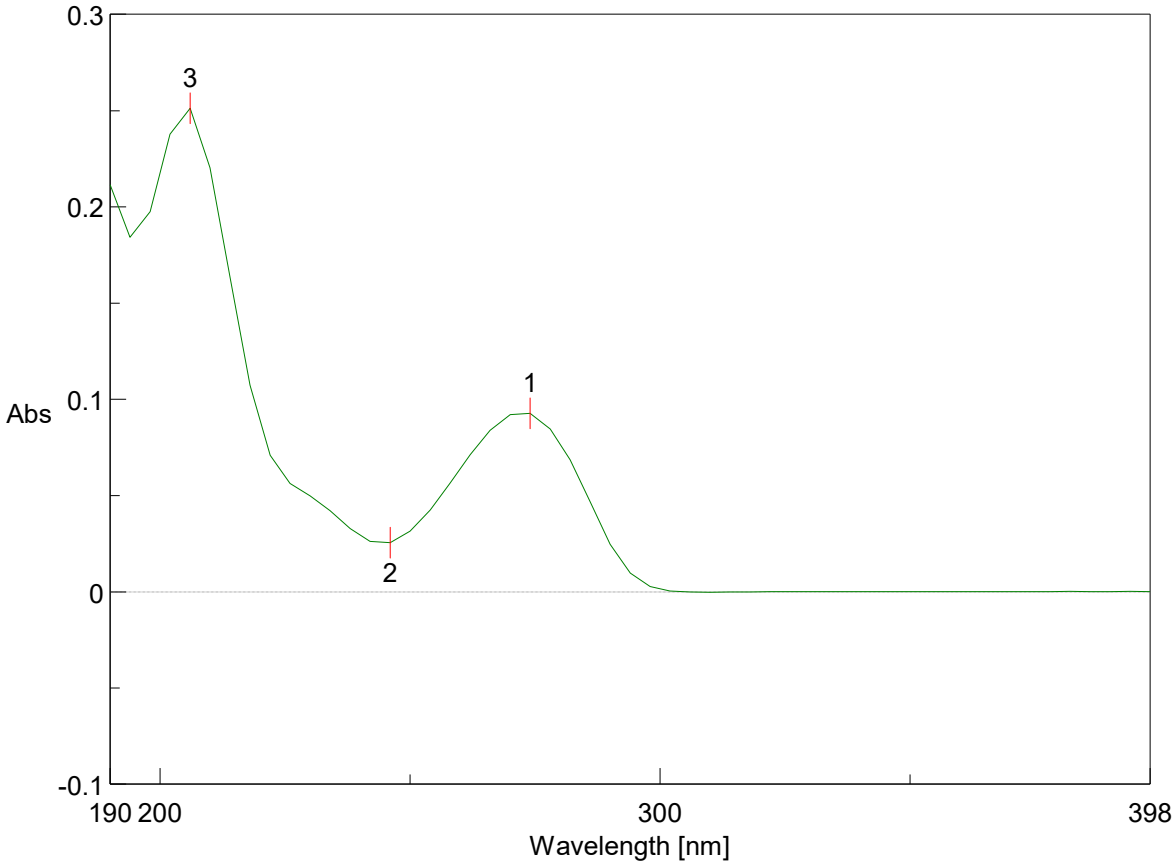

[Comments]

User	Administrator
Division	---
Company	DFL
Creation date	06/02/2018 14:27

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	190 nm
End	398 nm
Data interval	4 nm
Data points	53

[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A025161665
ROM version	1.02.02


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.092609	2	246	0.025412
3	206	0.251025			

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:33:46
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:30:15
Volume	30,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

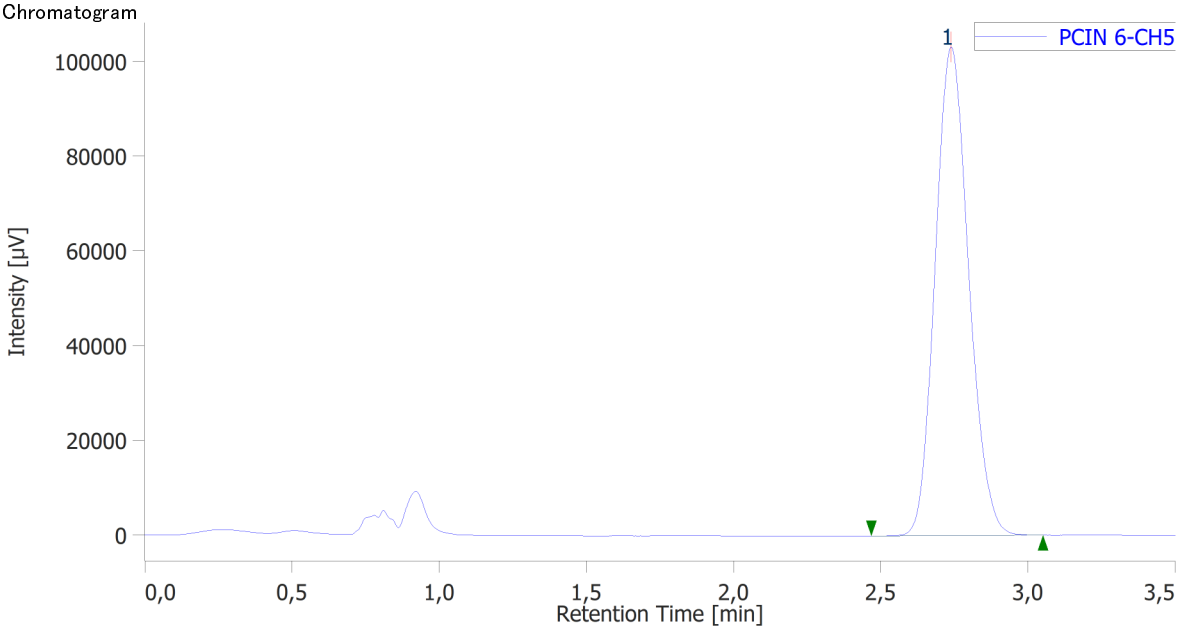

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,737	816821	103114	2757	N/A	1,149

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:18:16
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:14:44
Volume	30,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

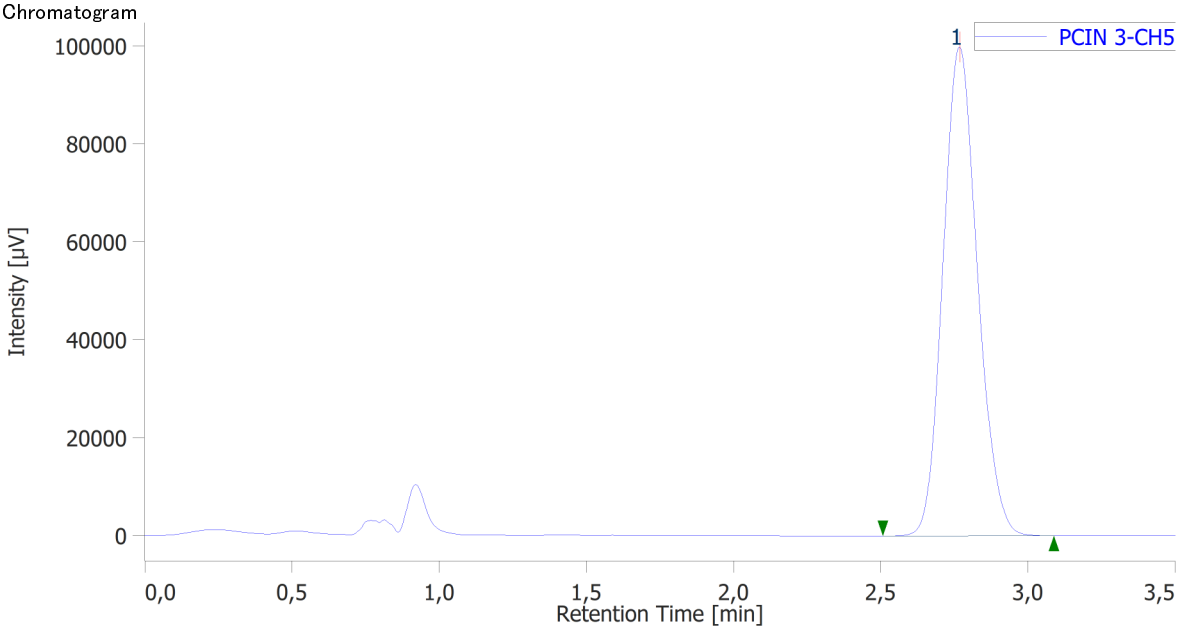

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,767	813697	99778	2693	N/A	1,130

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:14:22
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:10:51
Volume	30,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

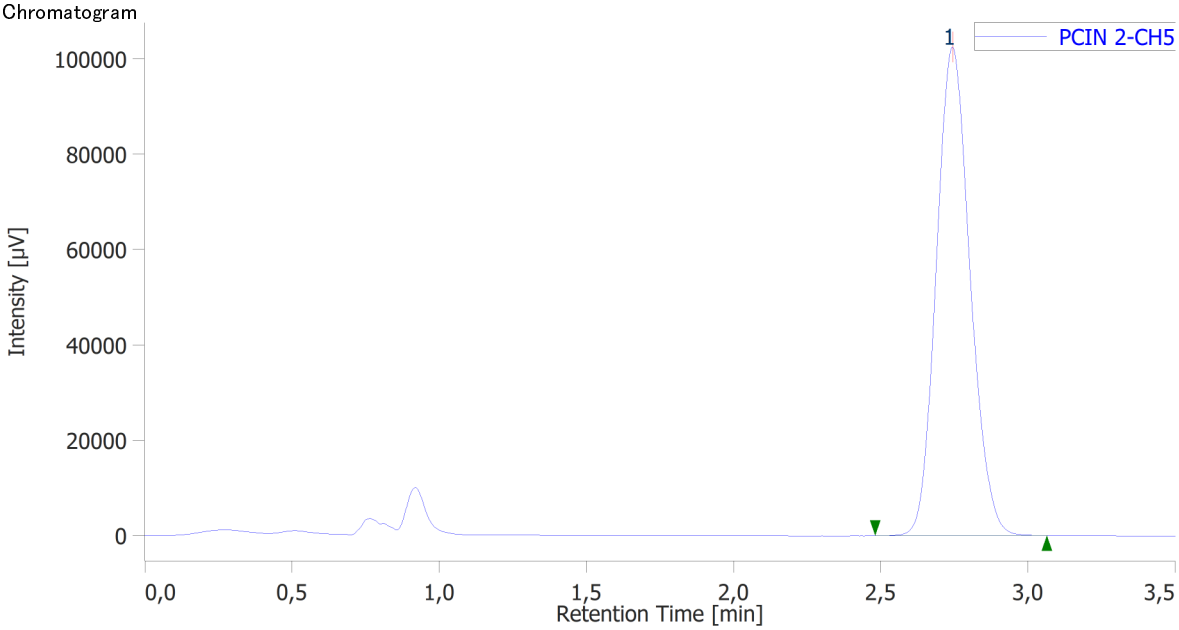

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,743	816436	102486	2754	N/A	1,117

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:19:04
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 16:13:30
Volume	30.00 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LDUV_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

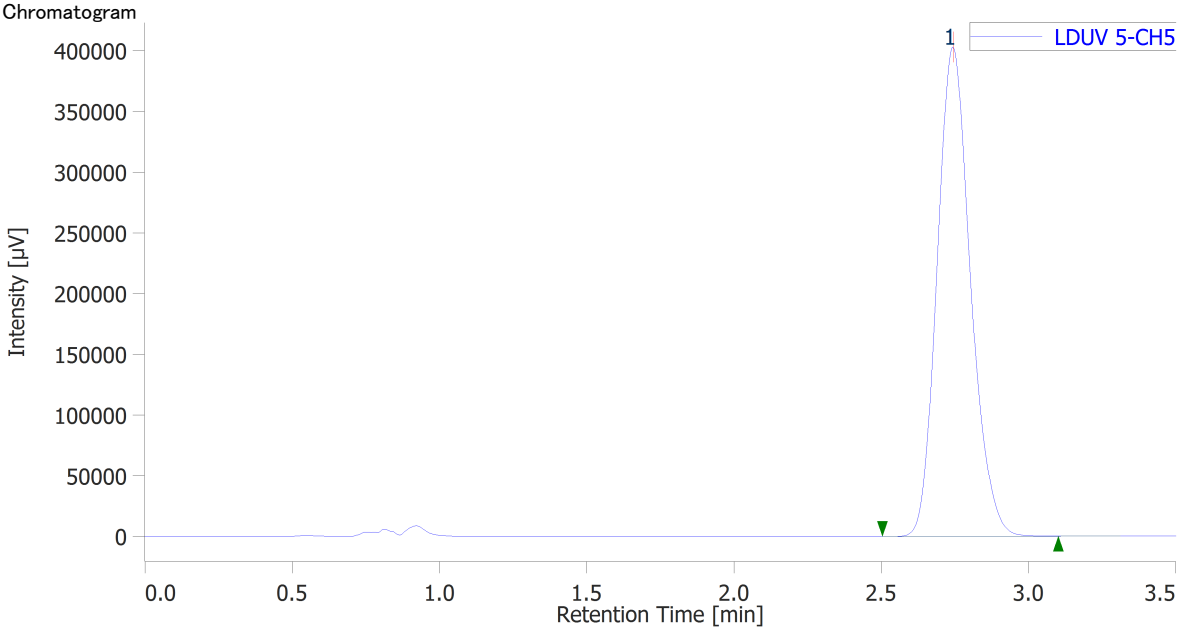

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2.743	3176306	402975	2874	N/A	1.153

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 15:29:54
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:26:22
Volume	30,00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação PCIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

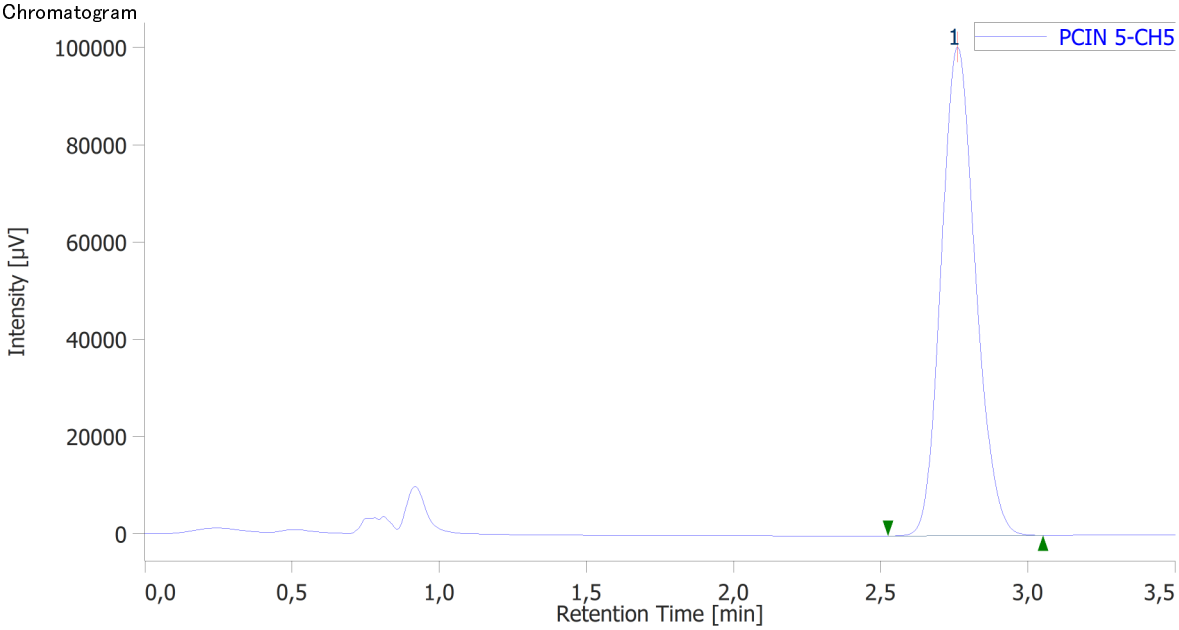

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,760	813120	100478	2711	N/A	1,137

Creator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 16:09:03
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 15:37:49
Volume	10,00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,5 [min]
Acquisition Sequence	Qualificação_20180206
Control Method	Qualificação LIN_20180206
Peak ID Table	Peak ID Table_20180206

Chromatogram

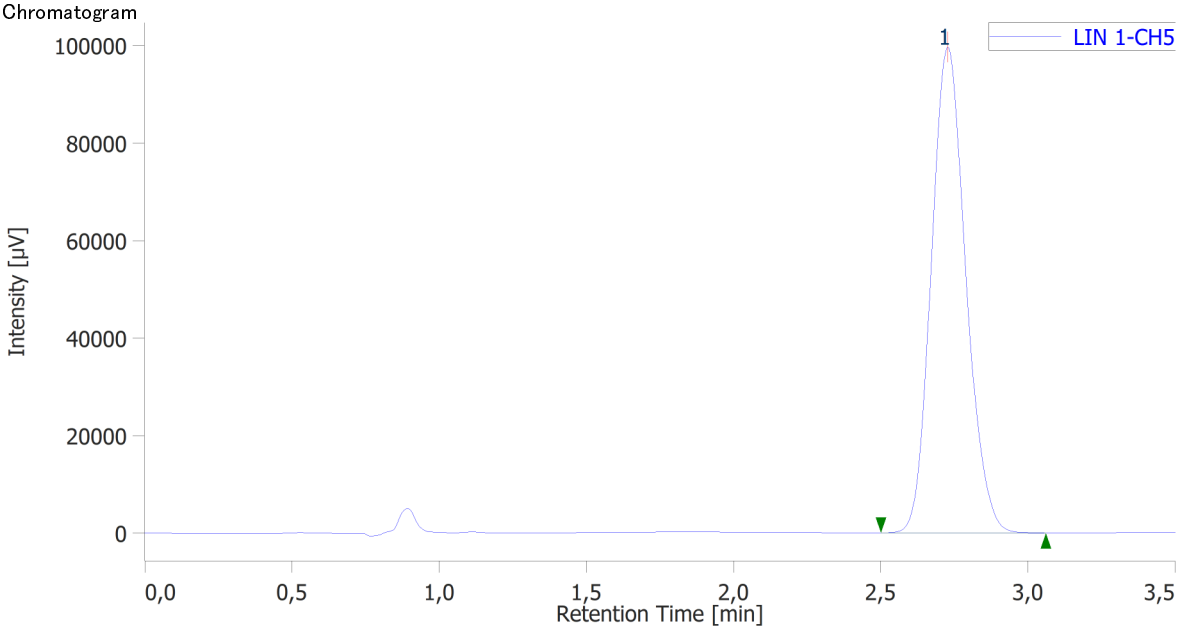

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	NTP	Resolution	Symmetry Factor
1	STD	5	2,727	812370	99669	2618	N/A	1,137

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	06/02/2018 19:12:26
Description	
HPLC System Name	RHPLC - PDA
Injection Date	06/02/2018 18:53:37
Volume	0,00 [µL]
Sample #	-
Project Name	JASCO
Acquisition Time	18,8 [min]
Acquisition Sequence	
Control Method	Qualificação GRO C-D_20180206
Peak ID Table	

Chromatogram

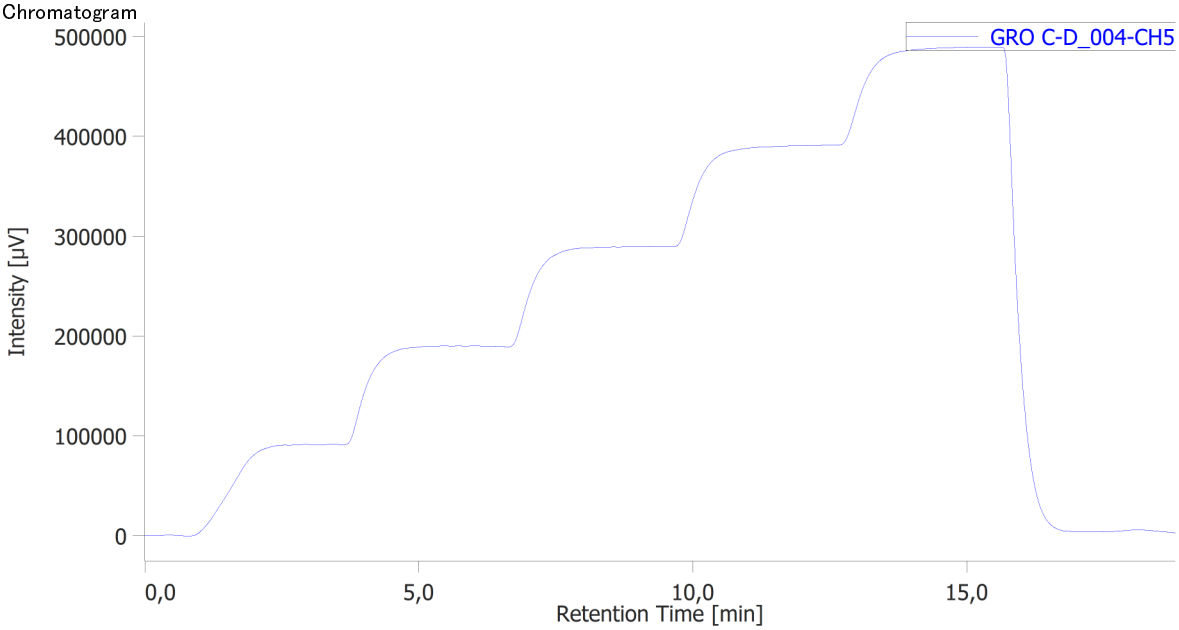

Peak Information - No data.

Creator Administrator
Reviewer
Approver