
Peak Find - EDUV.jws

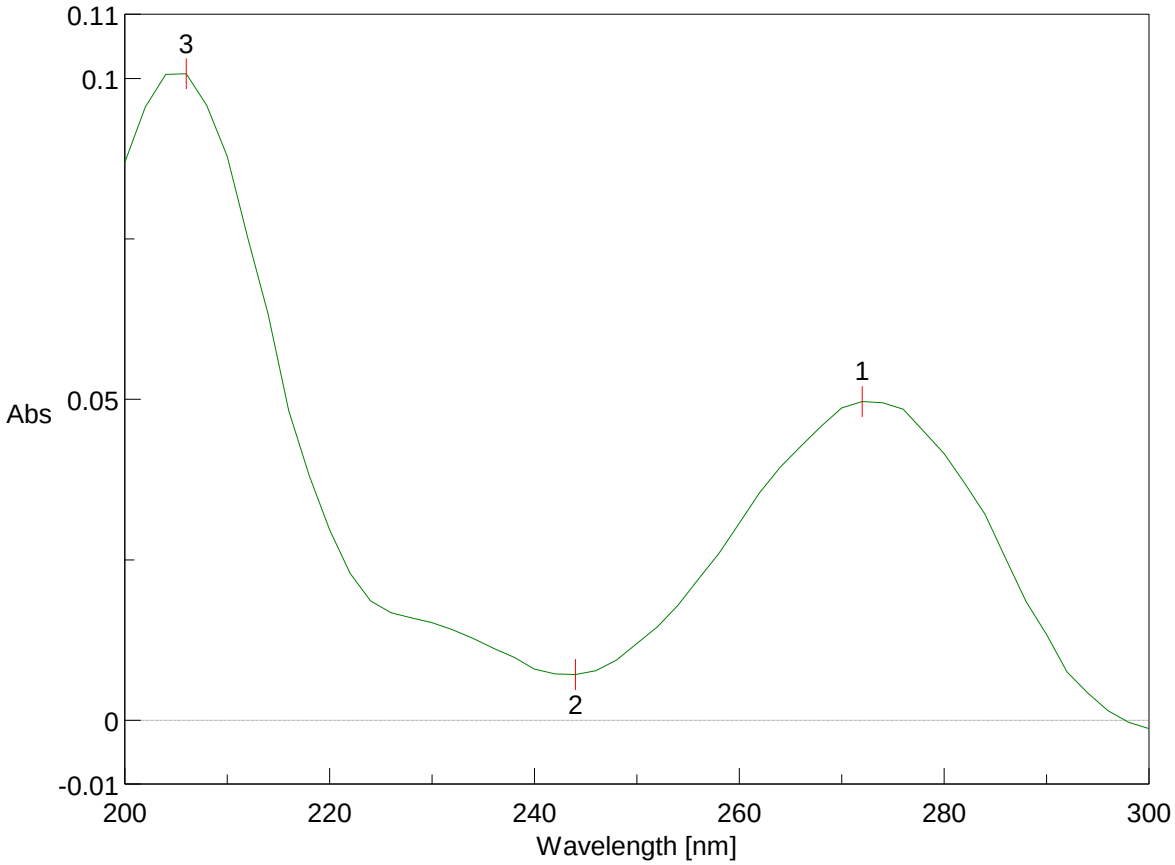

[Comments]

User	Administrator
Division	---
Company	TRB
Creation date	10/12/2019 10:41
Date modified	10/12/2019 10:41

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.0496075	2	244	0.00704396
3	206	0.100705			

Chromatogram

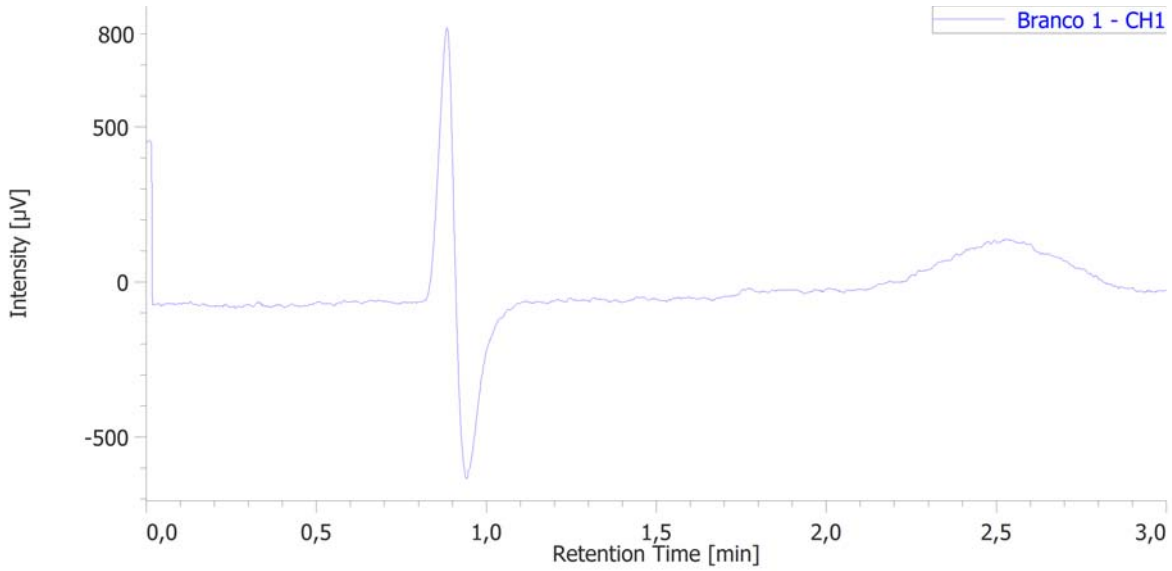


Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:41
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 15:54:53
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

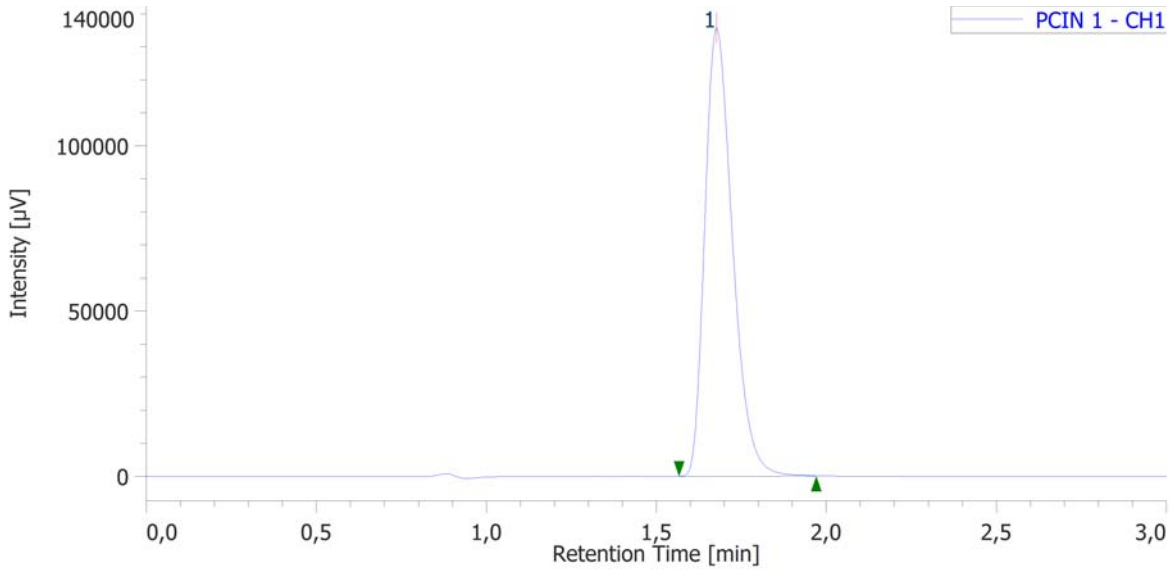

Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:42
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 15:58:16
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,677	767637	135596	100,000	100,000	N/A	2060	N/A	1,352	

Creator Administrator
Reviewer
Approver

Chromatogram

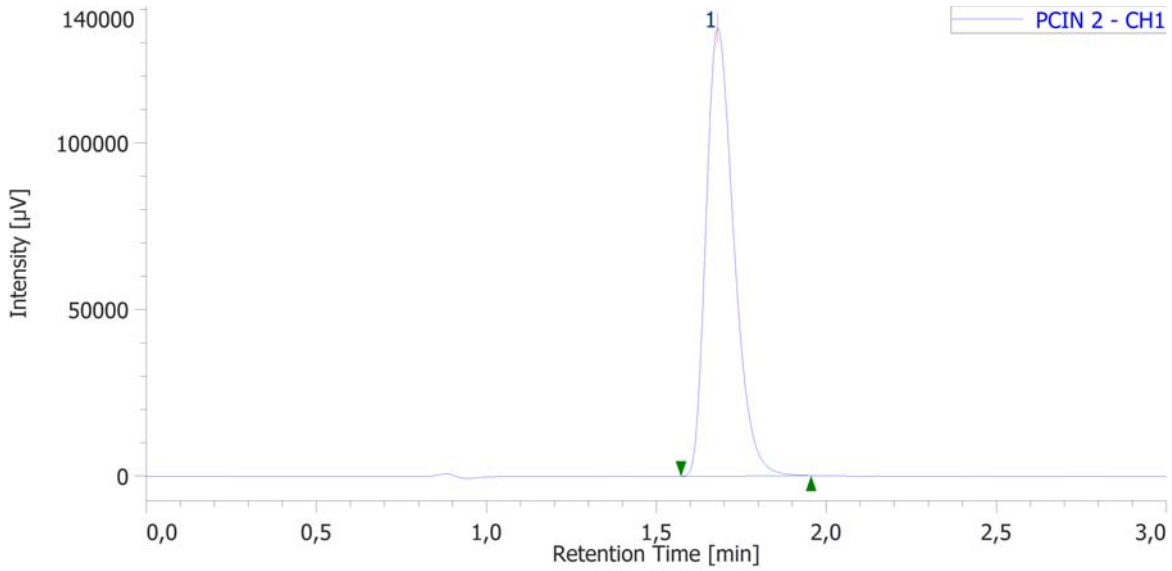

Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:42
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 16:01:36
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,680	765828	134462	100,000	100,000	N/A	2037	N/A	1,359	

Creator Administrator
Reviewer
Approver

Chromatogram

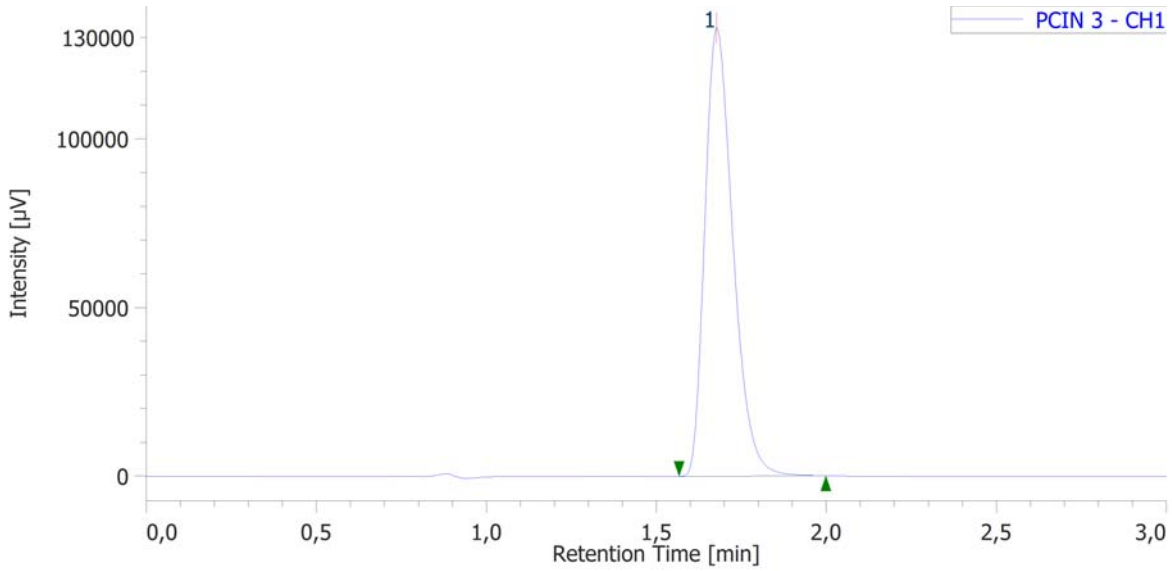

Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:42
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 16:04:56
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,677	763419	132808	100,000	100,000	N/A	2010	N/A	1,366	

Creator Administrator
Reviewer
Approver

Chromatogram

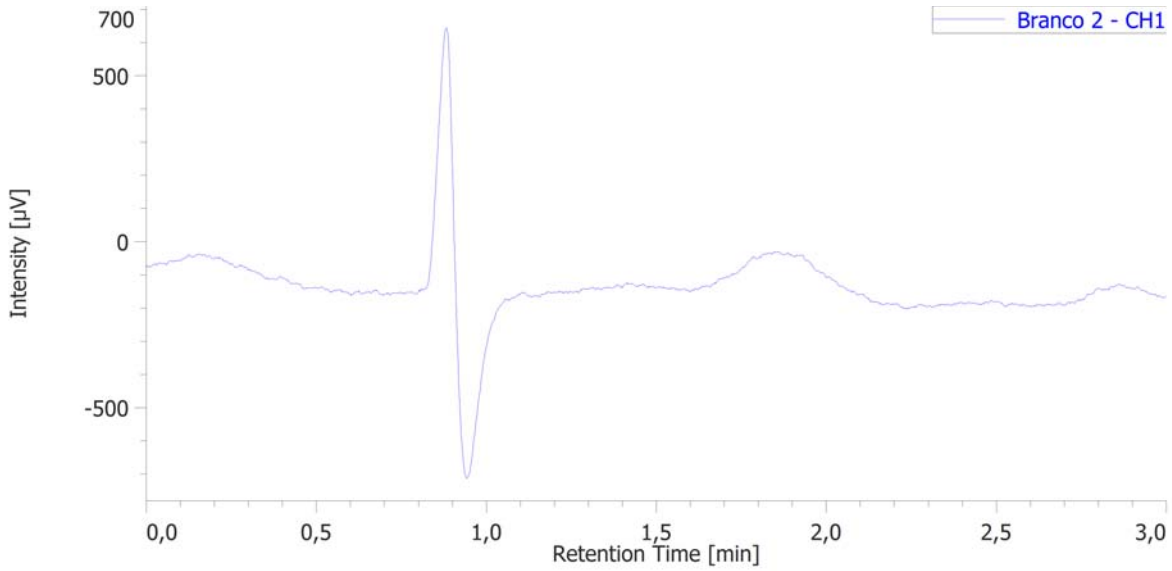


Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:43
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 16:08:16
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

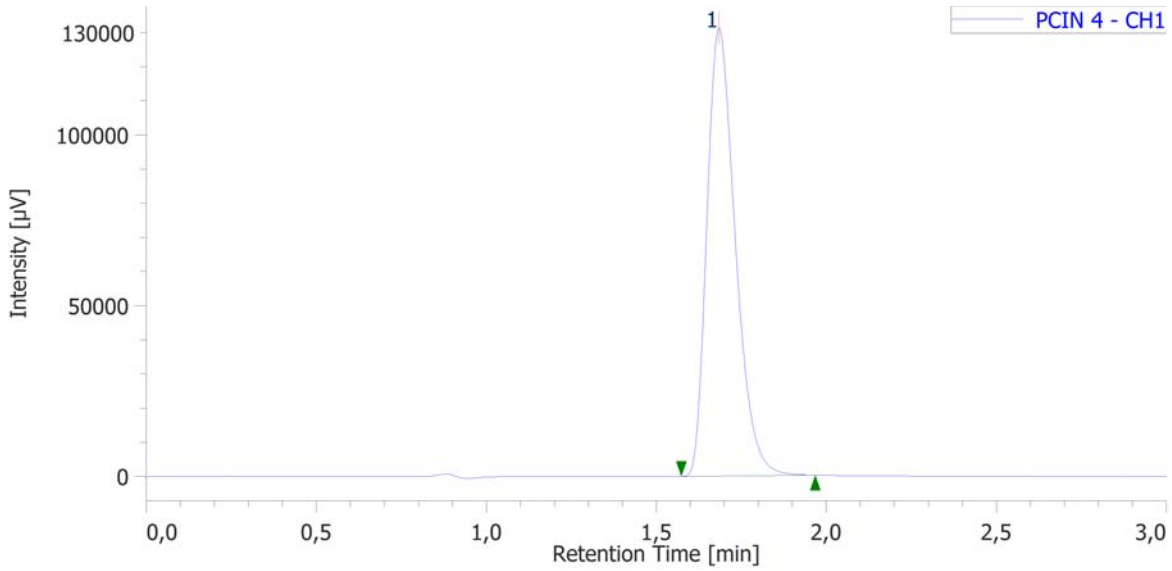

Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:43
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 16:11:36
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,683	763124	131193	100,000	100,000	N/A	1961	N/A	1,360	

Creator Administrator
Reviewer
Approver

Chromatogram

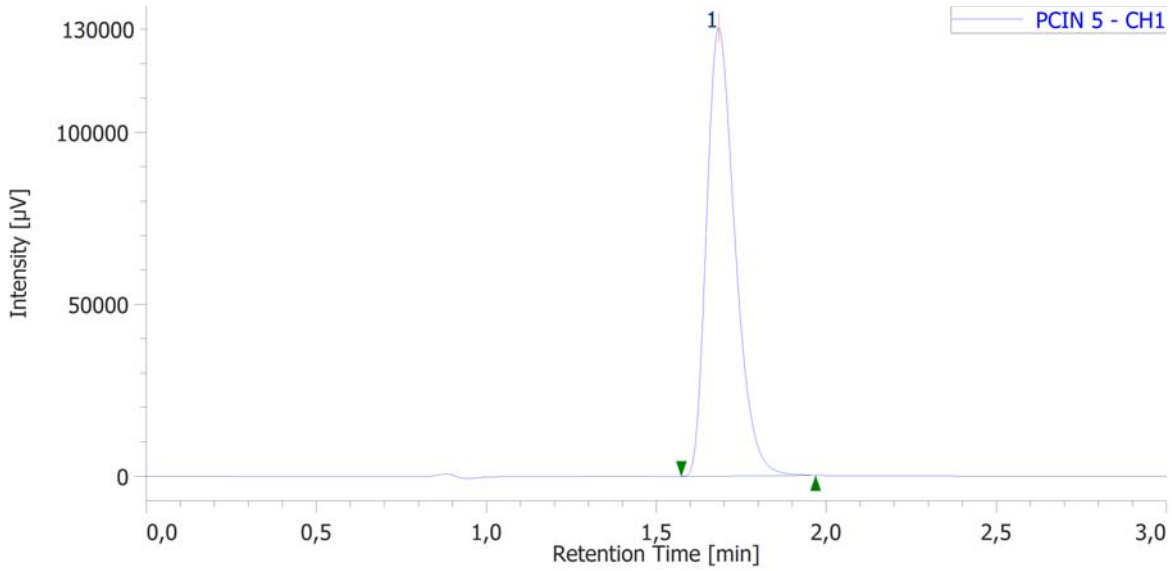

Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:44
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 16:14:58
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,683	759610	130286	100,000	100,000	N/A	1955	N/A	1,344	

Creator Administrator
Reviewer
Approver

Chromatogram

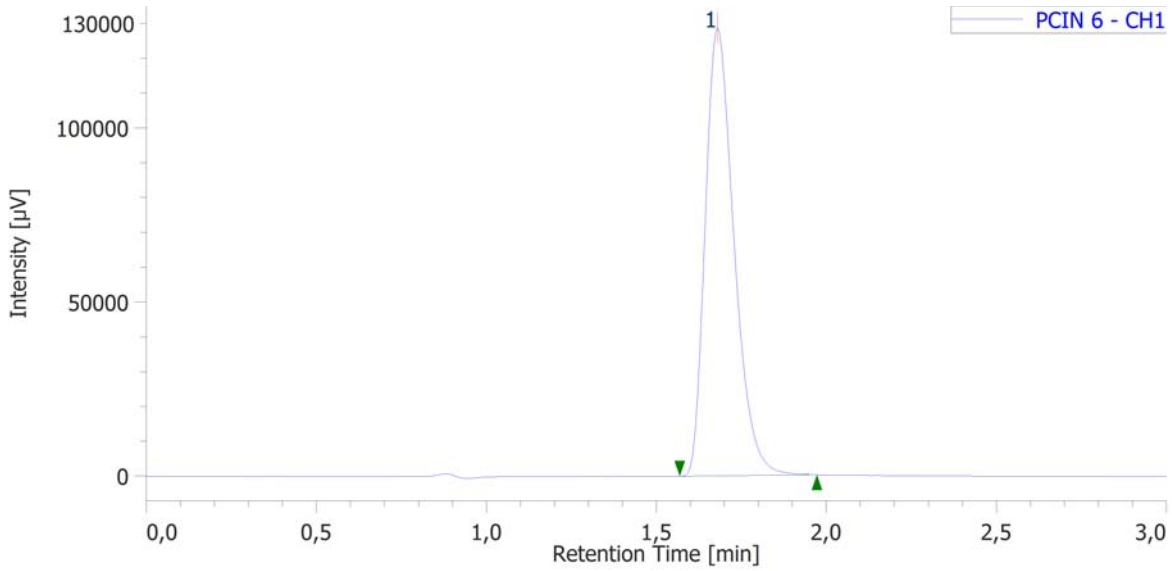

Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:44
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 16:18:21
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,680	757289	128580	100,000	100,000	N/A	1918	N/A	1,346	

Creator Administrator
Reviewer
Approver

Chromatogram

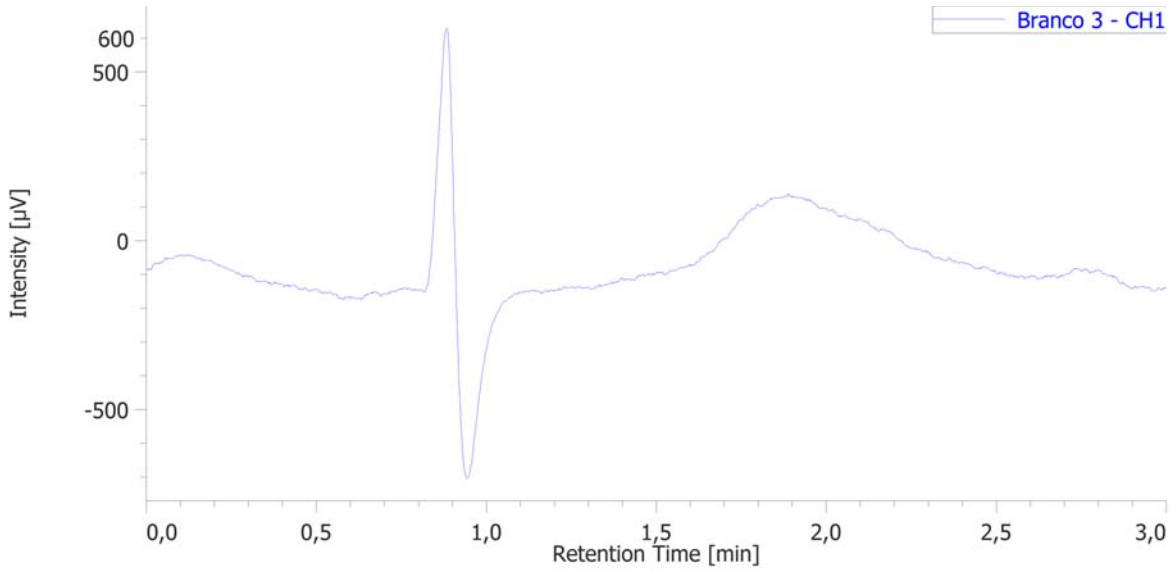


Chromatogram Information	
User Name	Administrator
Date Modified	09/12/2019 16:25:45
Description	
HPLC System Name	01-HP-02
Injection Date	09/12/2019 16:21:41
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

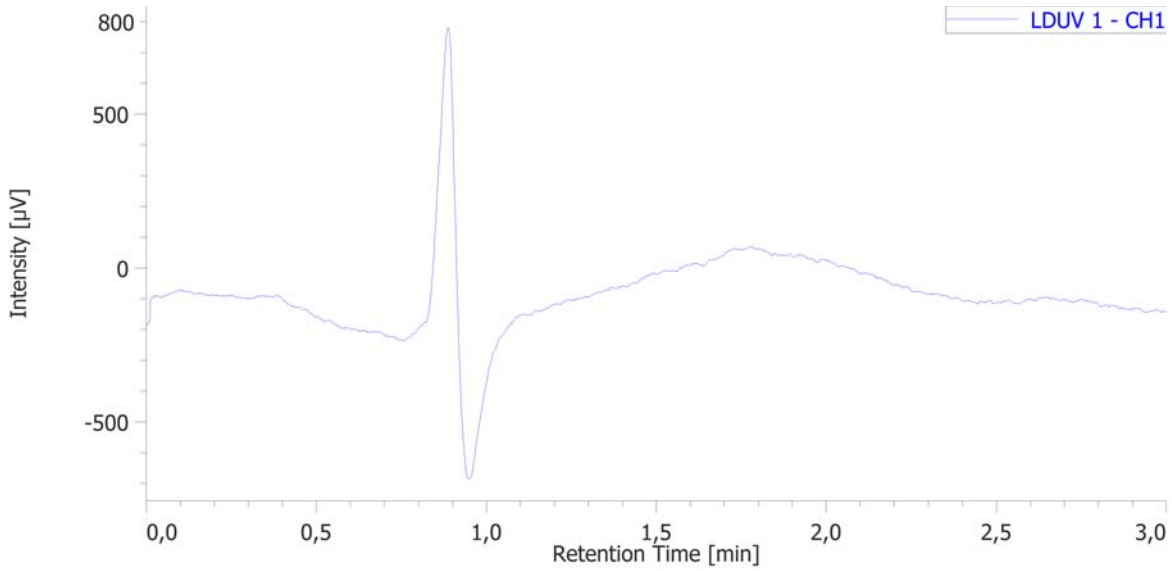


Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:23:28
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:03:31
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

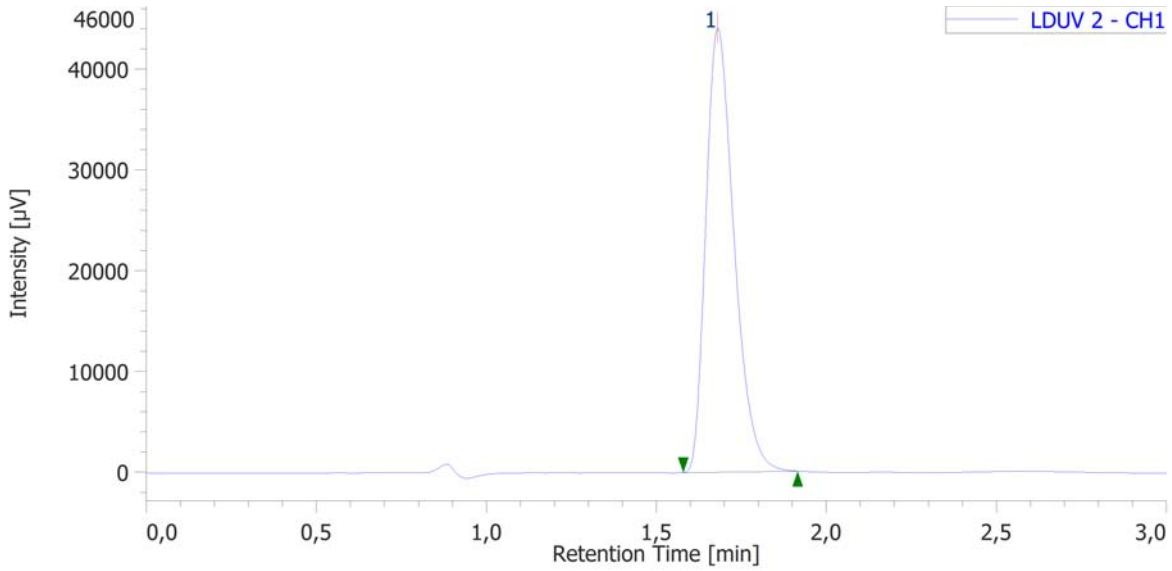

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:23:29
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:06:53
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,680	254193	44042	100,000	100,000	N/A	1990	N/A	1,375	

Creator Administrator
Reviewer
Approver

Chromatogram

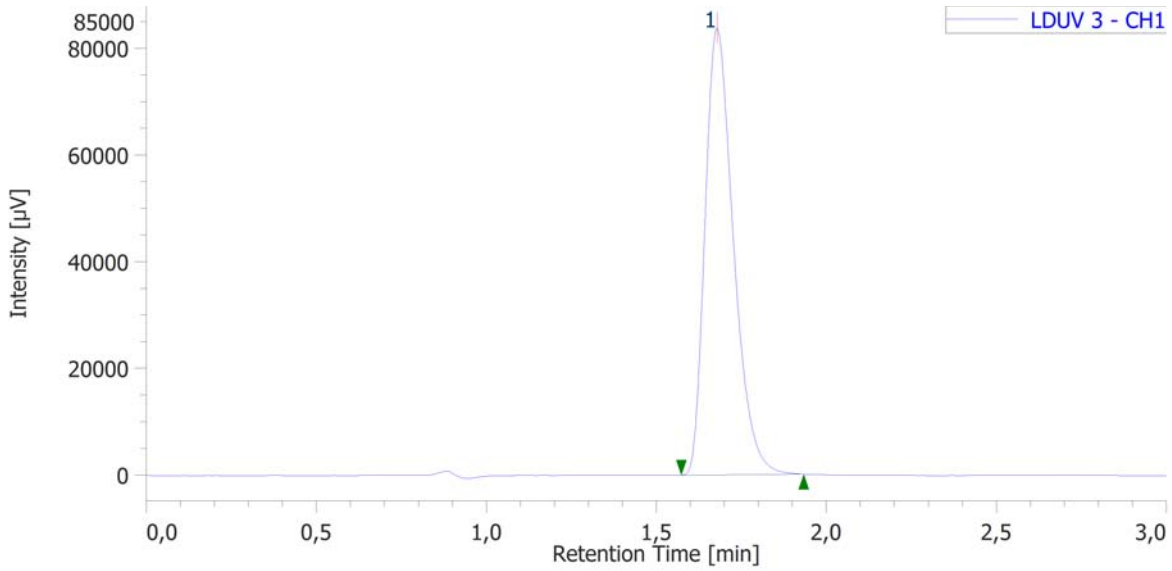

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:23:29
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:10:16
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,678	486226	83726	100,000	100,000	N/A	1961	N/A	1,371	

Creator Administrator
Reviewer
Approver

Chromatogram

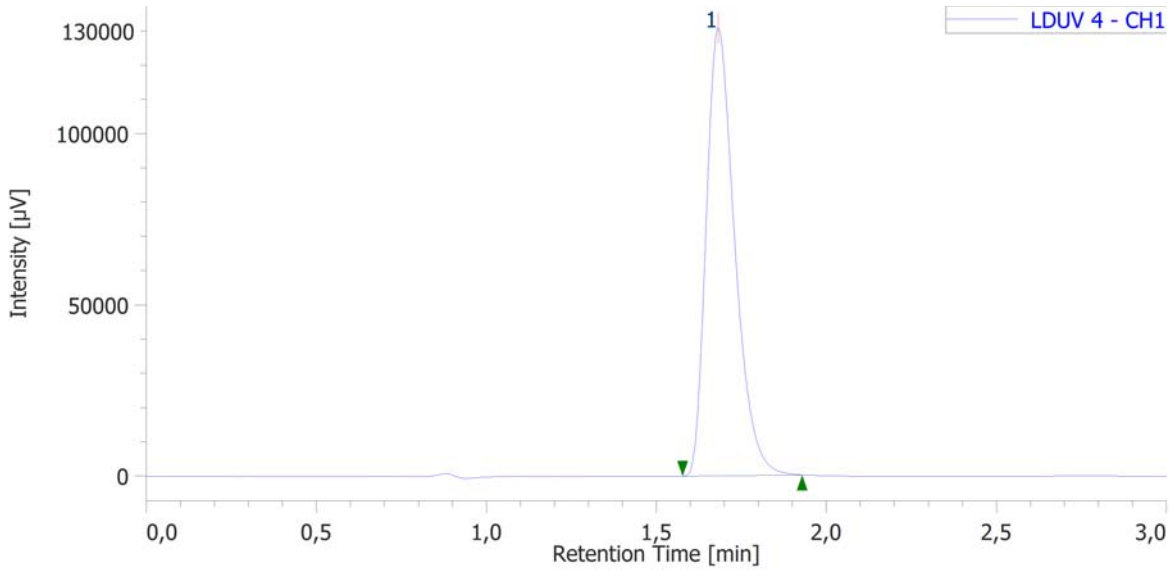

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:23:30
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:13:38
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,682	762410	130721	100,000	100,000	N/A	1967	N/A	1,380	

Creator Administrator
Reviewer
Approver

Chromatogram

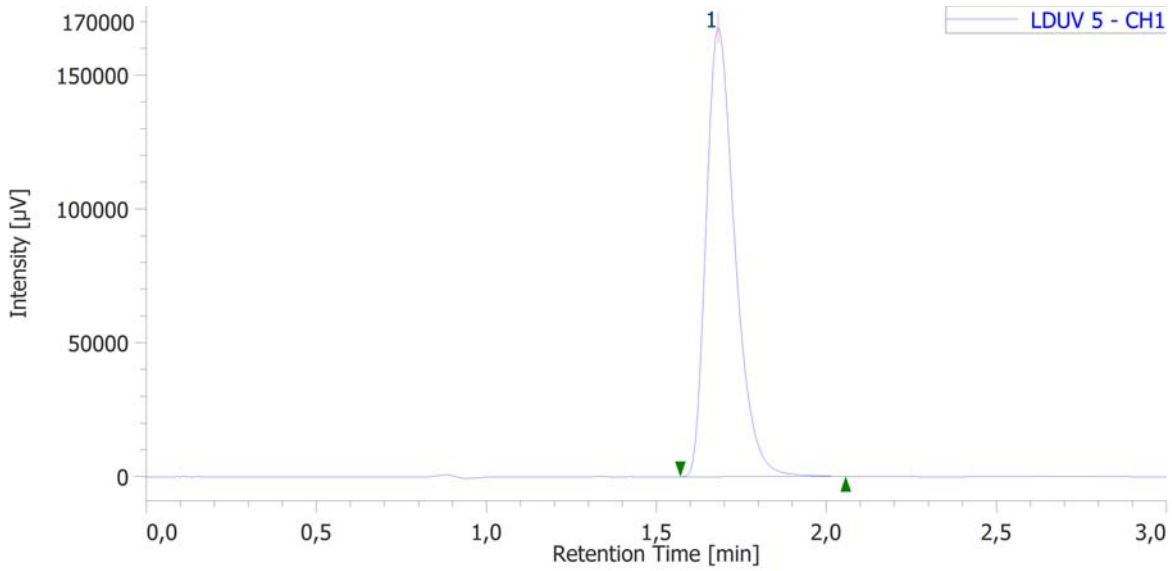

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:23:30
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:17:03
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,682	987072	167571	100,000	100,000	N/A	1955	N/A	1,390	

Creator Administrator
Reviewer
Approver

Chromatogram

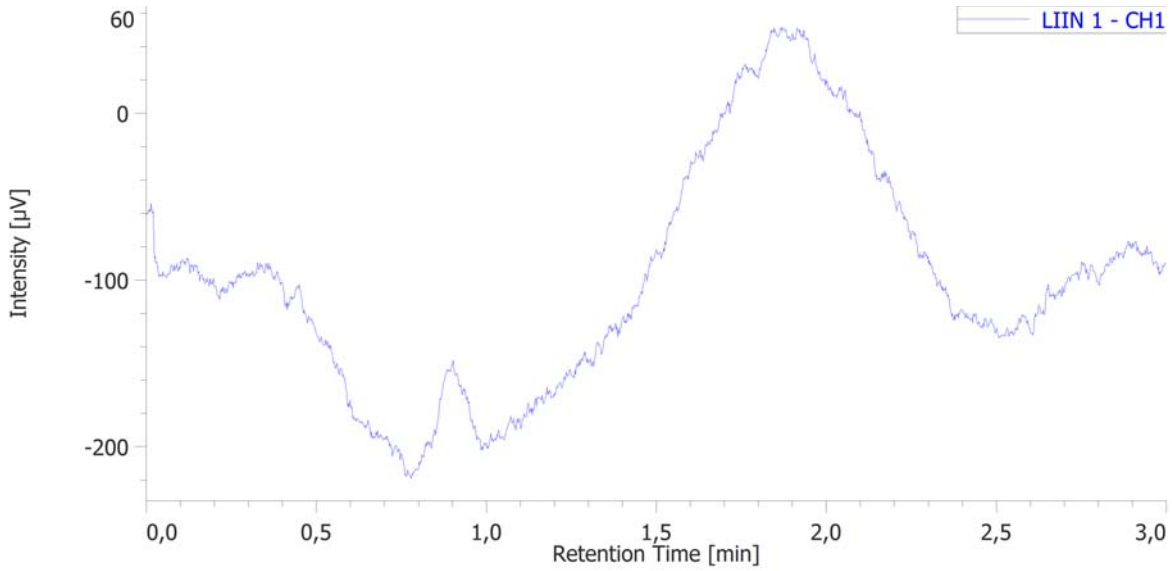


Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:48:04
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:26:57
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

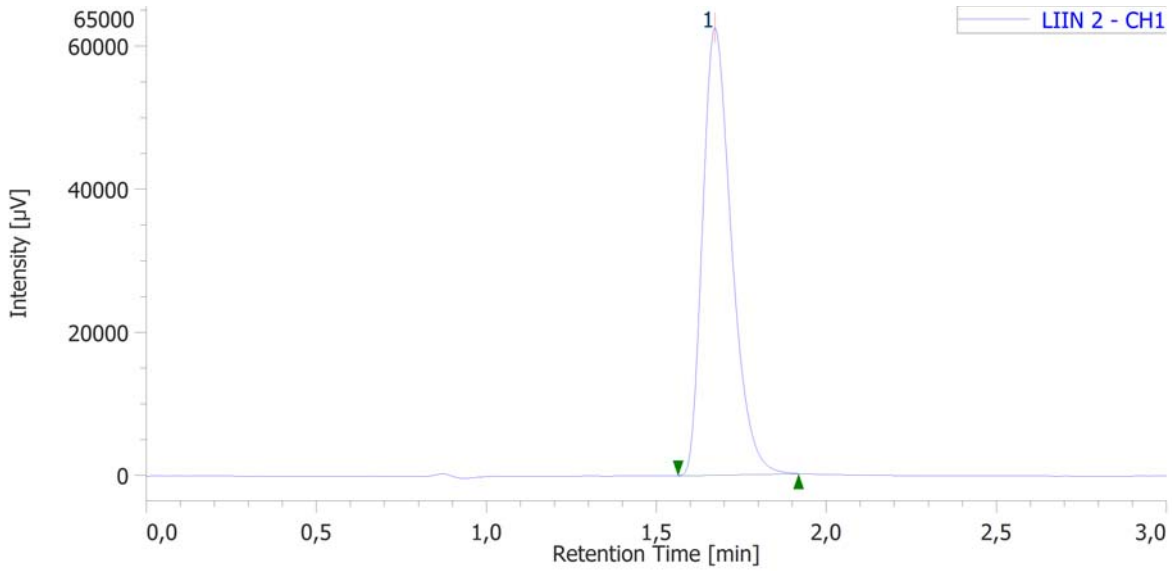

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:48:05
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:30:15
Volume	5,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,672	369421	62442	100,000	100,000	N/A	1886	N/A	1,364	

Creator Administrator
Reviewer
Approver

Chromatogram

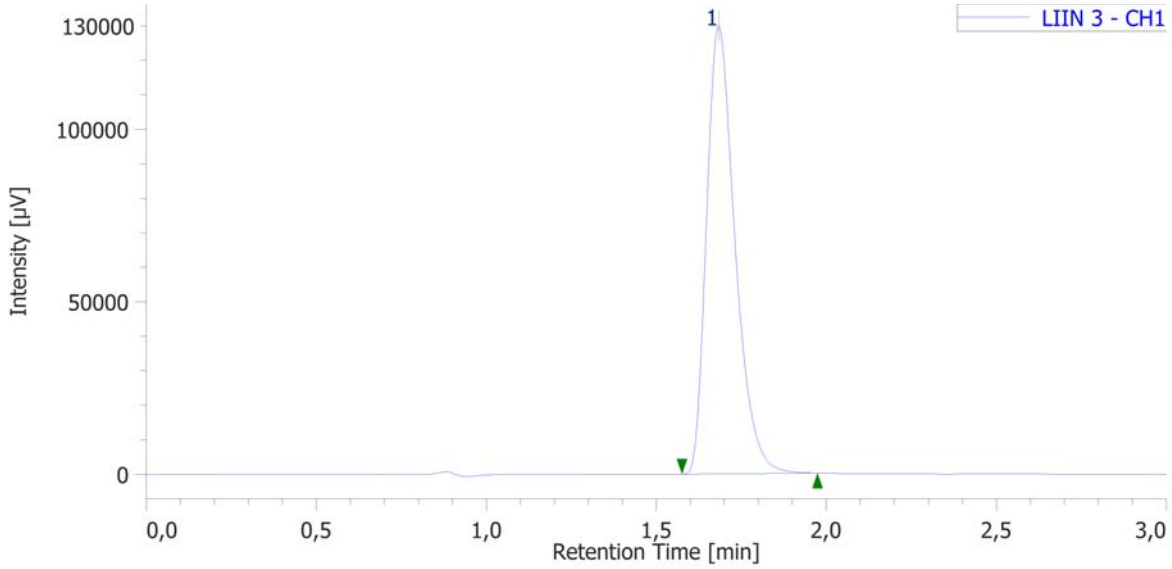

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:48:05
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:33:35
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,683	756888	129852	100,000	100,000	N/A	1991	N/A	1,368	

Creator Administrator
Reviewer
Approver

Chromatogram

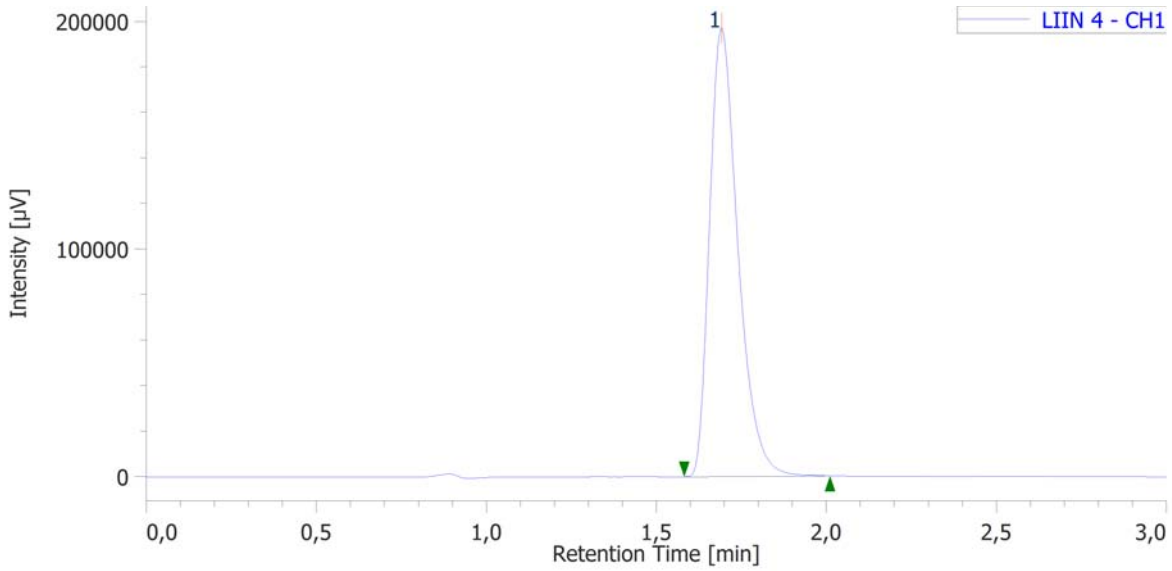

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:48:06
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:36:57
Volume	15,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,692	1142211	196875	100,000	100,000	N/A	2049	N/A	1,393	

Creator Administrator
Reviewer
Approver

Chromatogram

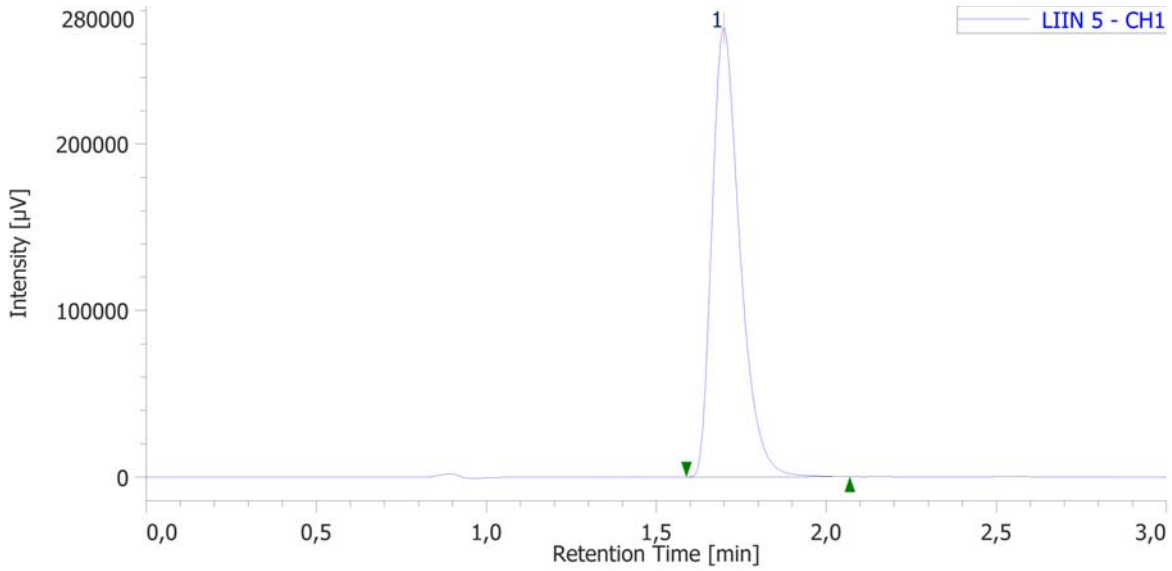

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 11:48:06
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 11:40:22
Volume	20,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,698	1540854	269441	100,000	100,000	N/A	2135	N/A	1,396	

Creator Administrator
Reviewer
Approver

Chromatogram

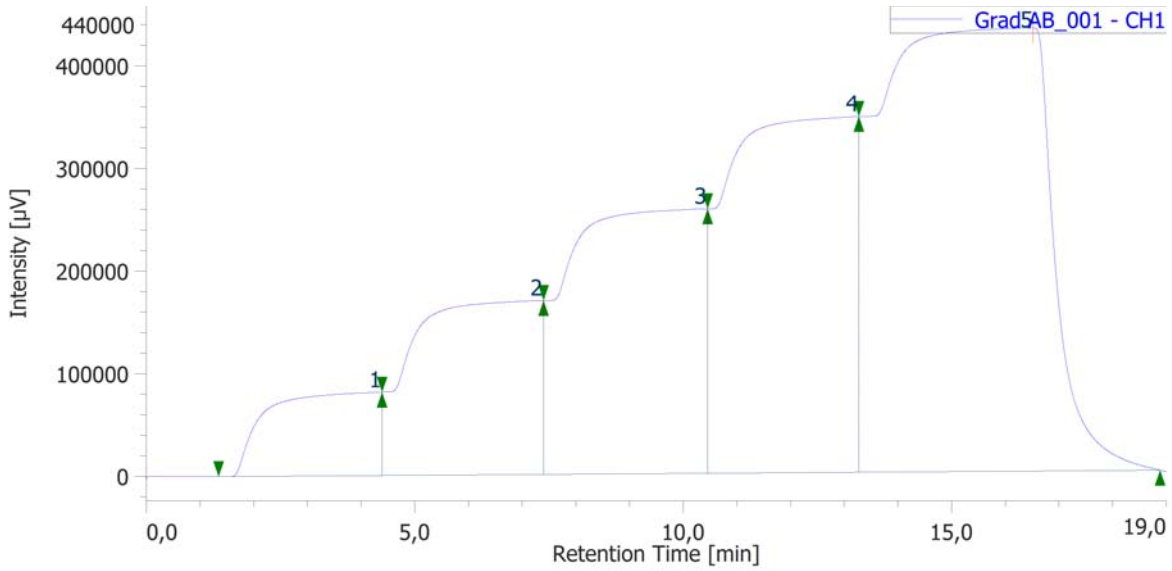

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 13:06:19
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 12:39:10
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Grad
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	1	4,385	81258	6,320	N/A	N/A	N/A	N/A	
2	40 %	1	7,390	169368	13,172	N/A	N/A	N/A	N/A	
3	60 %	1	10,448	257444	20,022	N/A	N/A	N/A	N/A	
4	80 %	1	13,267	346356	26,937	N/A	N/A	N/A	N/A	
5	100 %	1	16,515	431389	33,550	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver

Chromatogram

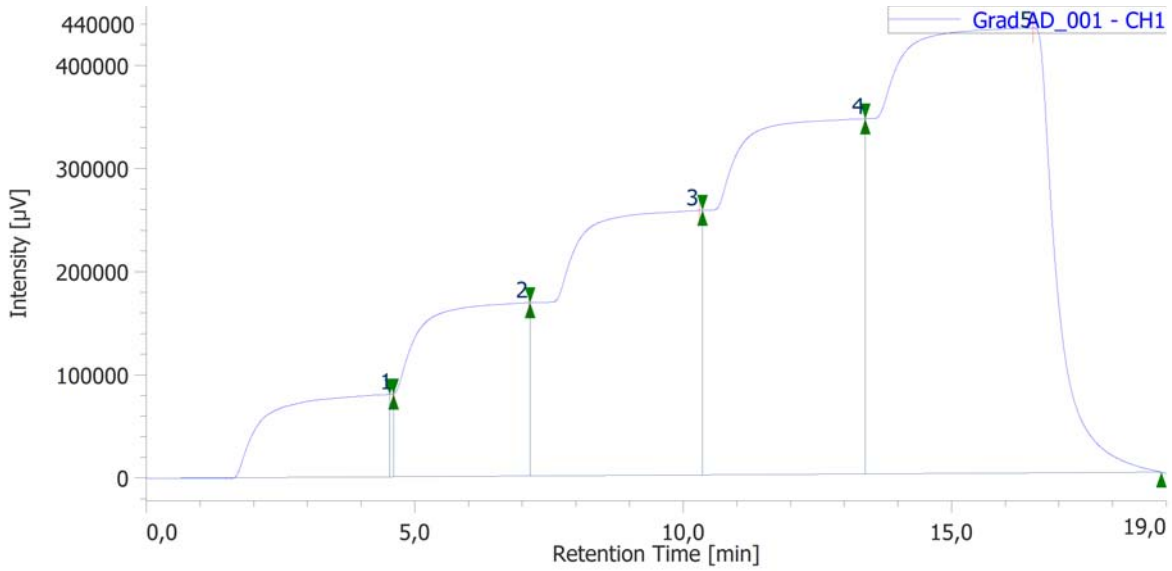

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 13:30:44
Description	
HPLC System Name	01-HP-02
Injection Date	10/12/2019 13:00:05
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AD
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad AD_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	1	4,588	79858	6,244	N/A	N/A	N/A	N/A	
2	40 %	1	7,123	167803	13,119	N/A	N/A	N/A	N/A	
3	60 %	1	10,297	256249	20,034	N/A	N/A	N/A	N/A	
4	80 %	1	13,382	344064	26,900	N/A	N/A	N/A	N/A	
5	100 %	1	16,512	431077	33,703	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver