
Peak Find - EDUV_001 UV_tR2,30 D.jws

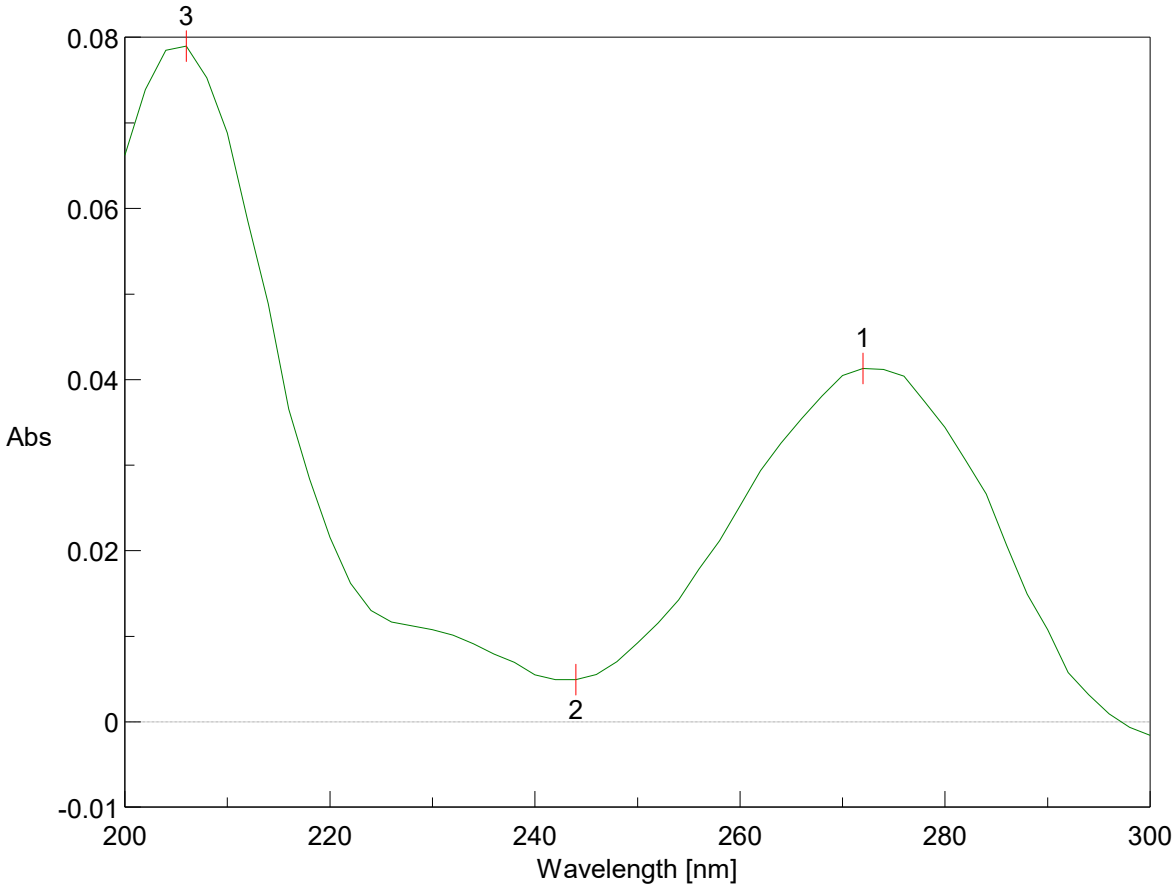

[Comments]

User	Administrator
Division	---
Company	TRB
Creation date	10/12/2019 08:32

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.041263	2	244	0.00488394
3	206	0.078959			

Chromatogram

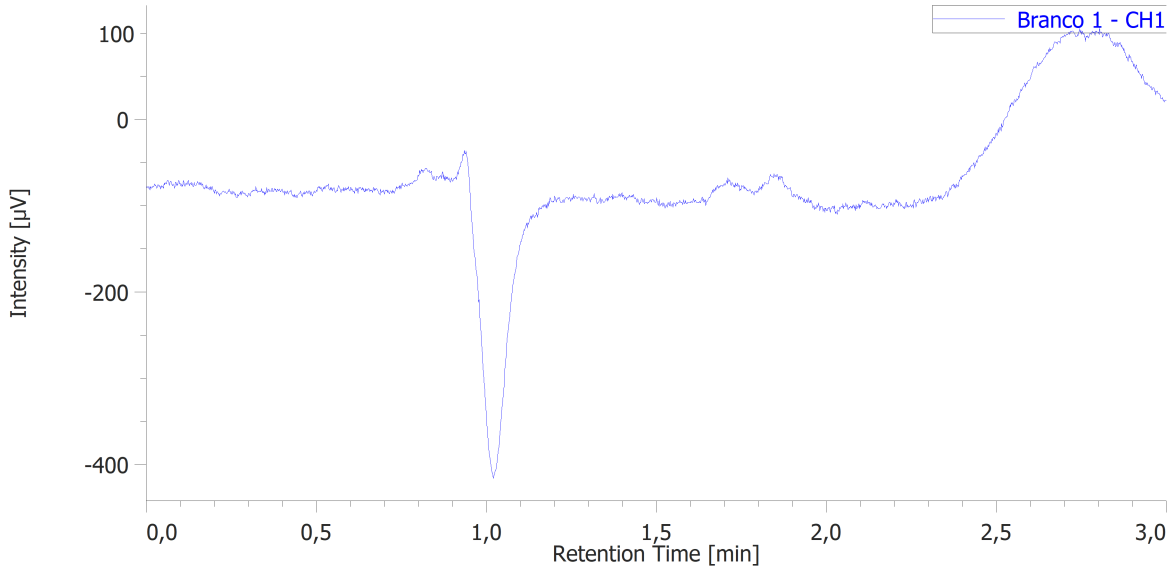


Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:16:30
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 08:56:56
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

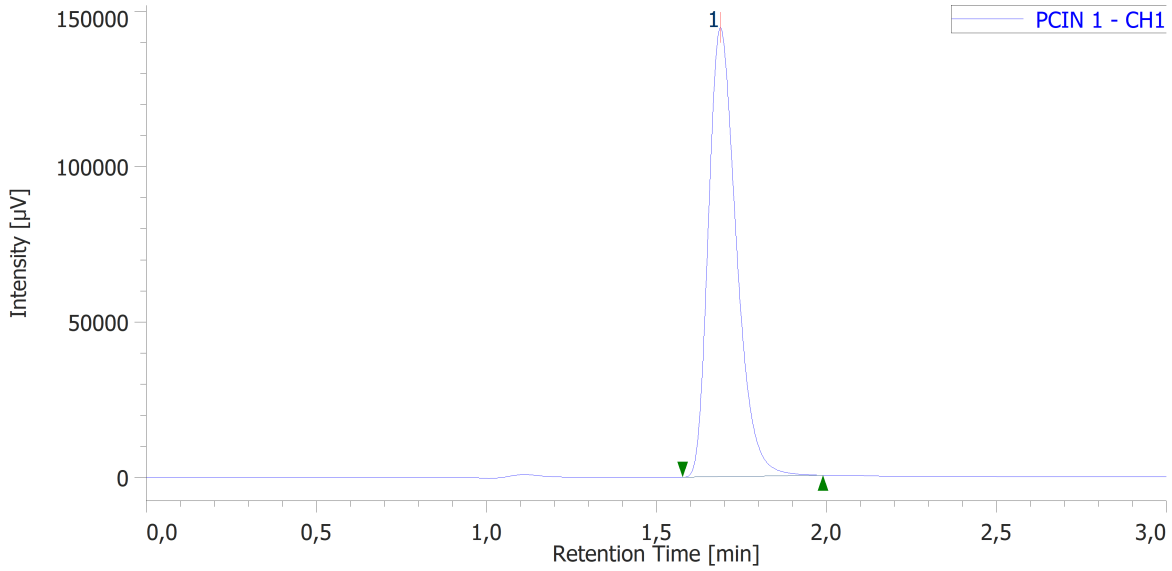

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:16:32
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:00:39
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,688	823800	144363	100,000	100,000	N/A	2081	N/A	1,331	

Creator Administrator
Reviewer
Approver

Chromatogram

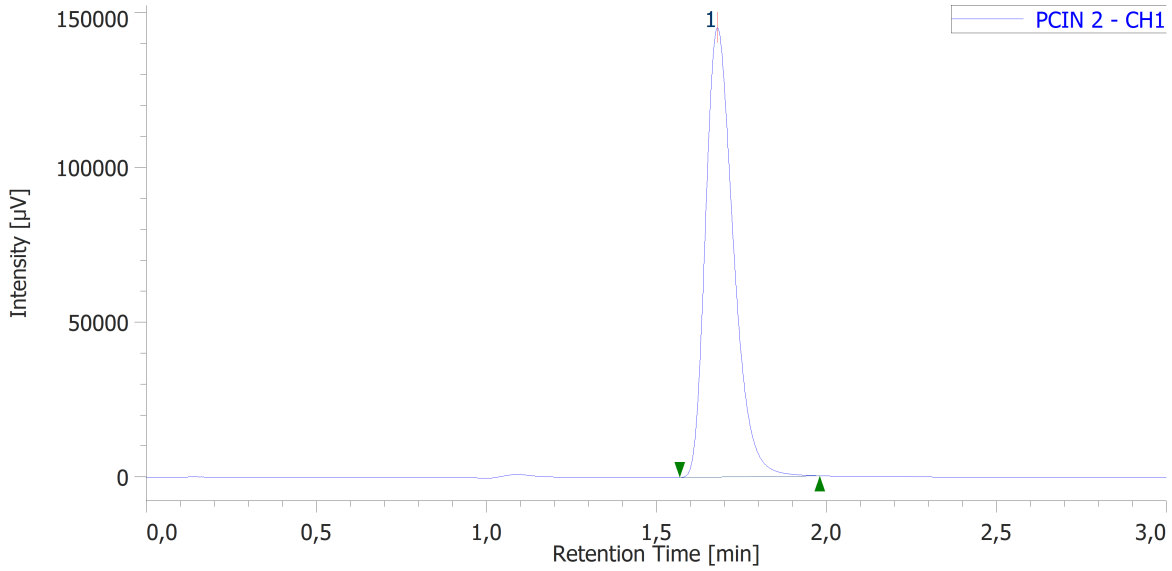

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:16:33
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:04:21
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,680	825188	145111	100,000	100,000	N/A	2075	N/A	1,326	

Creator Administrator
Reviewer
Approver

Chromatogram

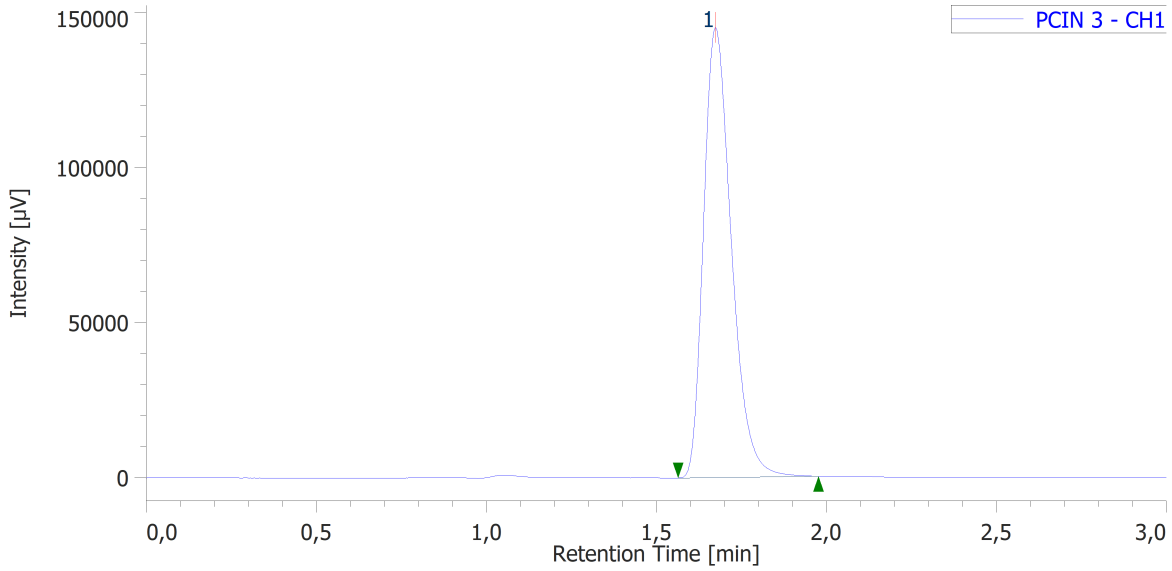

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:16:33
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:08:04
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,673	824294	144987	100,000	100,000	N/A	2060	N/A	1,343	

Creator Administrator
Reviewer
Approver

Chromatogram

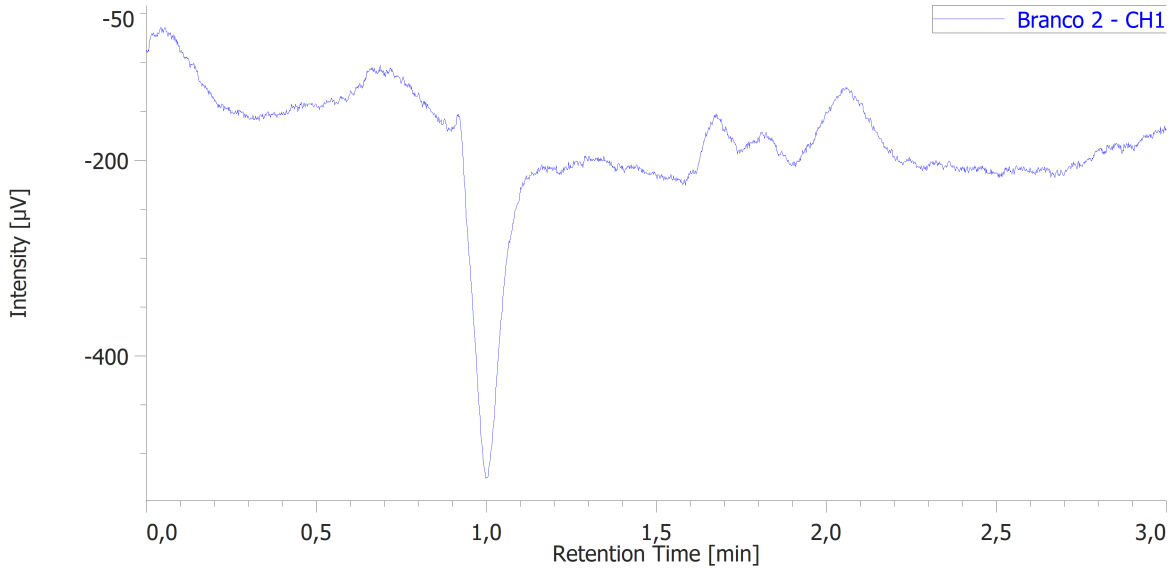


Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:16:34
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:11:47
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

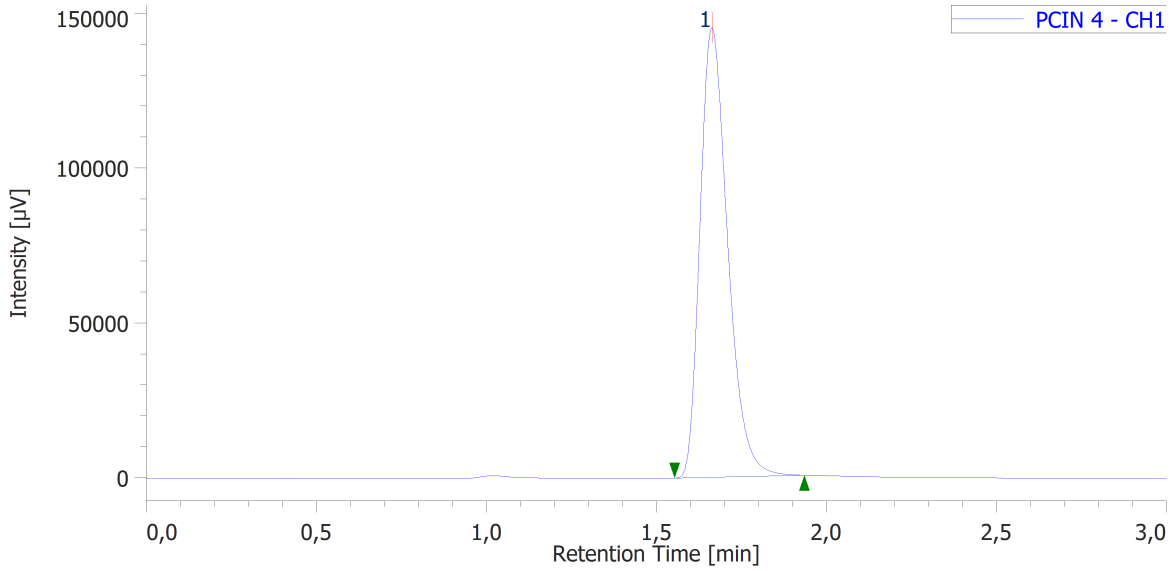

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:19:51
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:15:29
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,663	820247	145023	100,000	100,000	N/A	2049	N/A	1,330	

Creator Administrator
Reviewer
Approver

Chromatogram

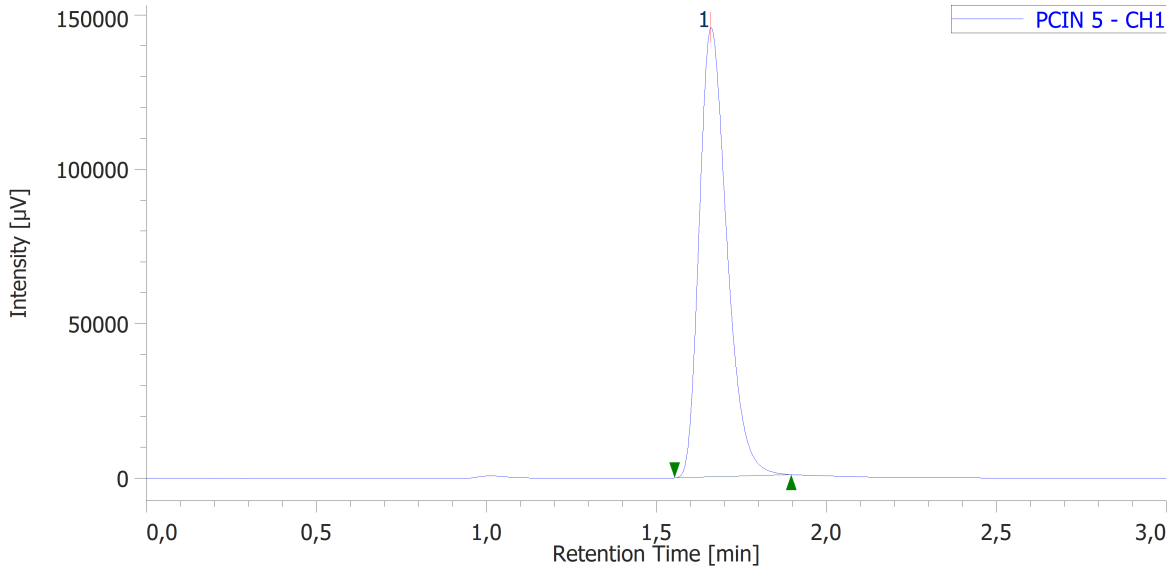

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:29:39
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:19:12
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,660	821041	145458	100,000	100,000	N/A	2041	N/A	1,350	

Creator Administrator
Reviewer
Approver

Chromatogram

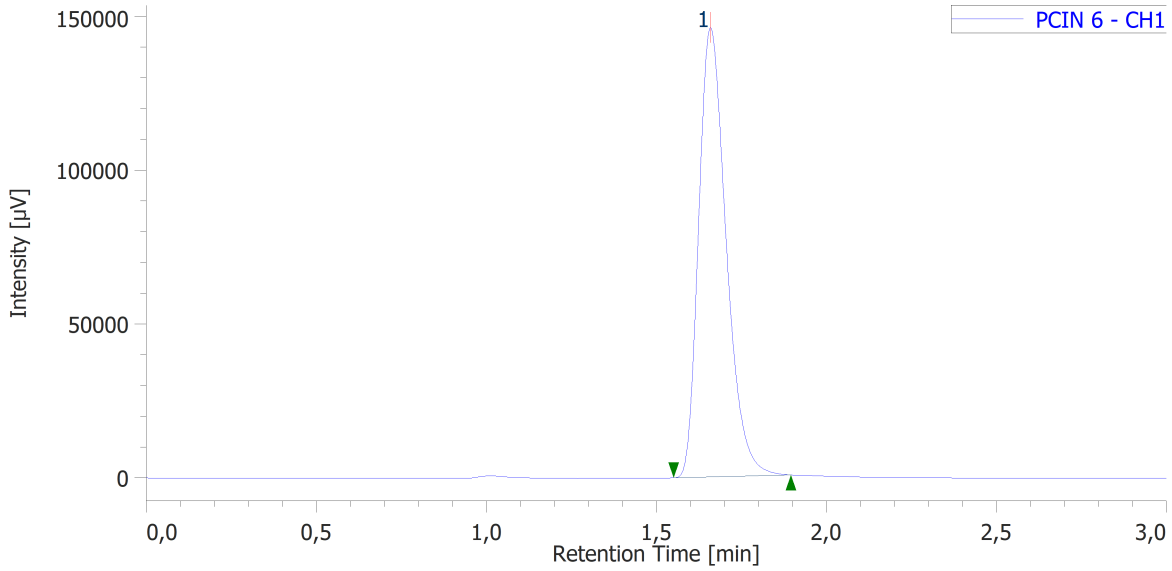

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:29:40
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:22:53
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,658	821395	145971	100,000	100,000	N/A	2047	N/A	1,340	

Creator Administrator
Reviewer
Approver

Chromatogram

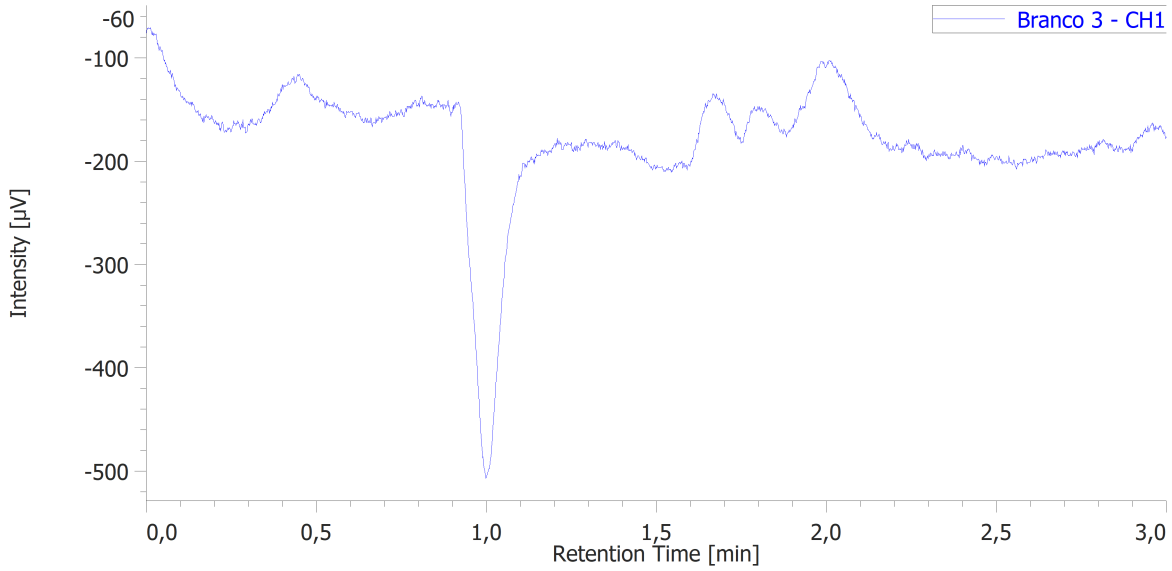


Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 09:43:26
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:26:33
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

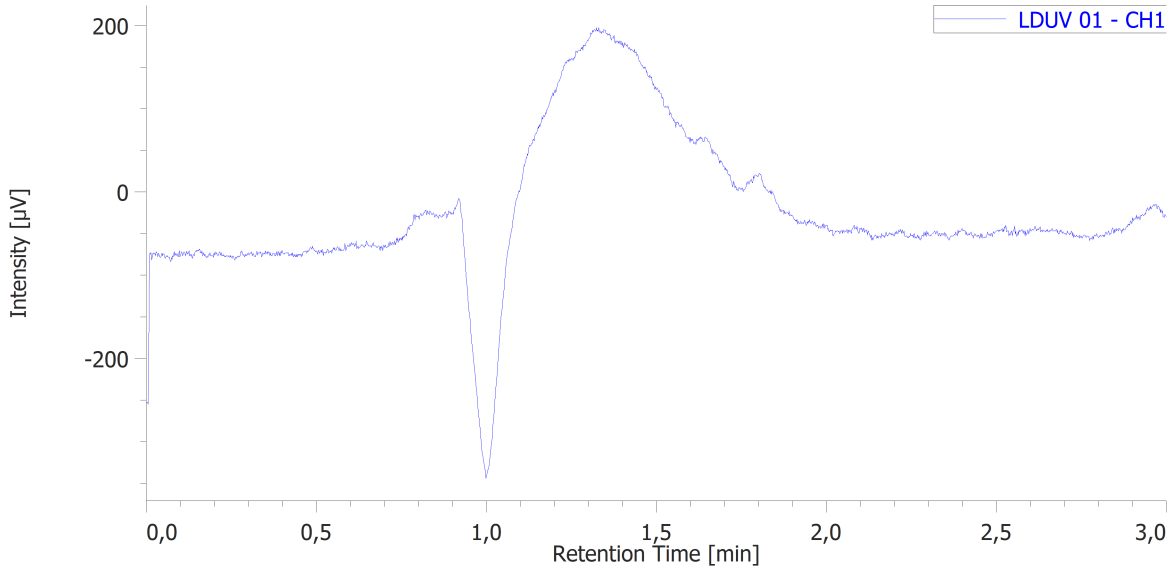


Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:00:55
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:37:45
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

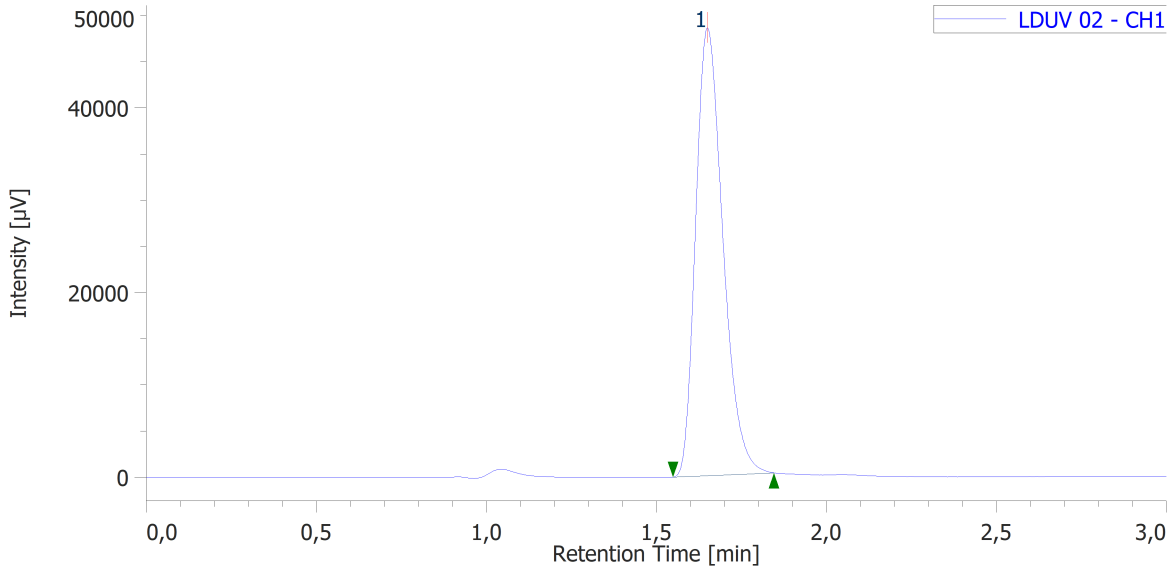

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:00:56
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:41:26
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,650	270014	48493	100,000	100,000	N/A	2047	N/A	1,316	

Creator Administrator
Reviewer
Approver

Chromatogram

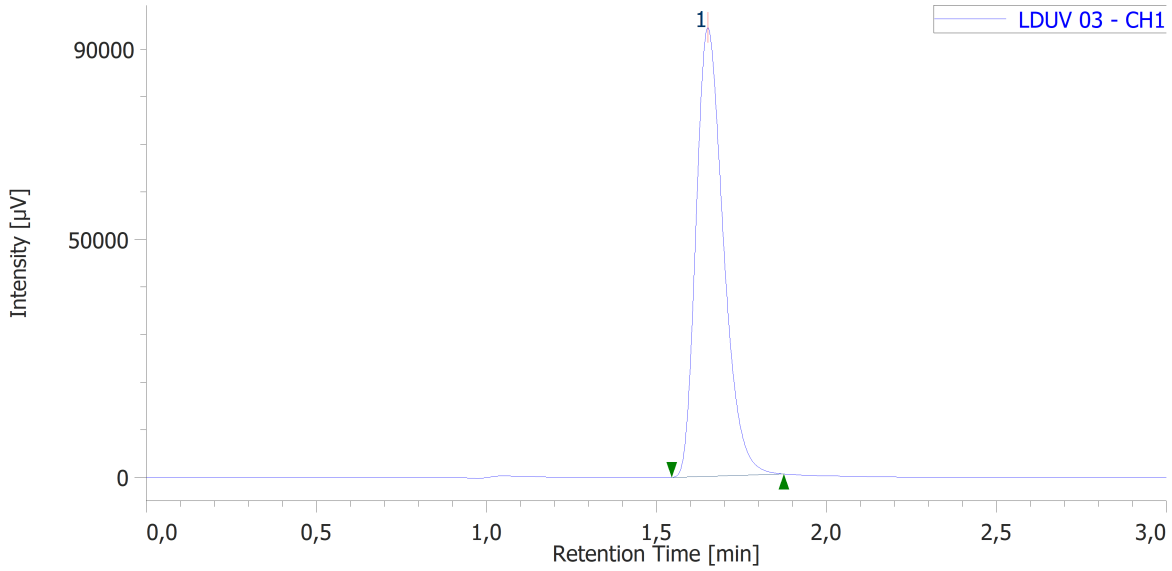

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:00:56
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:45:08
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,652	527157	94267	100,000	100,000	N/A	2051	N/A	1,314	

Creator Administrator
Reviewer
Approver

Chromatogram

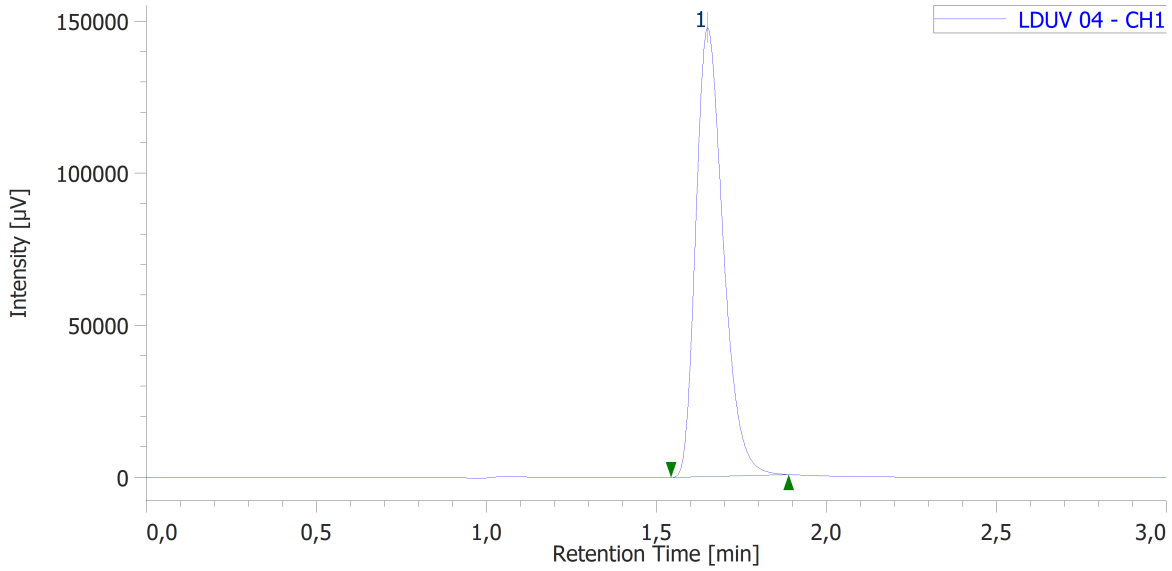

Chromatogram Information

User Name	Administrator
Date Modified	10/12/2019 10:00:57
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:48:51
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,650	824911	147507	100,000	100,000	N/A	2050	N/A	1,336	

Creator Administrator
Reviewer
Approver

Chromatogram

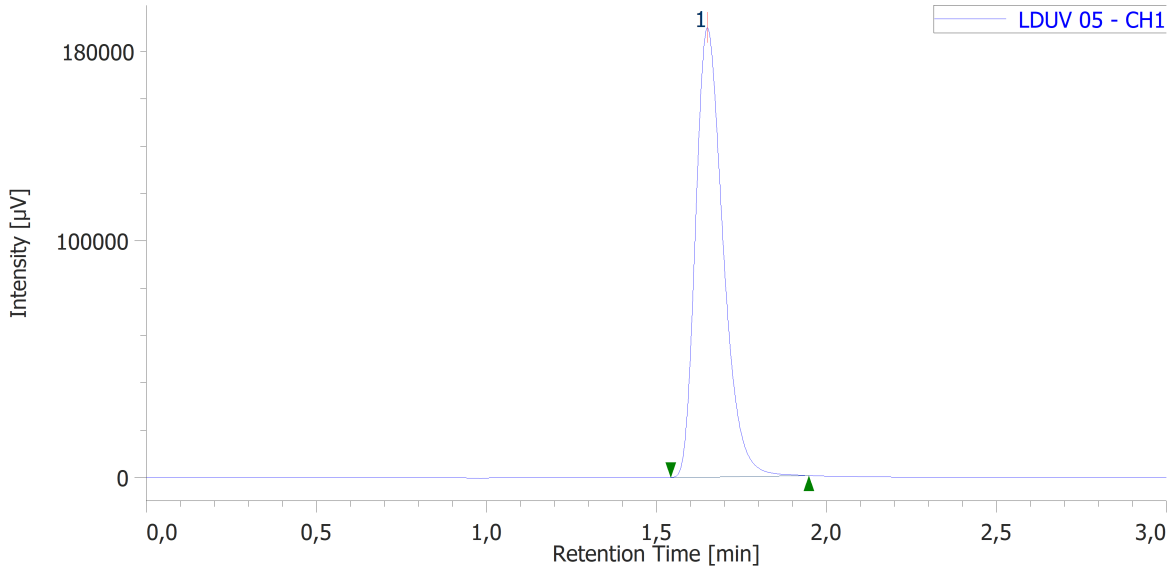

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:00:57
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 09:52:34
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,650	1065532	189808	100,000	100,000	N/A	2052	N/A	1,329	

Creator Administrator
Reviewer
Approver

Chromatogram

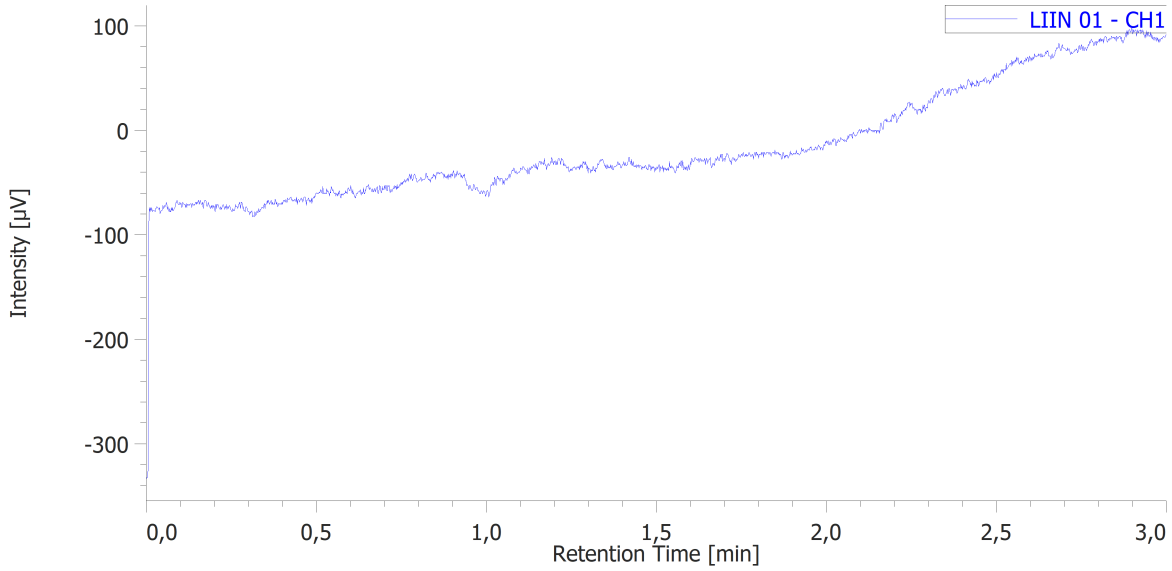


Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:39:30
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 10:19:40
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

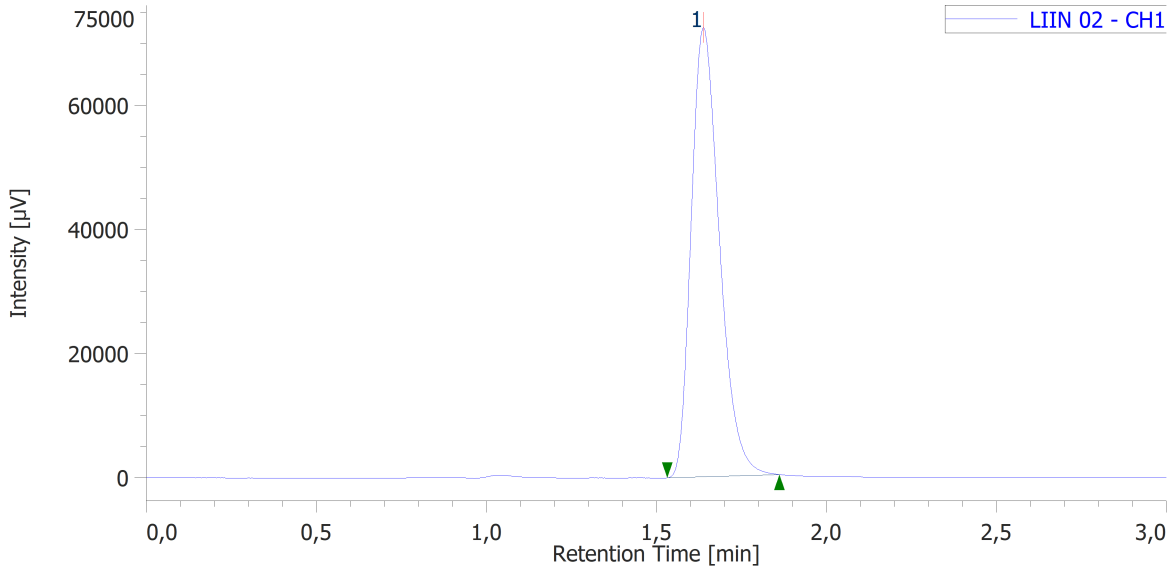

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:39:30
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 10:23:18
Volume	5,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,638	417747	72344	100,000	100,000	N/A	1886	N/A	1,314	

Creator Administrator
Reviewer
Approver

Chromatogram

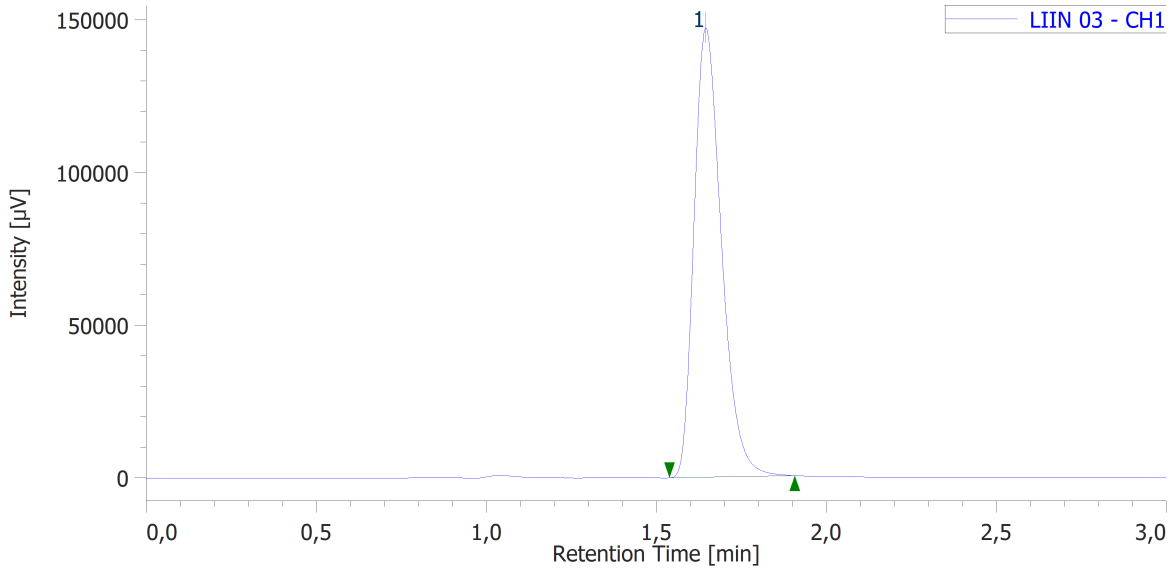

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:39:31
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 10:27:00
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,645	824967	147165	100,000	100,000	N/A	2036	N/A	1,335	

Creator Administrator
Reviewer
Approver

Chromatogram

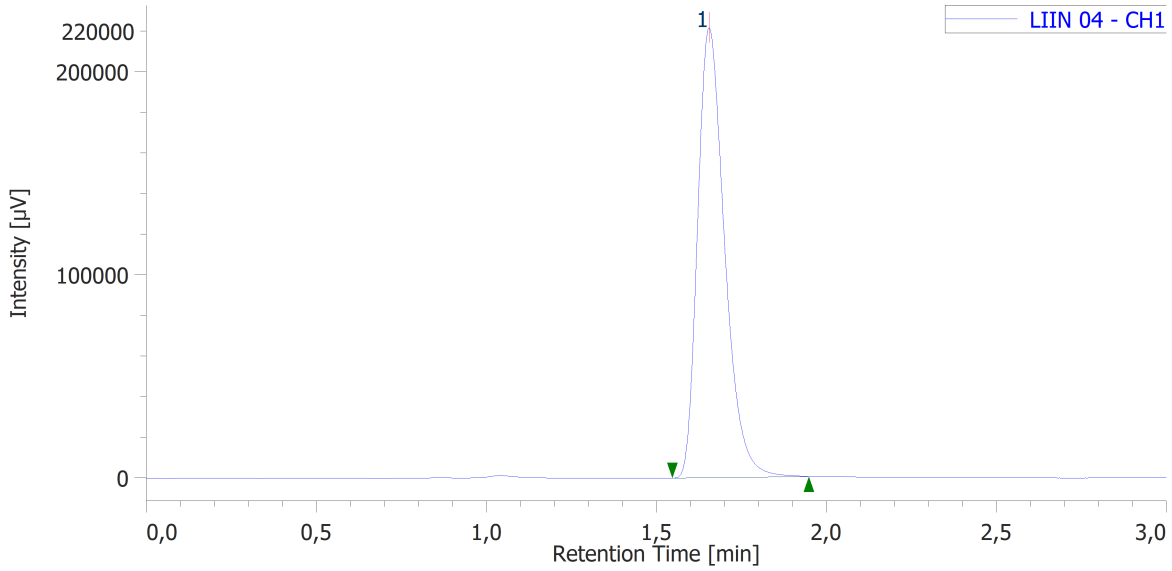

Chromatogram Information

User Name	Administrator
Date Modified	10/12/2019 10:39:31
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 10:30:48
Volume	15,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,655	1223274	221410	100,000	100,000	N/A	2142	N/A	1,349	

Creator Administrator
Reviewer
Approver

Chromatogram

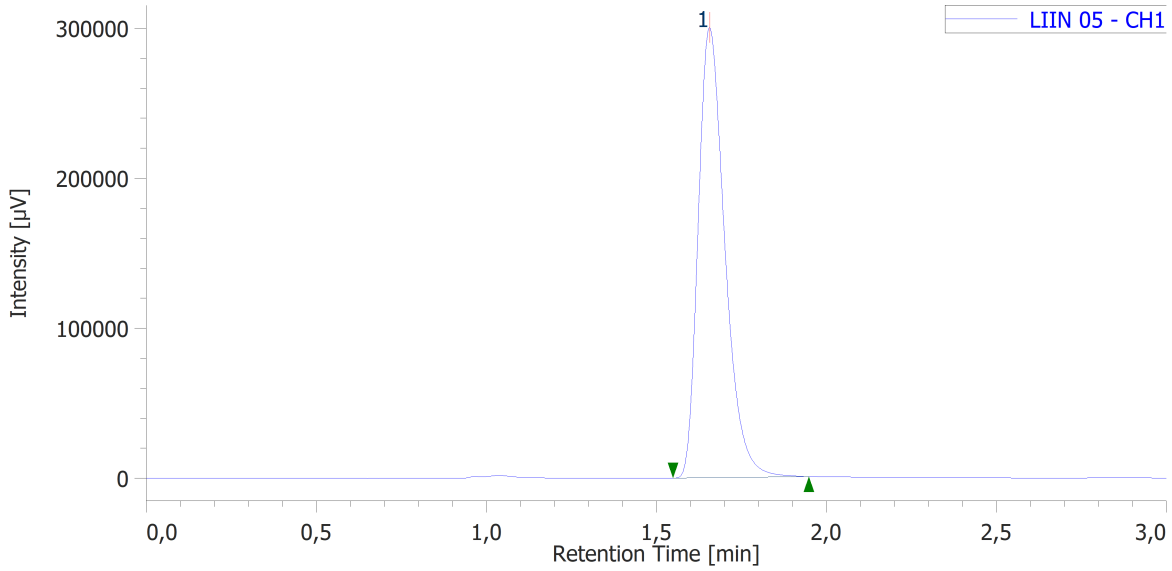

Chromatogram Information	
User Name	Administrator
Date Modified	10/12/2019 10:39:32
Description	
HPLC System Name	01-HP-01
Injection Date	10/12/2019 10:34:41
Volume	20,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,657	1634764	299858	100,000	100,000	N/A	2208	N/A	1,348	

Creator Administrator
Reviewer
Approver

Chromatogram

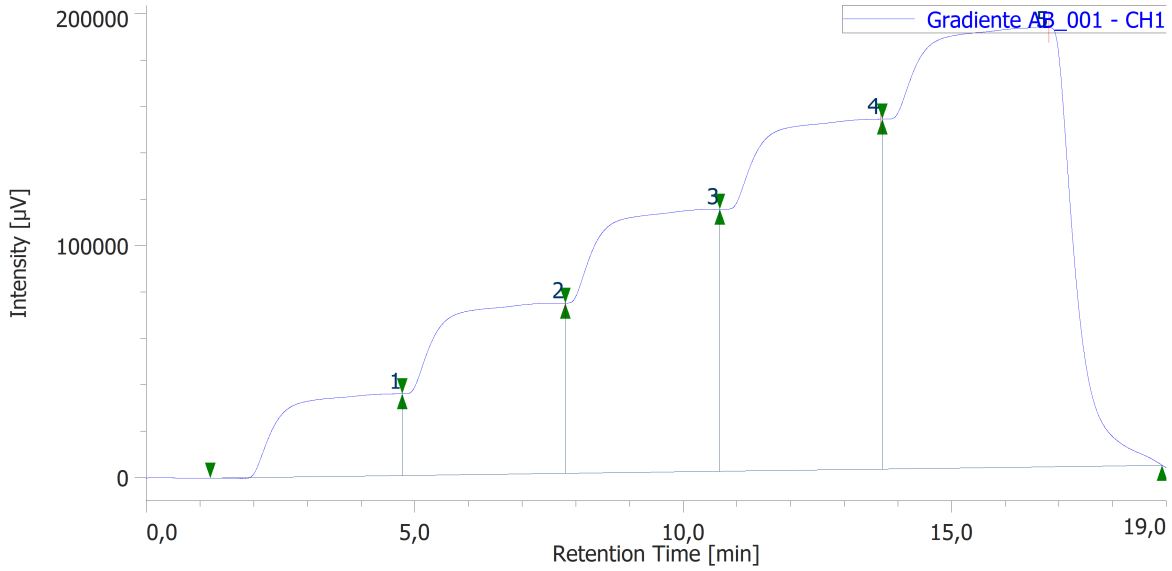

Chromatogram Information	
User Name	Administrator
Date Modified	11/12/2019 10:15:07
Description	
HPLC System Name	01-HP-01
Injection Date	11/12/2019 09:49:14
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	GradienteAB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	4,763	35248	6,278	N/A	N/A	N/A	N/A	
2	40%	1	7,797	73323	13,060	N/A	N/A	N/A	N/A	
3	60%	1	10,680	112893	20,108	N/A	N/A	N/A	N/A	
4	80%	1	13,670	150772	26,855	N/A	N/A	N/A	N/A	
5	100%	1	16,812	189193	33,698	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver

Chromatogram

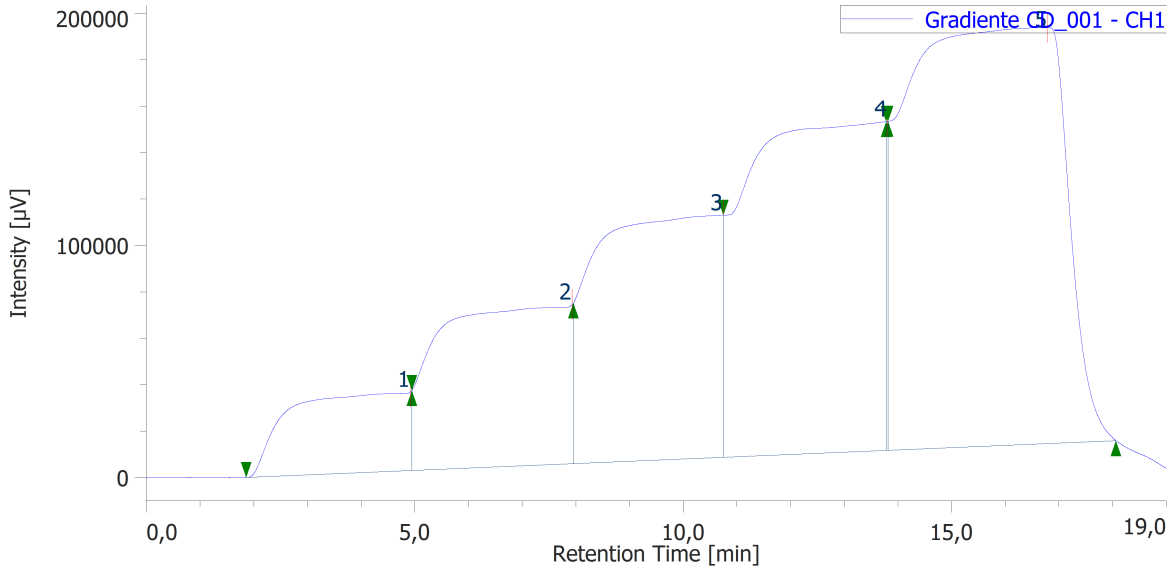

Chromatogram Information	
User Name	Administrator
Date Modified	11/12/2019 10:33:23
Description	
HPLC System Name	01-HP-01
Injection Date	11/12/2019 10:14:21
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	GradienteCD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	4,918	33957	6,437	N/A	N/A	N/A	N/A	
2	40%	1	7,930	68573	12,998	N/A	N/A	N/A	N/A	
3	60%	1	10,747	104262	19,763	N/A	N/A	N/A	N/A	
4	80%	1	13,800	141668	26,853	N/A	N/A	N/A	N/A	
5	100%	1	16,788	174028	33,949	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver