
Peak Find - EDUV.jws

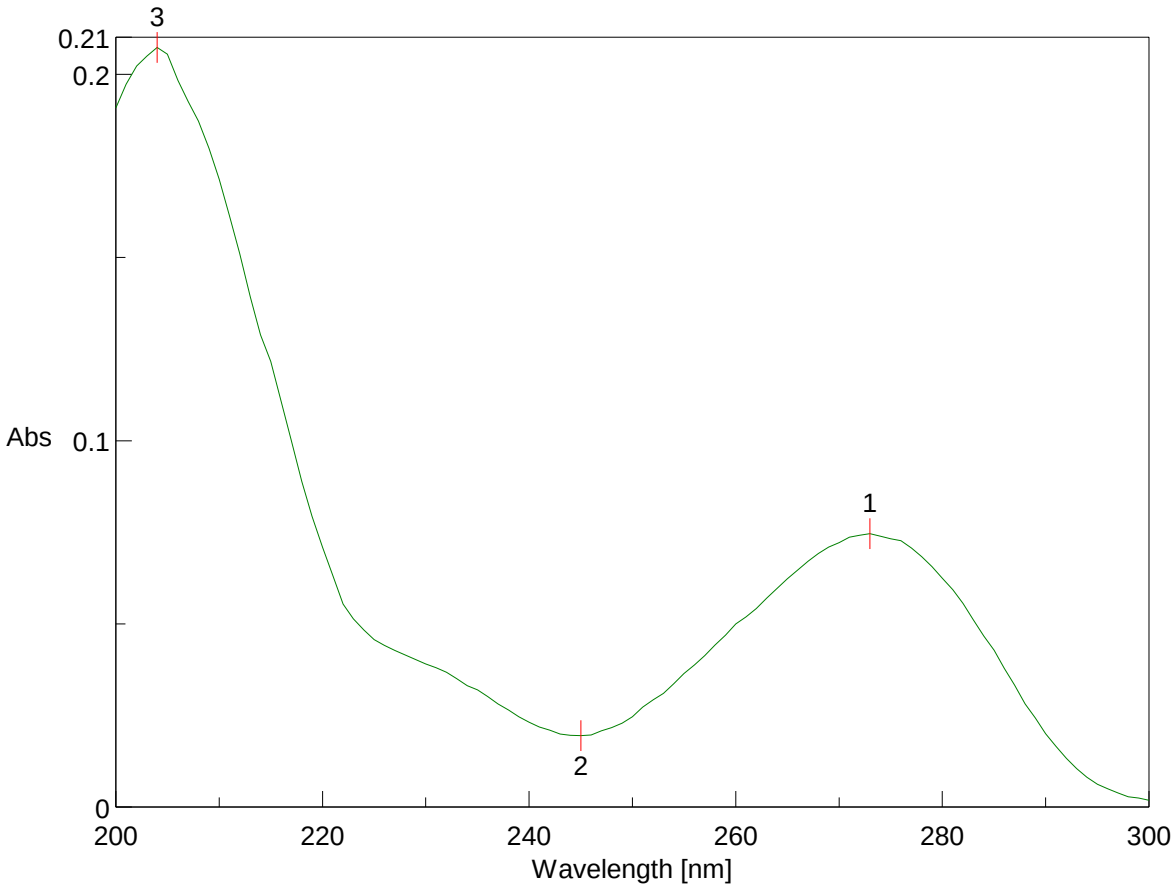

[Comments]

User	Administrator
Division	---
Company	SAUVET
Creation date	27/07/2020 13:38

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	0000000000
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.074602	2	245	0.019471
3	204	0.207166			

Chromatogram

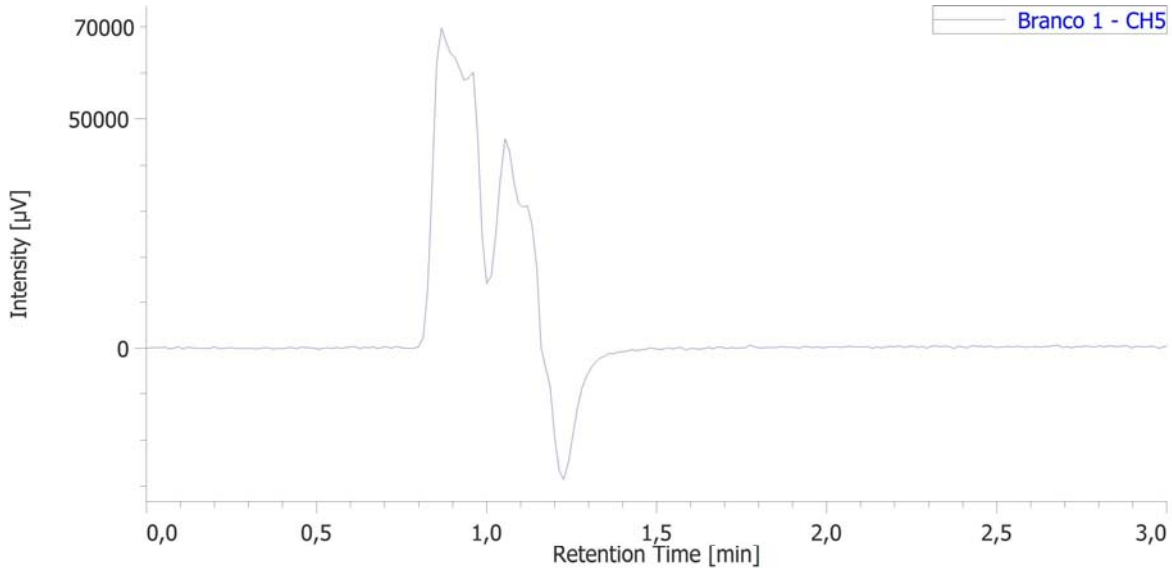


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:48
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 13:57:12
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

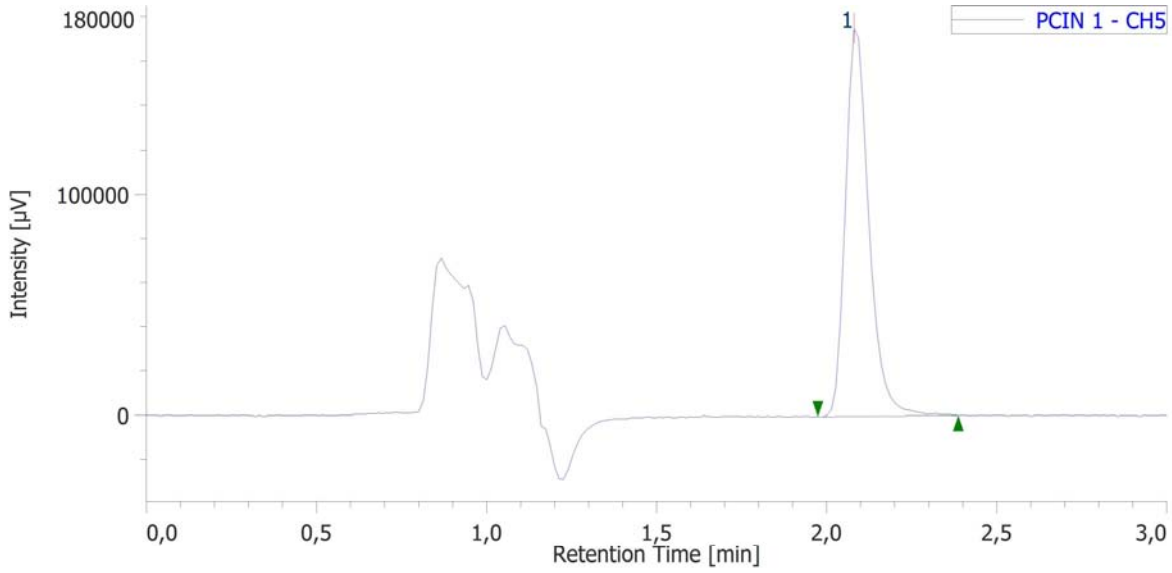


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:48
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:01:33
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,080	844686	175301	100,000	100,000	N/A	4575	N/A	

Chromatogram

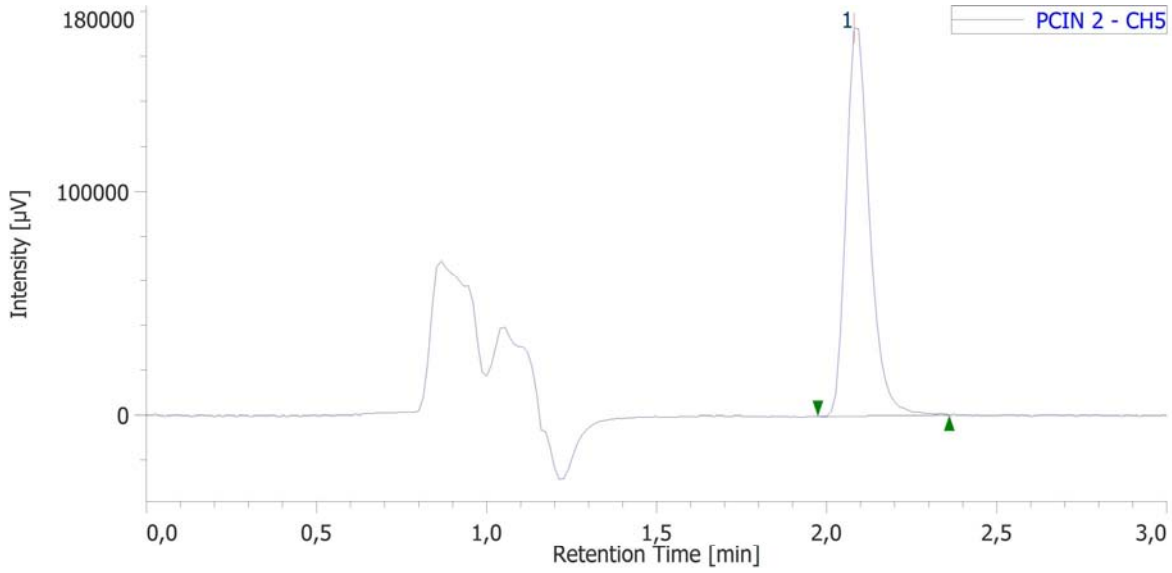


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:48
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:05:55
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,080	838092	172911	100,000	100,000	N/A	4509	N/A	

Chromatogram

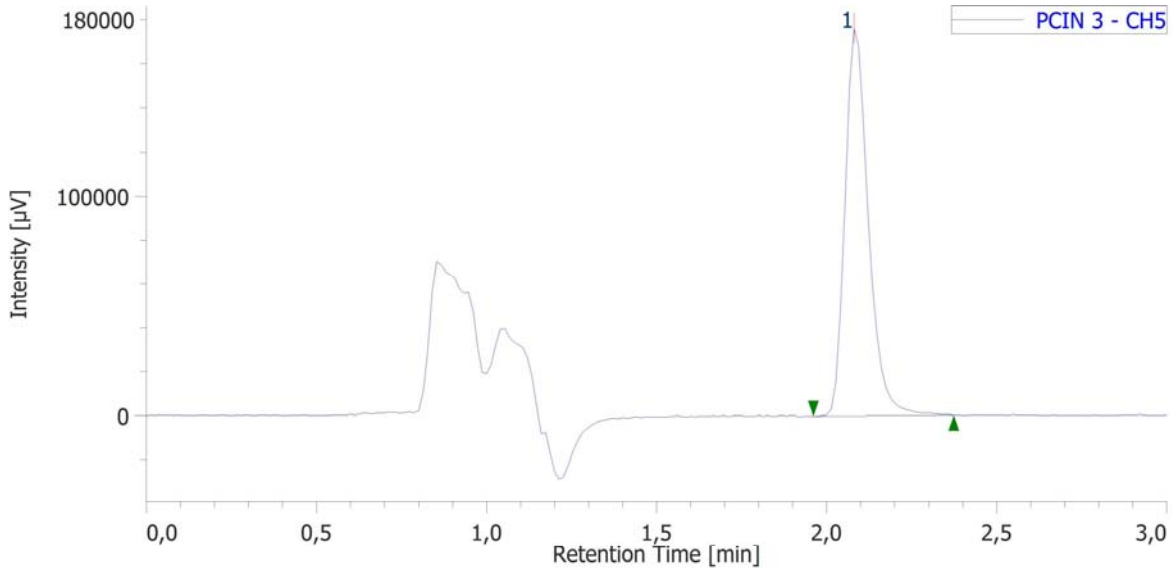


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:49
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:10:16
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,080	844276	176093	100,000	100,000	N/A	4583	N/A	

Chromatogram

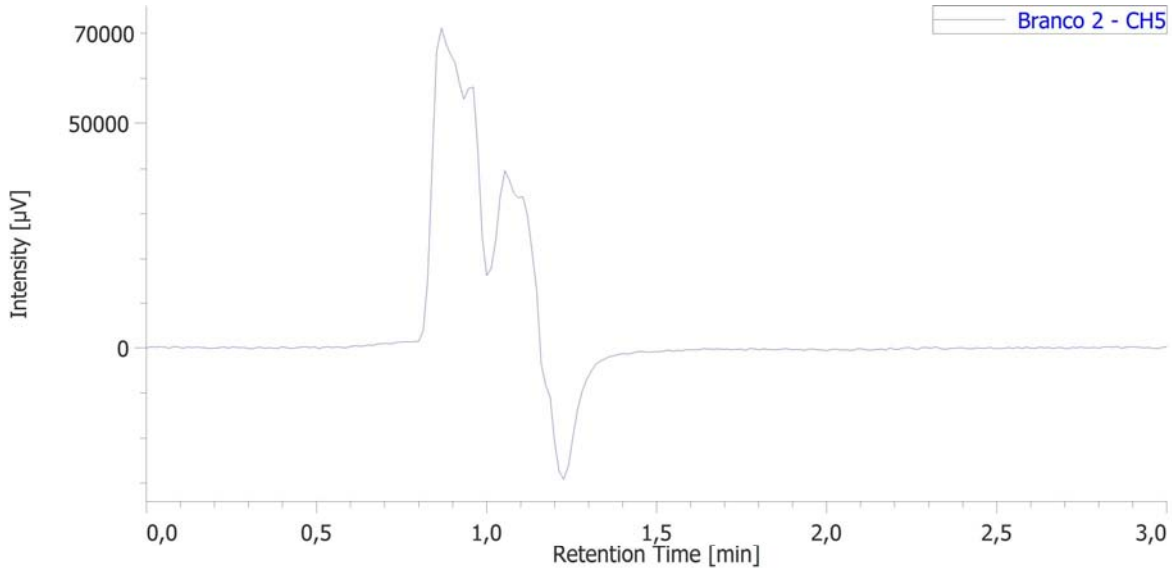


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:49
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:14:38
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

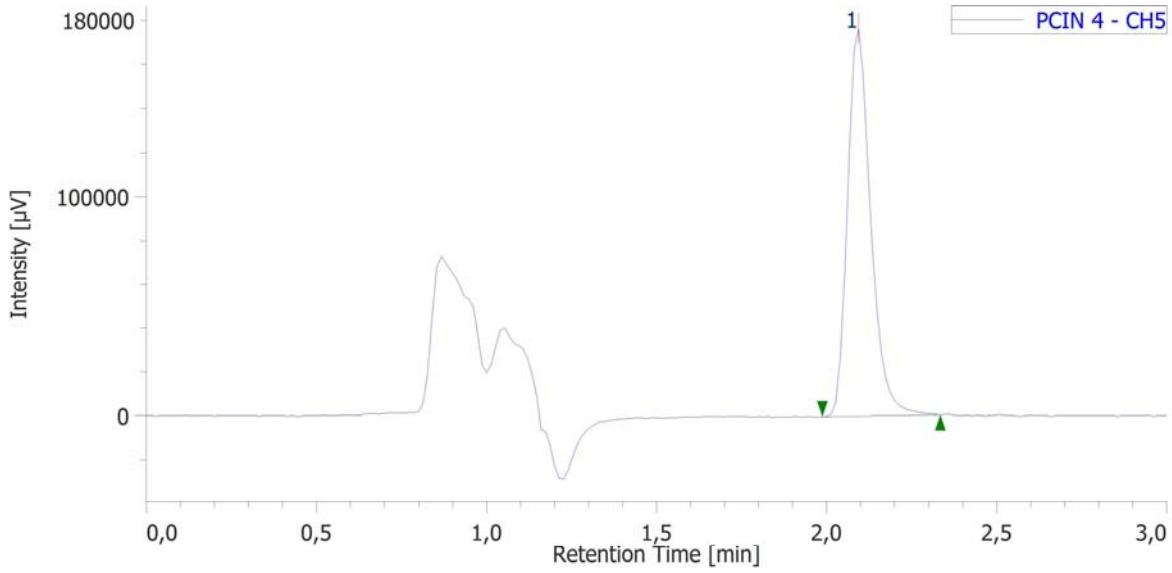


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:49
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:18:59
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,093	838434	176315	100,000	100,000	N/A	4680	N/A	

Chromatogram

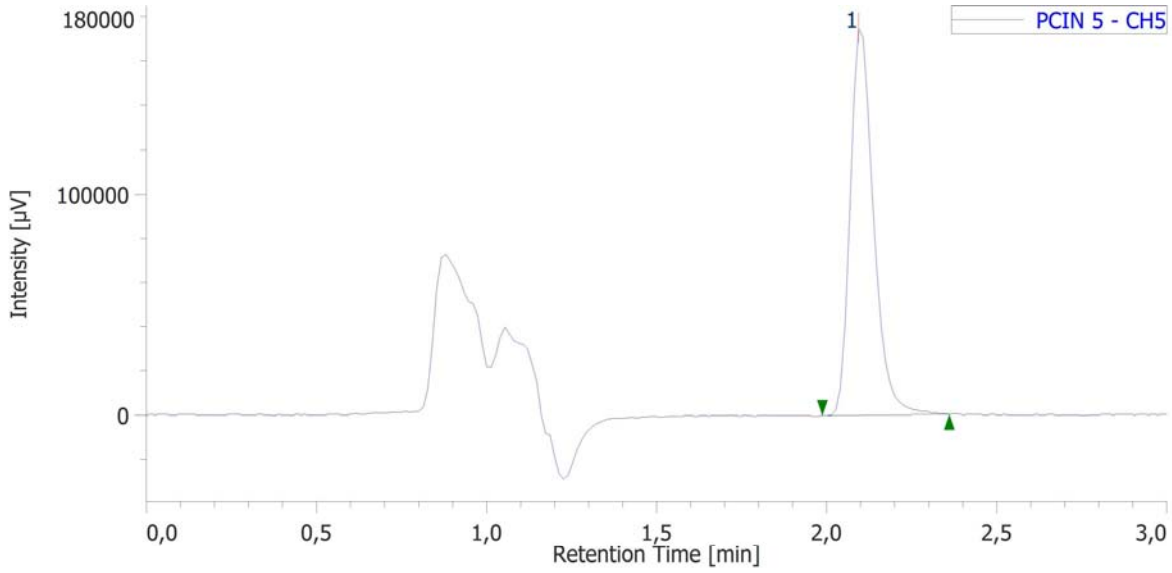


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:49
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:23:20
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,093	840517	174786	100,000	100,000	N/A	4591	N/A	

Chromatogram

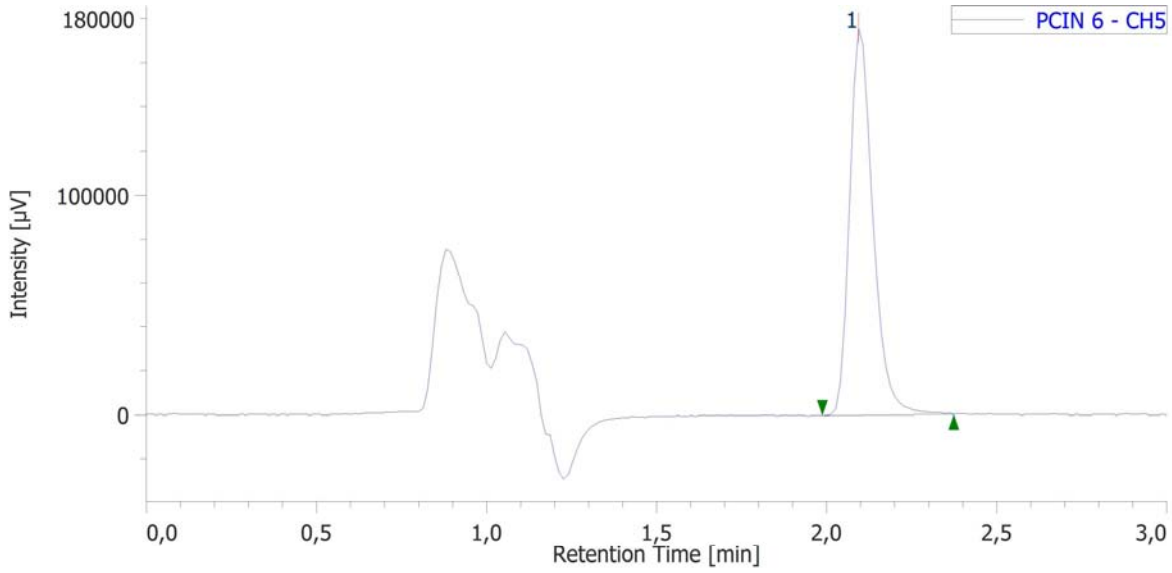


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:49
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:27:42
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,093	840152	175681	100,000	100,000	N/A	4640	N/A	

Chromatogram

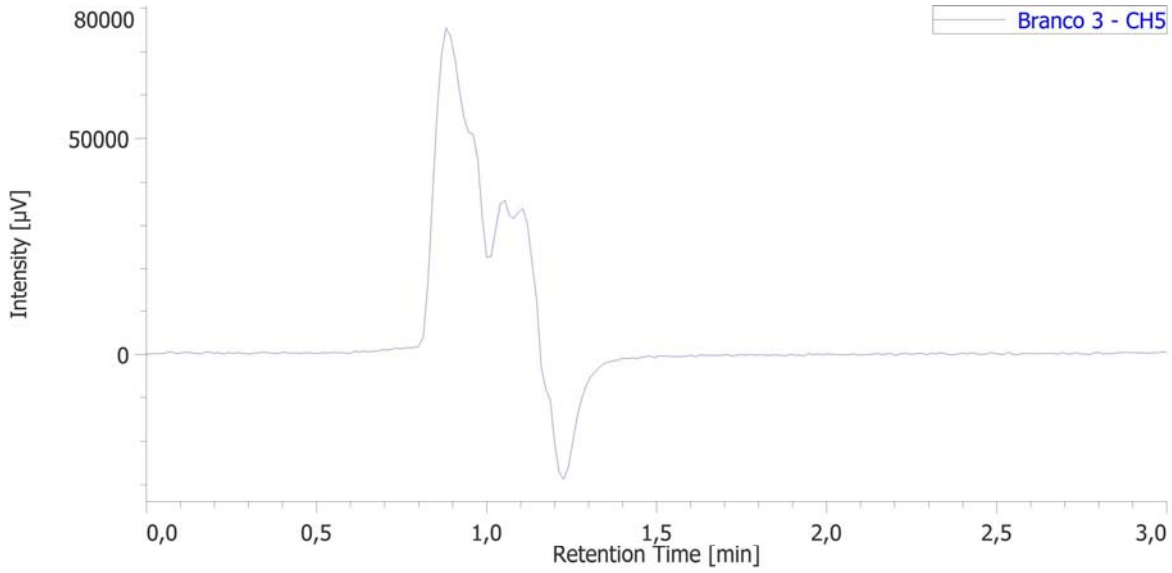


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 14:35:49
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:32:03
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

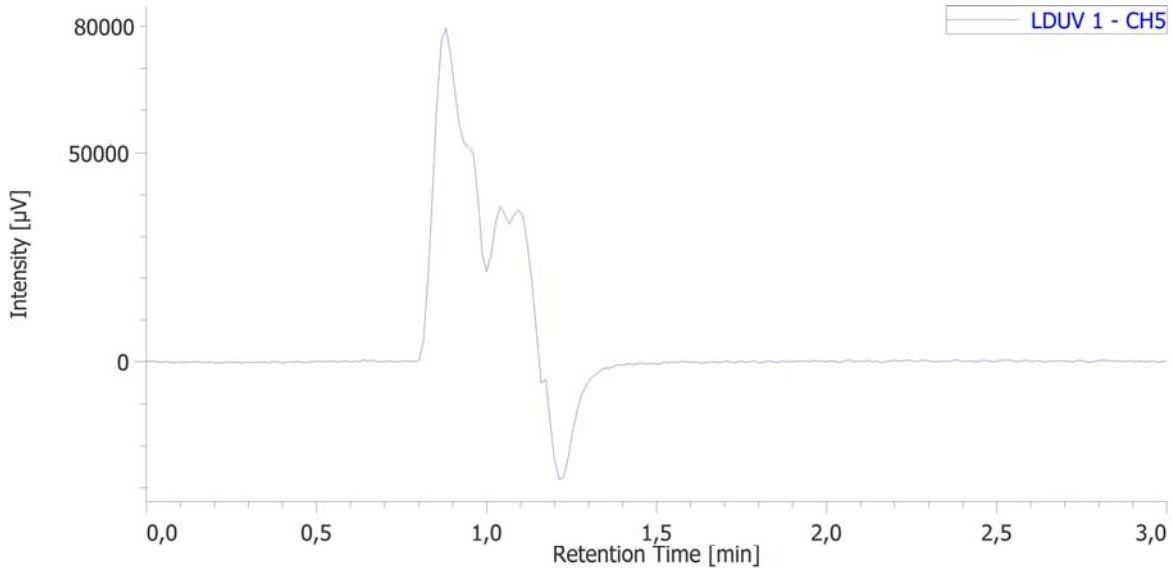


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:06:40
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:44:16
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

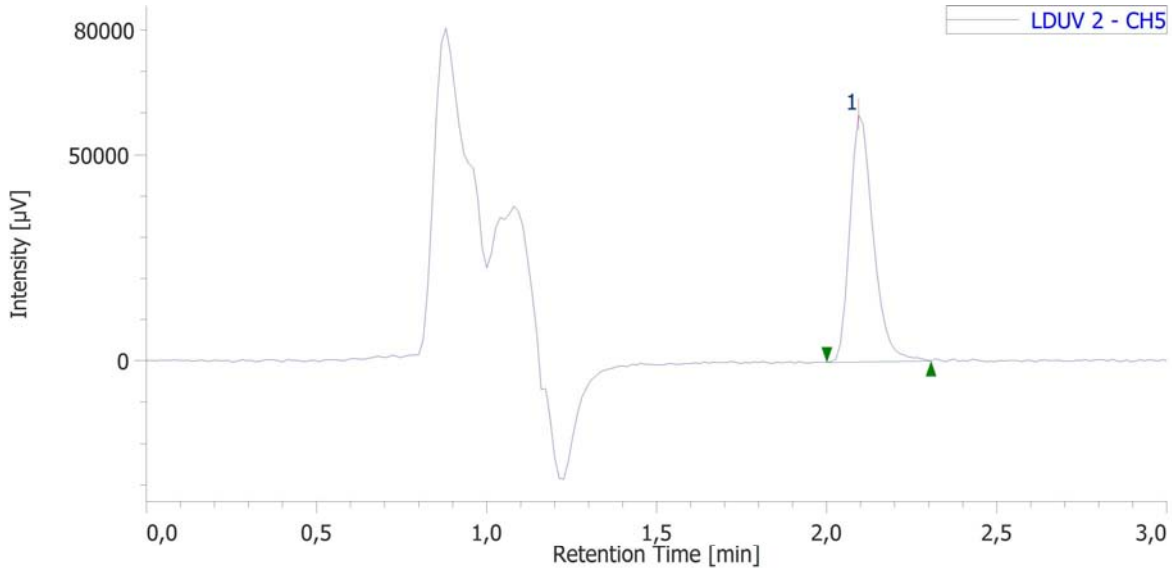


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:06:41
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:48:38
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,093	287371	59898	100,000	100,000	N/A	4584	N/A	

Chromatogram

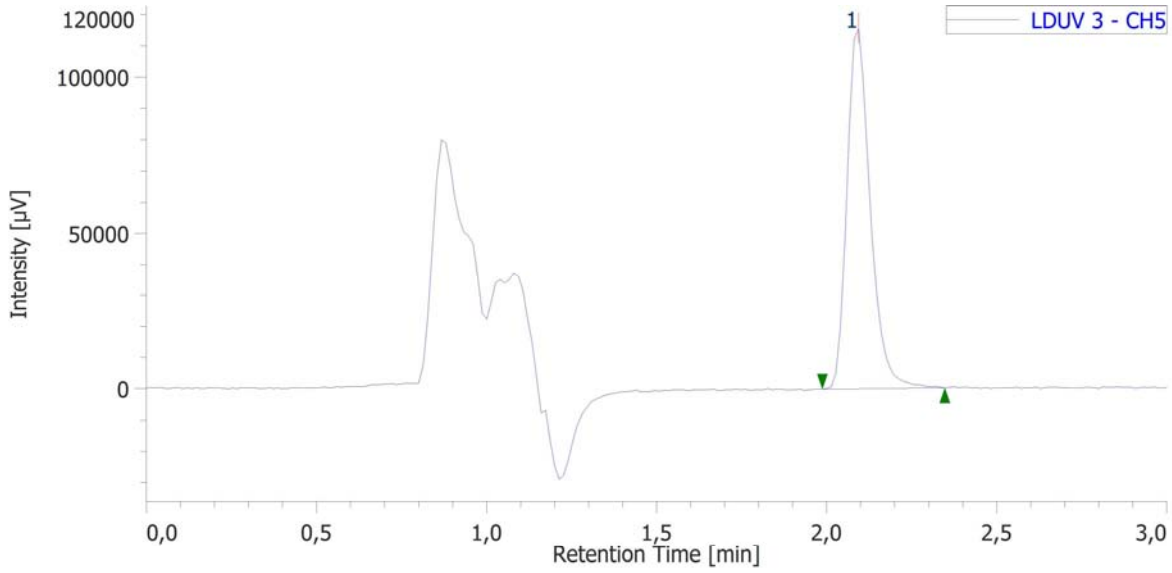


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:06:41
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:53:02
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,093	552665	115629	100,000	100,000	N/A	4666	N/A	

Chromatogram

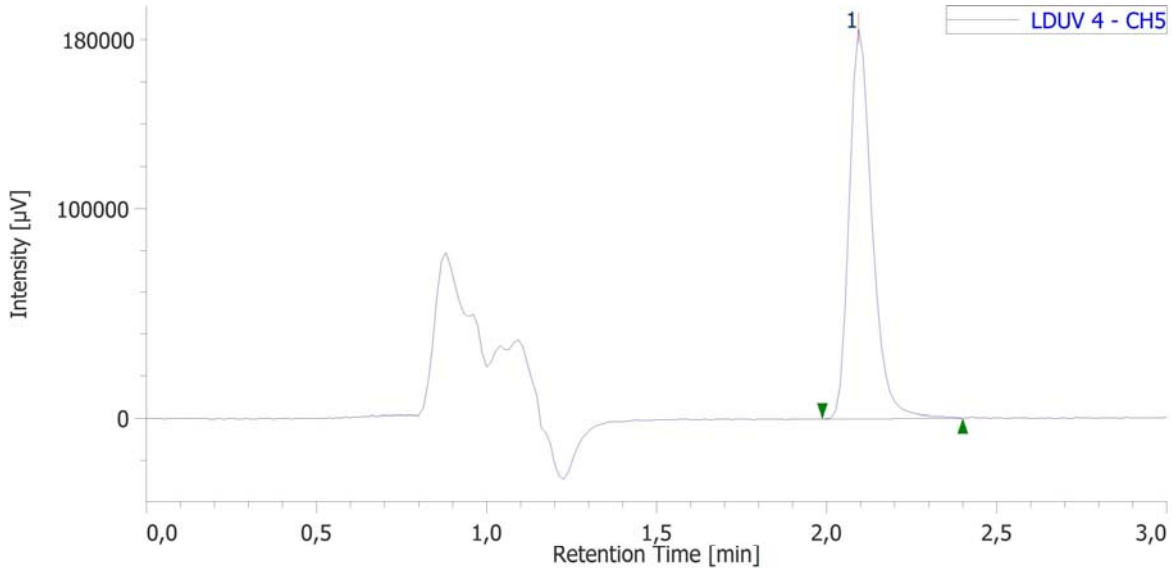


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:06:41
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 14:57:25
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,093	869734	185625	100,000	100,000	N/A	4893	N/A	

Chromatogram

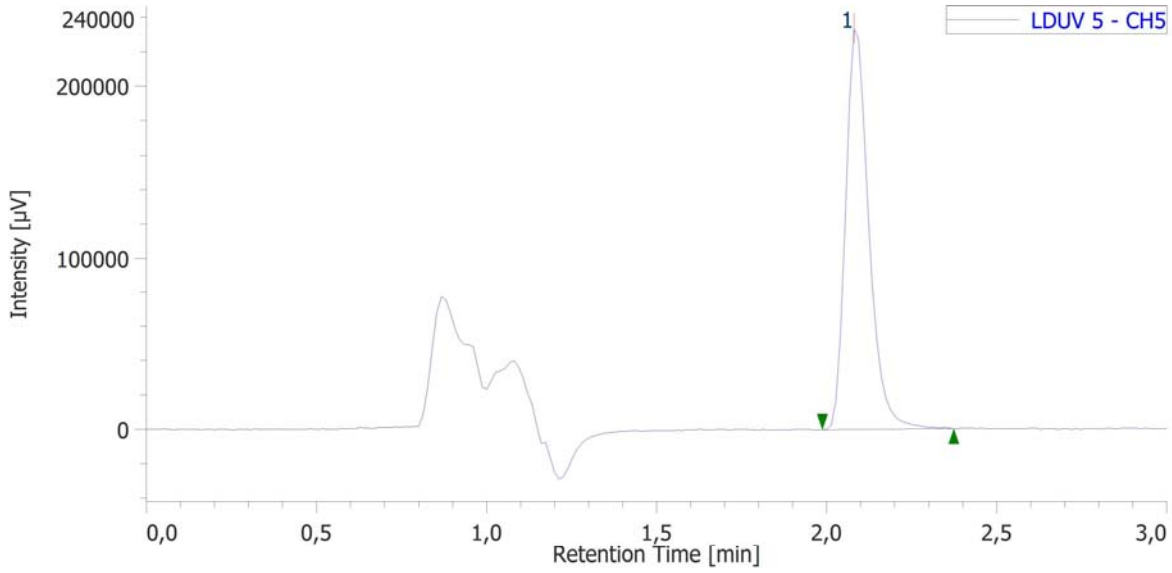


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:06:41
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 15:01:49
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,080	1112202	233500	100,000	100,000	N/A	4624	N/A	

Chromatogram

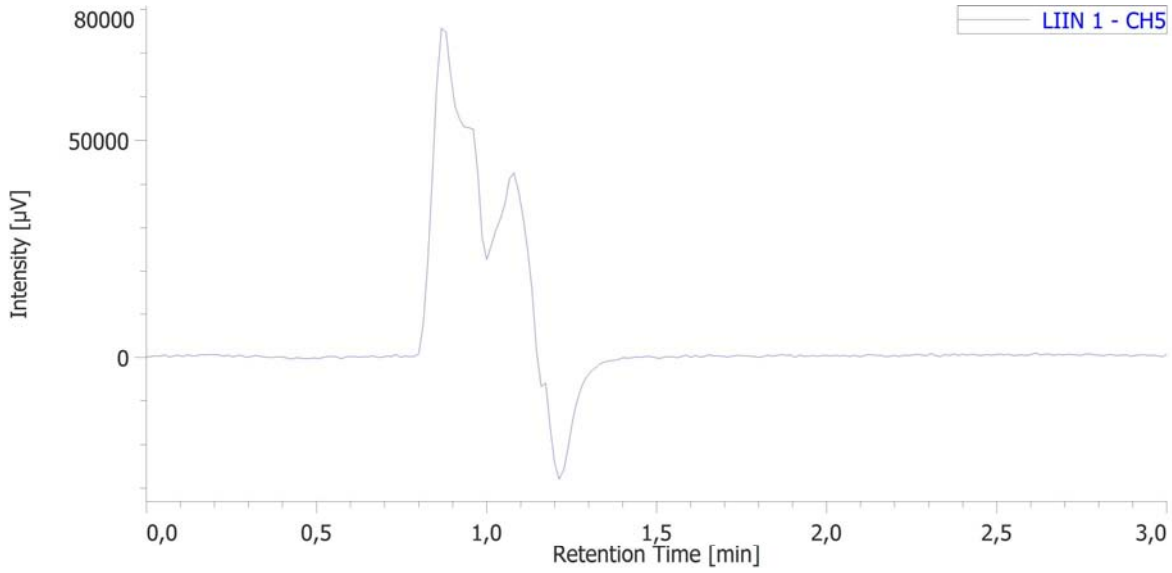


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:34:35
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 15:11:15
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

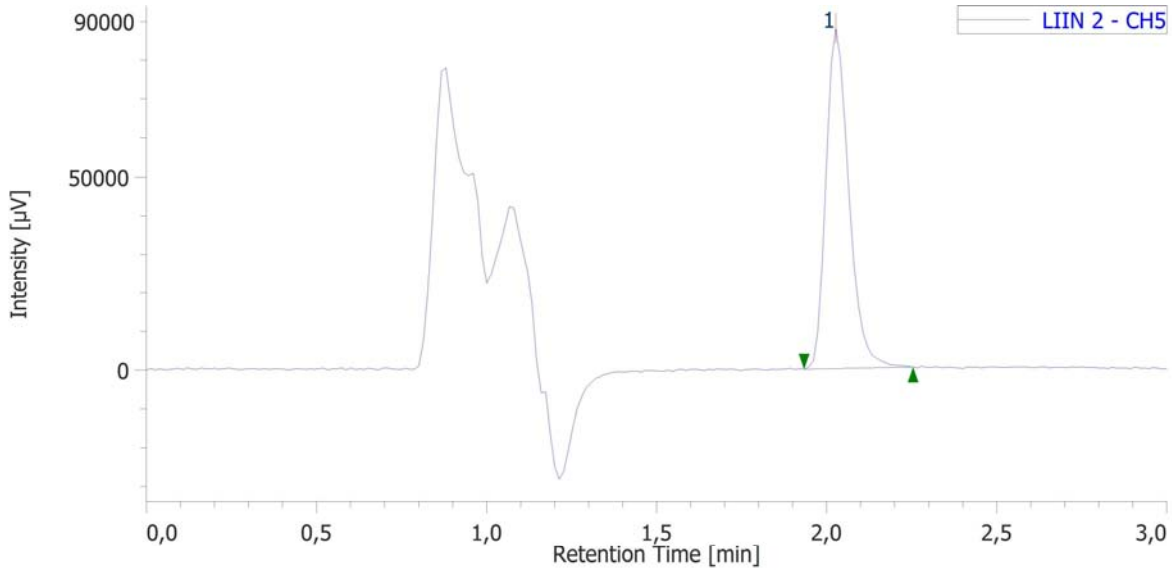


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:34:35
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 15:15:30
Volume	5,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,027	411756	87757	100,000	100,000	N/A	4464	N/A	

Chromatogram

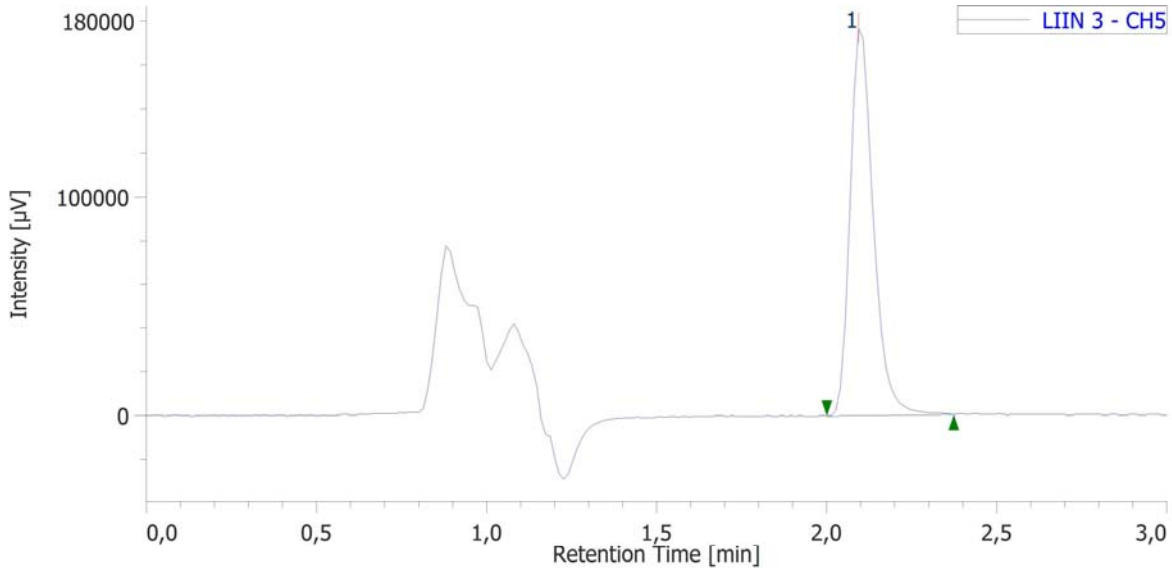


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:34:35
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 15:19:51
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,093	842031	176656	100,000	100,000	N/A	4691	N/A	

Chromatogram

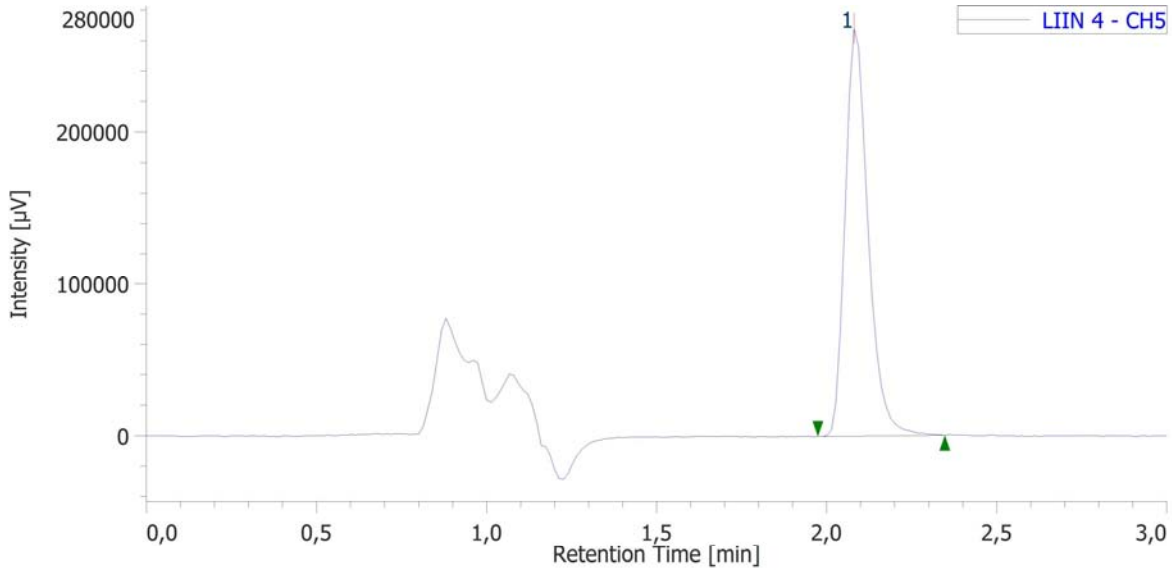


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:34:35
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 15:24:17
Volume	15,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,080	1265698	268164	100,000	100,000	N/A	4695	N/A	

Chromatogram

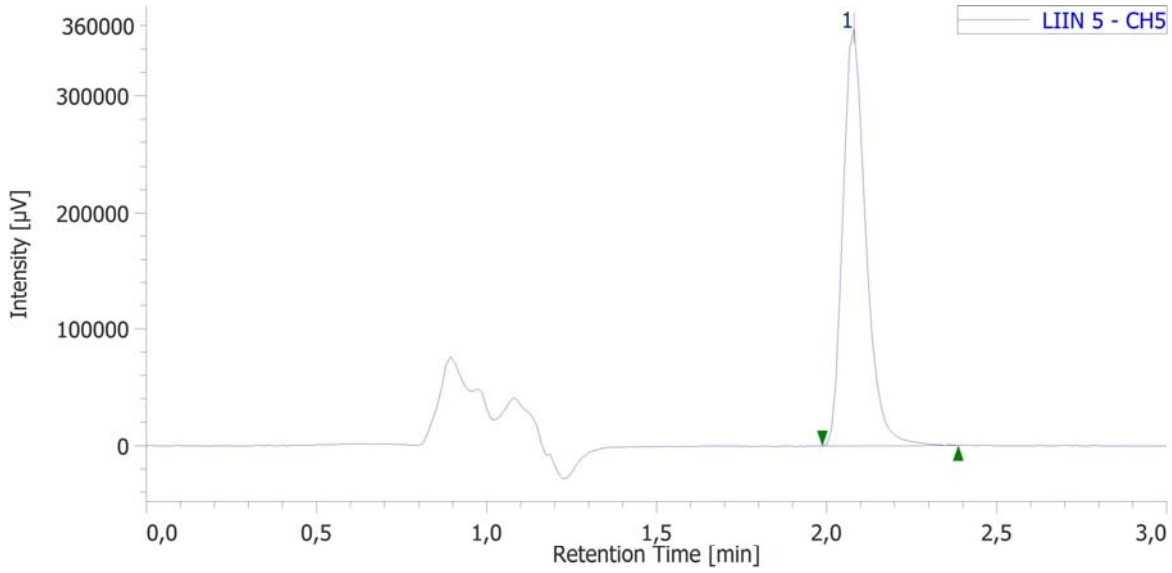


Chromatogram Information	
User Name	Administrator
Date Modified	27/07/2020 15:34:35
Description	
HPLC System Name	CQ 023
Injection Date	27/07/2020 15:28:50
Volume	20,00 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	Curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Warning
1	Cafeina	5	2,080	1683602	357826	100,000	100,000	N/A	4762	N/A	

Chromatogram

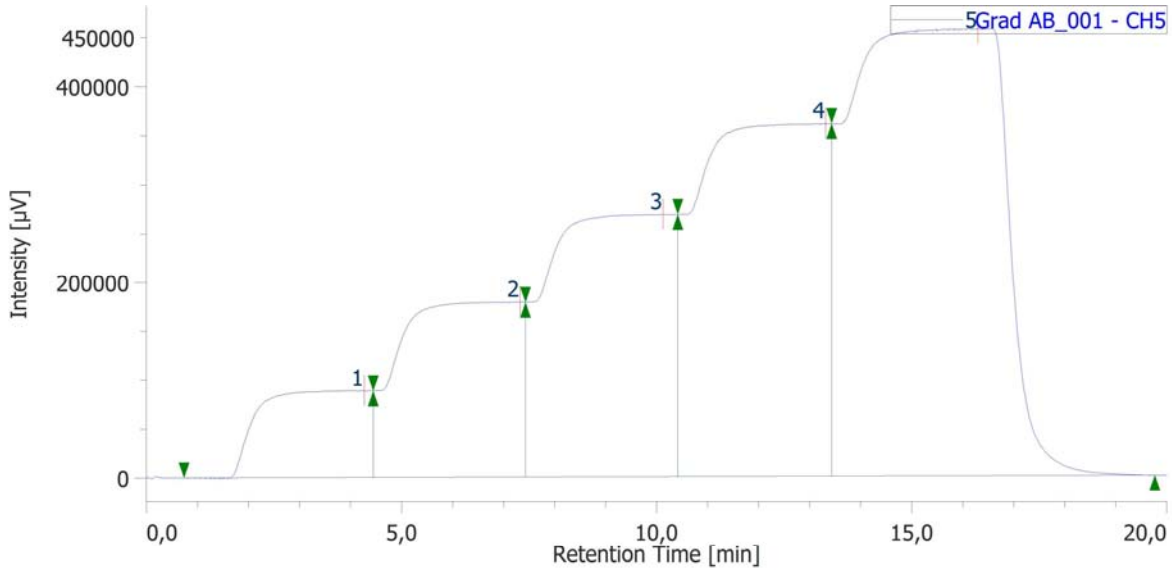


Chromatogram Information	
User Name	Administrator
Date Modified	28/07/2020 10:42:03
Description	
HPLC System Name	CQ 023
Injection Date	28/07/2020 10:18:13
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Warning
1	20 %	5	4,267	88500	6,538	N/A	N/A	N/A	
2	40 %	5	7,320	179101	13,230	N/A	N/A	N/A	
3	60 %	5	10,120	268850	19,860	N/A	N/A	N/A	
4	80 %	5	13,307	360372	26,621	N/A	N/A	N/A	
5	100 %	5	16,293	456891	33,751	N/A	N/A	N/A	

Chromatogram

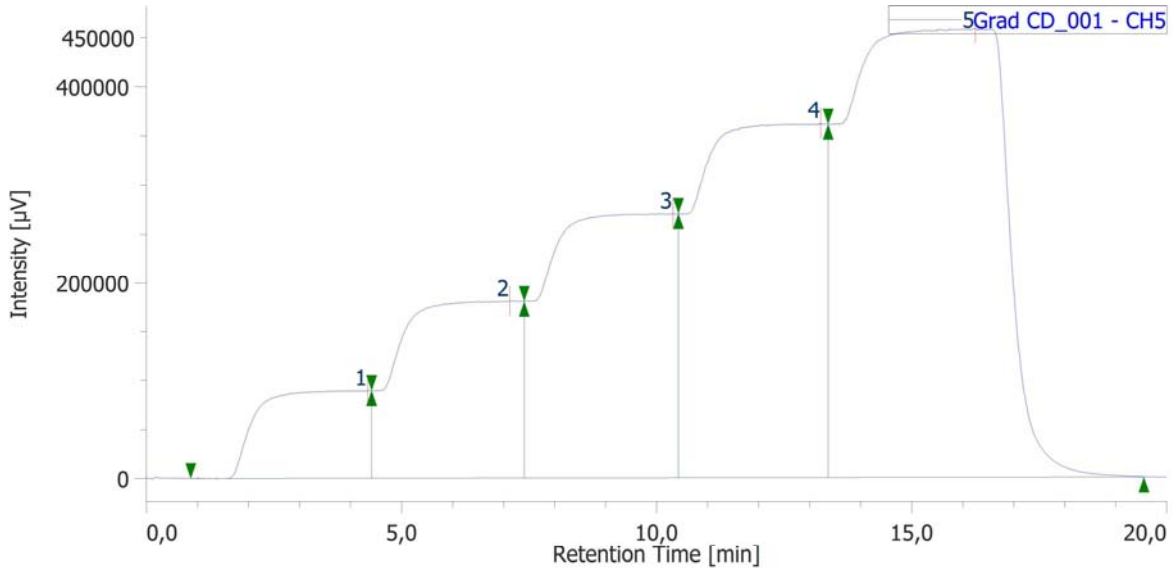

Chromatogram Information	
User Name	Administrator
Date Modified	28/07/2020 11:09:06
Description	
HPLC System Name	CQ 023
Injection Date	28/07/2020 10:44:06
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Warning
1	20 %	5	4,333	89391	6,571	N/A	N/A	N/A	
2	40 %	5	7,120	180748	13,287	N/A	N/A	N/A	
3	60 %	5	10,320	270330	19,872	N/A	N/A	N/A	
4	80 %	5	13,213	361795	26,596	N/A	N/A	N/A	
5	100 %	5	16,240	458069	33,673	N/A	N/A	N/A	