
Peak Find - EDUV_002 UV_tR1,88 D.jws

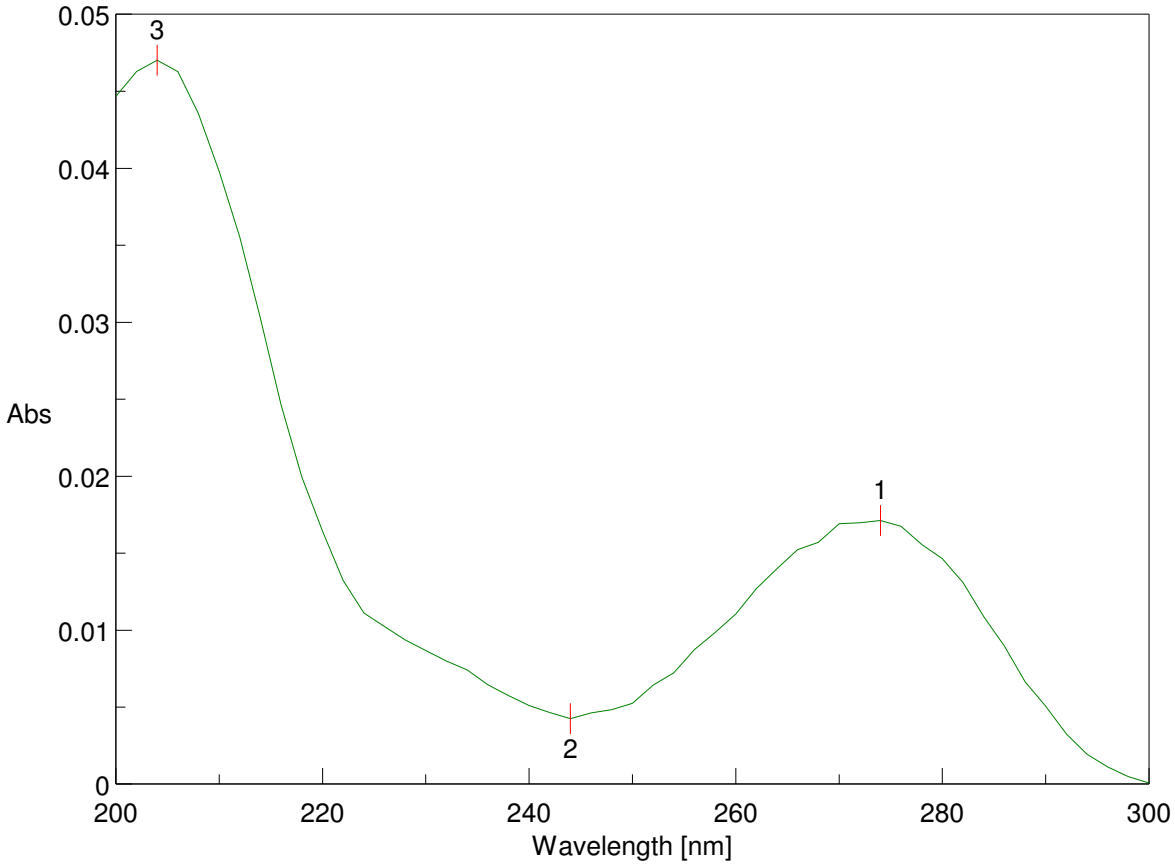

[Comments]

User	Administrator
Division	---
Company	HP Inc.
Creation date	25/08/2020 09:40

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0171145	2	244	0.004246
3	204	0.0469975			

Chromatogram

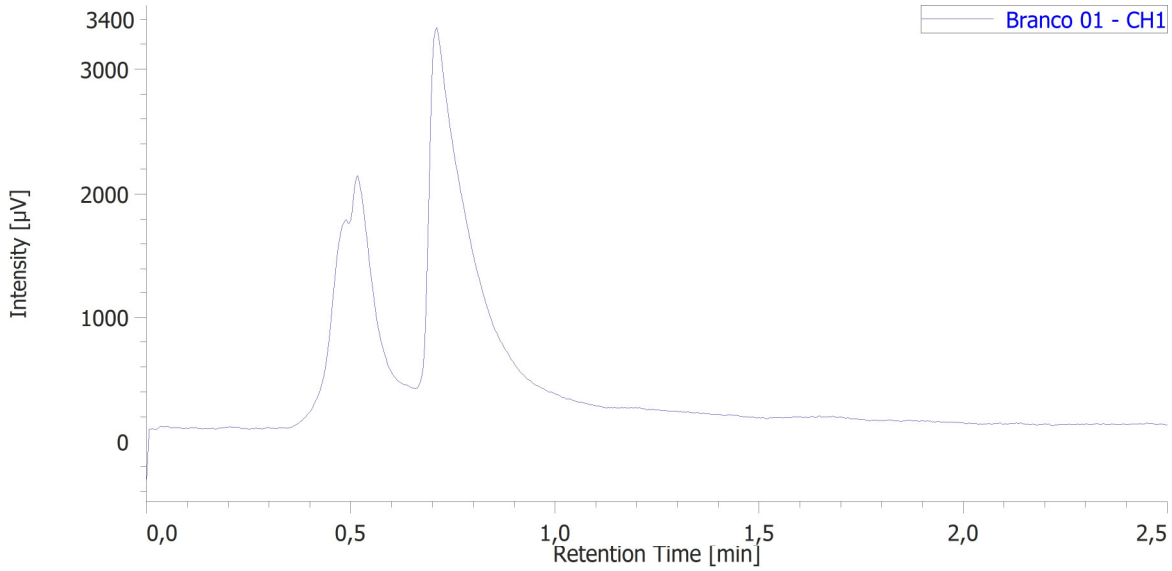


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 09:57:23
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	Branco 01
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

Chromatogram

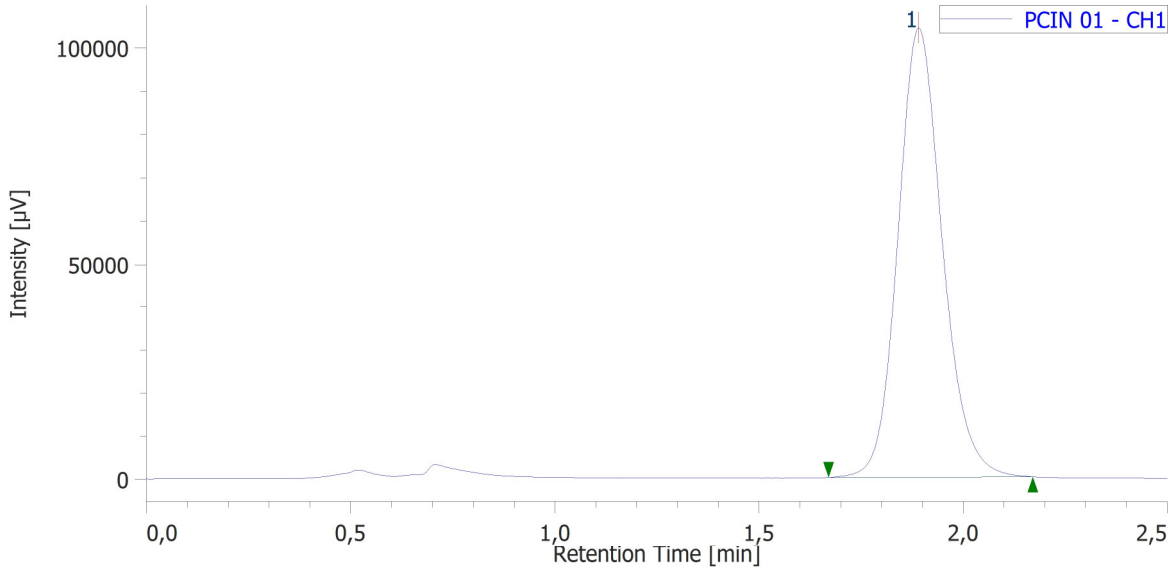


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:01:58
Volume	10,00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	PCIN 01
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,890	785761	104017	100,000	100,000	N/A	1516	N/A	1,153	

Chromatogram

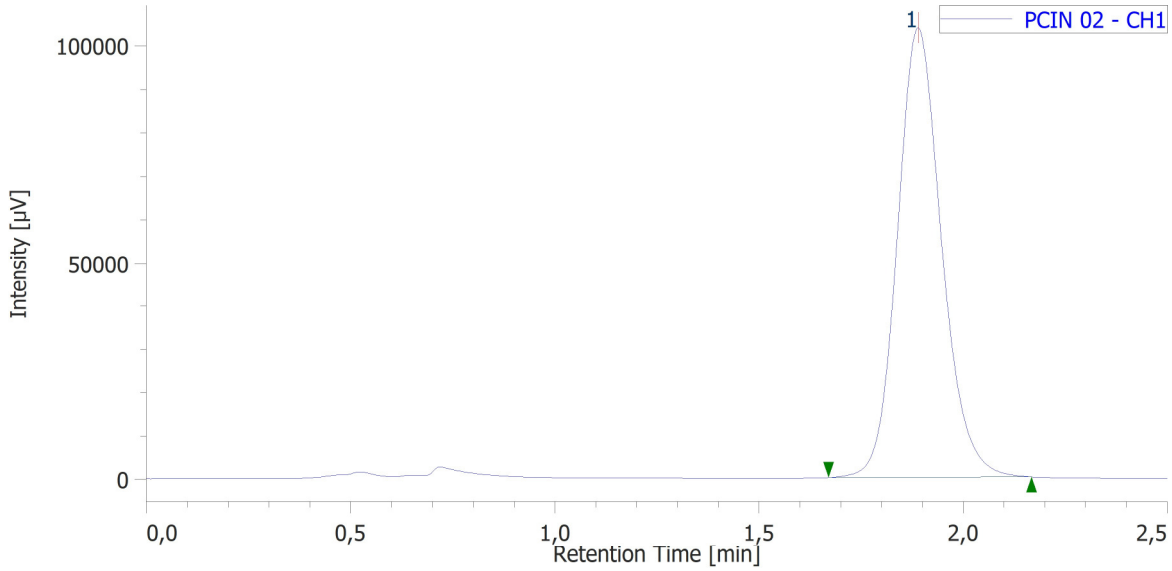


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:06:32
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	PCIN 02
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,890	780352	103580	100,000	100,000	N/A	1525	N/A	1,138	

Chromatogram

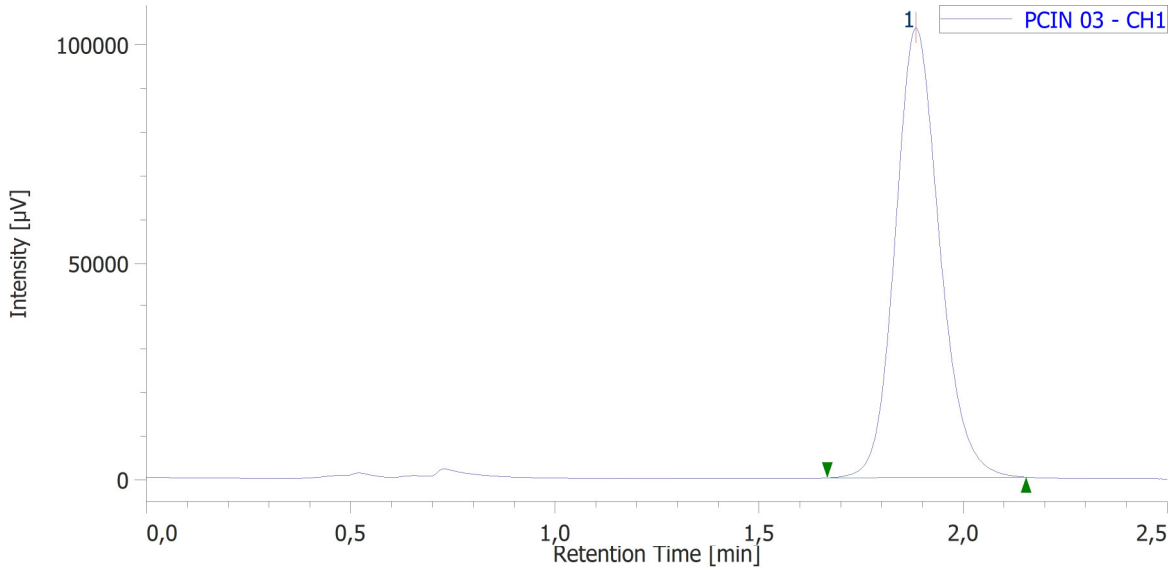


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:11:06
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	PCIN 03
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,883	780117	103301	100,000	100,000	N/A	1502	N/A	1,156	

Chromatogram

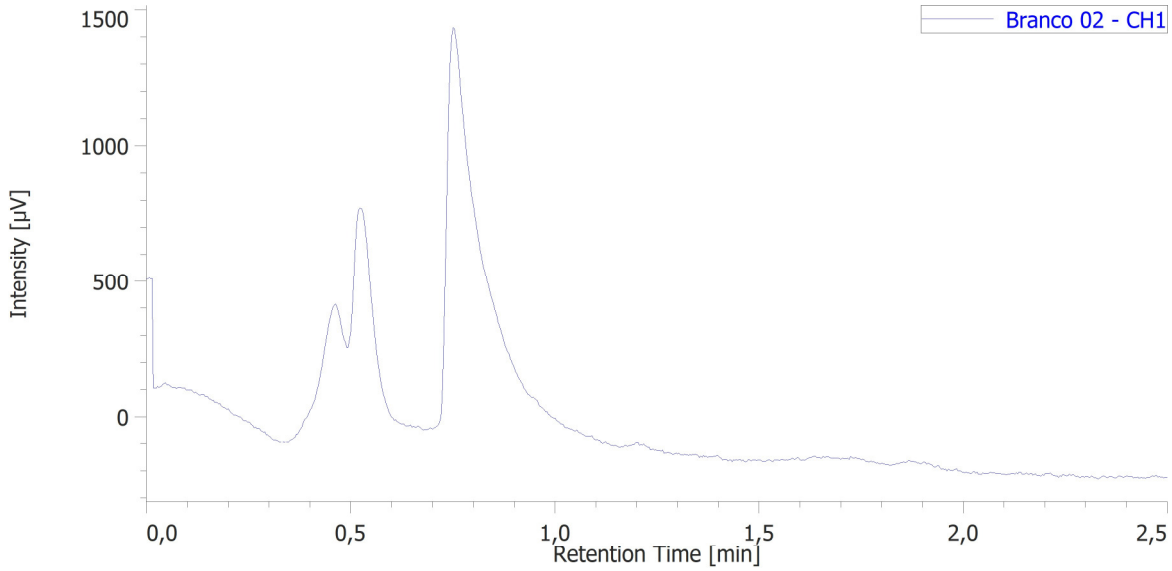


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:15:39
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	Branco 02
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

Chromatogram

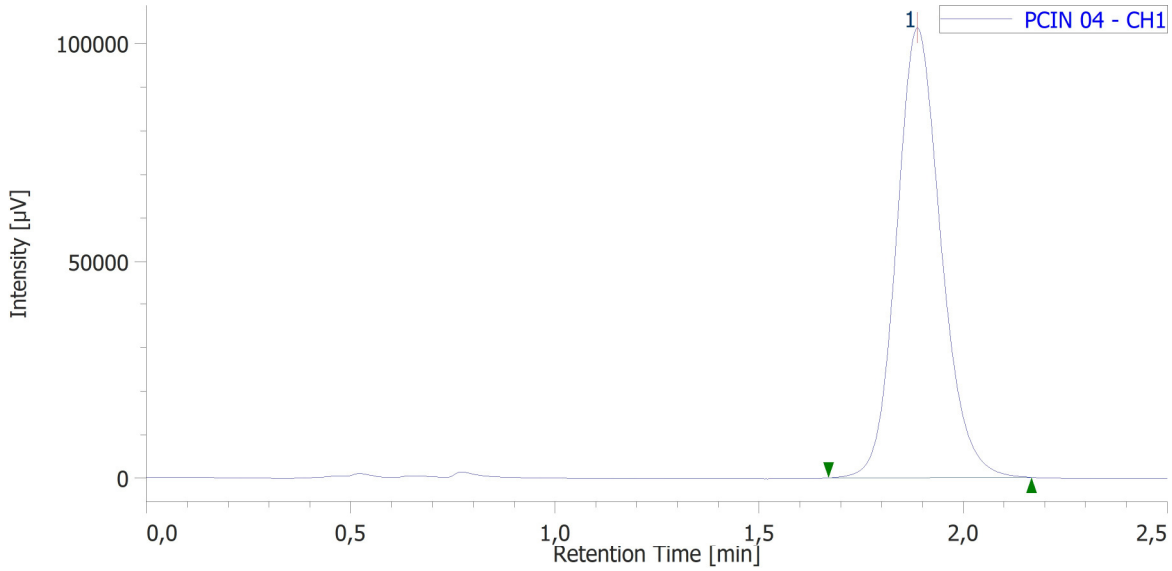


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:20:13
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	PCIN 04
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1.887	782831	103454	100.000	100.000	N/A	1502	N/A	1.152	

Chromatogram

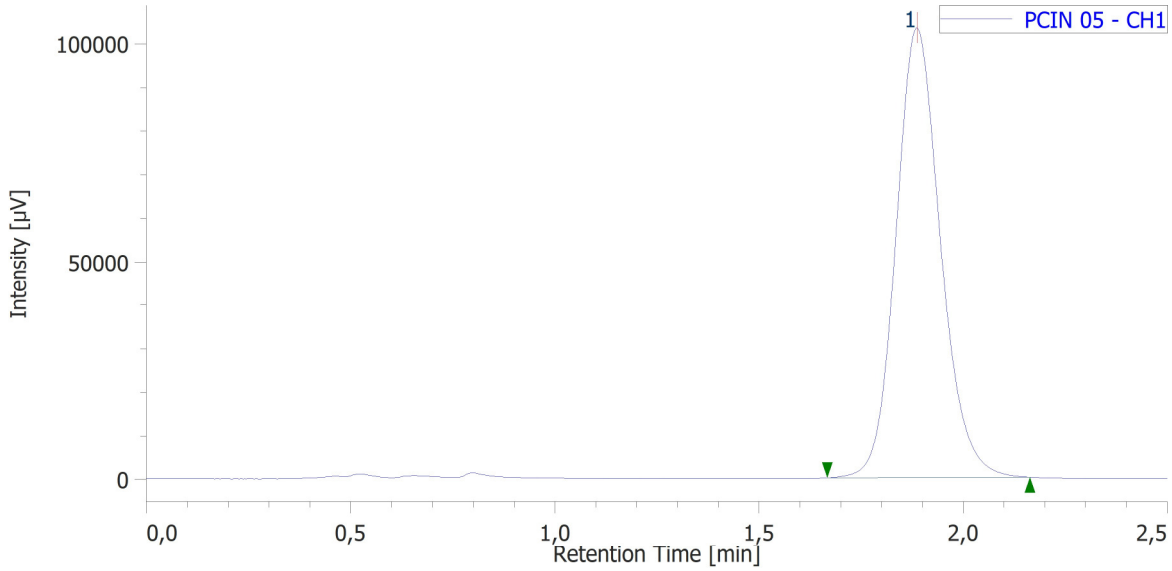


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:24:47
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	PCIN 05
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1.887	782286	103124	100.000	100.000	N/A	1496	N/A	1.137	

Chromatogram

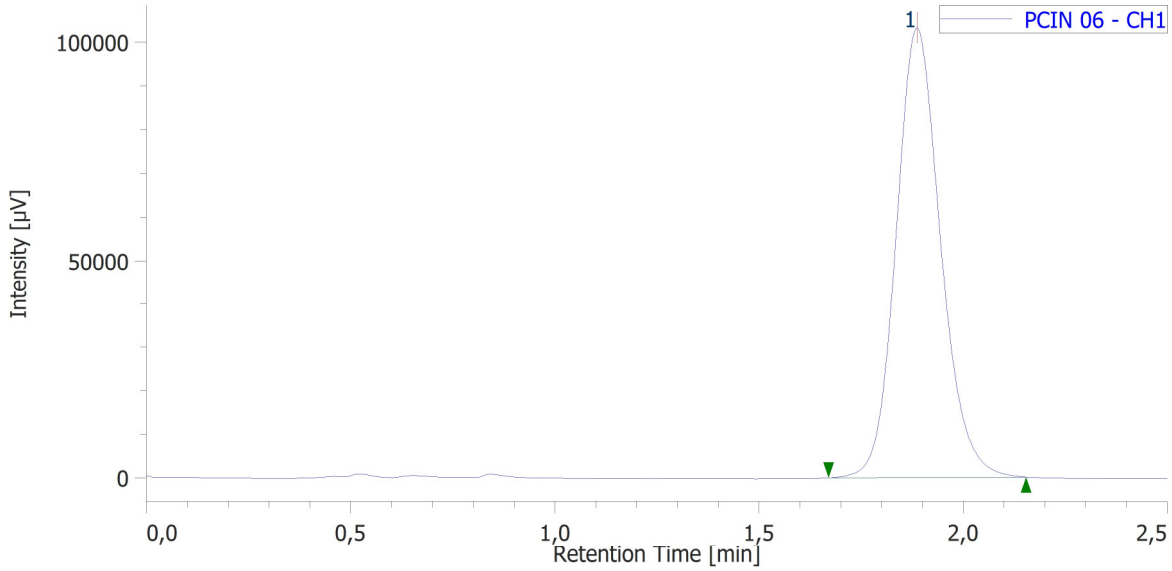


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:37:55
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:29:22
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	PCIN 06
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1.887	780657	103118	100.000	100.000	N/A	1499	N/A	1.140	

Chromatogram

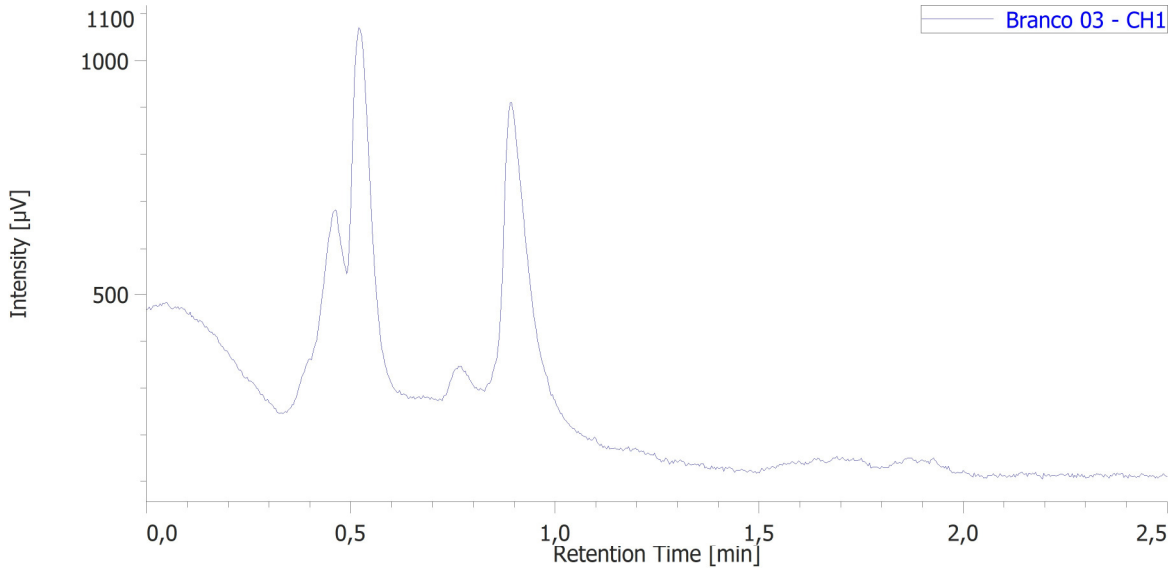


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:36:27
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:33:54
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	Branco 03
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

Chromatogram

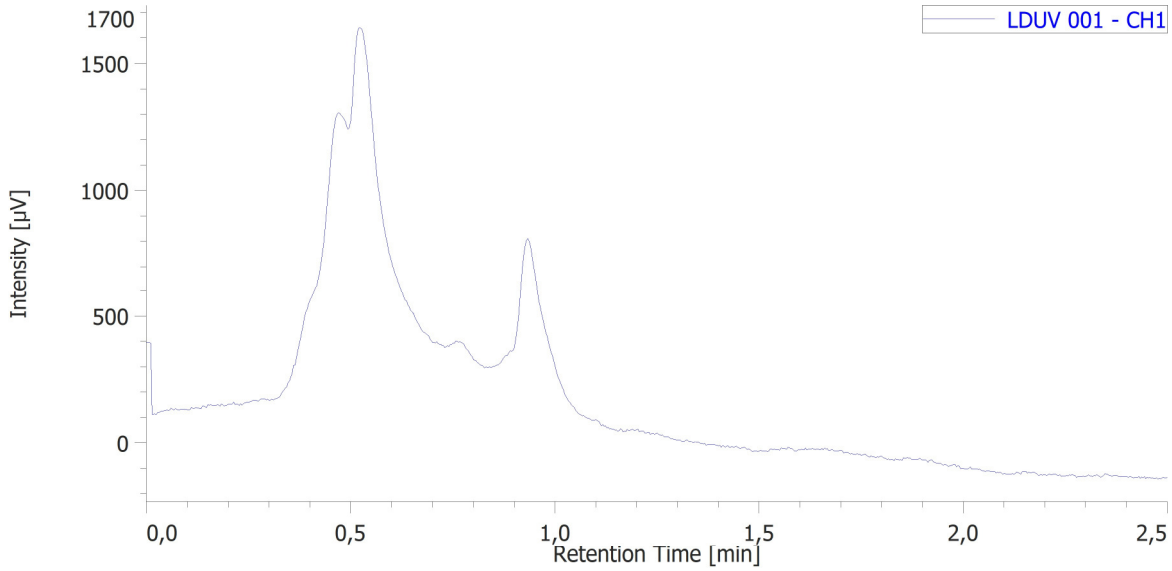


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:48:01
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:45:29
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 001-CH1
Sample Name	LDUV 001
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

Chromatogram

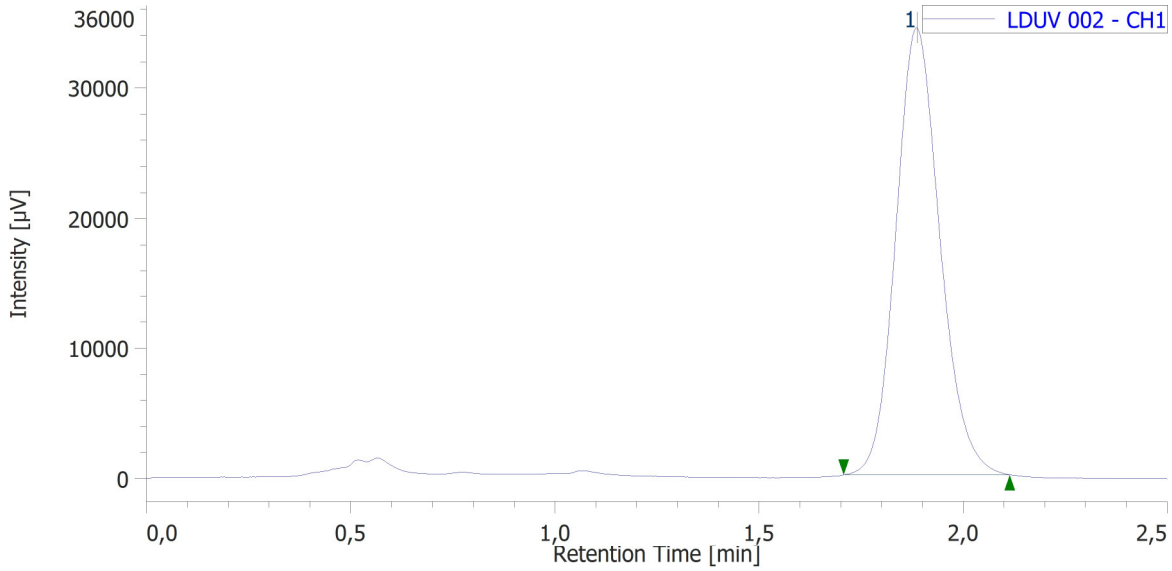


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:52:33
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:50:02
Volume	10.00 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 002-CH1
Sample Name	LDUV 002
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,887	257844	34282	100,000	100,000	N/A	1499	N/A	1,129	

Chromatogram

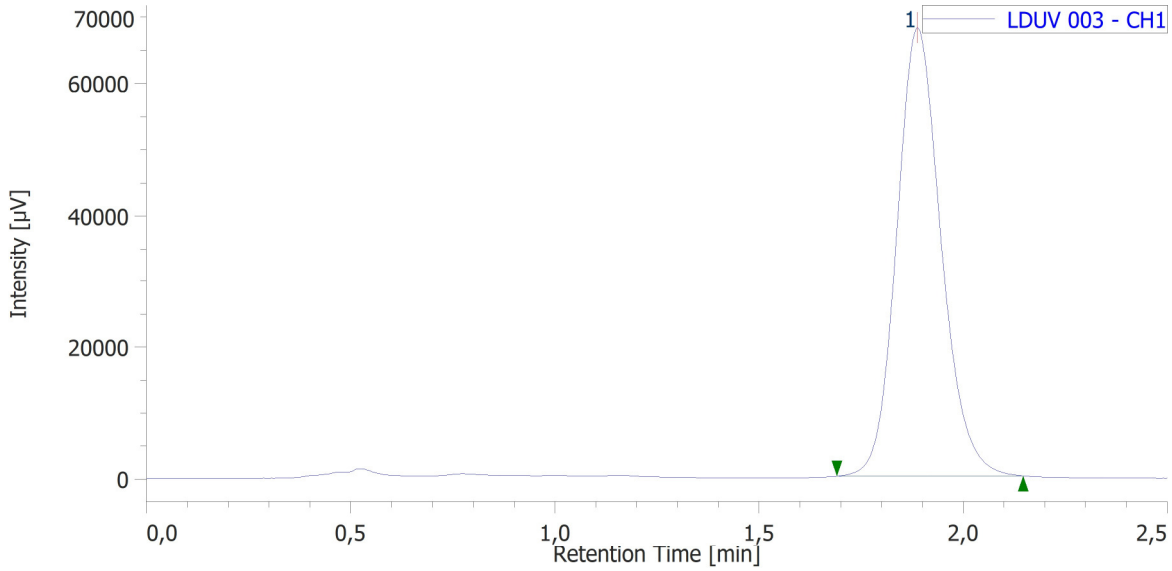


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 10:57:07
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:54:34
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 003-CH1
Sample Name	LDUV 003
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,887	513638	67901	100,000	100,000	N/A	1499	N/A	1,157	

Chromatogram

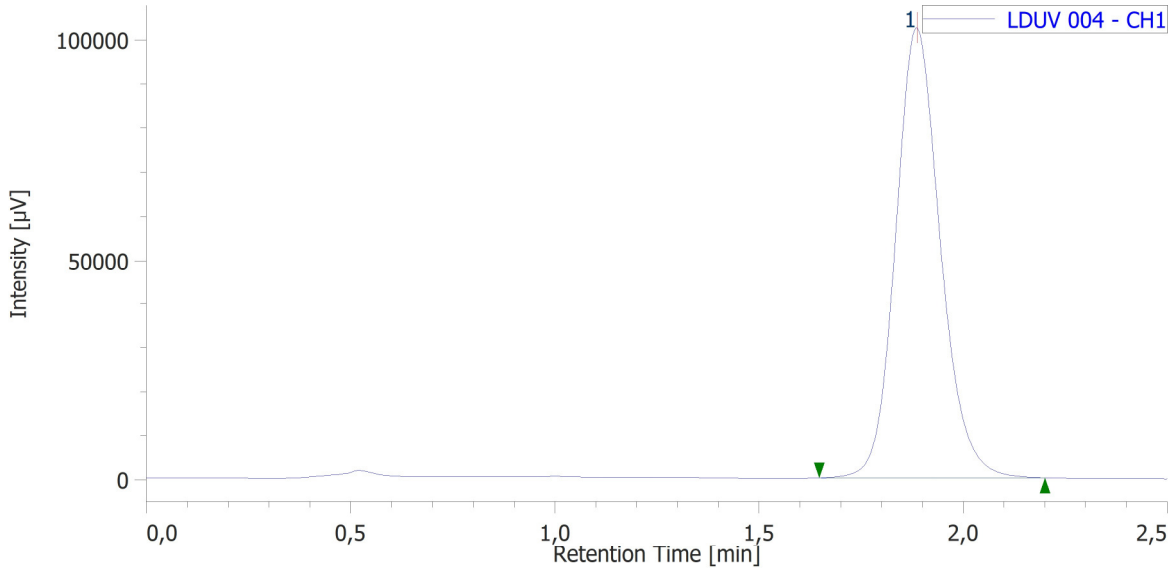


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 11:12:18
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 10:59:08
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação HPLC 1
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 004-CH1
Sample Name	LDUV 004
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,887	778719	102230	100,000	100,000	N/A	1491	N/A	1,133	

Chromatogram

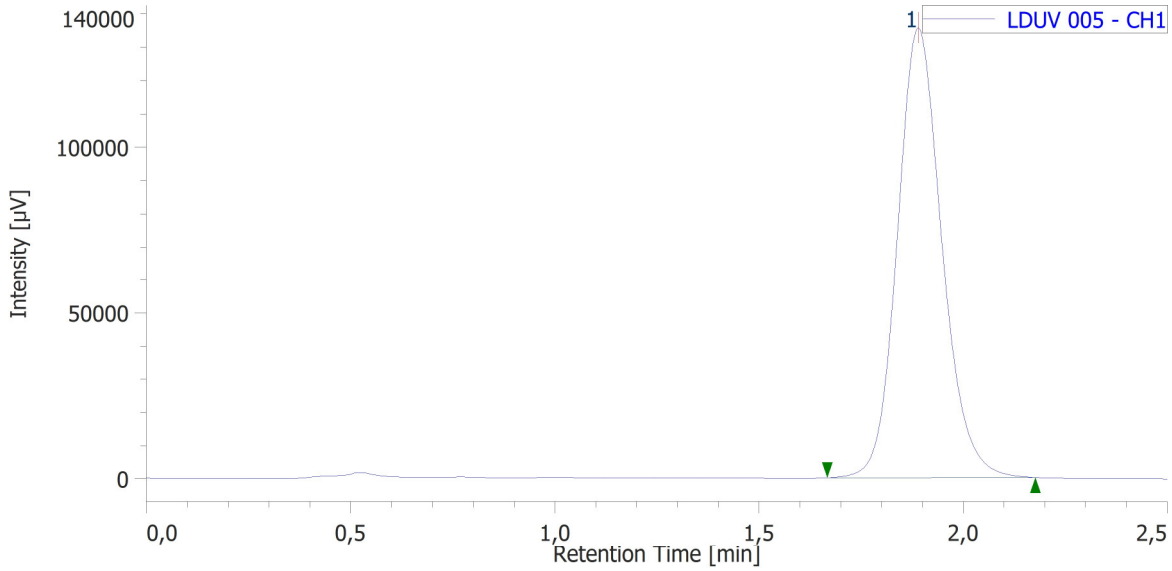


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 11:12:56
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 11:03:43
Volume	10.00 [µL]
Sample #	5
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 005-CH1
Sample Name	LDUV 005
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,890	1026223	135401	100,000	100,000	N/A	1506	N/A	1,138	

Chromatogram

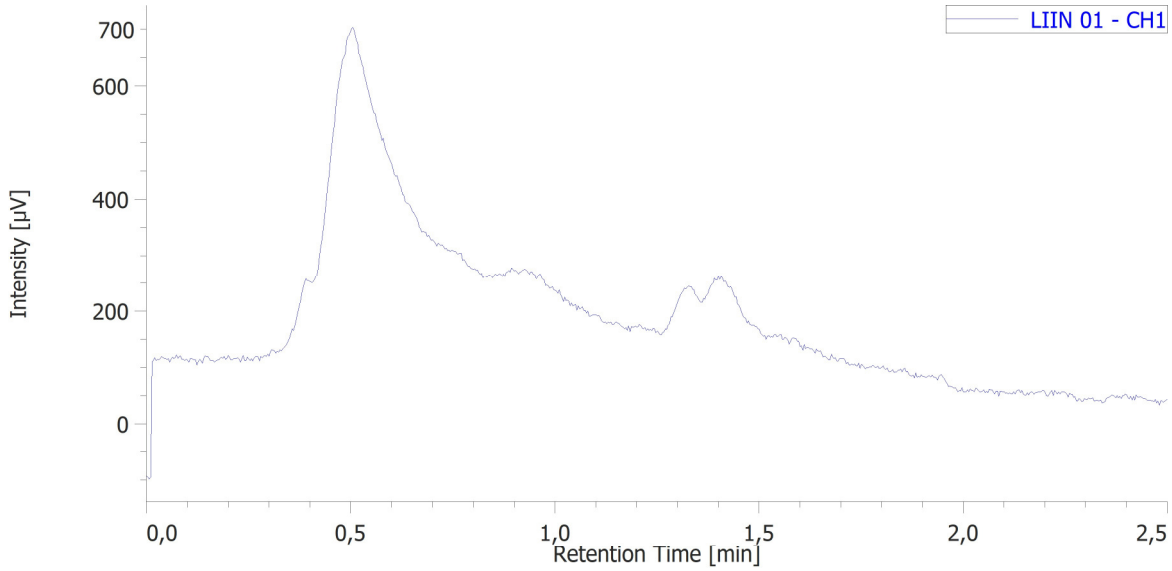


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 11:19:19
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 11:16:46
Volume	0.10 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2.5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	LIIN 01
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

Chromatogram

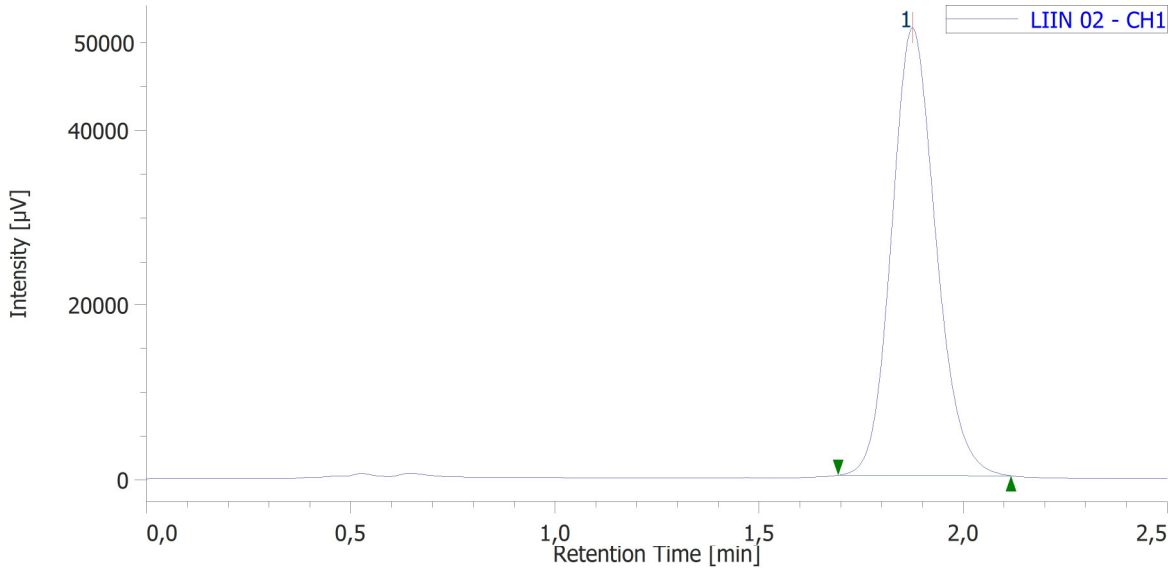


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 11:23:47
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 11:21:14
Volume	5,00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	LIIN 02
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,877	386480	51169	100,000	100,000	N/A	1473	N/A	1,127	

Chromatogram

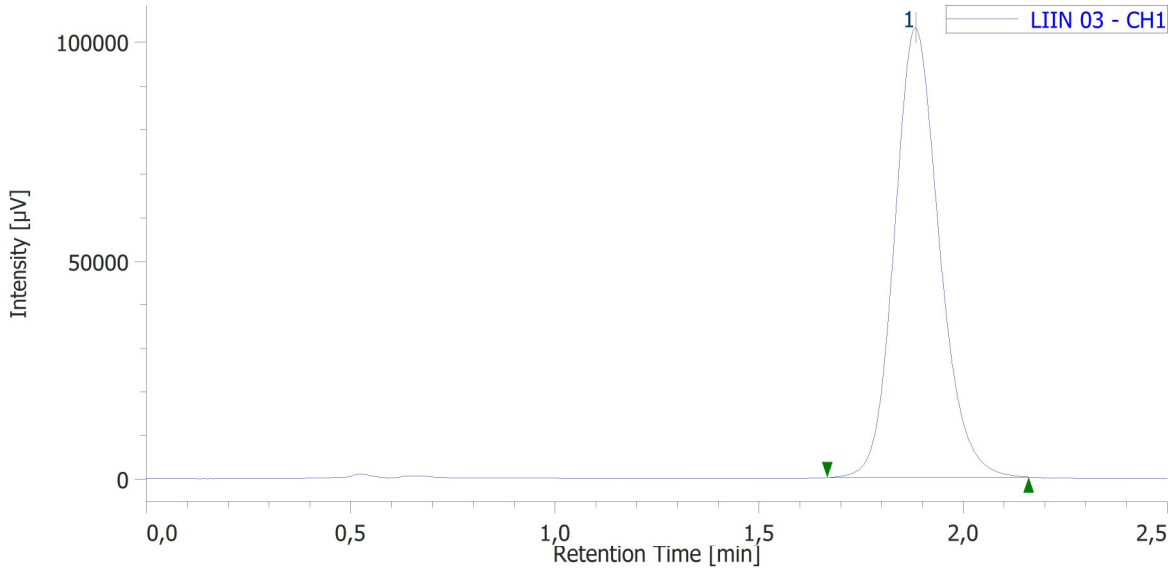


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 11:28:21
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 11:25:48
Volume	10,00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	LIIN 03
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,883	784358	102745	100,000	100,000	N/A	1469	N/A	1,144	

Chromatogram

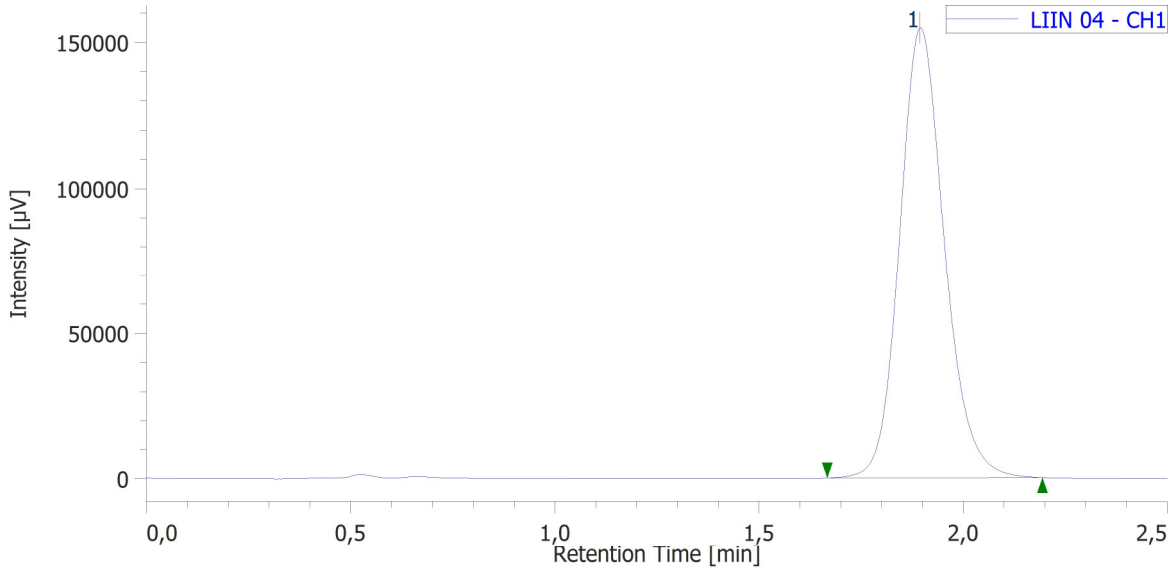


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 11:32:59
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 11:30:27
Volume	15,00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	LIIN 04
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,893	1178164	154594	100,000	100,000	N/A	1500	N/A	1,173	

Chromatogram

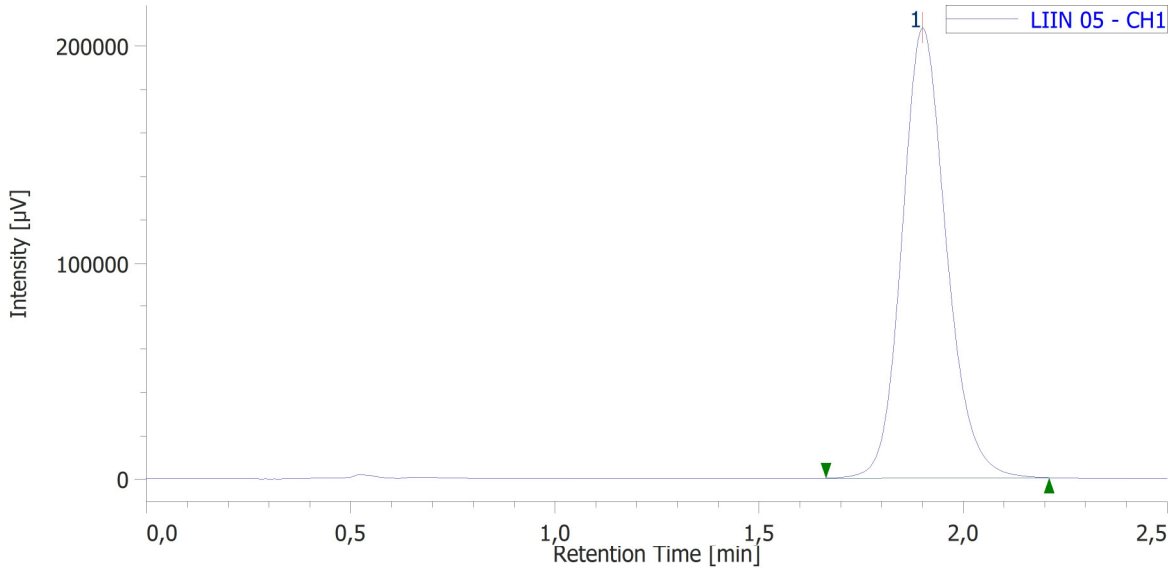


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 11:37:42
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 11:35:11
Volume	20,00 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	LIIN 05
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,900	1569876	207676	100,000	100,000	N/A	1538	N/A	1,159	

Chromatogram

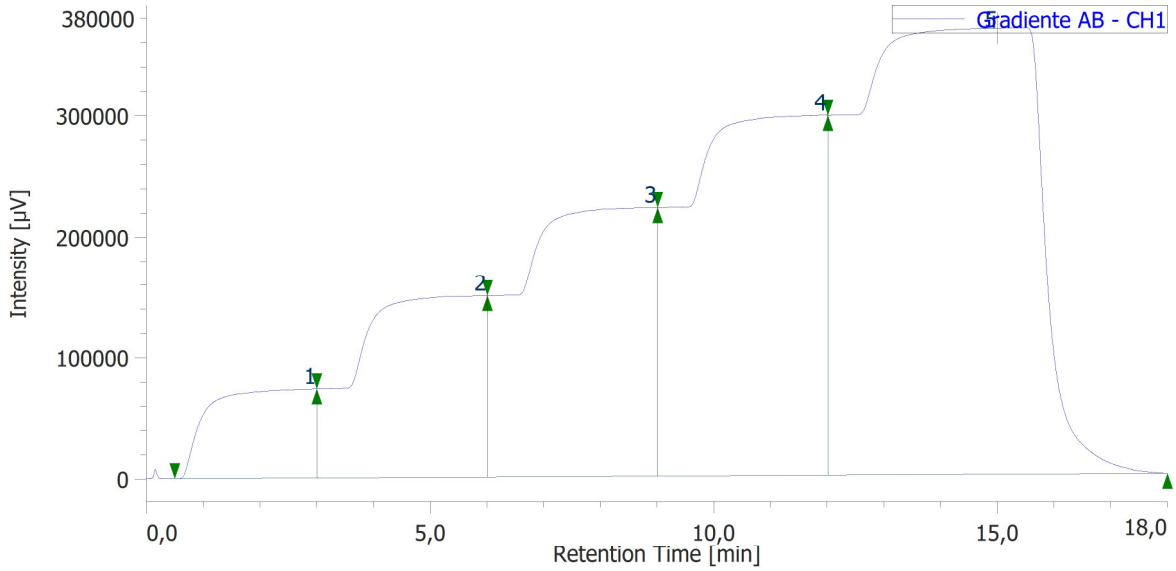

Chromatogram Information


User Name	Administrator
Date Modified	25/08/2020 14:04:45
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 13:00:12
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	18,0 [min]
Acquisition Sequence	Gradiente
Control Method	Teste de Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB-CH1
Sample Name	Gradiente AB
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,000	9018518	73633	4,509	6,631	N/A	N/A	N/A	N/A	
2	40%	1	6,000	22740060	149558	11,369	13,468	N/A	N/A	N/A	N/A	
3	60%	1	9,000	36017553	222346	18,008	20,023	N/A	N/A	N/A	N/A	
4	80%	1	12,000	49359820	297080	24,679	26,753	N/A	N/A	N/A	N/A	
5	100%	1	15,000	82875085	367818	41,435	33,124	N/A	N/A	N/A	N/A	

Chromatogram

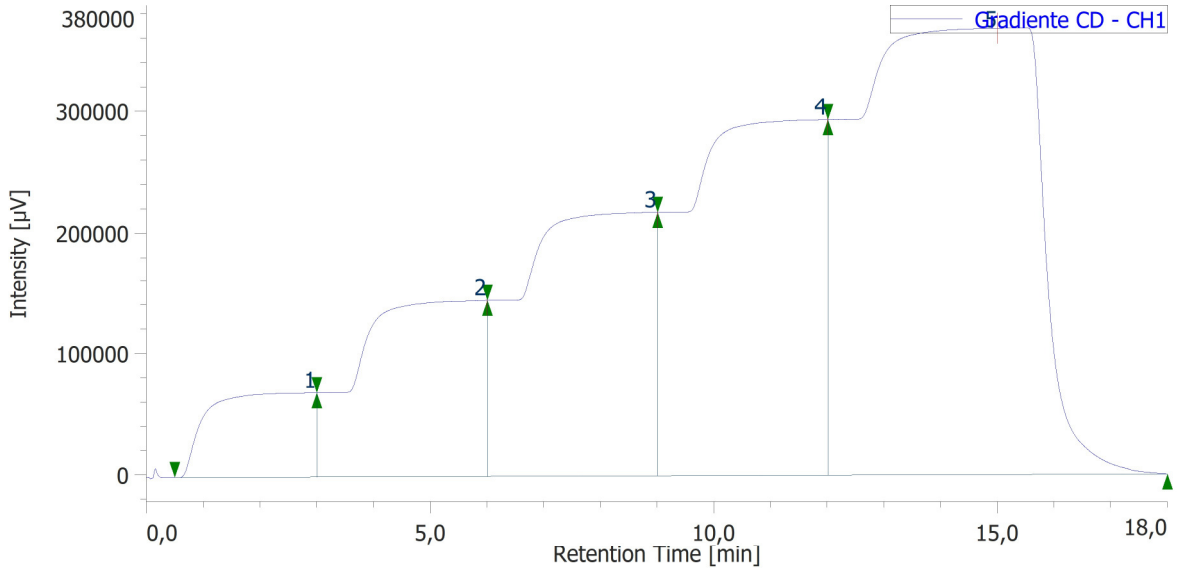

Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2020 14:04:45
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2020 13:40:48
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	18,0 [min]
Acquisition Sequence	Gradiente
Control Method	Teste de Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD-CH1
Sample Name	Gradiente CD
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,000	8550723	69538	4,347	6,365	N/A	N/A	N/A	N/A	
2	40%	1	6,000	21894833	144833	11,130	13,257	N/A	N/A	N/A	N/A	
3	60%	1	9,000	35131683	217554	17,859	19,913	N/A	N/A	N/A	N/A	
4	80%	1	12,000	48559445	293111	24,685	26,829	N/A	N/A	N/A	N/A	
5	100%	1	15,000	82577690	367461	41,978	33,635	N/A	N/A	N/A	N/A	