
Chromatogram

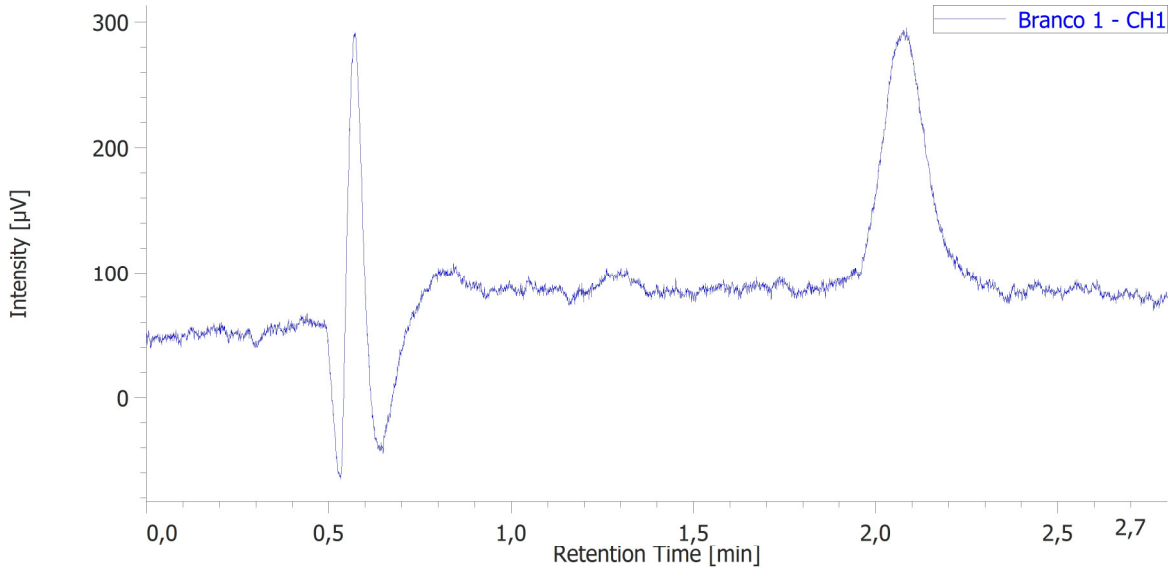


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:40
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 15:50:45
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

Chromatogram

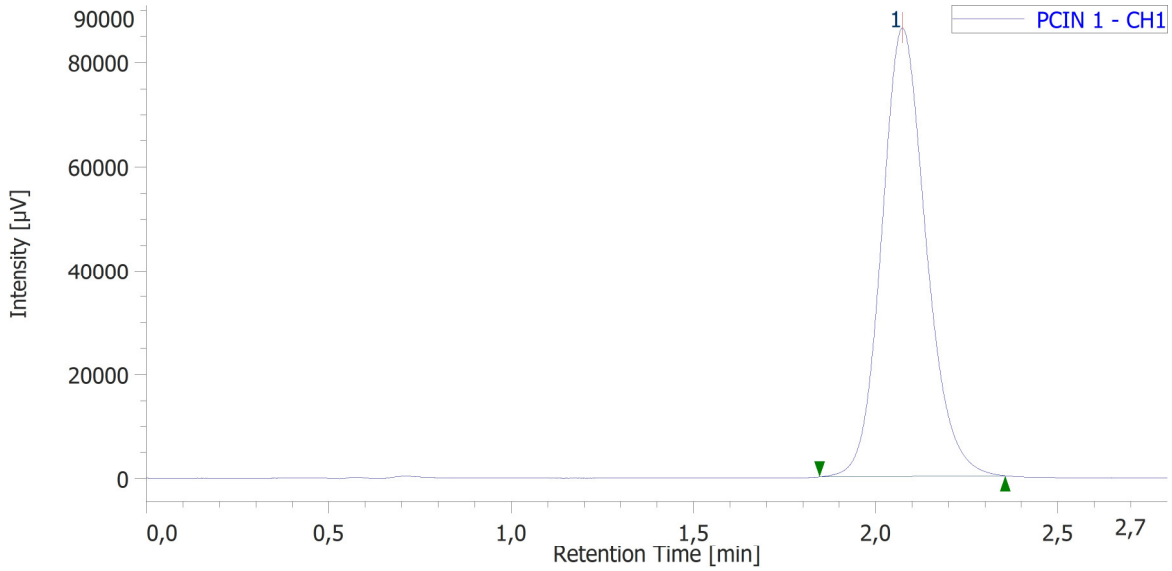


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:40
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 15:54:01
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.073	729839	86153	100.000	100.000	N/A	1445	N/A	1.142	

Chromatogram

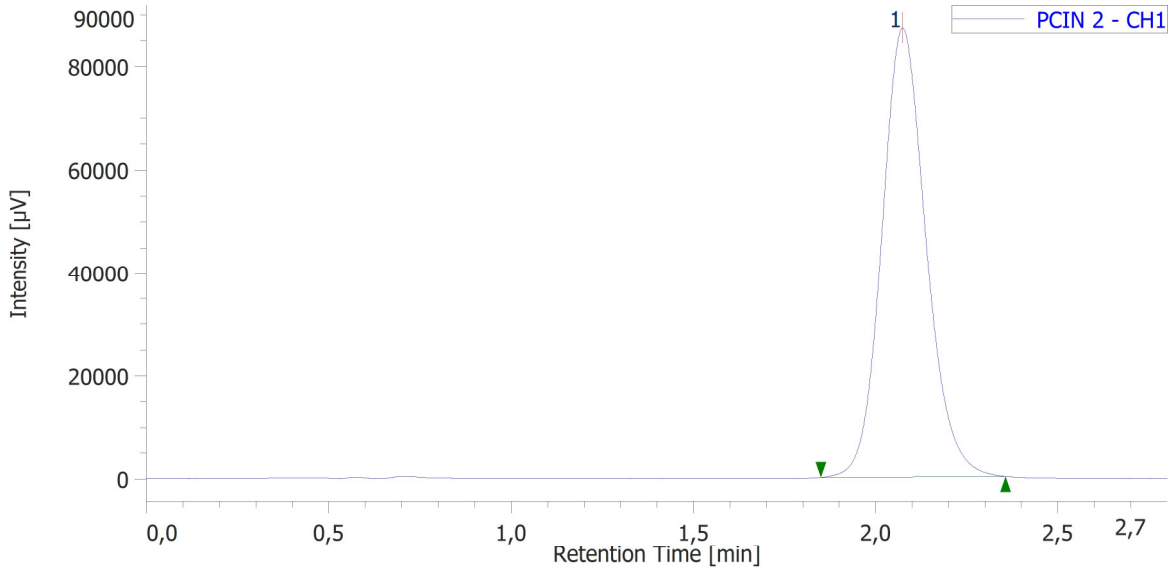


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:41
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 15:57:16
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.073	734058	87030	100.000	100.000	N/A	1454	N/A	1.144	

Chromatogram

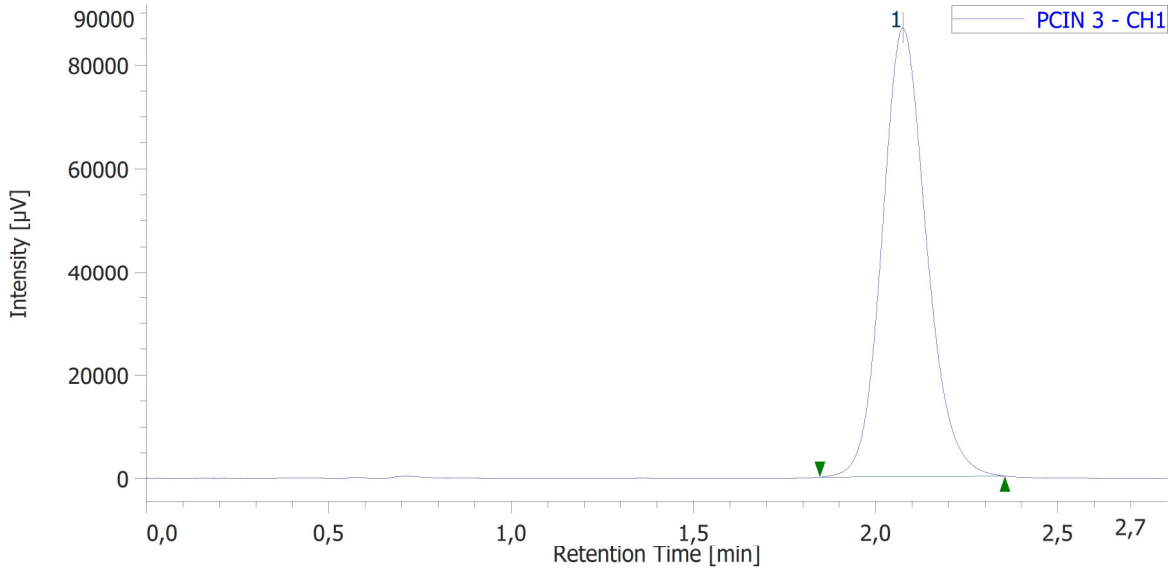


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:41
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:00:34
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.074	733219	86716	100.000	100.000	N/A	1449	N/A	1.143	

Chromatogram

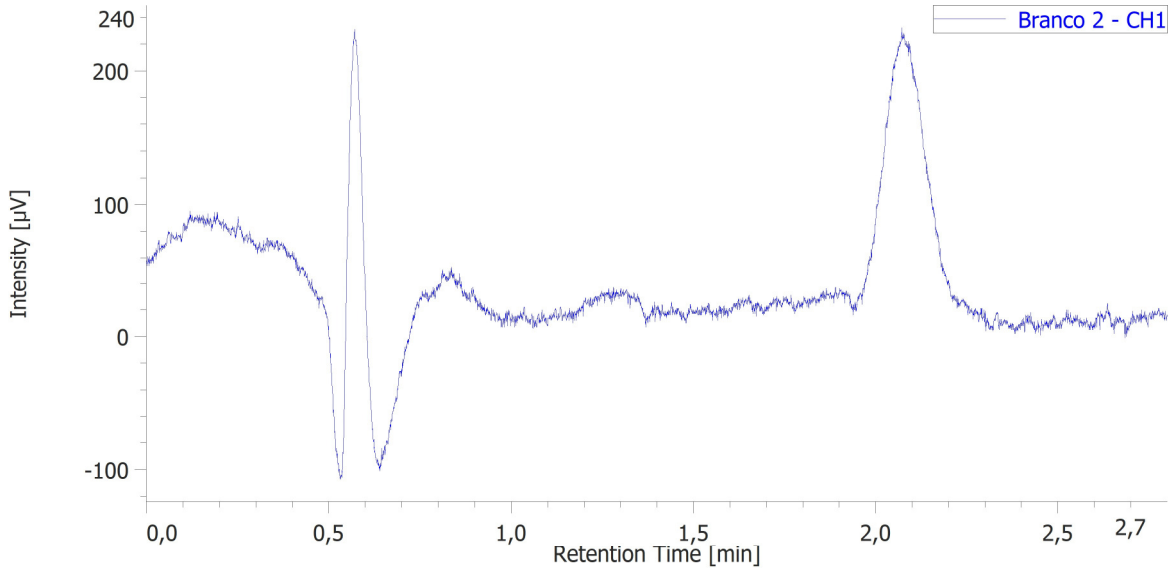


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:41
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:03:52
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

Chromatogram

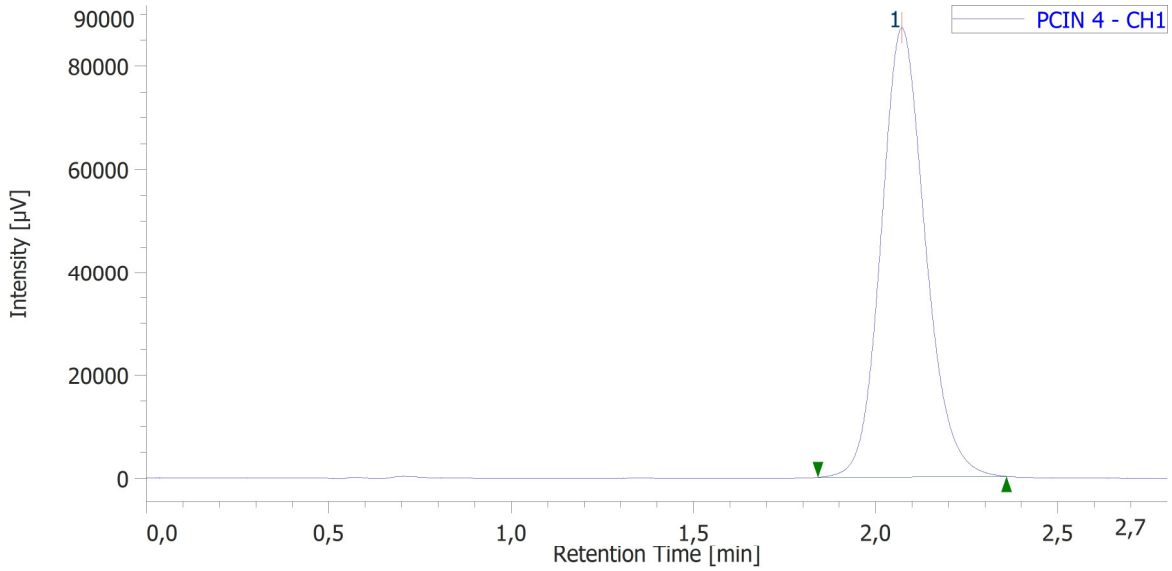


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:41
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:07:08
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.071	734605	87035	100.000	100.000	N/A	1453	N/A	1.141	

Chromatogram

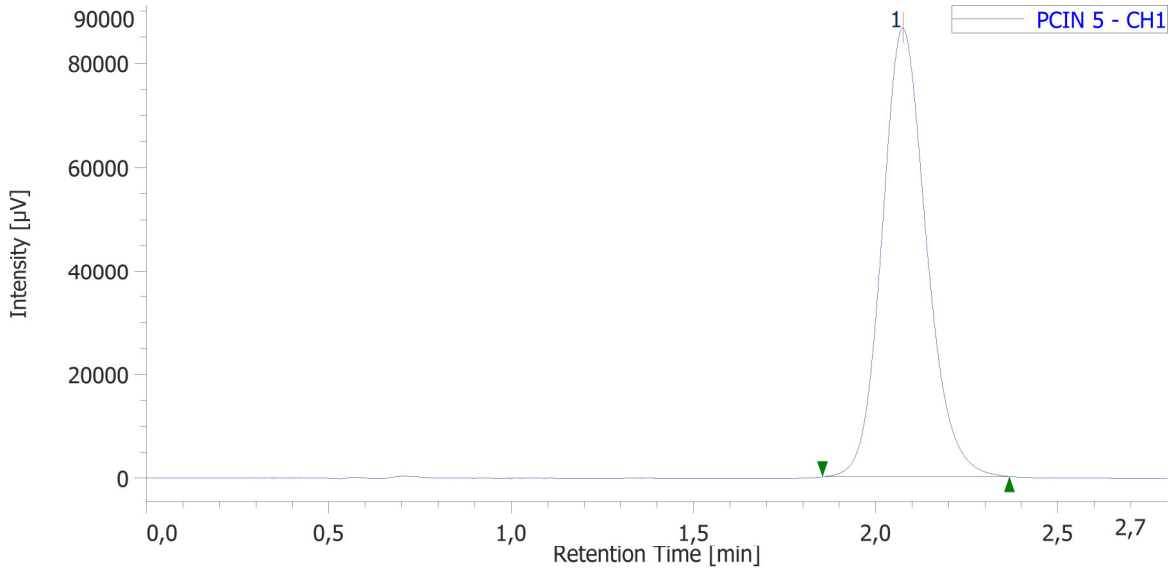


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:41
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:10:26
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.074	733089	86462	100.000	100.000	N/A	1443	N/A	1.144	

Chromatogram

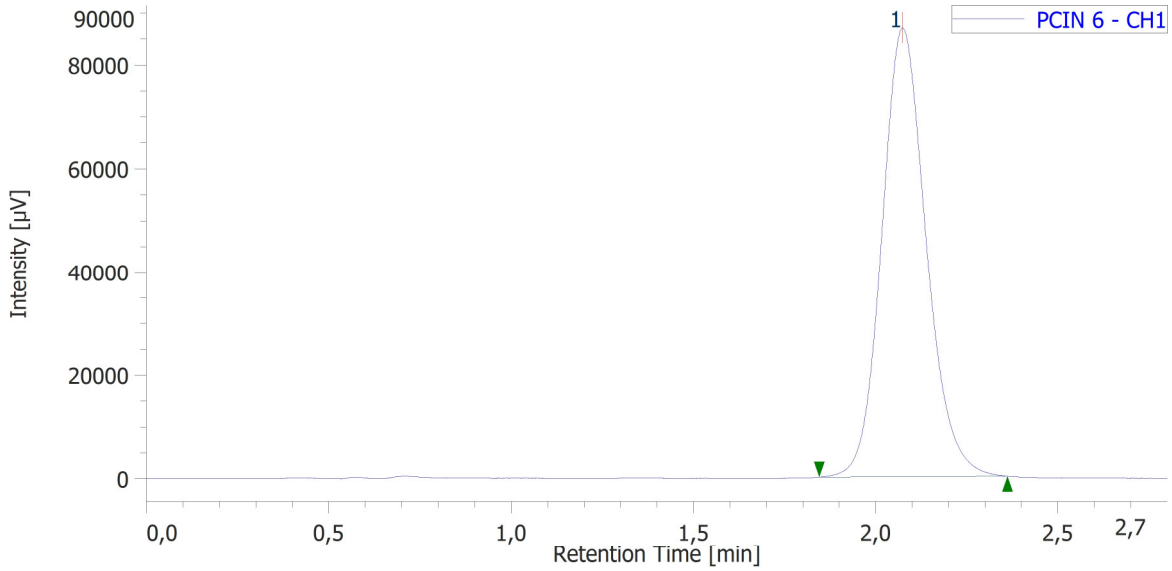


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:41
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:13:42
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.073	733755	86710	100.000	100.000	N/A	1447	N/A	1.142	

Chromatogram

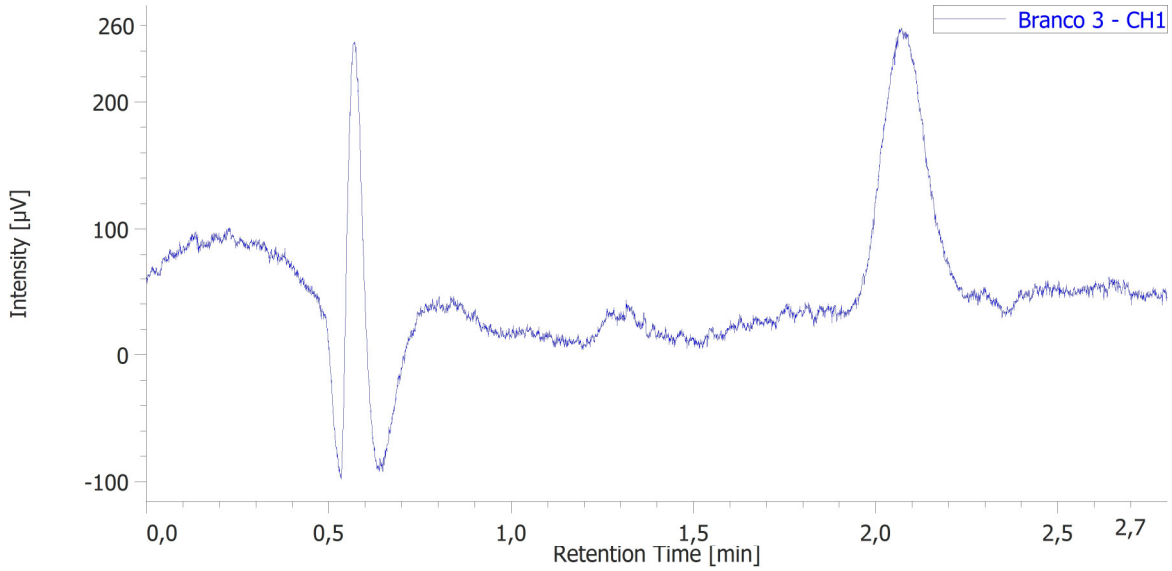


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:20:41
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:16:57
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

Chromatogram

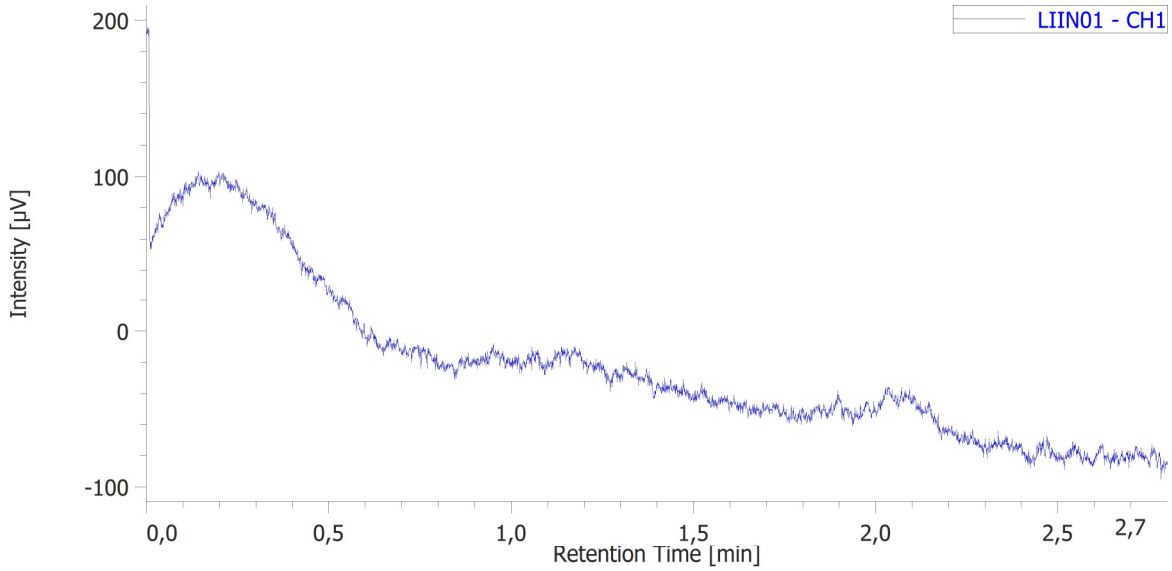


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:26:21
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:23:29
Volume	0.10 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN01-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

Chromatogram

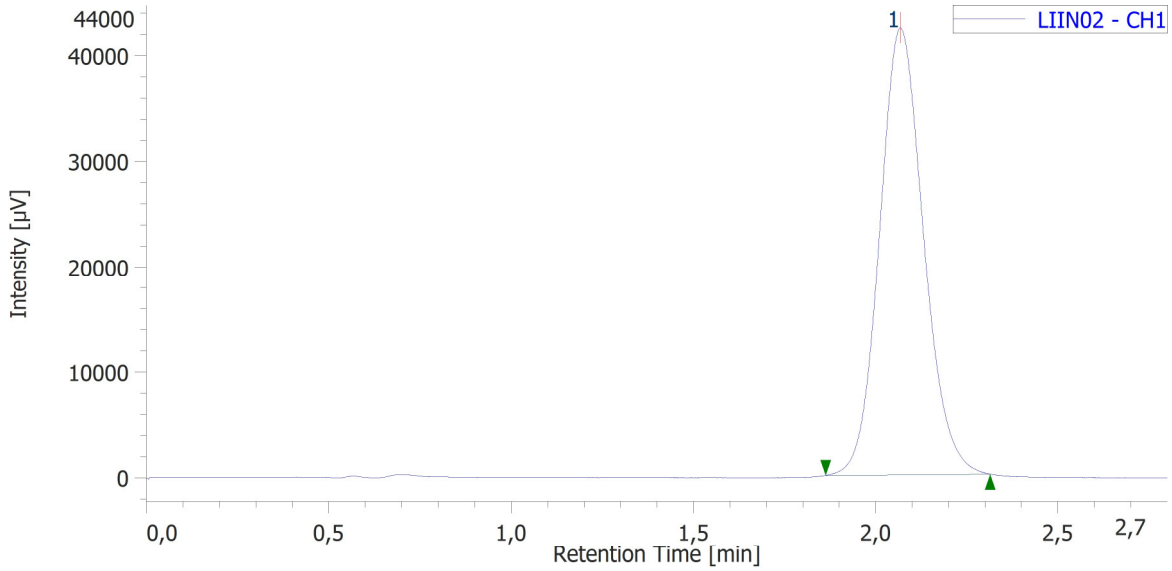


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:29:33
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:26:42
Volume	5,00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2,8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN02-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,067	355090	42318	100,000	100,000	N/A	1438	N/A	1,118	

Chromatogram

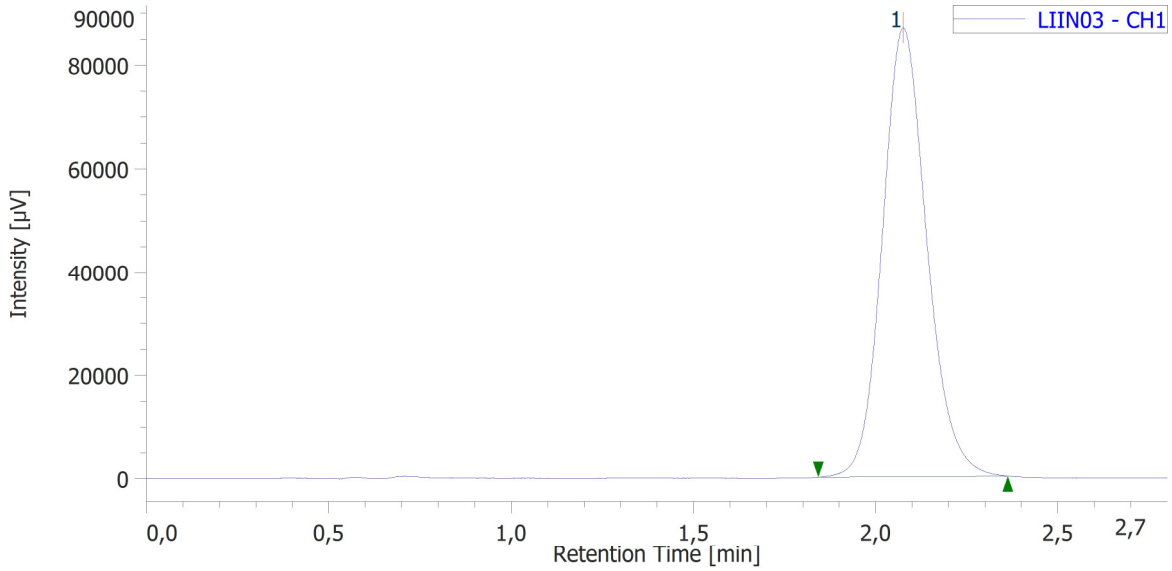


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:32:50
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:30:00
Volume	10.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN03-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.075	735908	86729	100.000	100.000	N/A	1443	N/A	1.145	

Chromatogram

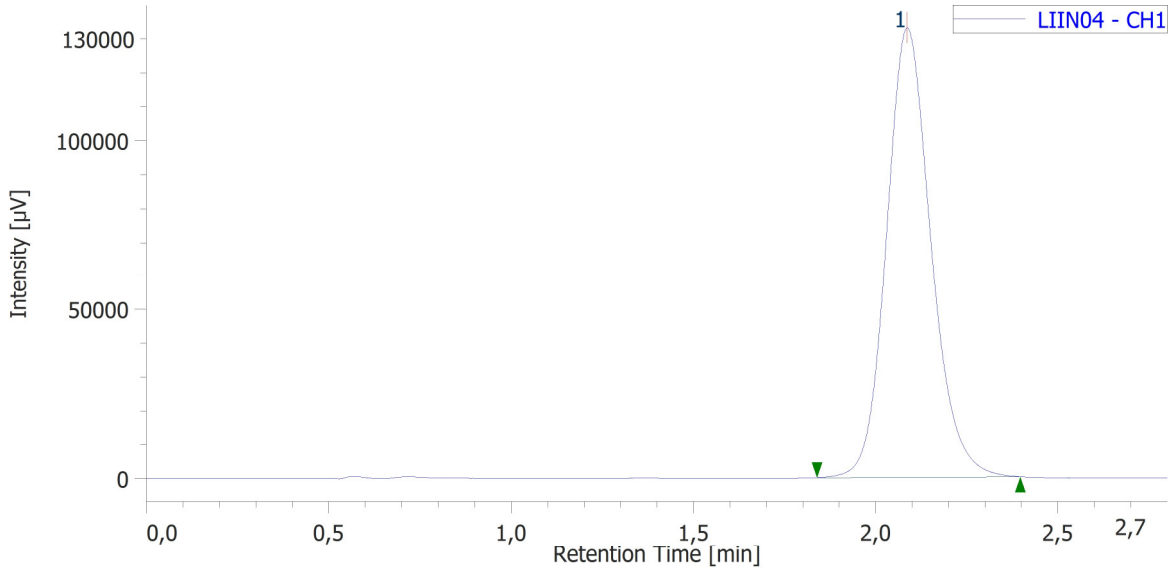


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:36:12
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:33:21
Volume	15,00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2,8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN04-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,086	1126833	132734	100,000	100,000	N/A	1470	N/A	1,154	

Chromatogram

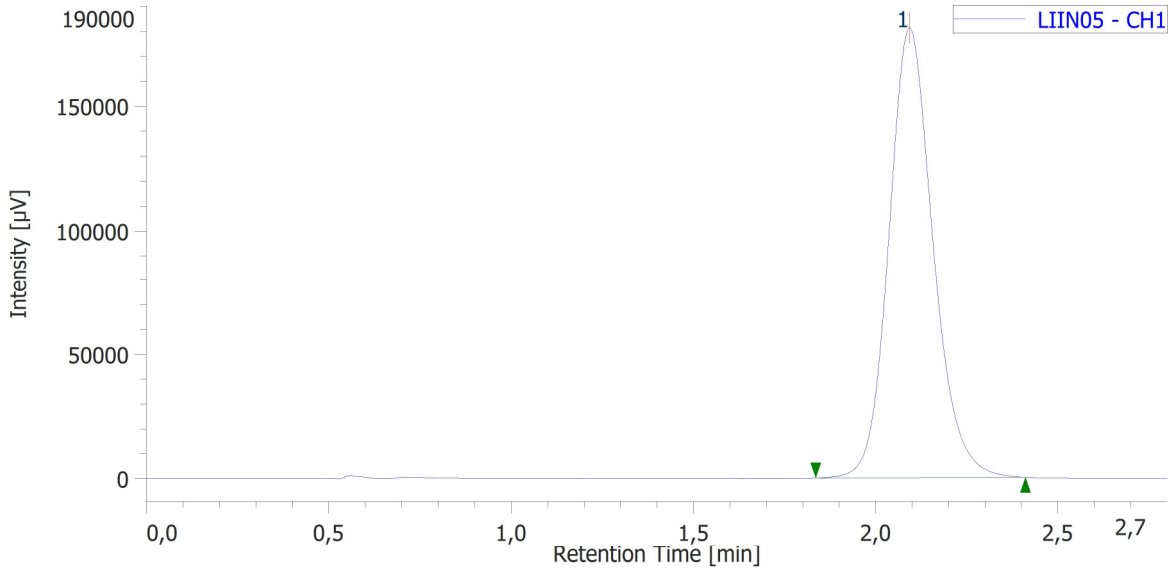


Chromatogram Information	
User Name	Giovana
Date Modified	26/08/2020 16:39:34
Description	
HPLC System Name	HPLC 002 RI
Injection Date	26/08/2020 16:36:44
Volume	20.00 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2.8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN05-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Integração_Cafeína_20200826

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.093	1525134	180982	100.000	100.000	N/A	1503	N/A	1.151	

Chromatogram

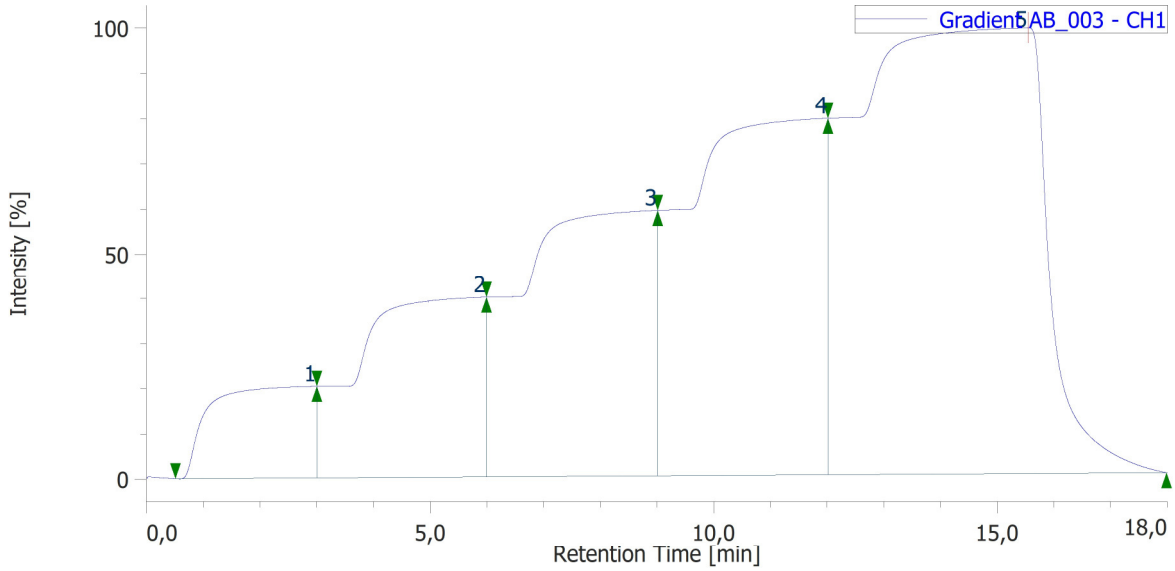


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2020 12:26:10
Description	
HPLC System Name	HPLC 002 RI
Injection Date	27/08/2020 12:08:08
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação HPLC 2
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradient AB_003-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,000	8920252	73814	4,584	6,832	N/A	N/A	N/A	N/A	
2	40%	1	5,987	21676729	144783	11,138	13,401	N/A	N/A	N/A	N/A	
3	60%	1	9,008	34592640	214756	17,775	19,878	N/A	N/A	N/A	N/A	
4	80%	1	12,010	47437211	287693	24,375	26,629	N/A	N/A	N/A	N/A	
5	100%	1	15,539	81984119	359342	42,127	33,260	N/A	N/A	N/A	N/A	

Chromatogram

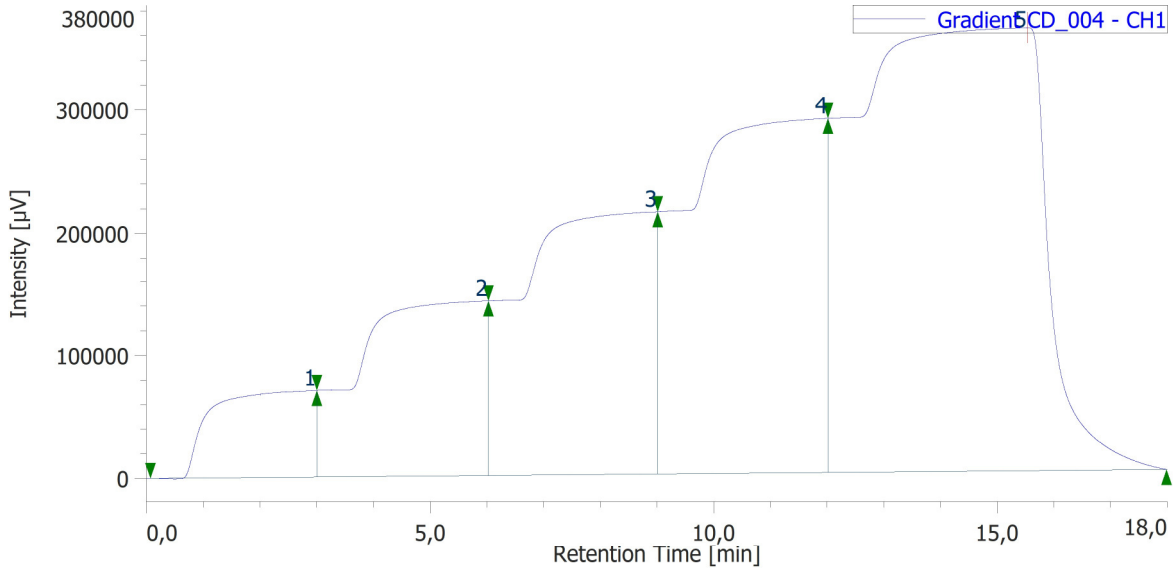

Chromatogram Information


User Name	Giovana
Date Modified	27/08/2020 12:58:10
Description	
HPLC System Name	HPLC 002 RI
Injection Date	27/08/2020 12:40:08
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação HPLC 2
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradient CD_004-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,002	8385840	70415	4,336	6,555	N/A	N/A	N/A	N/A	
2	40%	1	6,022	21430408	141758	11,080	13,197	N/A	N/A	N/A	N/A	
3	60%	1	9,008	34042047	213854	17,600	19,909	N/A	N/A	N/A	N/A	
4	80%	1	12,011	47439146	288130	24,527	26,824	N/A	N/A	N/A	N/A	
5	100%	1	15,531	82118948	359982	42,457	33,514	N/A	N/A	N/A	N/A	

Chromatogram

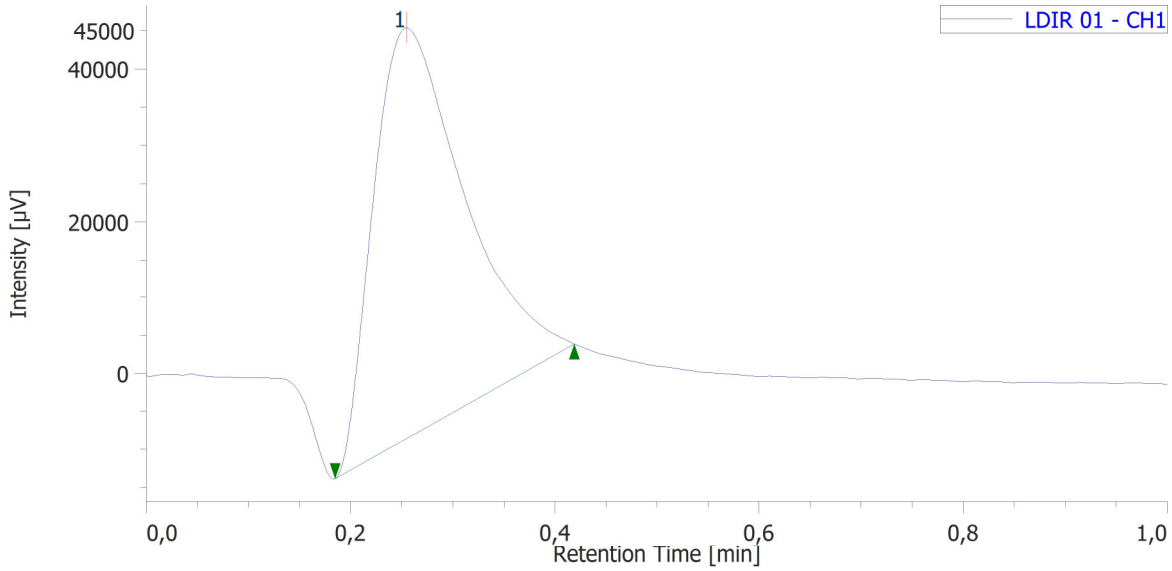


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2020 16:00:52
Description	
HPLC System Name	HPLC 002 RI
Injection Date	27/08/2020 14:17:34
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	1.0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 01-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.255	333796	53883	100.000	100.000	N/A	39	N/A	1.702	

Chromatogram

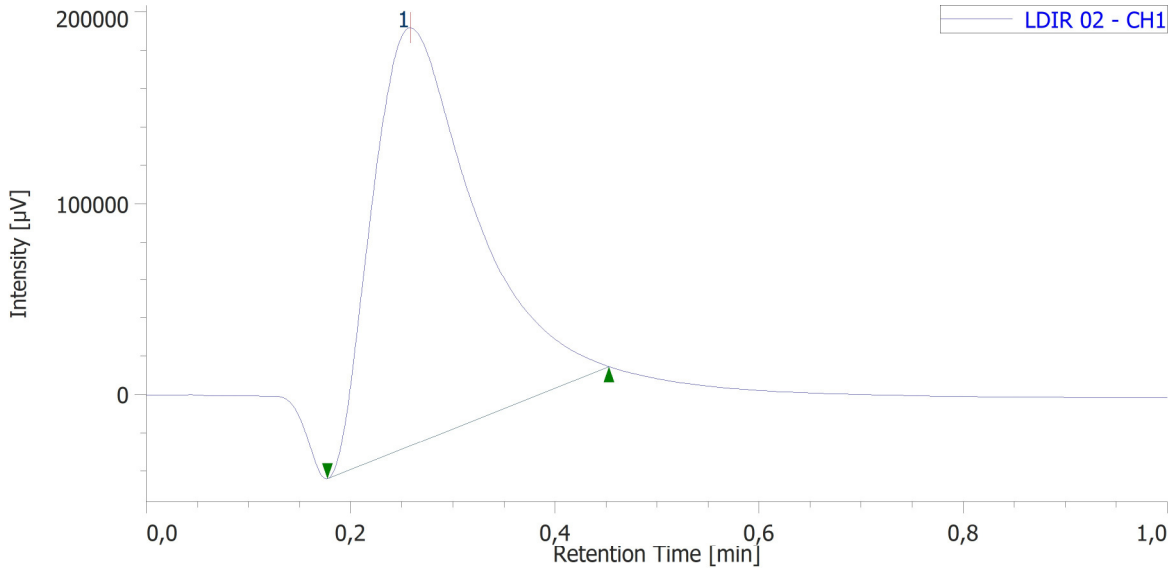


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2020 16:00:52
Description	
HPLC System Name	HPLC 002 RI
Injection Date	27/08/2020 14:20:53
Volume	10.00 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	1.0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	Cafeína Peak ID Table_20200826-b
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 02-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.259	1523893	218321	100.000	100.000	N/A	33	N/A	1.707	

Chromatogram

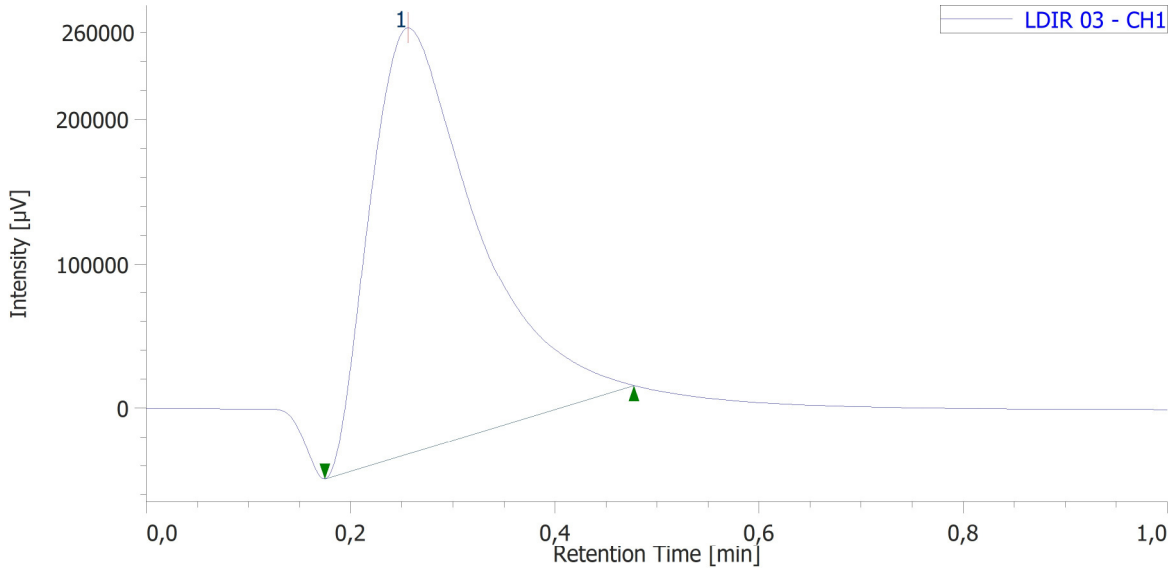


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2020 16:00:52
Description	
HPLC System Name	HPLC 002 RI
Injection Date	27/08/2020 14:23:58
Volume	10.00 [µL]
Sample #	3
Project Name	Qualificação HPLC 2
Acquisition Time	1.0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 03-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.256	2137207	294347	100.000	100.000	N/A	30	N/A	1.840	

Chromatogram

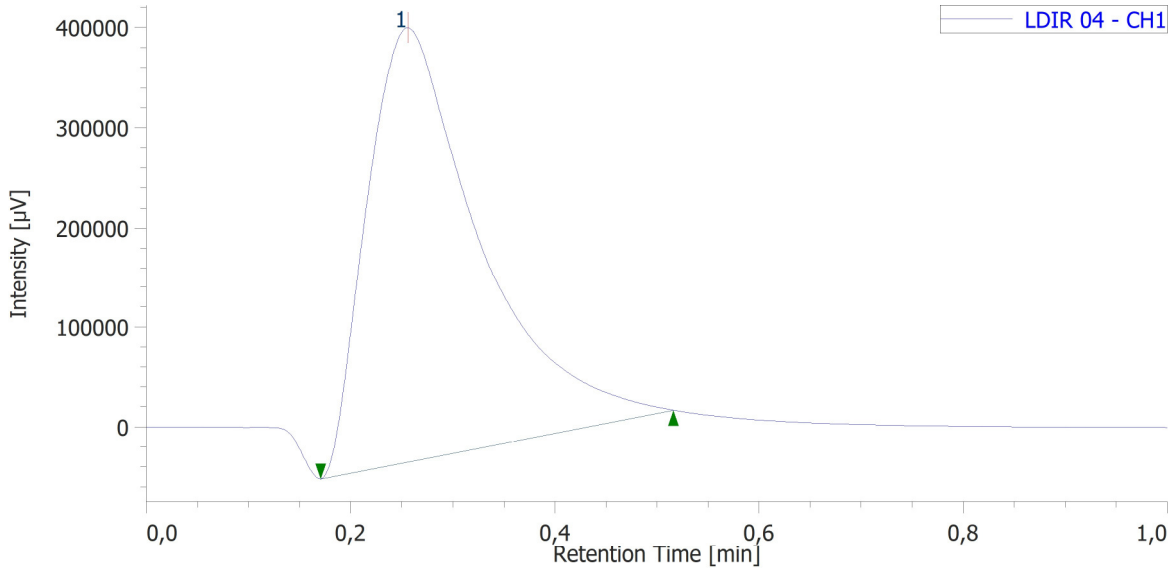


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2020 16:00:52
Description	
HPLC System Name	HPLC 002 RI
Injection Date	27/08/2020 14:27:03
Volume	10.00 [µL]
Sample #	4
Project Name	Qualificação HPLC 2
Acquisition Time	1.0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 04-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.256	3340668	434593	100.000	100.000	N/A	28	N/A	1.922	

Chromatogram

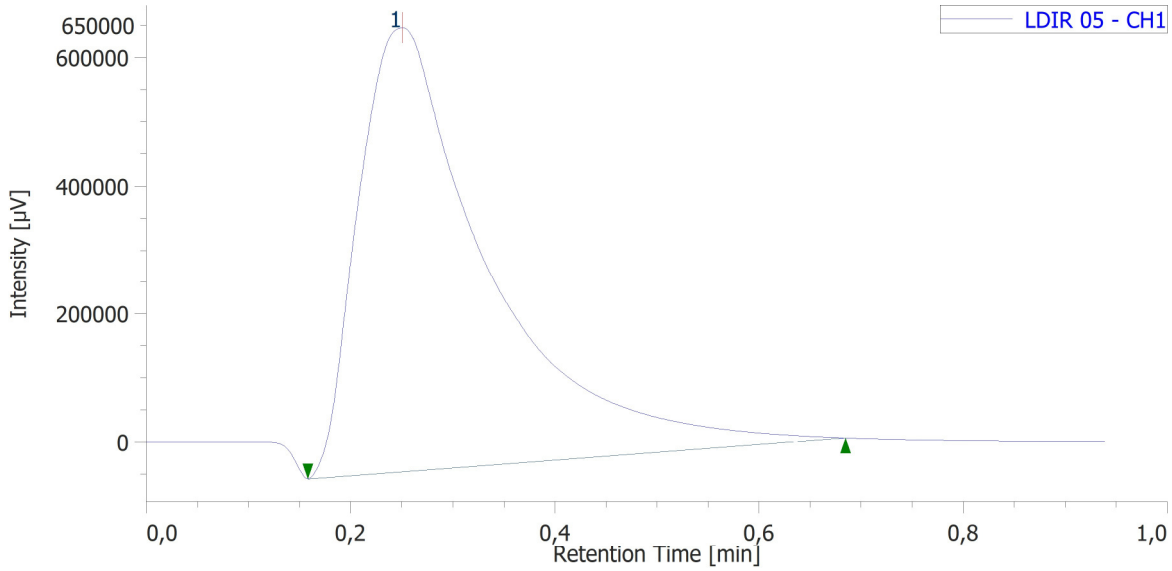

Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2020 16:00:53
Description	
HPLC System Name	HPLC 002 RI
Injection Date	27/08/2020 14:30:07
Volume	10.00 [µL]
Sample #	5
Project Name	Qualificação HPLC 2
Acquisition Time	1.0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 05-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.251	6189730	691694	100.000	100.000	N/A	23	N/A	2.382	