
Peak Find - EDUV_001 UV_tR2,14 D

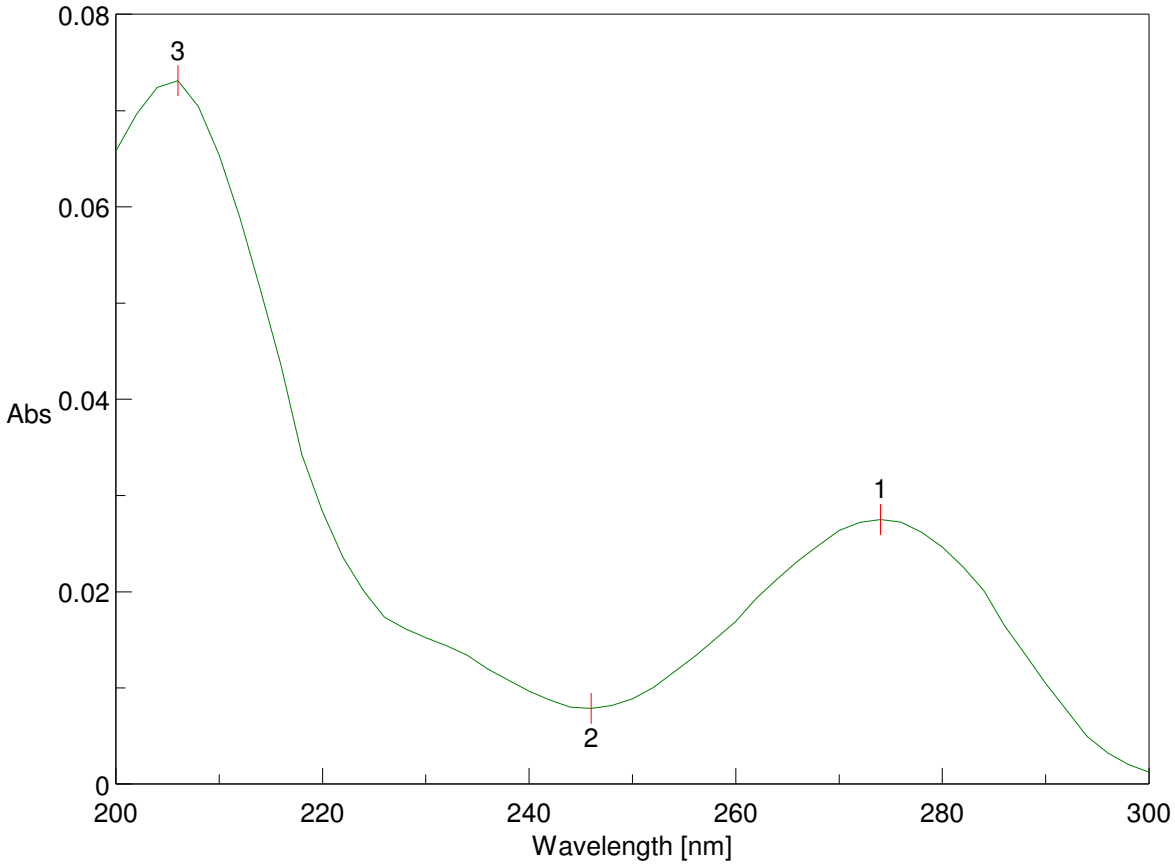

[Comments]

User	Administrator
Division	---
Company	JP
Creation date	27/08/2020 09:27

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	370 nm
Data interval	2 nm
Data points	86


[Measurement Information]

Instrument Name	UV-4070
Model Name	UV-4070
Serial No.	A010760888
ROM version	1.00.18

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.027466	2	246	0.00784171
3	206	0.0730841			

Peak Find - EDUV_001 PDA_2,1833

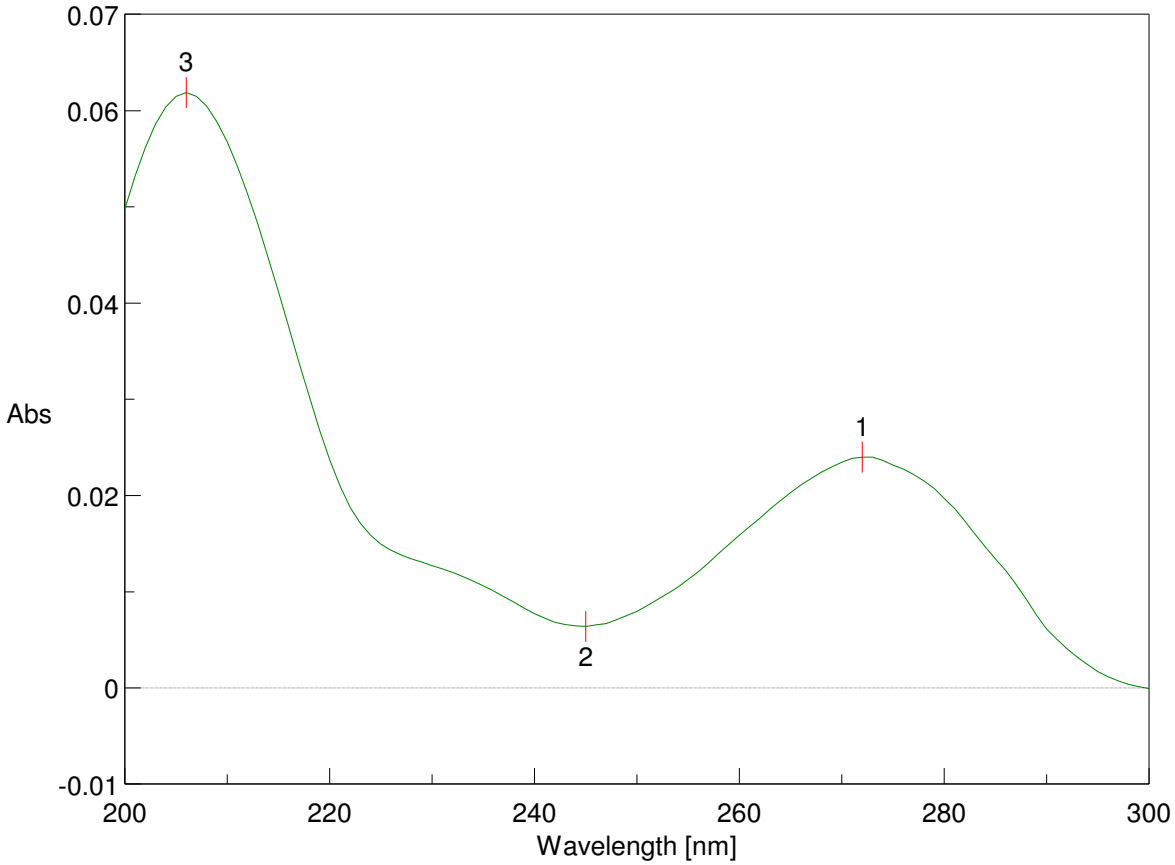

[Comments]

User	Administrator
Division	---
Company	JP
Creation date	27/08/2020 09:13

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2018
Model Name	MD-2018
Serial No.	A023761331
ROM version	V1.05.01

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.023974	2	245	0.006352
3	206	0.06186			

Chromatogram

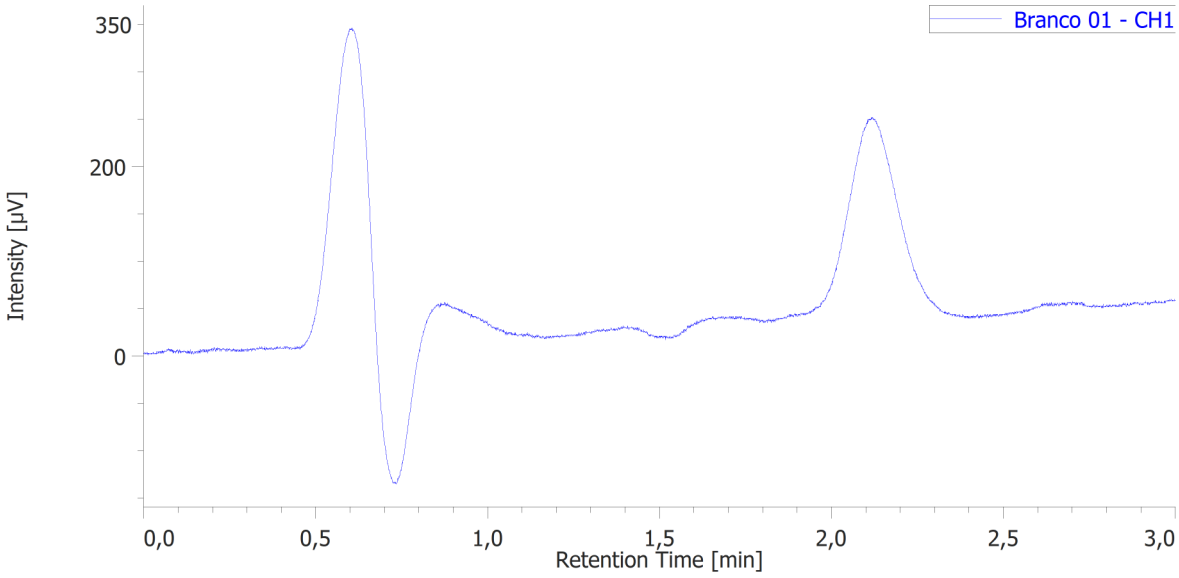


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 09:52:22
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 09:49:19
Volume	10.00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

Chromatogram

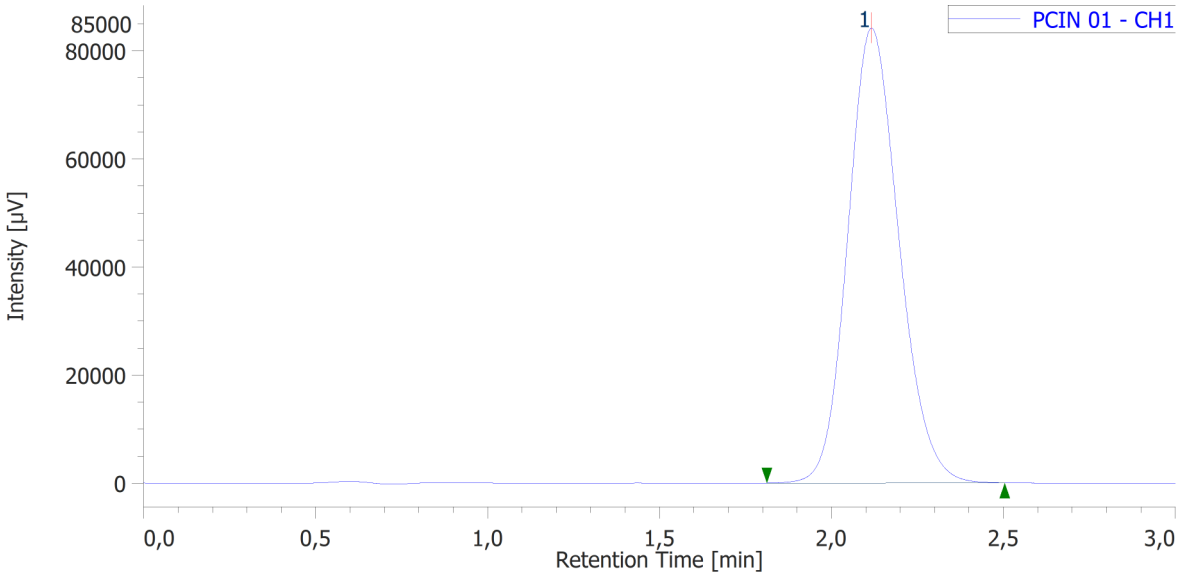

Chromatogram Information


User Name	Administrator
Date Modified	27/08/2020 09:55:34
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 09:52:32
Volume	10.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.116	868863	84122	100.000	100.000	N/A	986	N/A	1.149	

Chromatogram

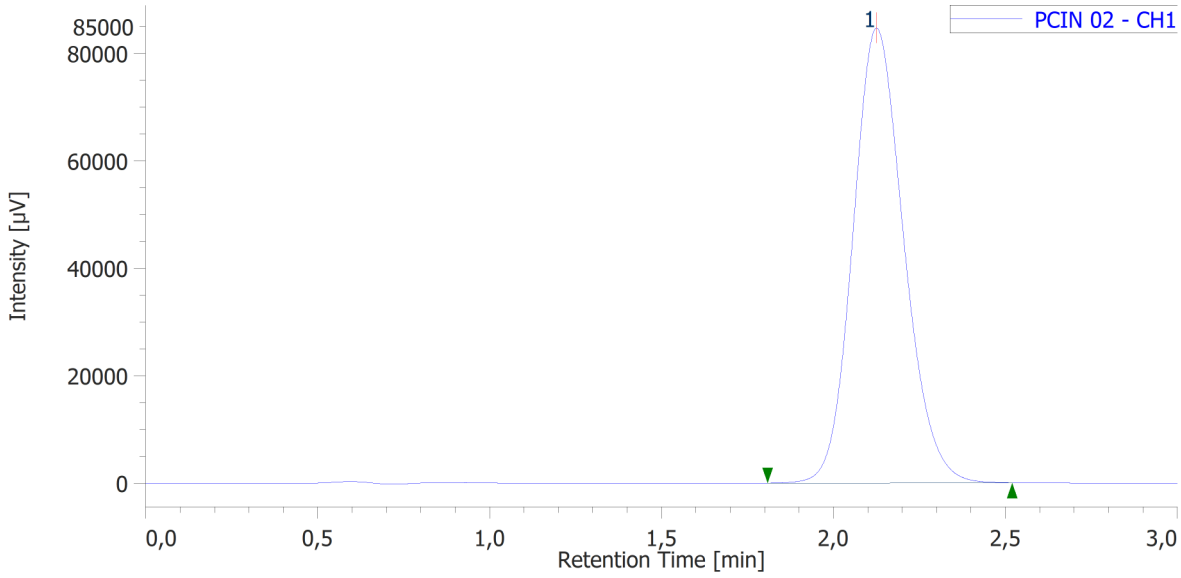


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 09:58:46
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 09:55:44
Volume	10.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.125	868941	84627	100.000	100.000	N/A	1008	N/A	1.145	

Chromatogram

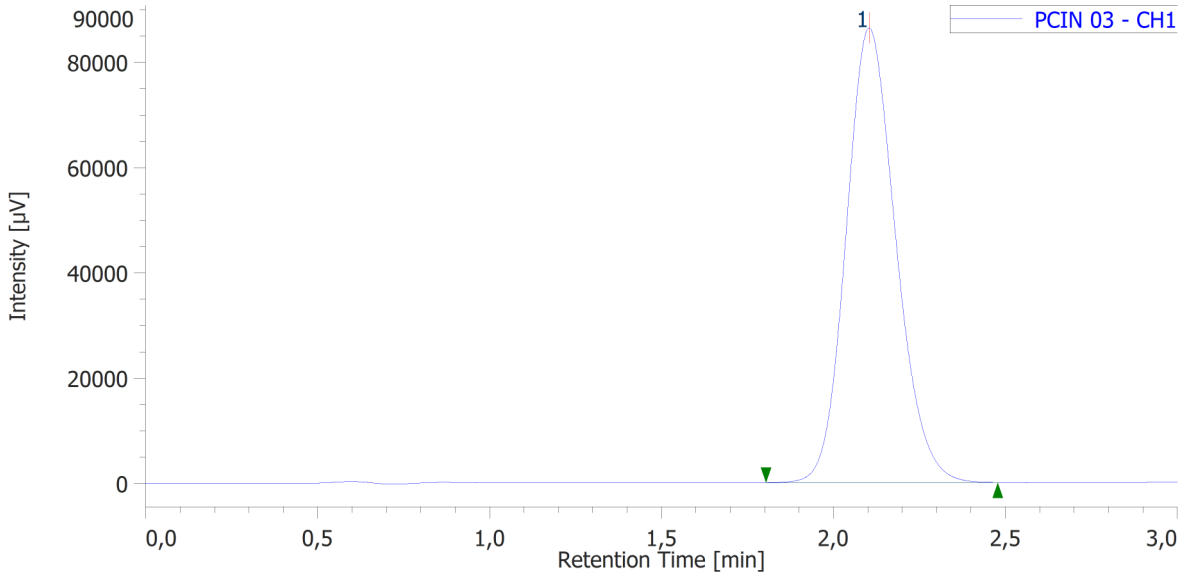

Chromatogram Information


User Name	Administrator
Date Modified	27/08/2020 10:01:58
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 09:58:56
Volume	10.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.103	867865	86371	100.000	100.000	N/A	1031	N/A	1.150	

Chromatogram

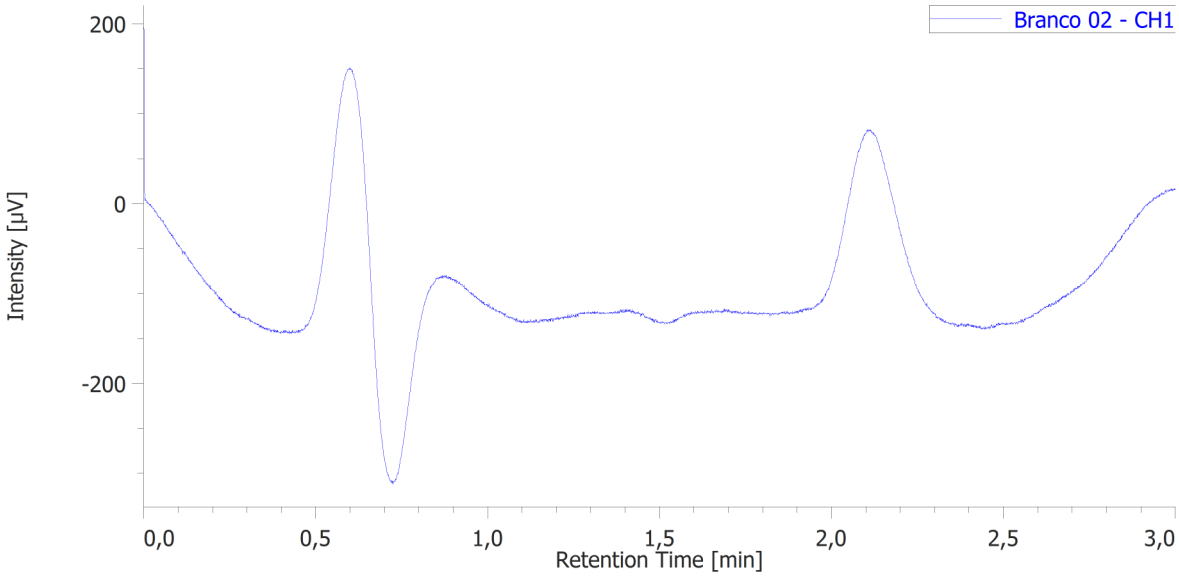


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:05:10
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:02:08
Volume	10.00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

Chromatogram

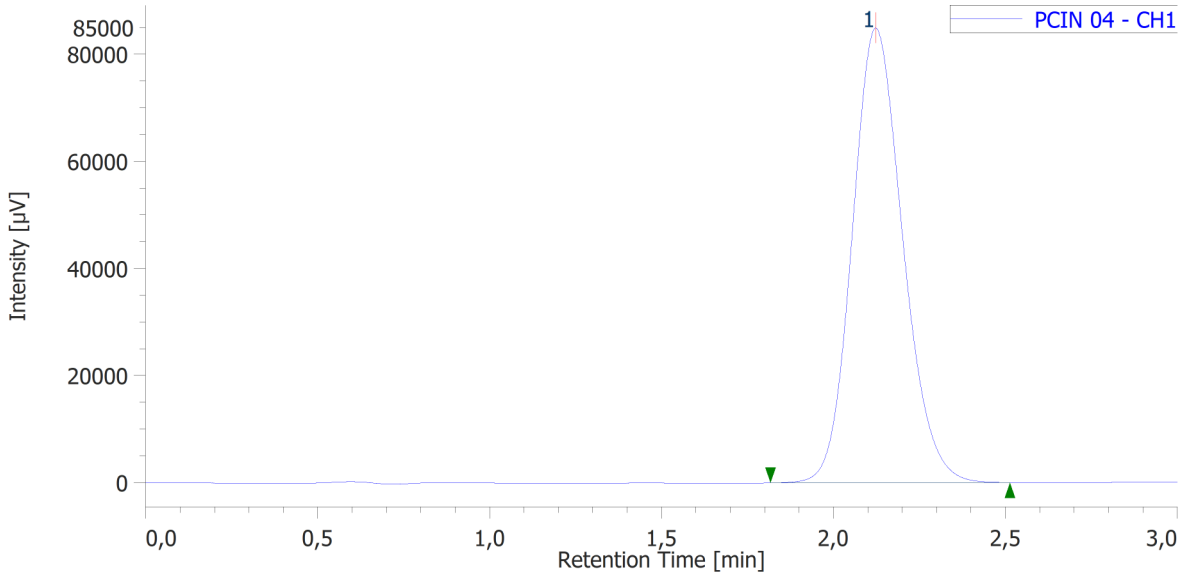

Chromatogram Information


User Name	Administrator
Date Modified	27/08/2020 10:08:22
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:05:20
Volume	10.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.122	867018	84880	100.000	100.000	N/A	1015	N/A	1.150	

Chromatogram

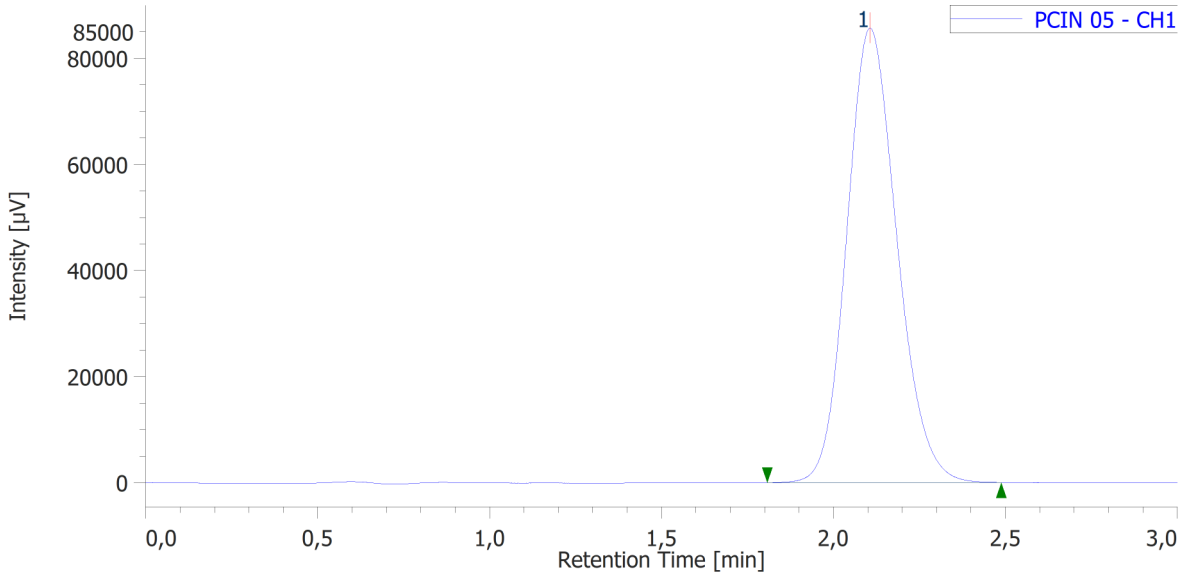


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:11:34
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:08:33
Volume	10.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.106	868492	85669	100.000	100.000	N/A	1015	N/A	1.150	

Chromatogram

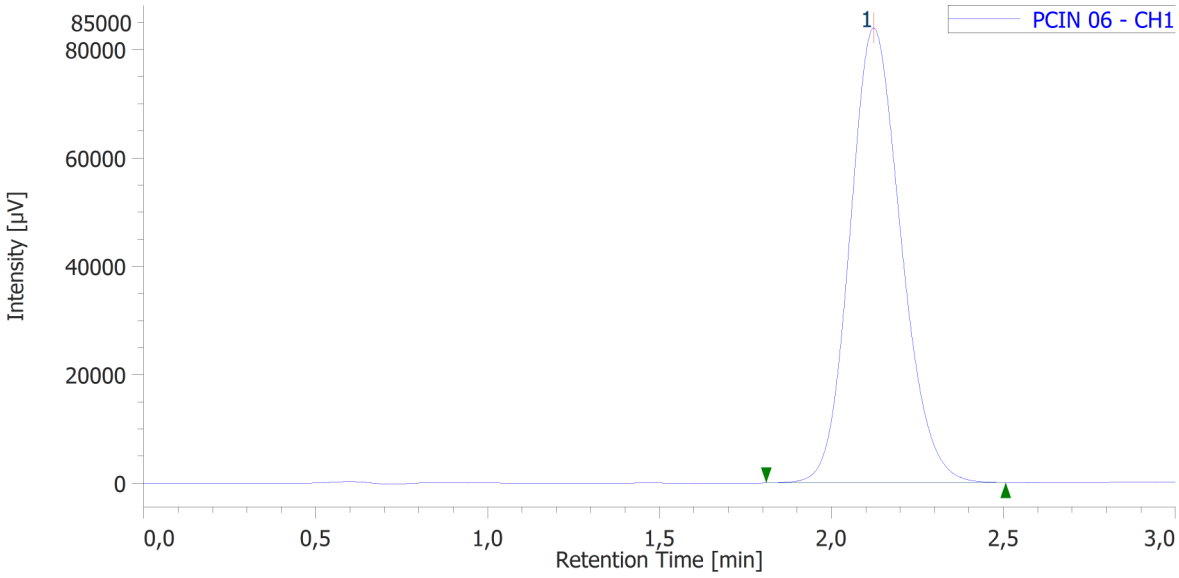

Chromatogram Information


User Name	Administrator
Date Modified	27/08/2020 10:14:46
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:11:45
Volume	10.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.122	867231	83866	100.000	100.000	N/A	990	N/A	1.149	

Chromatogram

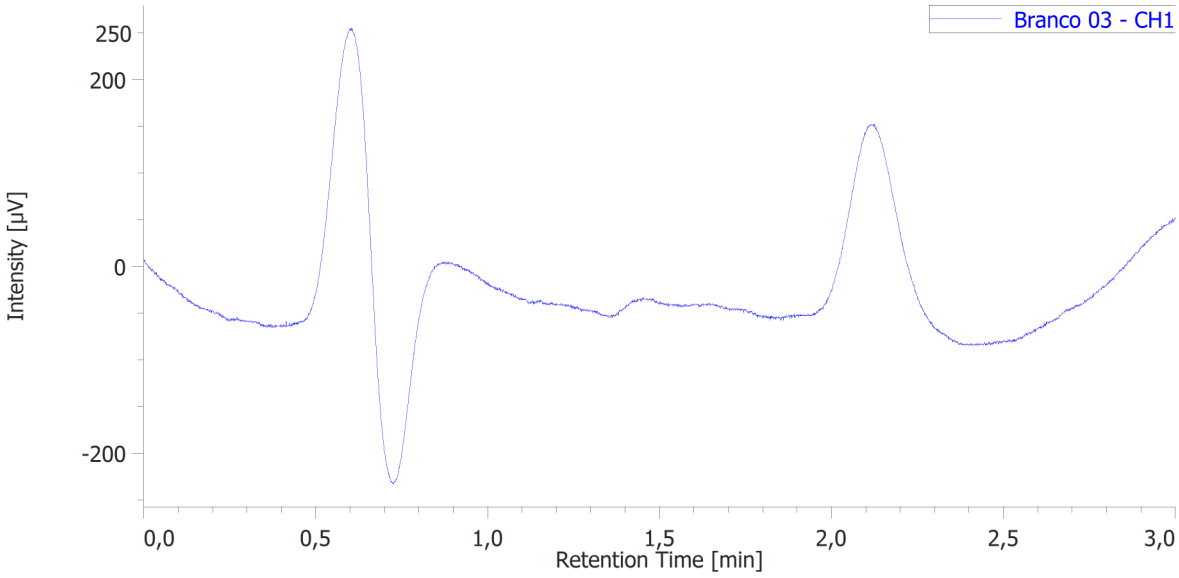


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:18:00
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:14:57
Volume	10.00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

Chromatogram

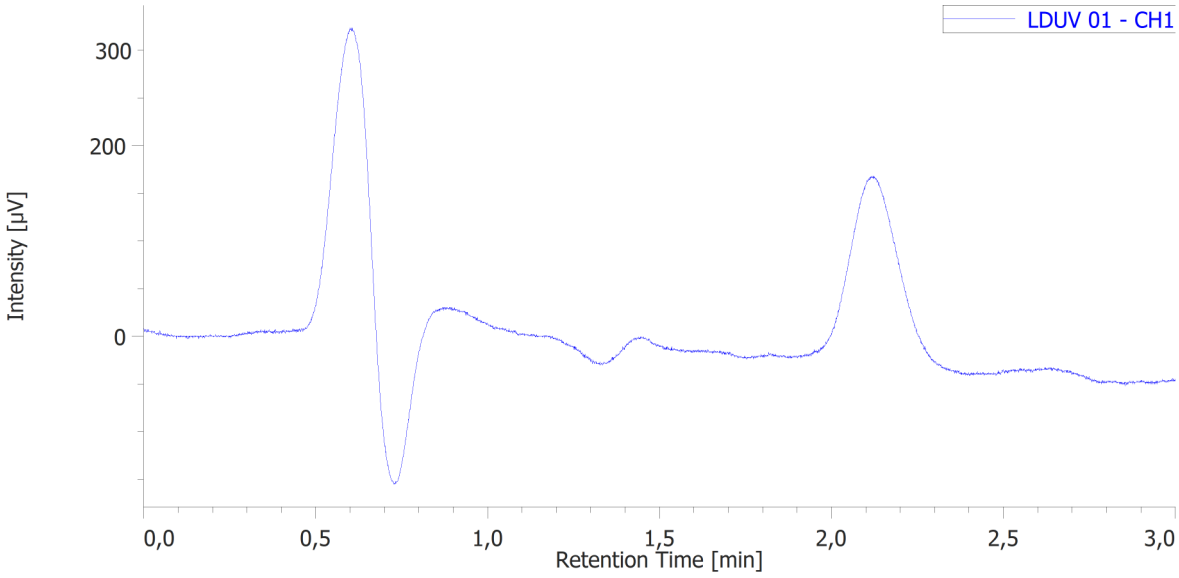


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:24:40
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:21:37
Volume	10.00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

Chromatogram

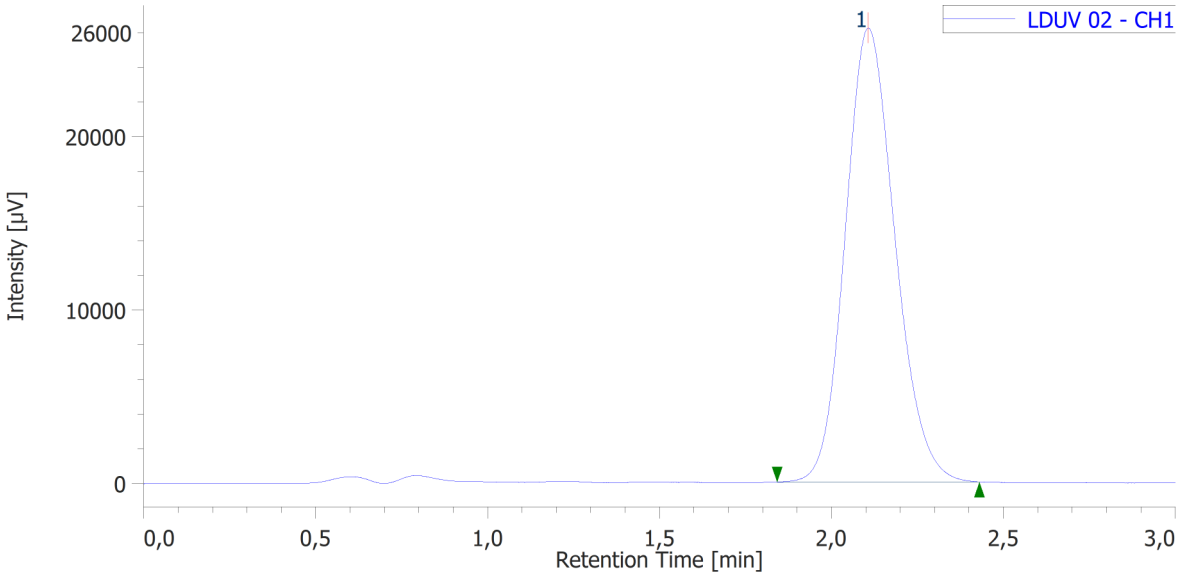


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:27:52
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:24:49
Volume	10.00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.107	263300	26178	100.000	100.000	N/A	1030	N/A	1.153	

Chromatogram

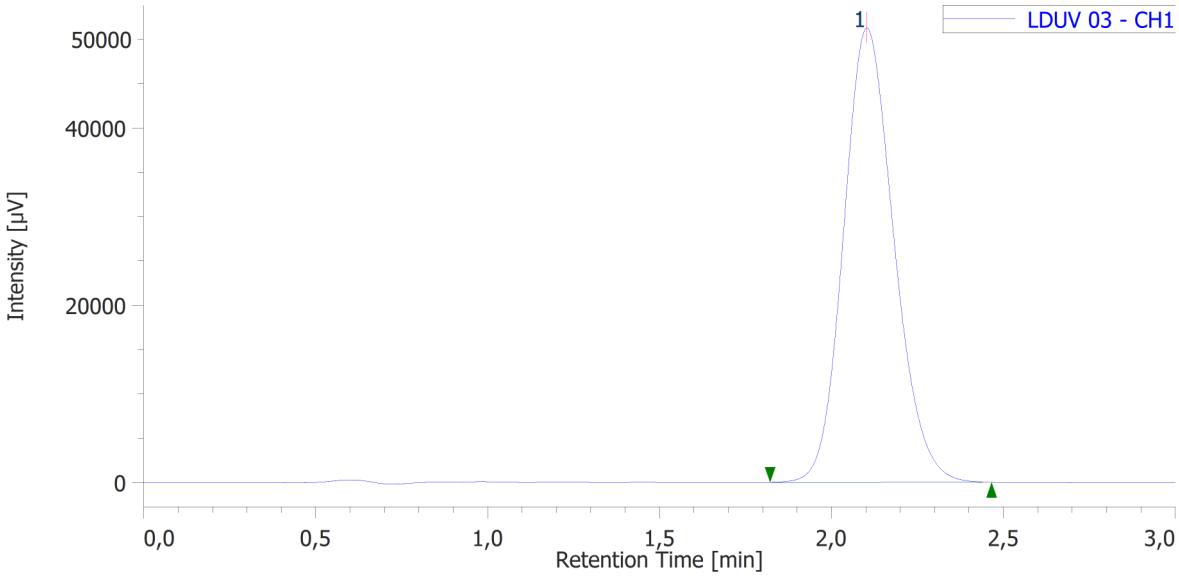


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:31:04
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:28:01
Volume	10.00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.102	521641	51203	100.000	100.000	N/A	1001	N/A	1.156	

Chromatogram

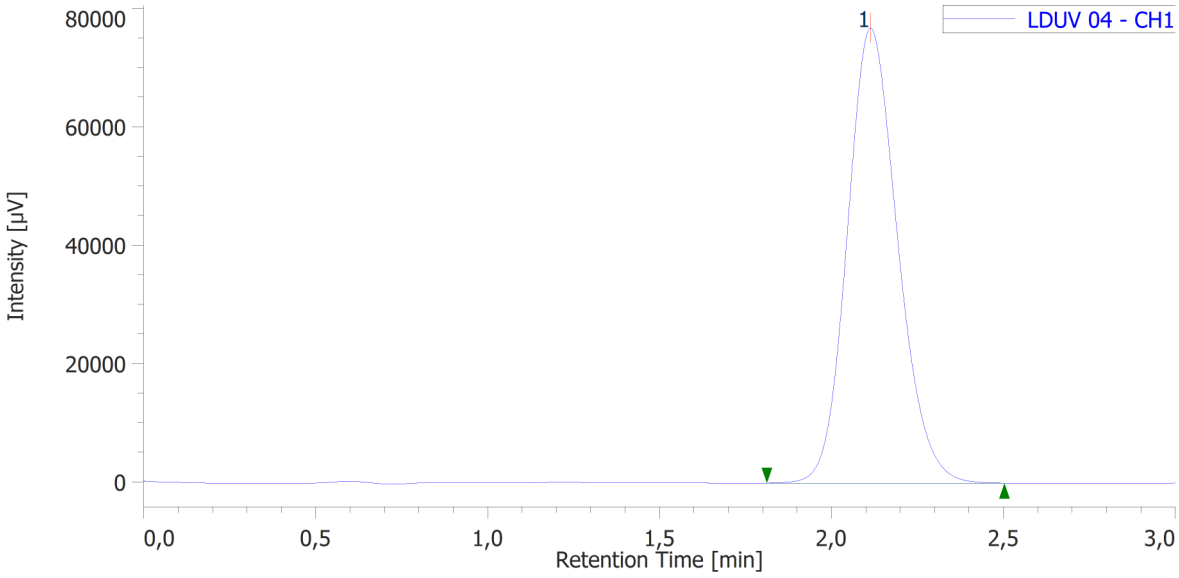


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:42:05
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:31:13
Volume	10.00 [µL]
Sample #	4
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.113	782714	76839	100.000	100.000	N/A	1015	N/A	1.152	

Chromatogram

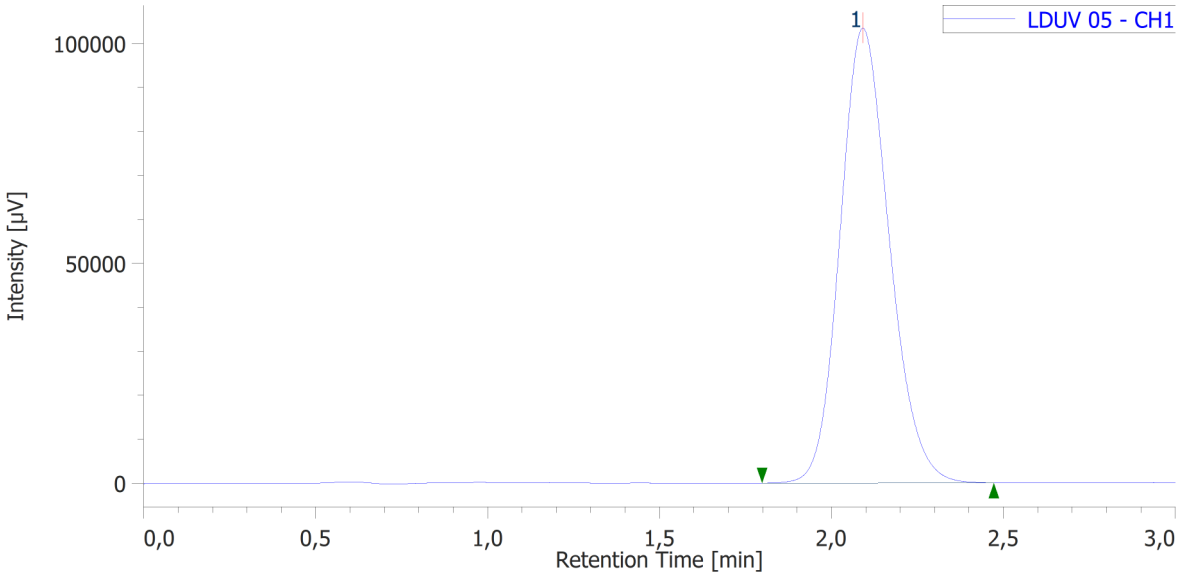


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:42:29
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:34:25
Volume	10.00 [µL]
Sample #	5
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.091	1031282	103455	100.000	100.000	N/A	1037	N/A	1.159	

Chromatogram

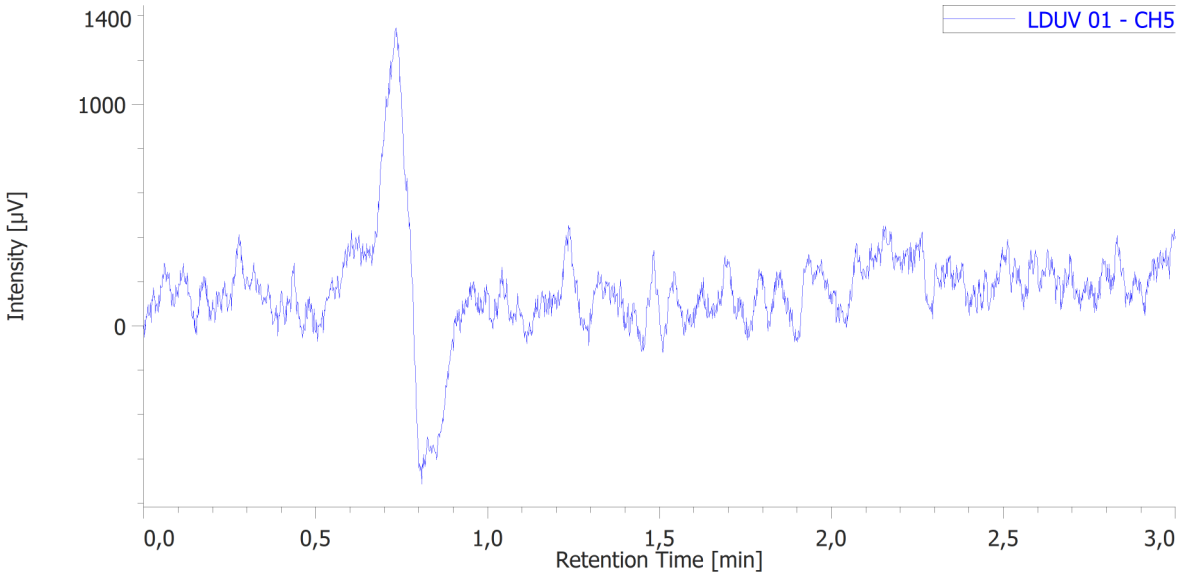


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:24:40
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:21:37
Volume	10.00 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Peak CH5

Chromatogram

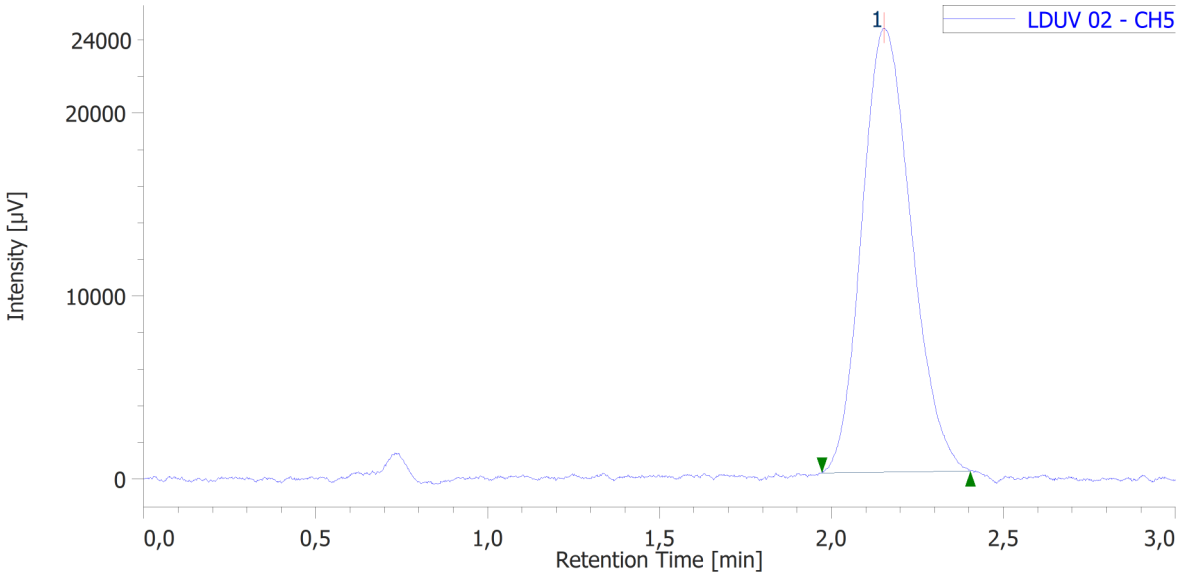


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:27:52
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:24:49
Volume	10.00 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Peak CH5

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.152	242571	24271	100.000	100.000	N/A	1049	N/A	1.192	

Chromatogram

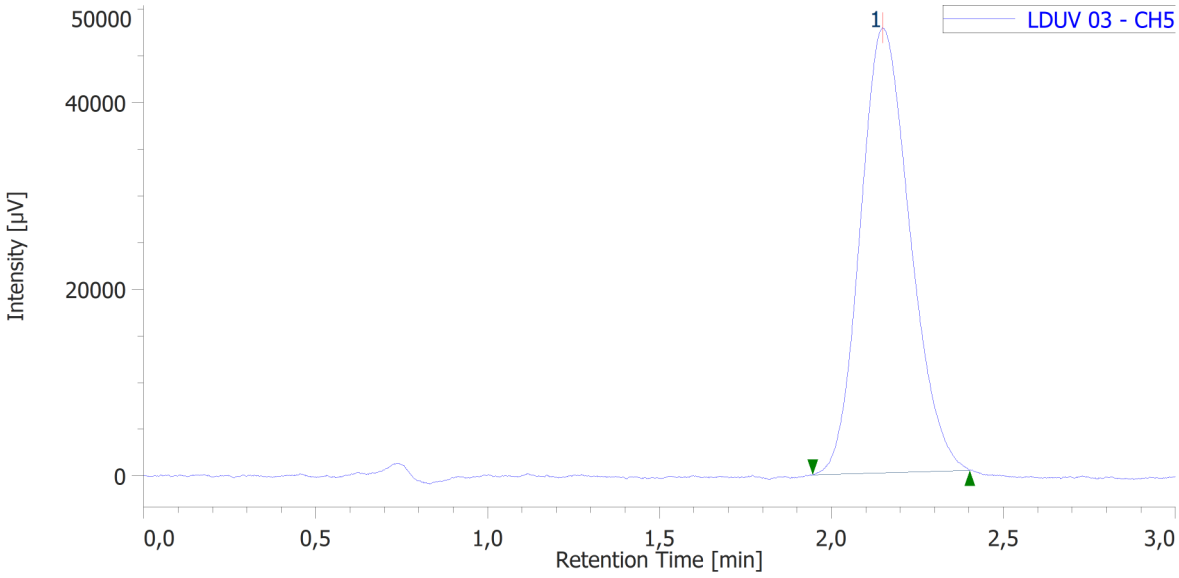


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:31:04
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:28:01
Volume	10.00 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Peak CH5

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.148	479839	47669	100.000	100.000	N/A	1053	N/A	1.177	

Chromatogram

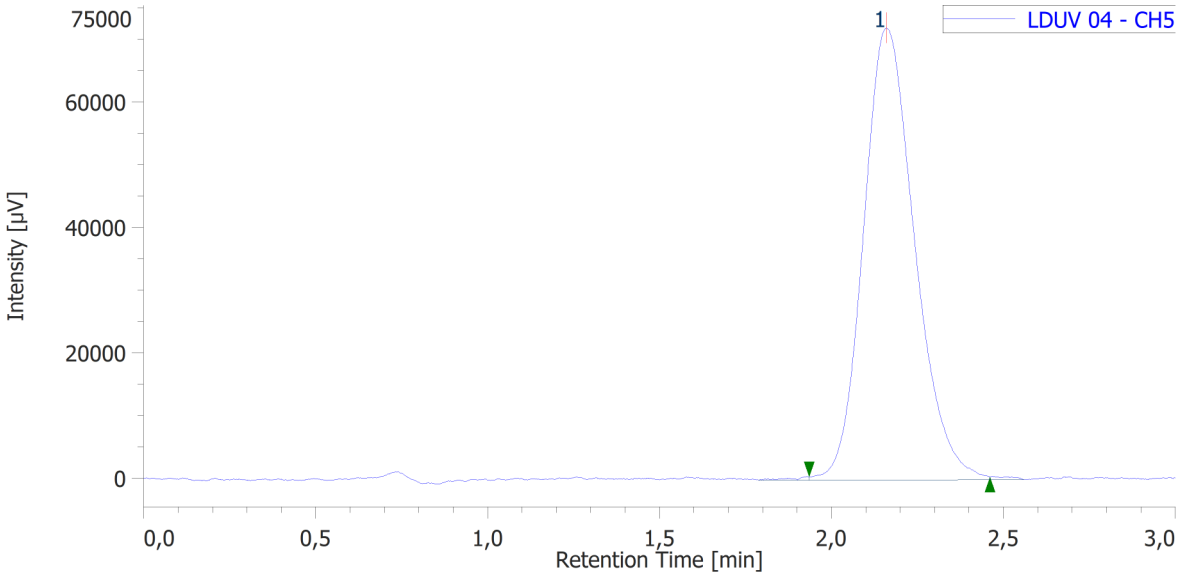


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:42:05
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:31:13
Volume	10.00 [µL]
Sample #	4
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Peak CH5

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.160	746643	72091	100.000	100.000	N/A	1042	N/A	1.196	

Chromatogram

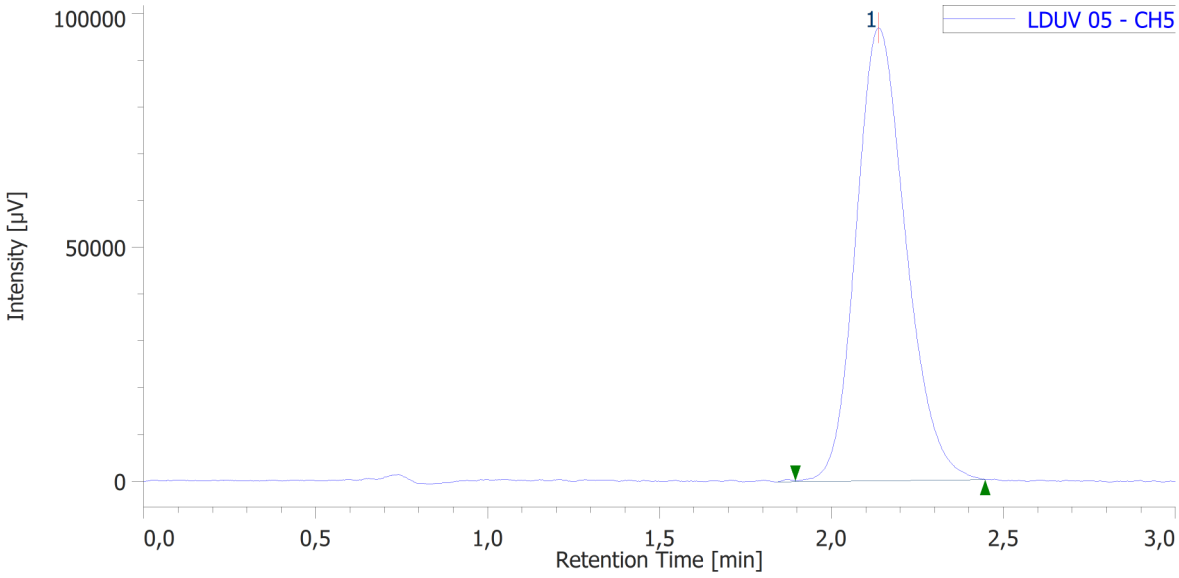


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:42:29
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:34:25
Volume	10.00 [µL]
Sample #	5
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Peak CH5

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.135	974841	96784	100.000	100.000	N/A	1063	N/A	1.204	

Chromatogram

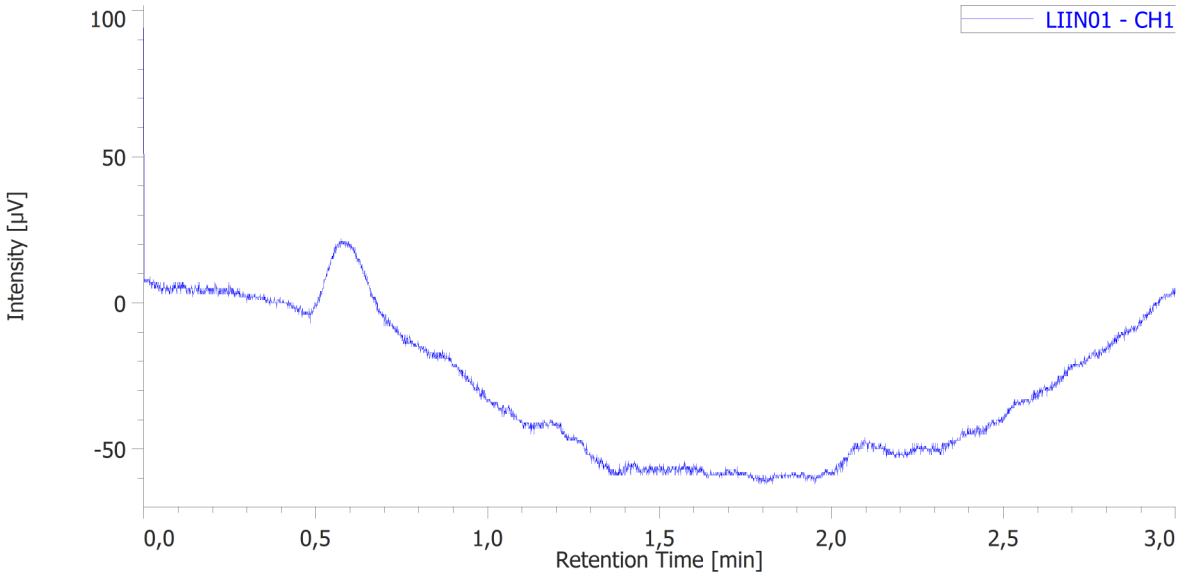


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:47:47
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:44:45
Volume	0.10 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

Chromatogram

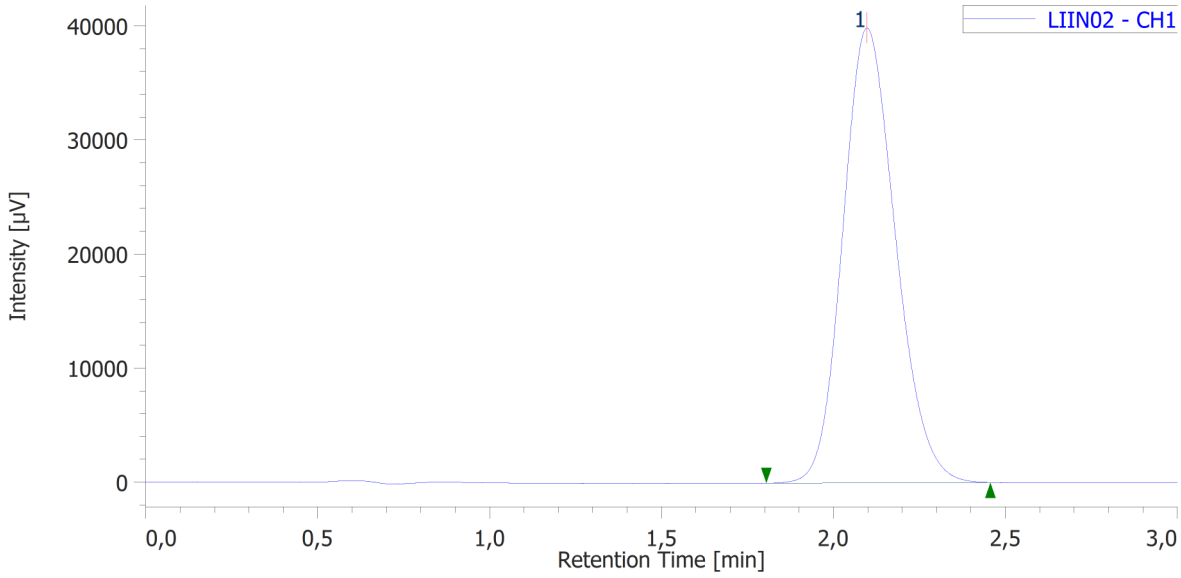


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:50:59
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:47:57
Volume	5.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.097	426054	39858	100.000	100.000	N/A	897	N/A	1.166	

Chromatogram

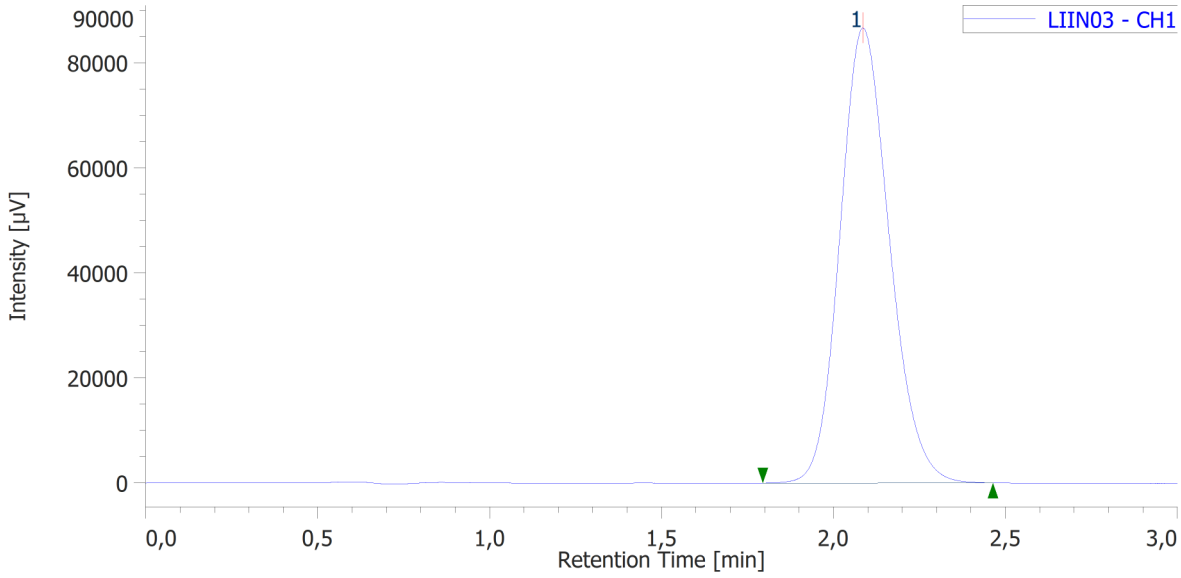

Chromatogram Information


User Name	Administrator
Date Modified	27/08/2020 10:54:12
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:51:10
Volume	10.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.085	865971	86589	100.000	100.000	N/A	1023	N/A	1.152	

Chromatogram

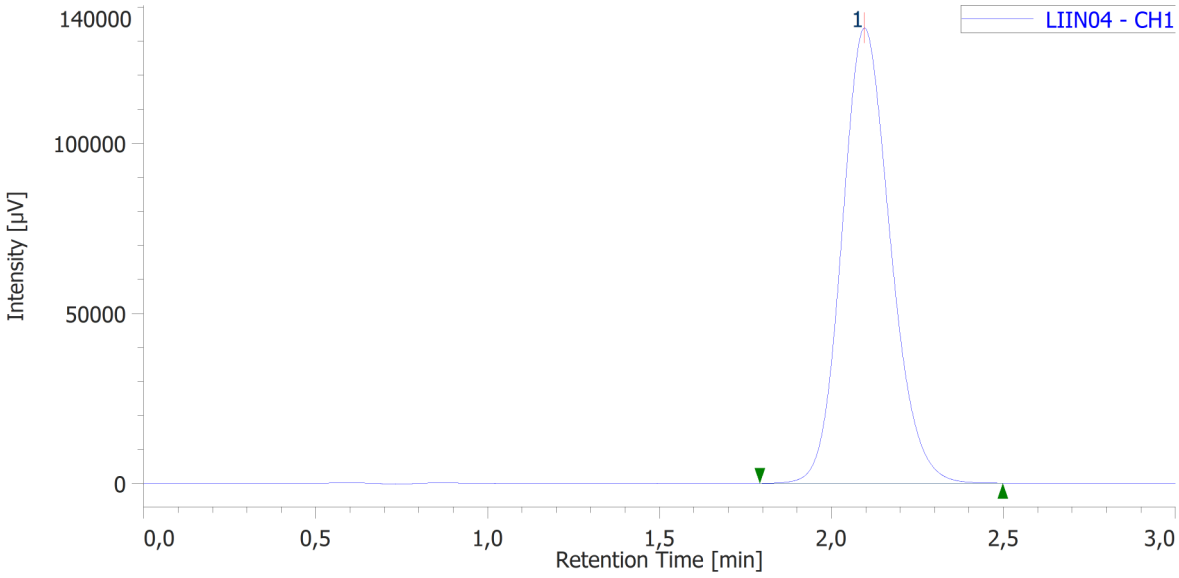


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 10:57:23
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:54:22
Volume	15,00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,095	1308282	133726	100,000	100,000	N/A	1085	N/A	1,144	

Chromatogram

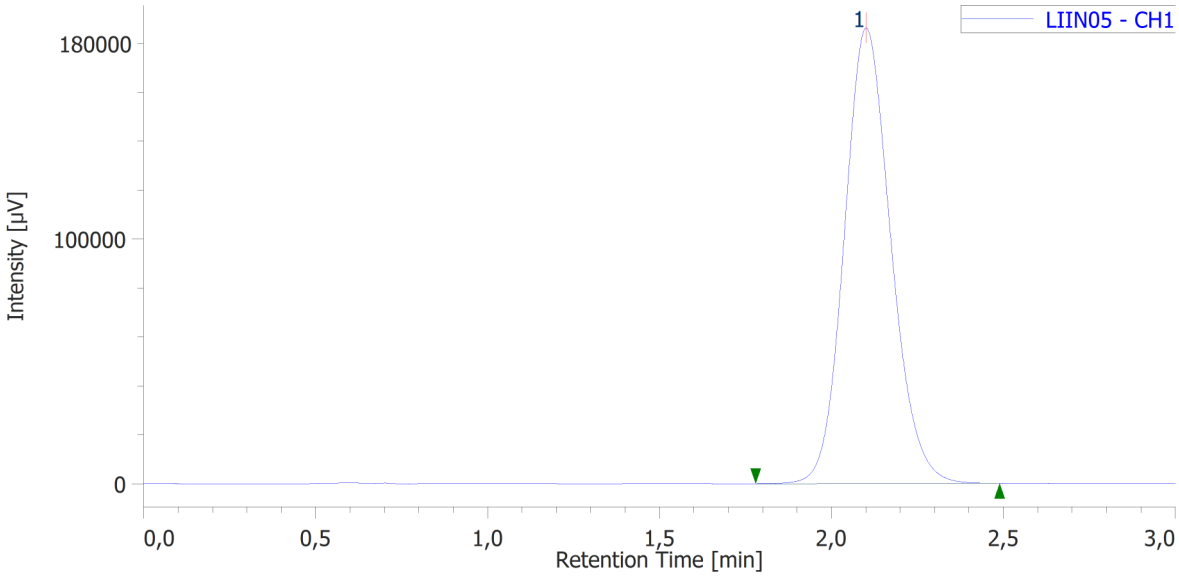


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 11:00:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 10:57:34
Volume	20.00 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Peak CH1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.100	1751885	186153	100.000	100.000	N/A	1180	N/A	1.135	

Chromatogram

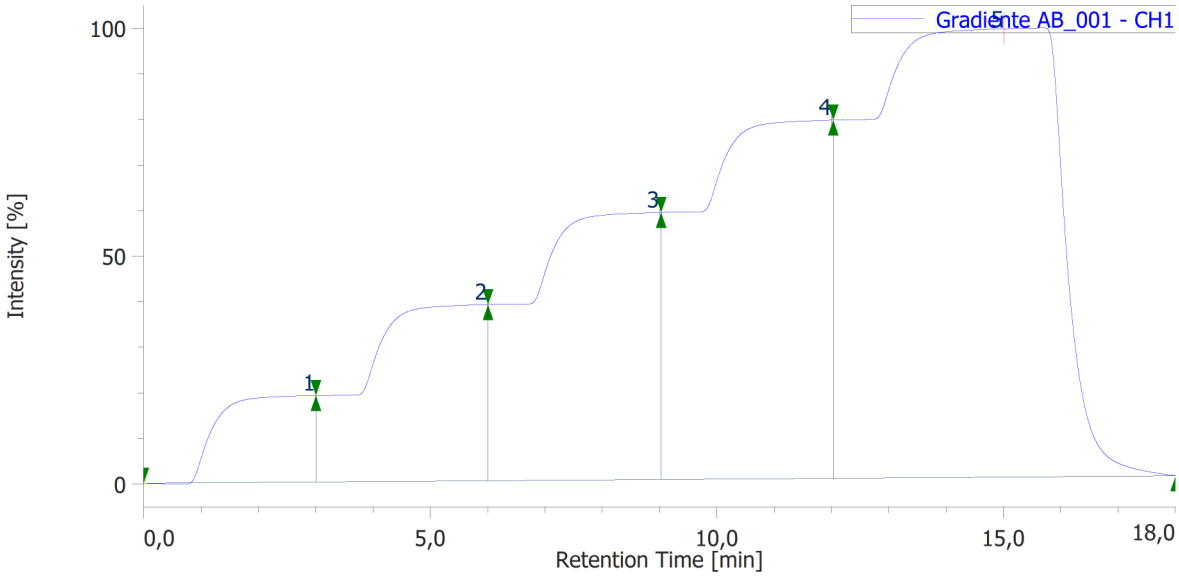


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 11:47:07
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 11:29:05
Volume	0,00 [µL]
Sample #	-
Project Name	JASCO
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,000	7678082	70265	3,919	6,466	N/A	N/A	N/A	N/A	
2	40%	1	6,000	20769743	143303	10,601	13,188	N/A	N/A	N/A	N/A	
3	60%	1	9,000	34260385	217186	17,487	19,987	N/A	N/A	N/A	N/A	
4	80%	1	12,000	47447110	291308	24,218	26,809	N/A	N/A	N/A	N/A	
5	100%	1	15,000	85764669	364560	43,775	33,550	N/A	N/A	N/A	N/A	

Chromatogram

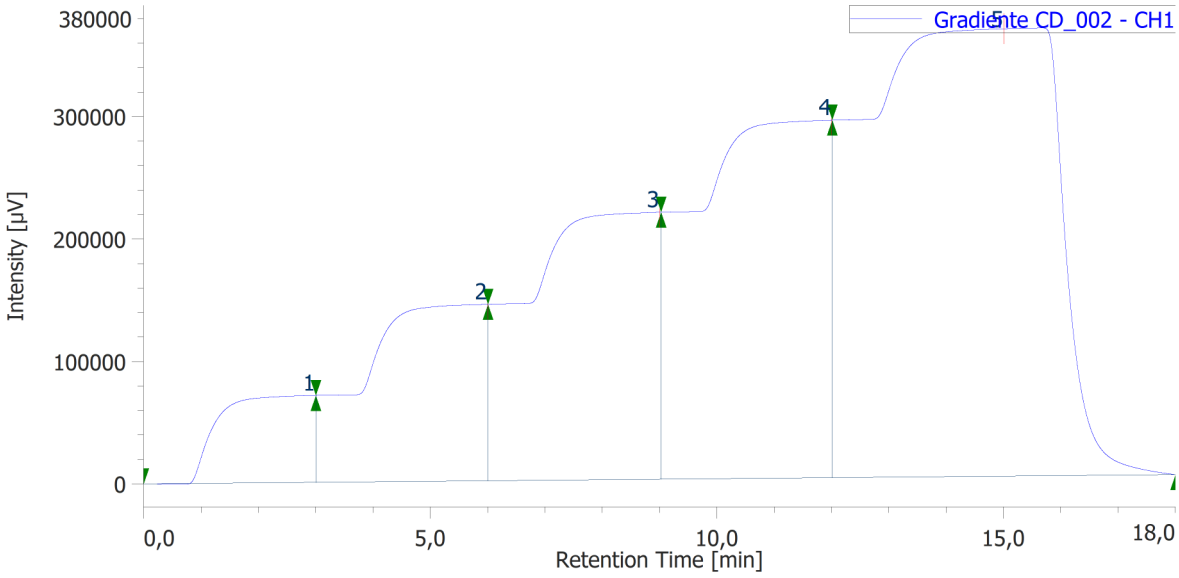

Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2020 12:12:14
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2020 11:54:12
Volume	0,00 [µL]
Sample #	-
Project Name	JASCO
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,000	7765400	71007	3,955	6,515	N/A	N/A	N/A	N/A	
2	40%	1	6,000	20911499	144071	10,651	13,219	N/A	N/A	N/A	N/A	
3	60%	1	9,000	34396298	217969	17,519	20,000	N/A	N/A	N/A	N/A	
4	80%	1	12,000	47257740	291757	24,070	26,770	N/A	N/A	N/A	N/A	
5	100%	1	15,000	86002611	365056	43,804	33,496	N/A	N/A	N/A	N/A	