
Peak Find - Comp Onda.jws

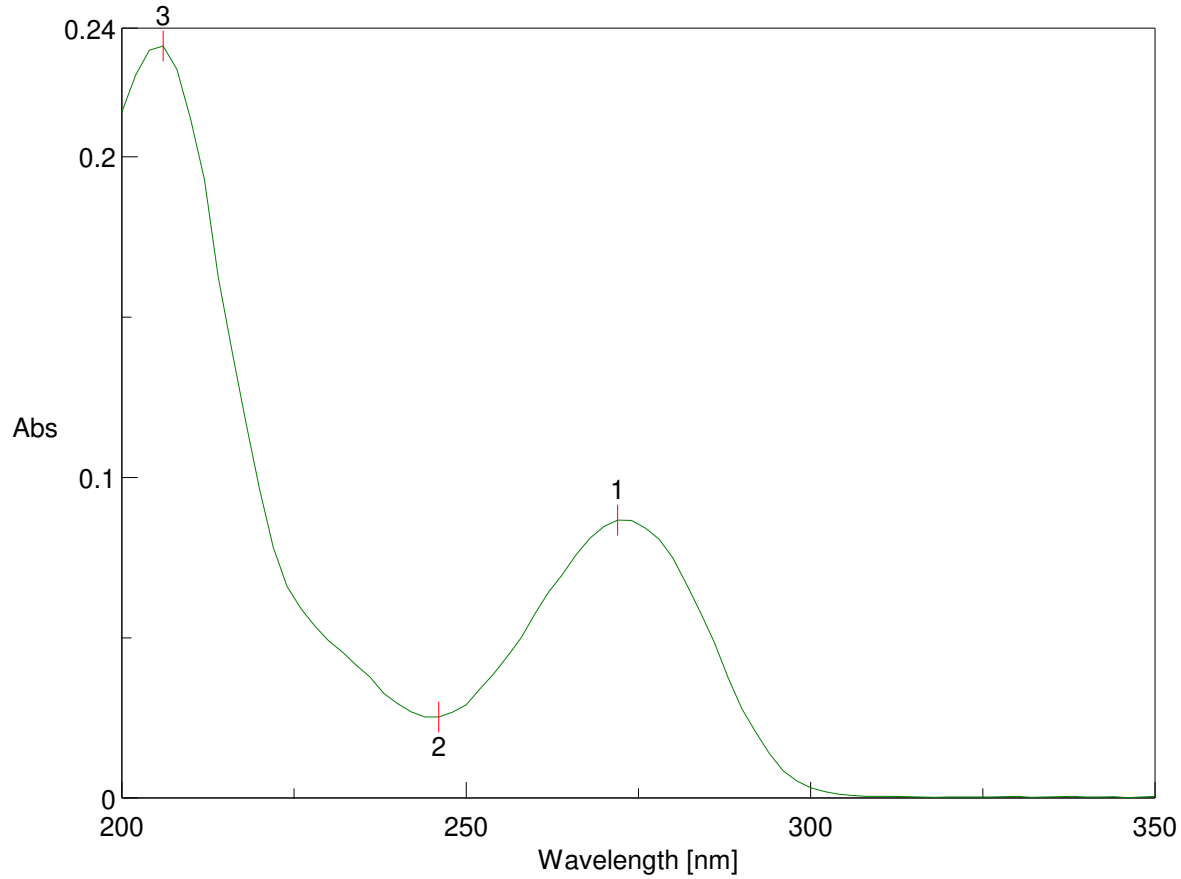

[Comments]

User	Administrator
Division	---
Company	QPack
Creation date	15/10/2020 12:11

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.08657	2	246	0.025246
3	206	0.234399			

Chromatogram

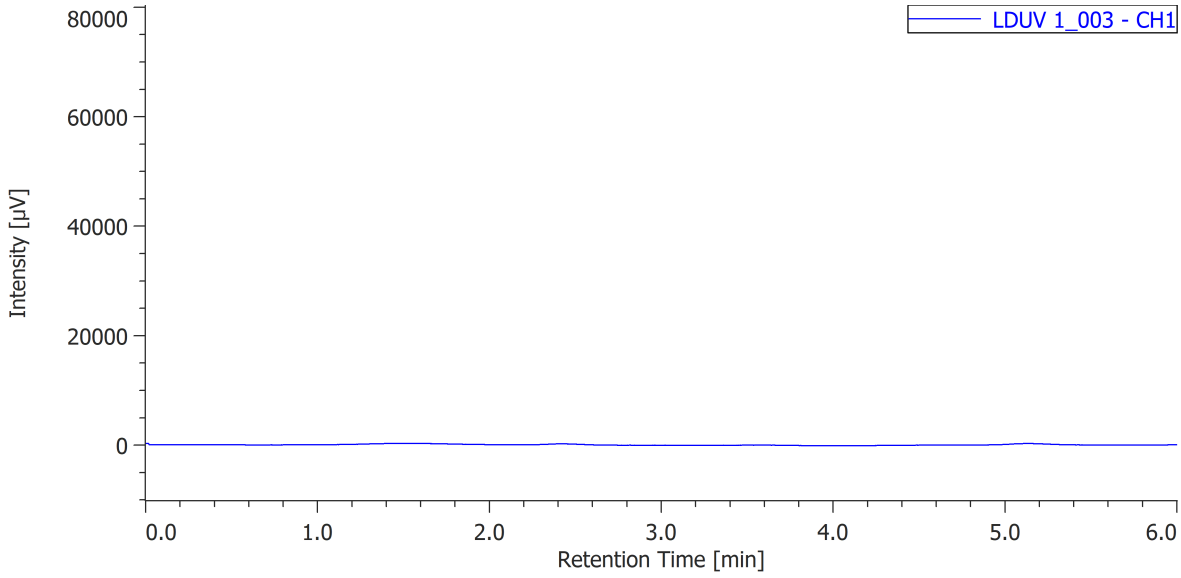


Chromatogram Information	
User Name	Administrator
Date Modified	15/10/2020 12:15:31
Description	
HPLC System Name	HPLC 0001
Injection Date	15/10/2020 11:18:00
Volume	10.0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	6.0 [min]
Acquisition Sequence	
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	

Chromatogram

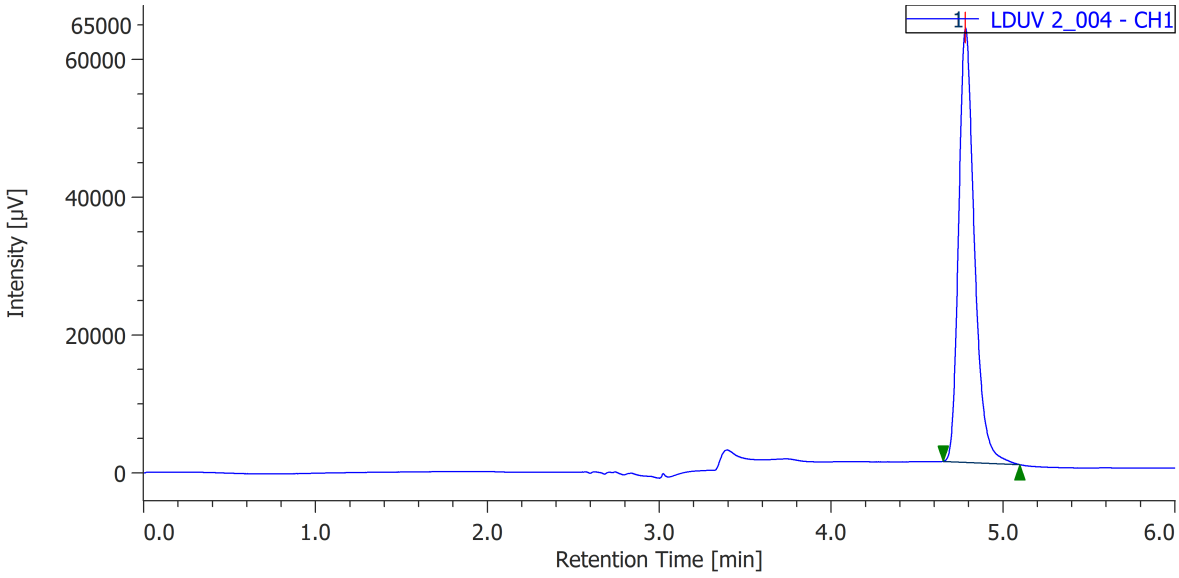


Chromatogram Information	
User Name	Administrator
Date Modified	15/10/2020 12:15:30
Description	
HPLC System Name	HPLC 0001
Injection Date	15/10/2020 11:28:43
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	6.0 [min]
Acquisition Sequence	
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 2_004-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	4.780	403371	63066	100.000	100.000	N/A	14016	N/A	1.322	

Chromatogram

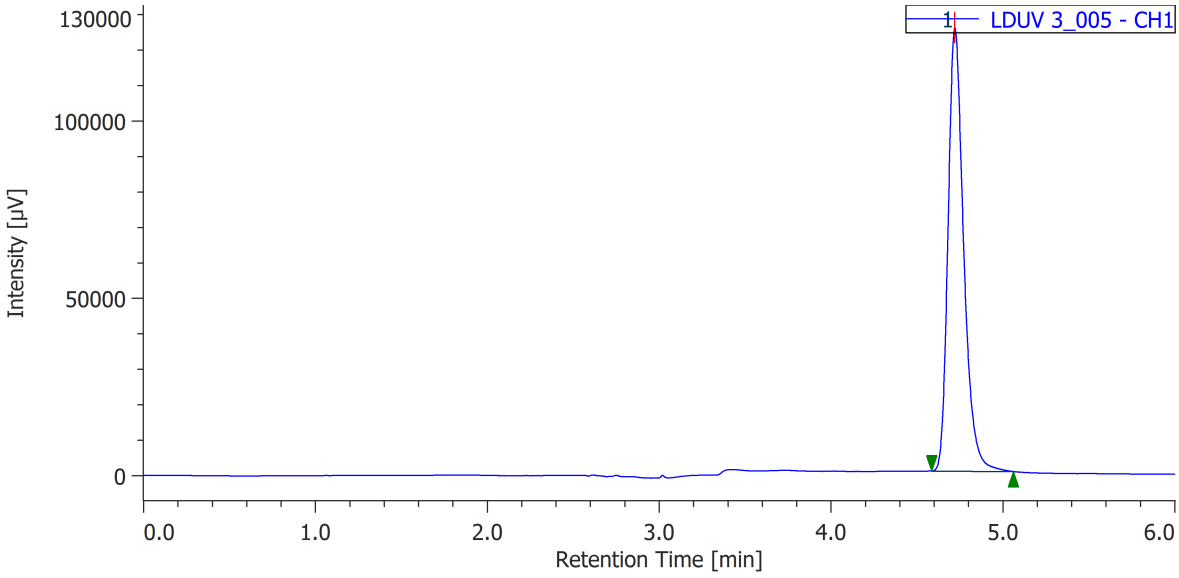


Chromatogram Information	
User Name	Administrator
Date Modified	15/10/2020 12:15:31
Description	
HPLC System Name	HPLC 0001
Injection Date	15/10/2020 11:38:50
Volume	10.0 [µL]
Sample #	13
Project Name	Qualificação
Acquisition Time	6.0 [min]
Acquisition Sequence	
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 3_005-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	4.718	810611	125009	100.000	100.000	N/A	13862	N/A	1.307	

Chromatogram

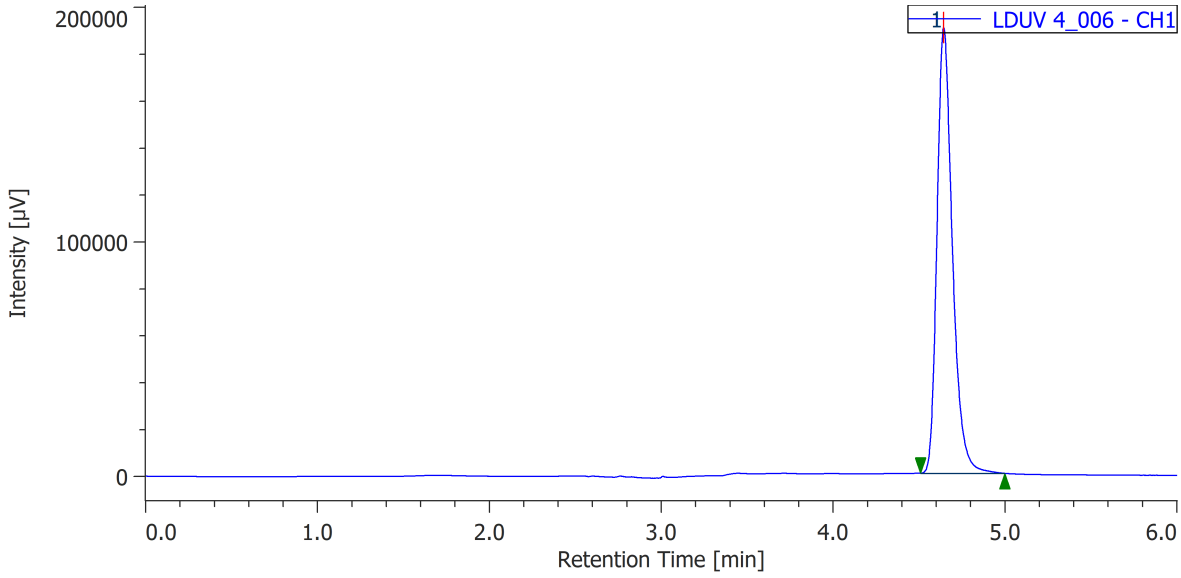


Chromatogram Information	
User Name	Administrator
Date Modified	15/10/2020 12:15:31
Description	
HPLC System Name	HPLC 0001
Injection Date	15/10/2020 11:52:52
Volume	10.0 [µL]
Sample #	14
Project Name	Qualificação
Acquisition Time	6.0 [min]
Acquisition Sequence	
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 4_006-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	4.642	1181061	189912	100.000	100.000	N/A	13868	N/A	1.312	

Chromatogram

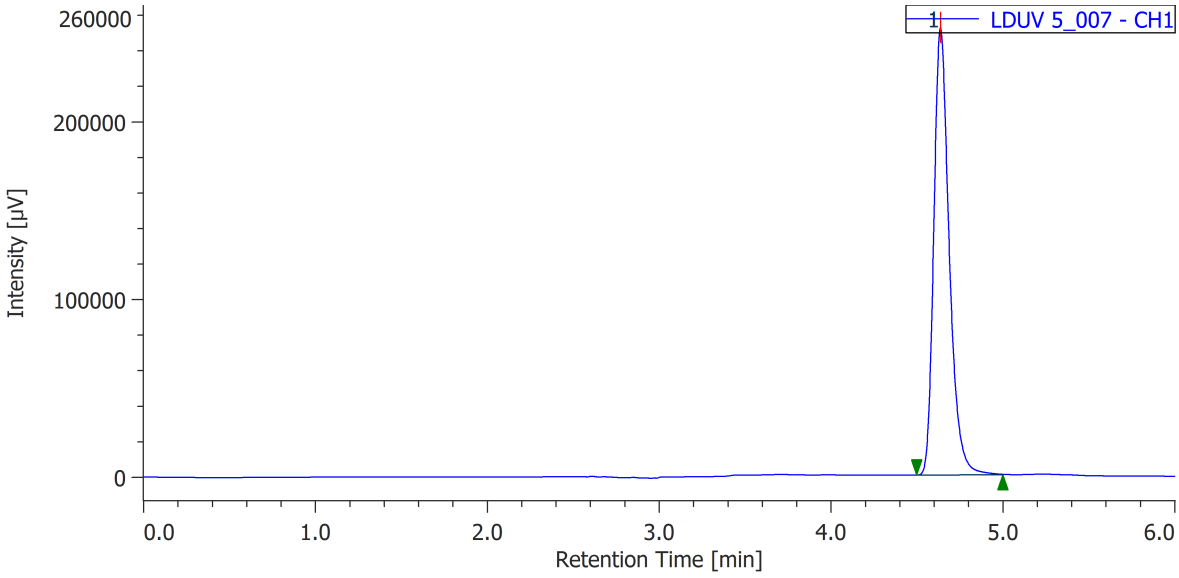

Chromatogram Information	
User Name	Administrator
Date Modified	15/10/2020 12:15:31
Description	
HPLC System Name	HPLC 0001
Injection Date	15/10/2020 12:03:05
Volume	10.0 [µL]
Sample #	15
Project Name	Qualificação
Acquisition Time	6.0 [min]
Acquisition Sequence	
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 5_007-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	4.635	1570029	251592	100.000	100.000	N/A	13707	N/A	1.311	